


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052419\
 Data File : BM020551.D
 Acq On : 24 May 2019 21:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 16:07:05 2019

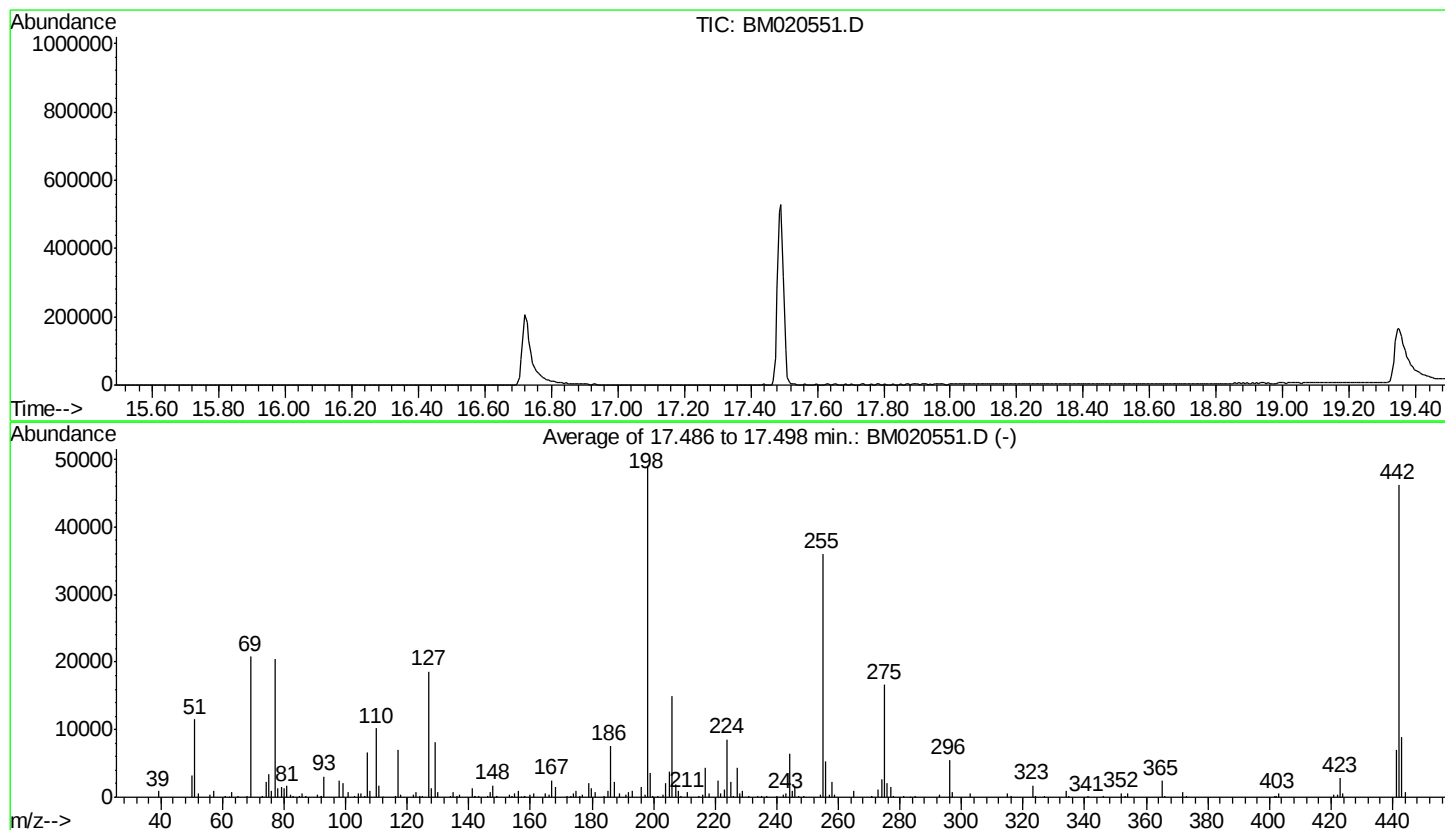

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	11479	PASS
68	69	0.00	2	1.3	260	PASS
69	198	0.00	100	42.3	20744	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.8	18550	PASS
197	198	0.00	2	0.7	330	PASS
198	198	100	100	100.0	49032	PASS
199	198	5	9	7.2	3539	PASS
275	198	10	60	33.9	16599	PASS
365	198	1	100	4.8	2376	PASS
441	198	0.01	100	14.5	7094	PASS
442	198	50	100	94.3	46261	PASS
443	442	15	24	19.1	8848	PASS