

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030175.D
 Acq On : 26 May 2021 18:46
 Operator : CG/JU
 Sample : M2495-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB439

Quant Time: May 27 02:40:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 26 15:30:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	185771	20.00	ng/ul	0.00
20) Naphthalene-d8	10.669	136	798337	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	545977	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	1176257	20.00	ng/ul	0.00
79) Chrysene-d12	21.392	240	1193183	20.00	ng/ul	0.00
88) Perylene-d12	23.686	264	1071870	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	24488	5.39	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.034	99	137123	8.40	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	418866	40.63	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	421491	34.45	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	271291	20.92	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	255363	49.00	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	249313	50.23	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.286	165	511597	39.95	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	35627	1.87	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	1983224	47.51	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	2413663	44.86	ng/ul	0.00
54) 4-Nitrophenol-d4	14.674	143	55667	8.25	ng/ul	0.00
60) Fluorene-d10	15.492	176	1778530	48.81	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	268037	47.01	ng/ul	0.00
73) Anthracene-d10	17.333	188	3122689	53.64	ng/ul	0.00
81) Pyrene-d10	19.615	212	3609258	56.43	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.544	264	3301213	54.33	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.951	163	65449	1.59	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030175.D
Acq On : 26 May 2021 18:46
Operator : CG/JU
Sample : M2495-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB439

Quant Time: May 27 02:40:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 26 15:30:24 2021
Response via : Initial Calibration

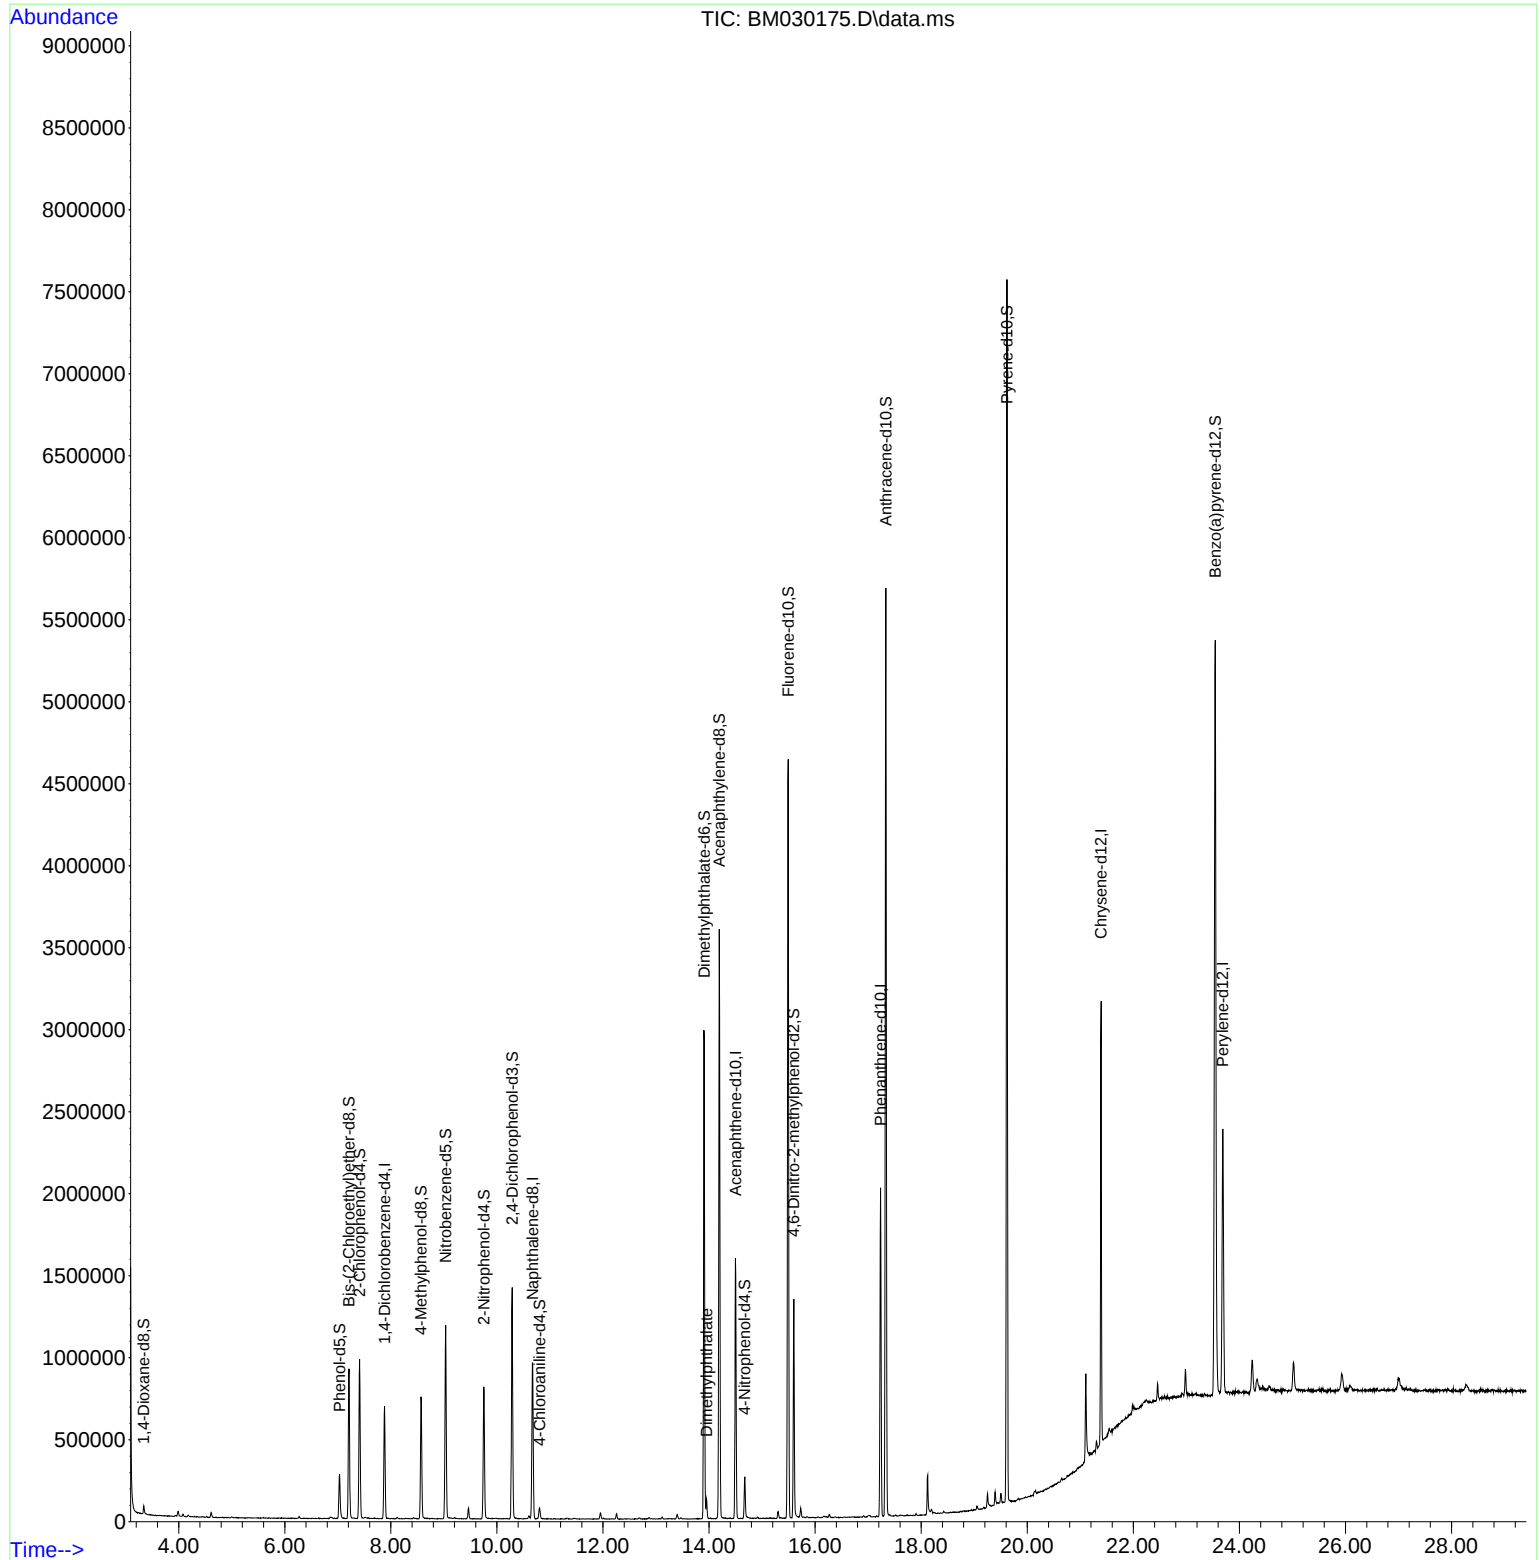

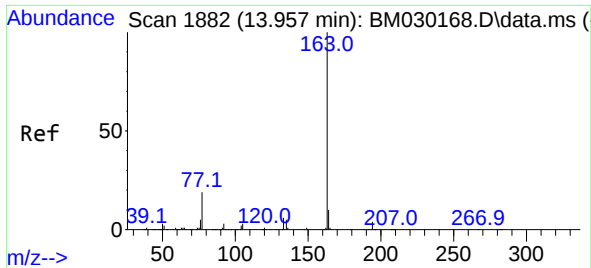

#47
 Dimethylphthalate
 Concen: 1.59 ng/ul
 RT: 13.951 min Scan# 1847
 Delta R.T. -0.006 min
 Lab File: BM030175.D
 Acq: 26 May 2021 18:46

Instrument :
 BNA_M
 ClientSampleId :
 GB439

Tgt Ion:163	Resp:	65449
Ion	Ratio	Lower Upper
163	100	
194	4.1	3.4 5.0
164	11.2	8.2 12.2

