

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030181.D
 Acq On : 26 May 2021 23:05
 Operator : CG/JU
 Sample : M2495-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB440

Quant Time: May 27 02:41:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 26 15:30:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	249004	20.00	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1084200	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	746835	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	1657348	20.00	ng/ul	0.00
79) Chrysene-d12	21.386	240	1801156	20.00	ng/ul	0.00
88) Perylene-d12	23.686	264	1726639	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	24789	4.07	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	
7) Phenol-d5	7.028	99	140410	6.41	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	394180	28.52	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	405823	24.75	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	271958	15.64	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	243796	34.45	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	236737	35.12	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	493897	28.40	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	38943	1.51	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1916891	33.57	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	2337660	31.76	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	58913	6.39	ng/ul	-0.01
60) Fluorene-d10	15.486	176	1746077	35.03	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	260630	32.44	ng/ul	0.00
73) Anthracene-d10	17.327	188	2972956	36.24	ng/ul	0.00
81) Pyrene-d10	19.615	212	3500653	36.26	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	3466805	35.42	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.951	163	61330	1.09	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030181.D
Acq On : 26 May 2021 23:05
Operator : CG/JU
Sample : M2495-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB440

Quant Time: May 27 02:41:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 26 15:30:24 2021
Response via : Initial Calibration

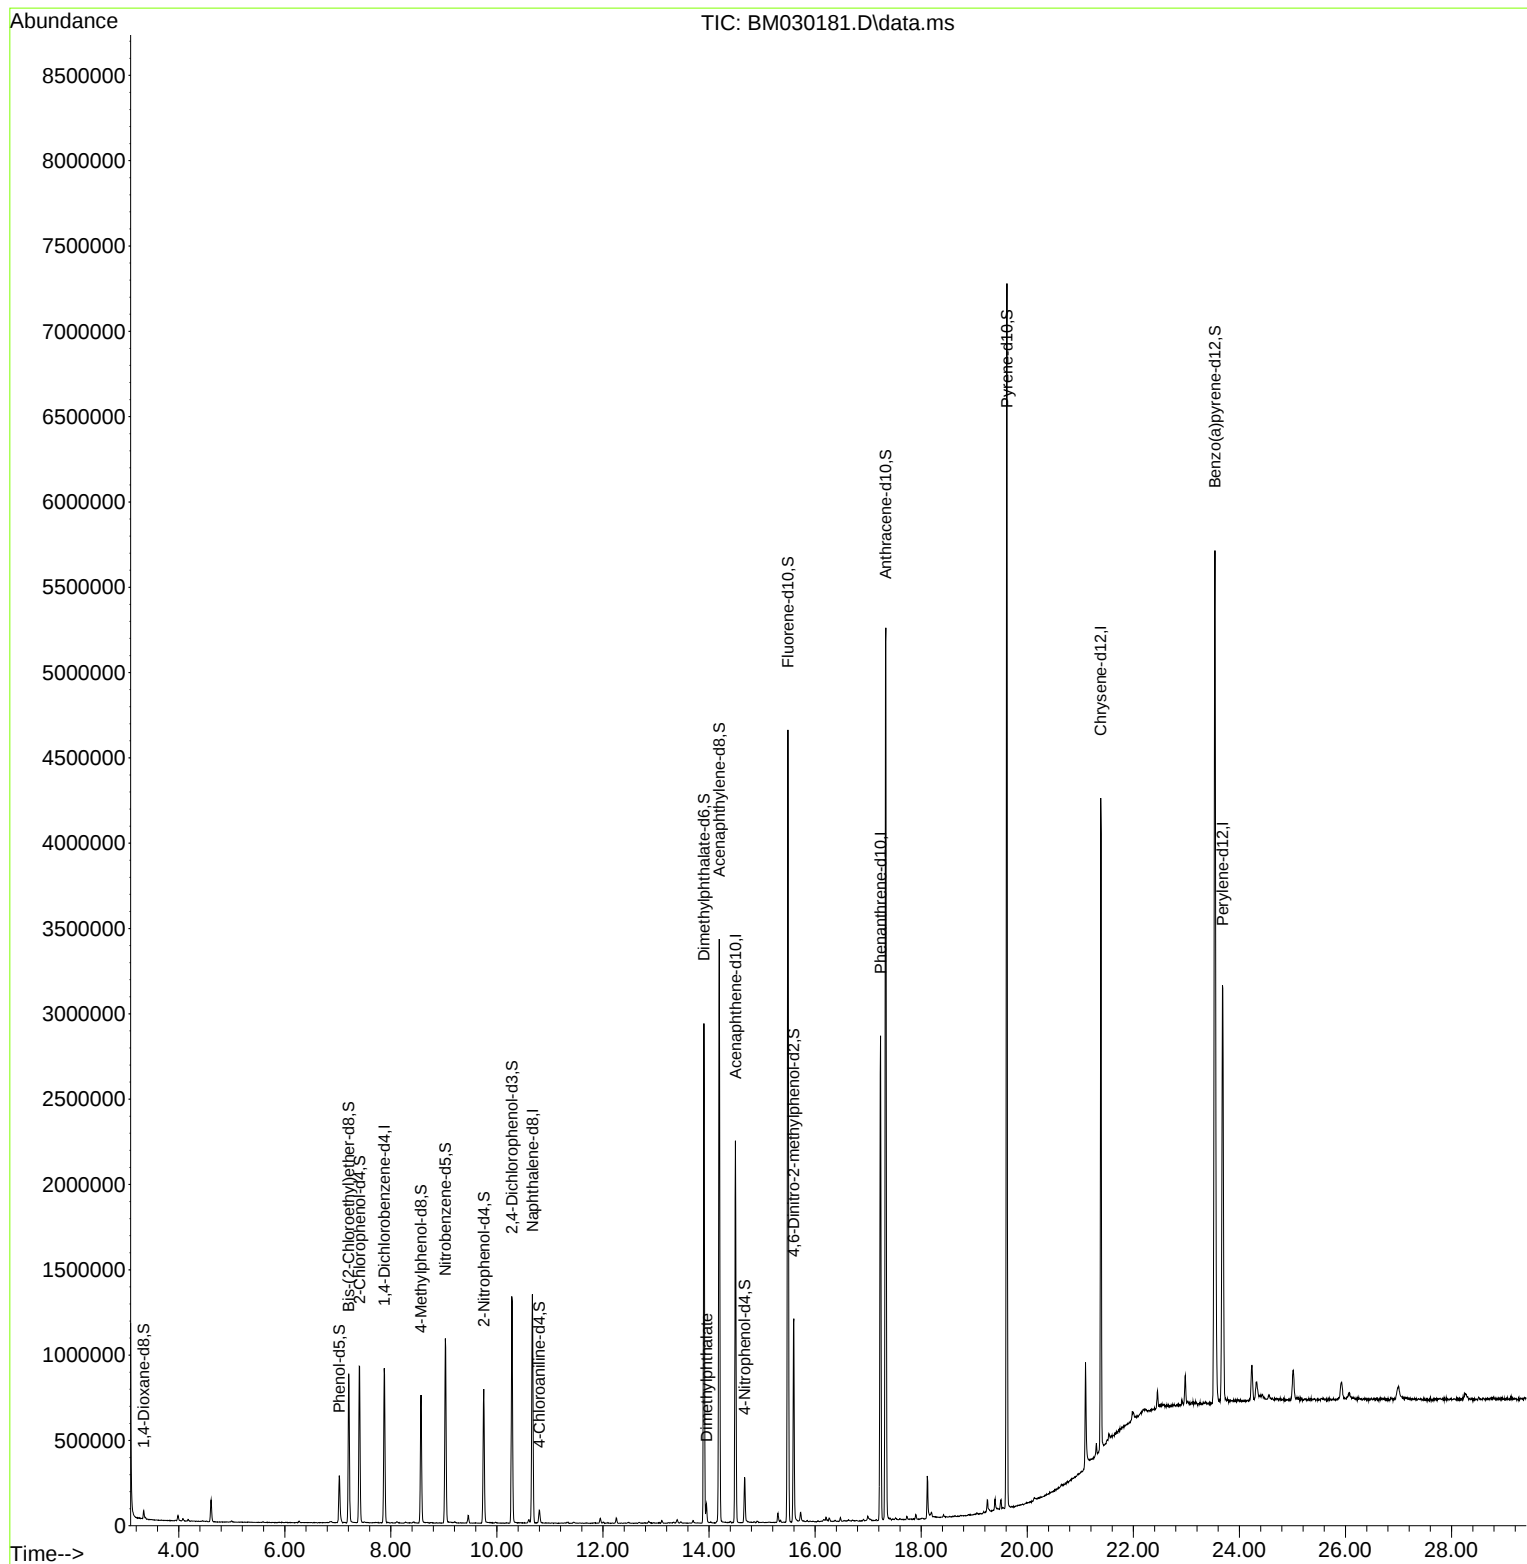

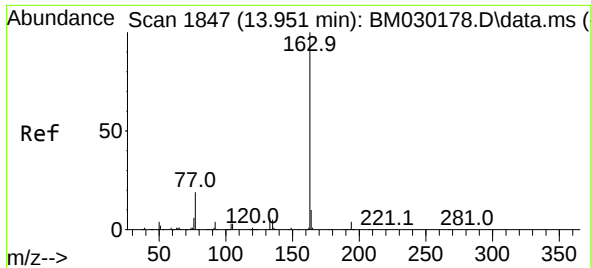

#47
 Dimethylphthalate
 Concen: 1.09 ng/ul
 RT: 13.951 min Scan# 1847
 Delta R.T. -0.006 min
 Lab File: BM030181.D
 Acq: 26 May 2021 23:05

Instrument :
 BNA_M
 ClientSampleId :
 GB440

Tgt Ion:163 Resp: 61330
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.4 5.0
 164 11.4 8.2 12.2

