

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030173.D
 Acq On : 26 May 2021 17:31
 Operator : CG/JU
 Sample : PB136652BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030173.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	53	rVB	81016	116089	1.41%	0.150%
2	3.752	109	113	140	rBV	818003	1465706	17.80%	1.893%
3	4.081	166	169	173	rVB3	12037	16141	0.20%	0.021%
4	7.034	663	671	682	rBV	1168707	1859841	22.59%	2.402%
5	7.210	692	701	710	rBV	916832	1480631	17.98%	1.912%
6	7.410	726	735	743	rBV	1167261	1869002	22.70%	2.414%
7	7.881	807	815	825	rVB	861015	1370486	16.65%	1.770%
8	8.569	925	932	946	rBV	1421247	2320700	28.19%	2.997%
9	9.034	1003	1011	1019	rBV	1093043	1813570	22.03%	2.342%
10	9.751	1126	1133	1147	rBV	764969	1274872	15.49%	1.646%
11	10.286	1215	1224	1234	rBV	1442682	2365360	28.73%	3.055%
12	10.669	1281	1289	1303	rVB	1192267	2107675	25.60%	2.722%
13	10.798	1303	1311	1322	rBV	1514106	2605298	31.65%	3.365%
14	12.257	1550	1559	1563	rBV2	31136	52636	0.64%	0.068%
15	13.910	1832	1840	1851	rBV	2887462	4079681	49.55%	5.269%
16	14.192	1880	1888	1901	rBV	3237806	4804561	58.36%	6.205%
17	14.498	1931	1940	1948	rBV	2062810	3103258	37.69%	4.008%
18	14.674	1961	1970	1985	rBV	1237097	1853941	22.52%	2.394%
19	15.316	2073	2079	2082	rBV7	5462	9775	0.12%	0.013%
20	15.486	2101	2108	2115	rBV	4159519	6114272	74.27%	7.896%
21	15.598	2120	2127	2137	rBV	1027908	1422764	17.28%	1.837%
22	15.727	2144	2149	2156	rVB2	51255	77951	0.95%	0.101%
23	16.168	2218	2224	2226	rBV7	6356	9601	0.12%	0.012%
24	16.268	2235	2241	2245	rBV5	16698	25693	0.31%	0.033%
25	16.910	2347	2350	2357	rVB8	8746	13853	0.17%	0.018%
26	17.015	2364	2368	2374	rBV3	10756	18880	0.23%	0.024%
27	17.233	2398	2405	2412	rBV	2685627	3794370	46.09%	4.900%
28	17.333	2415	2422	2433	rBV	4808128	6802502	82.63%	8.785%
29	18.121	2553	2556	2564	rBV7	21416	44674	0.54%	0.058%
30	19.251	2744	2748	2752	rBV	62686	86444	1.05%	0.112%
31	19.503	2787	2791	2794	rBV	46210	60436	0.73%	0.078%
32	19.615	2804	2810	2822	rBV	6160129	8232636	100.00%	10.632%
33	21.392	3107	3112	3117	rBV	3402990	4258155	51.72%	5.499%
34	23.544	3471	3478	3492	rVB2	4027640	7948100	96.54%	10.265%
35	23.691	3497	3503	3512	rVB2	2127843	3951062	47.99%	5.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030173.D
Acq On : 26 May 2021 17:31
Operator : CG/JU
Sample : PB136652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Title : SVOA CALIBRATION




Sum of corrected areas: 77430616

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030173.D
Acq On : 26 May 2021 17:31
Operator : CG/JU
Sample : PB136652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

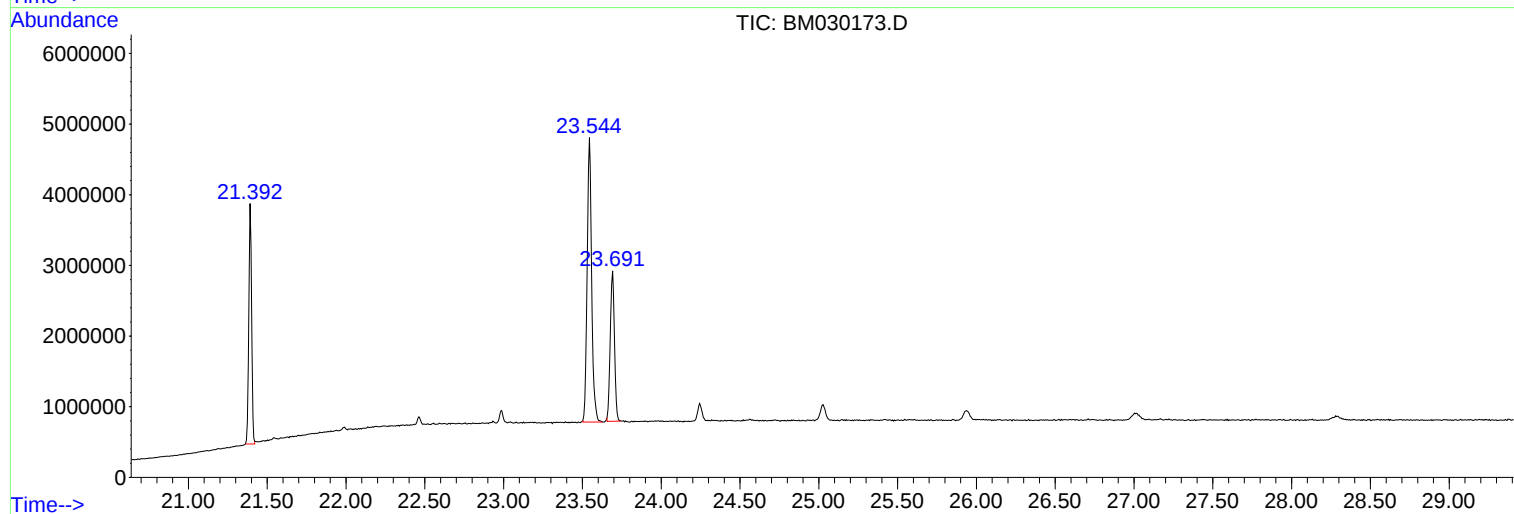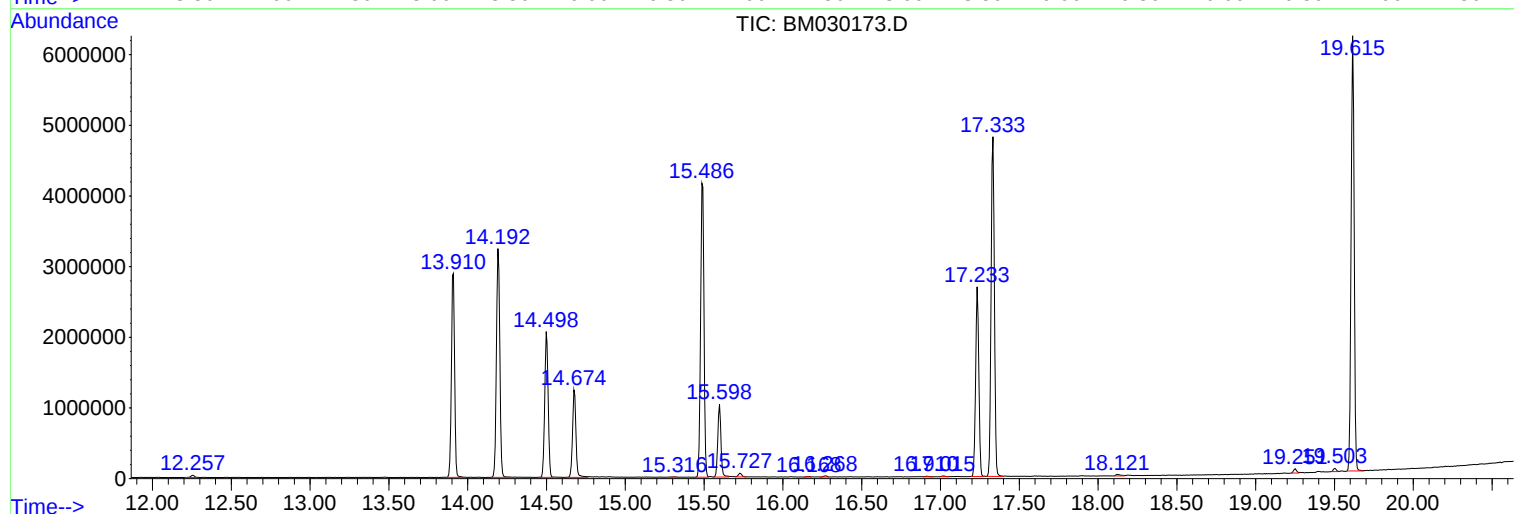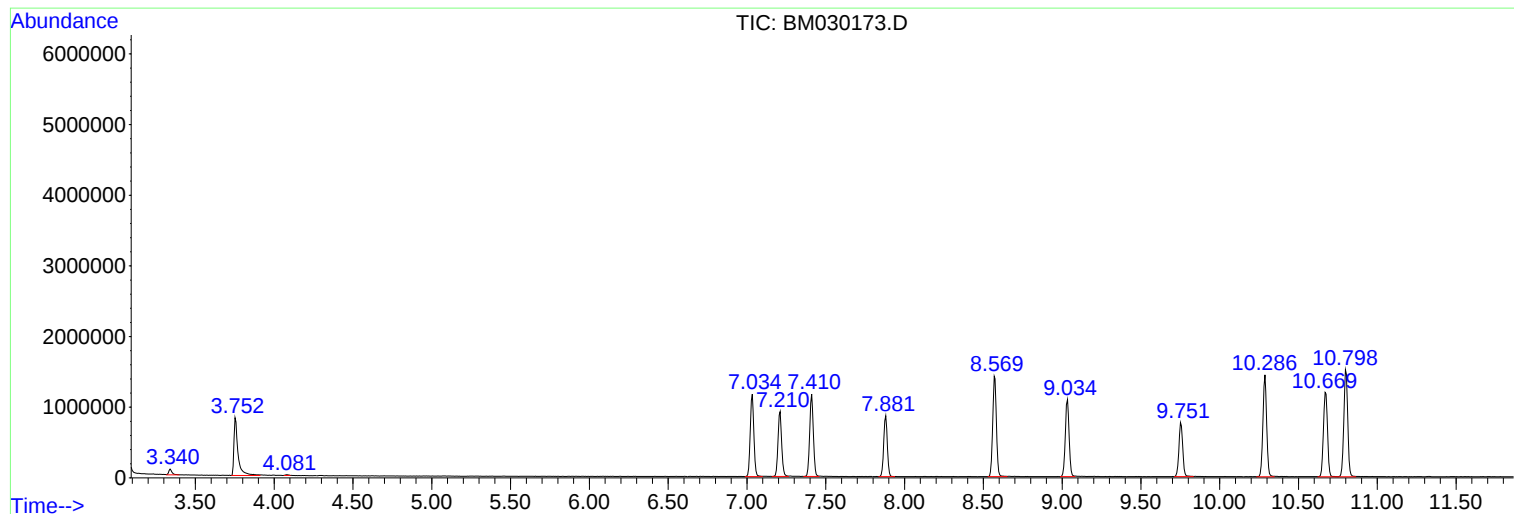

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030173.D
Acq On : 26 May 2021 17:31
Operator : CG/JU
Sample : PB136652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030173.D
Acq On : 26 May 2021 17:31
Operator : CG/JU
Sample : PB136652BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc