

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030185.D
 Acq On : 27 May 2021 01:32
 Operator : CG/JU
 Sample : M2495-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030185.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rBV	50133	61052	0.90%	0.097%
2	3.934	140	144	146	rBV3	7796	11659	0.17%	0.018%
3	3.987	149	153	161	rVB	34220	50241	0.74%	0.079%
4	4.081	166	169	174	rVB2	14581	17110	0.25%	0.027%
5	4.181	182	186	191	rBV5	13343	18596	0.27%	0.029%
6	4.522	240	244	250	rVB	13795	19777	0.29%	0.031%
7	4.610	253	259	266	rBV	40489	64517	0.95%	0.102%
8	4.993	320	324	329	rBV4	7001	11431	0.17%	0.018%
9	6.269	534	541	548	rBV3	12379	24492	0.36%	0.039%
10	7.028	662	670	681	rBV	321637	529569	7.79%	0.838%
11	7.204	694	700	713	rBV	1060831	1695367	24.92%	2.681%
12	7.404	728	734	747	rBV	1076797	1782816	26.21%	2.820%
13	7.504	749	751	757	rVB6	6746	8351	0.12%	0.013%
14	7.875	806	814	822	rBV	854755	1375916	20.23%	2.176%
15	8.110	851	854	860	rBV8	4691	7722	0.11%	0.012%
16	8.281	879	883	892	rBV8	5051	11567	0.17%	0.018%
17	8.569	923	932	940	rBV	831307	1336767	19.65%	2.114%
18	9.028	999	1010	1019	rBV	1282270	2120510	31.17%	3.354%
19	9.122	1024	1026	1031	rVB6	4917	9258	0.14%	0.015%
20	9.463	1075	1084	1089	rBV	27847	44741	0.66%	0.071%
21	9.751	1125	1133	1147	rBV	924509	1495149	21.98%	2.365%
22	9.963	1165	1169	1175	rBV7	6438	12038	0.18%	0.019%
23	10.281	1216	1223	1233	rBV	1496340	2515395	36.98%	3.978%
24	10.669	1280	1289	1296	rBV	1203533	2002918	29.44%	3.168%
25	11.445	1416	1421	1426	rBV6	13084	25363	0.37%	0.040%
26	11.945	1498	1506	1511	rBV	22521	40341	0.59%	0.064%
27	11.998	1511	1515	1524	rVB6	10301	18915	0.28%	0.030%
28	12.251	1551	1558	1566	rVB2	33643	60480	0.89%	0.096%
29	12.863	1656	1662	1667	rBV4	14482	24741	0.36%	0.039%
30	13.110	1699	1704	1710	rBV2	25670	40916	0.60%	0.065%
31	13.404	1747	1754	1759	rVB7	6263	11112	0.16%	0.018%
32	13.463	1759	1764	1769	rBV5	9604	12736	0.19%	0.020%
33	13.698	1800	1804	1809	rBV6	5056	8686	0.13%	0.014%
34	13.904	1832	1839	1850	rBV	2890386	3946029	58.01%	6.241%
35	14.027	1856	1860	1866	rVB9	5093	11229	0.17%	0.018%
36	14.192	1876	1888	1900	rBV	3302367	4821904	70.89%	7.626%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030185.D
 Acq On : 27 May 2021 01:32
 Operator : CG/JU
 Sample : M2495-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB456

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	14.498	1933	1940	1951	rVB	1833722	2685123	39.47%	4.247%
38	14.669	1963	1969	1974	rBV	199290	301315	4.43%	0.477%
39	14.716	1974	1977	1982	rVB2	12951	18218	0.27%	0.029%
40	14.904	2006	2009	2014	rBV6	8098	11678	0.17%	0.018%
41	15.233	2059	2065	2072	rBV	141141	192579	2.83%	0.305%
42	15.298	2072	2076	2083	rVB2	33407	60293	0.89%	0.095%
43	15.486	2098	2108	2116	rBV	4381740	6140064	90.26%	9.711%
44	15.592	2120	2126	2139	rBV	1017340	1391400	20.45%	2.201%
45	15.727	2144	2149	2154	rVB	47278	74636	1.10%	0.118%
46	15.845	2163	2169	2174	rBV9	9667	17156	0.25%	0.027%
47	16.163	2220	2223	2226	rBV5	4783	6902	0.10%	0.011%
48	16.263	2237	2240	2244	rBV2	15223	21918	0.32%	0.035%
49	16.910	2347	2350	2355	rBV6	9488	13177	0.19%	0.021%
50	17.015	2366	2368	2374	rVB2	7624	12382	0.18%	0.020%
51	17.227	2398	2404	2414	rBV	1994287	2909449	42.77%	4.602%
52	17.327	2414	2421	2433	rBV	4505271	6280997	92.34%	9.934%
53	17.515	2449	2453	2458	rVB3	10742	14595	0.21%	0.023%
54	17.898	2515	2518	2522	rVB6	9302	12778	0.19%	0.020%
55	18.115	2551	2555	2561	rBV3	32870	53591	0.79%	0.085%
56	18.192	2564	2568	2573	rVB	29421	44673	0.66%	0.071%
57	19.245	2743	2747	2750	rBV	47689	66415	0.98%	0.105%
58	19.386	2768	2771	2778	rBV7	25098	39618	0.58%	0.063%
59	19.498	2786	2790	2794	rBV	41123	58345	0.86%	0.092%
60	19.609	2803	2809	2820	rBV	4950439	6802381	100.00%	10.759%
61	21.386	3106	3111	3121	rBV	2257051	2877127	42.30%	4.550%
62	23.533	3469	3476	3488	rBV2	3069970	6124285	90.03%	9.686%
63	23.680	3495	3501	3510	rVB2	1436087	2746471	40.38%	4.344%


Sum of corrected areas: 63226977

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030185.D
Acq On : 27 May 2021 01:32
Operator : CG/JU
Sample : M2495-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB456

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

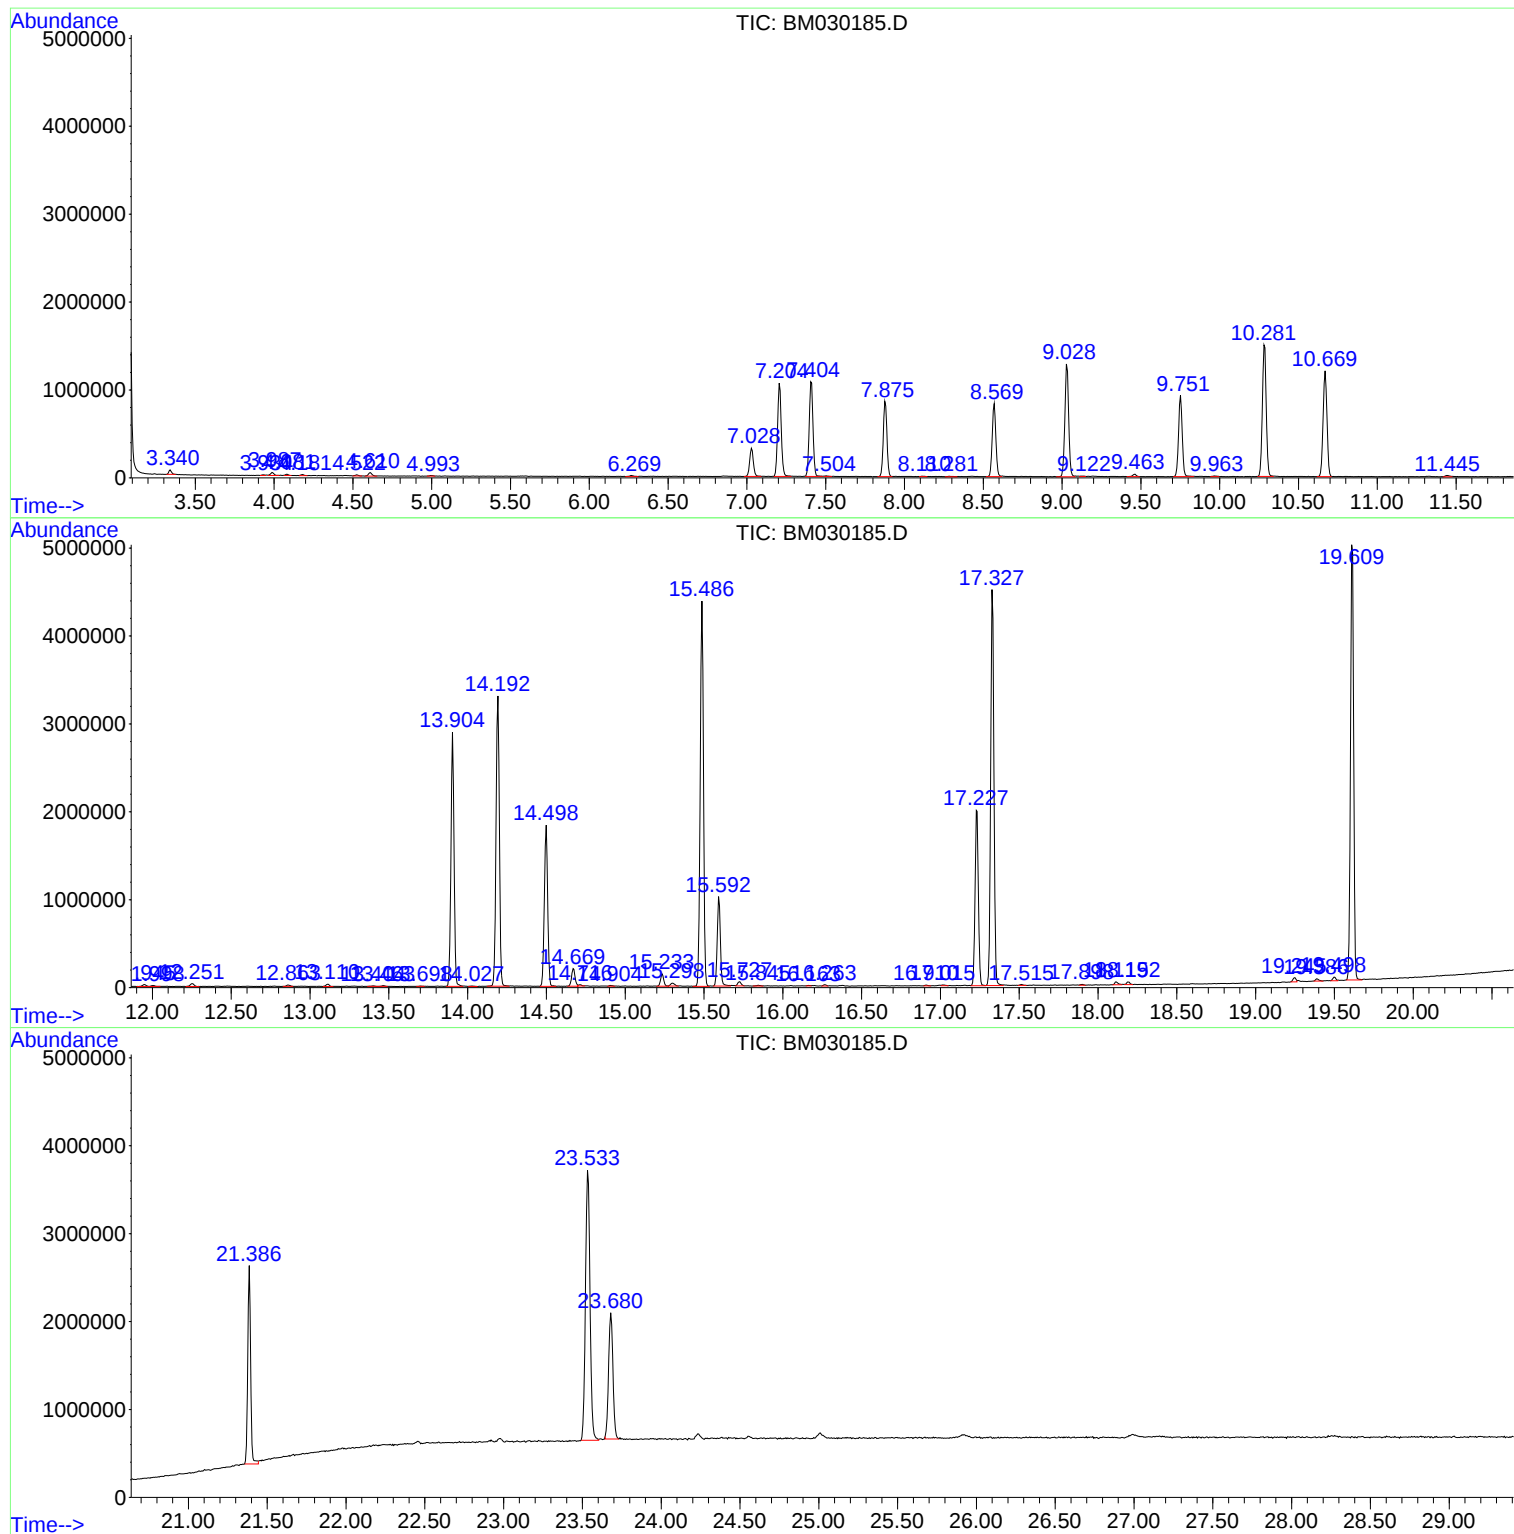

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030185.D
Acq On : 27 May 2021 01:32
Operator : CG/JU
Sample : M2495-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB456

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030185.D
Acq On : 27 May 2021 01:32
Operator : CG/JU
Sample : M2495-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB456

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------