

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030189.D
 Acq On : 27 May 2021 03:58
 Operator : CG/JU
 Sample : M2495-17
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB459

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030189.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	47	rBV	45954	61758	0.97%	0.102%
2	3.381	47	50	53	rVB	18693	22373	0.35%	0.037%
3	3.987	147	153	159	rVB2	31431	48833	0.76%	0.080%
4	4.081	165	169	173	rVB	18515	22821	0.36%	0.038%
5	4.175	181	185	192	rVB	27489	39573	0.62%	0.065%
6	4.516	241	243	250	rVB6	5142	8776	0.14%	0.014%
7	5.705	441	445	450	rBV2	8373	11851	0.19%	0.020%
8	6.269	536	541	543	rBV	10348	12436	0.19%	0.020%
9	6.558	585	590	593	rBV6	3567	6780	0.11%	0.011%
10	7.028	662	670	680	rVB	264310	411899	6.44%	0.679%
11	7.205	694	700	714	rBV	962611	1542890	24.12%	2.543%
12	7.405	727	734	744	rBV	994733	1600228	25.01%	2.637%
13	7.875	807	814	822	rBV	1011175	1603199	25.06%	2.642%
14	8.569	920	932	944	rBV	716539	1153917	18.04%	1.902%
15	8.699	951	954	958	rVB6	5803	7776	0.12%	0.013%
16	9.028	1001	1010	1018	rBV	1166001	1893198	29.59%	3.120%
17	9.269	1047	1051	1057	rVB3	9411	15261	0.24%	0.025%
18	9.751	1125	1133	1142	rBV	787250	1319332	20.62%	2.174%
19	9.963	1165	1169	1173	rBV6	4889	9042	0.14%	0.015%
20	10.281	1215	1223	1231	rBV	1351437	2228415	34.83%	3.672%
21	10.475	1250	1256	1261	rBV7	6969	14102	0.22%	0.023%
22	10.669	1281	1289	1297	rBV	1330202	2274109	35.54%	3.748%
23	10.810	1311	1313	1319	rVB7	5690	6537	0.10%	0.011%
24	11.322	1393	1400	1406	rVB8	6589	14509	0.23%	0.024%
25	11.445	1416	1421	1429	rBV7	15112	30926	0.48%	0.051%
26	11.922	1495	1502	1509	rBV	63673	106900	1.67%	0.176%
27	11.998	1509	1515	1521	rVB7	14629	29615	0.46%	0.049%
28	12.251	1552	1558	1563	rVB	28760	48637	0.76%	0.080%
29	12.863	1657	1662	1669	rBV6	11027	19303	0.30%	0.032%
30	12.951	1673	1677	1680	rVV6	4732	6559	0.10%	0.011%
31	13.039	1687	1692	1697	rBV	17891	26165	0.41%	0.043%
32	13.110	1699	1704	1711	rVB3	18207	26545	0.41%	0.044%
33	13.398	1745	1753	1758	rBV7	10407	18363	0.29%	0.030%
34	13.469	1761	1765	1769	rVB5	6803	10988	0.17%	0.018%
35	13.698	1799	1804	1813	rBV5	3800	10334	0.16%	0.017%
36	13.904	1832	1839	1852	rBV	2467816	3379637	52.82%	5.570%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030189.D
 Acq On : 27 May 2021 03:58
 Operator : CG/JU
 Sample : M2495-17
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB459

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	14.051	1859	1864	1872	rVB7	21586	36281	0.57%	0.060%
38	14.192	1875	1888	1895	rBV	2803909	4139111	64.69%	6.821%
39	14.498	1928	1940	1949	rBV	1956992	2989285	46.72%	4.926%
40	14.669	1963	1969	1974	rBV	168882	256511	4.01%	0.423%
41	14.710	1974	1976	1980	rVV2	32361	41771	0.65%	0.069%
42	14.751	1980	1983	1988	rVB6	5990	9622	0.15%	0.016%
43	14.904	2006	2009	2014	rBV6	8264	12673	0.20%	0.021%
44	15.239	2061	2066	2070	rBV5	5155	8132	0.13%	0.013%
45	15.304	2071	2077	2081	rVV2	19305	36727	0.57%	0.061%
46	15.486	2101	2108	2115	rBV	3791521	5312638	83.04%	8.755%
47	15.592	2120	2126	2138	rBV	884156	1210316	18.92%	1.995%
48	15.722	2143	2148	2153	rVB	43933	69062	1.08%	0.114%
49	15.845	2166	2169	2173	rBV6	10917	13988	0.22%	0.023%
50	15.939	2182	2185	2192	rVB6	10335	15270	0.24%	0.025%
51	16.051	2200	2204	2208	rBV6	4688	8155	0.13%	0.013%
52	16.175	2221	2225	2227	rBV5	6292	7132	0.11%	0.012%
53	16.269	2234	2241	2247	rBV5	12885	23420	0.37%	0.039%
54	16.827	2333	2336	2340	rBV4	9591	12782	0.20%	0.021%
55	16.916	2347	2351	2354	rVB5	5236	7521	0.12%	0.012%
56	17.016	2366	2368	2372	rVB2	10804	11475	0.18%	0.019%
57	17.151	2387	2391	2395	rBV6	5790	6707	0.10%	0.011%
58	17.227	2398	2404	2415	rVV	2197969	3179371	49.69%	5.240%
59	17.327	2415	2421	2432	rBV	3945773	5587168	87.33%	9.208%
60	17.510	2450	2452	2457	rVB2	12333	12484	0.20%	0.021%
61	17.898	2514	2518	2520	rBV5	8232	10239	0.16%	0.017%
62	18.116	2551	2555	2562	rBV5	21412	35648	0.56%	0.059%
63	18.192	2563	2568	2573	rVB	43054	59191	0.93%	0.098%
64	19.245	2743	2747	2755	rBV2	46719	80001	1.25%	0.132%
65	19.386	2769	2771	2776	rVB6	16776	19347	0.30%	0.032%
66	19.498	2787	2790	2795	rVB	36168	45489	0.71%	0.075%
67	19.610	2803	2809	2816	rBV	4758529	6242254	97.57%	10.287%
68	21.386	3106	3111	3116	rBV	2601558	3267226	51.07%	5.384%
69	23.533	3469	3476	3488	rVB	3442237	6397955	100.00%	10.544%
70	23.680	3494	3501	3514	rVB2	1744061	3470760	54.25%	5.720%




Sum of corrected areas: 60679299

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030189.D
Acq On : 27 May 2021 03:58
Operator : CG/JU
Sample : M2495-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB459

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

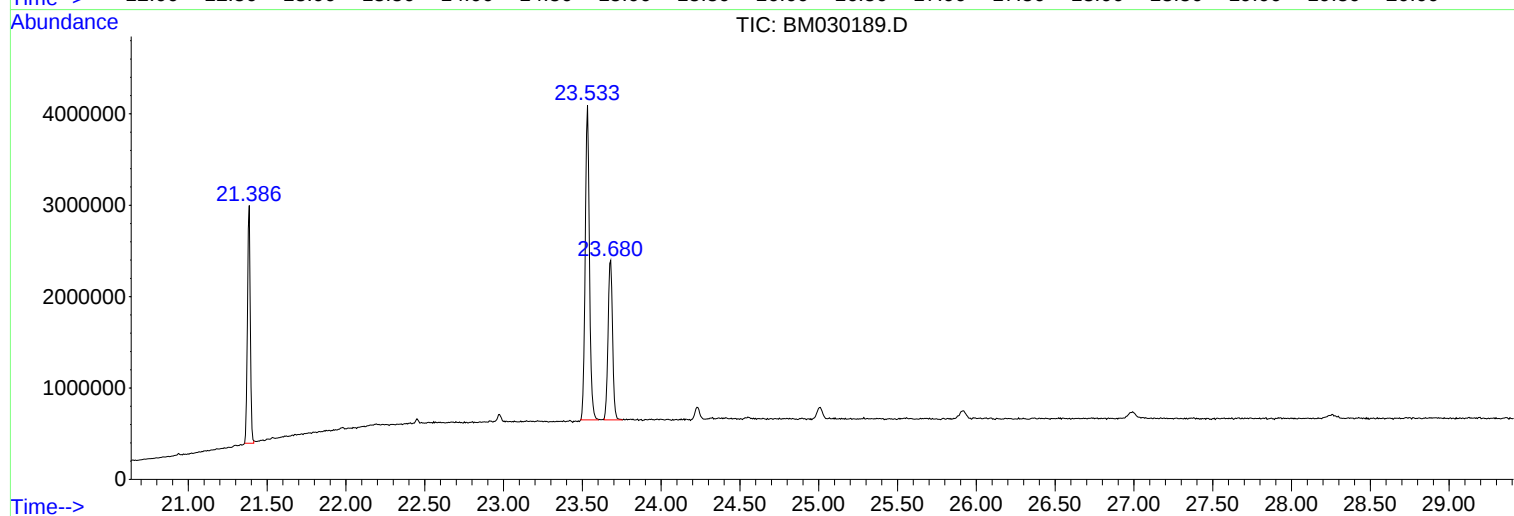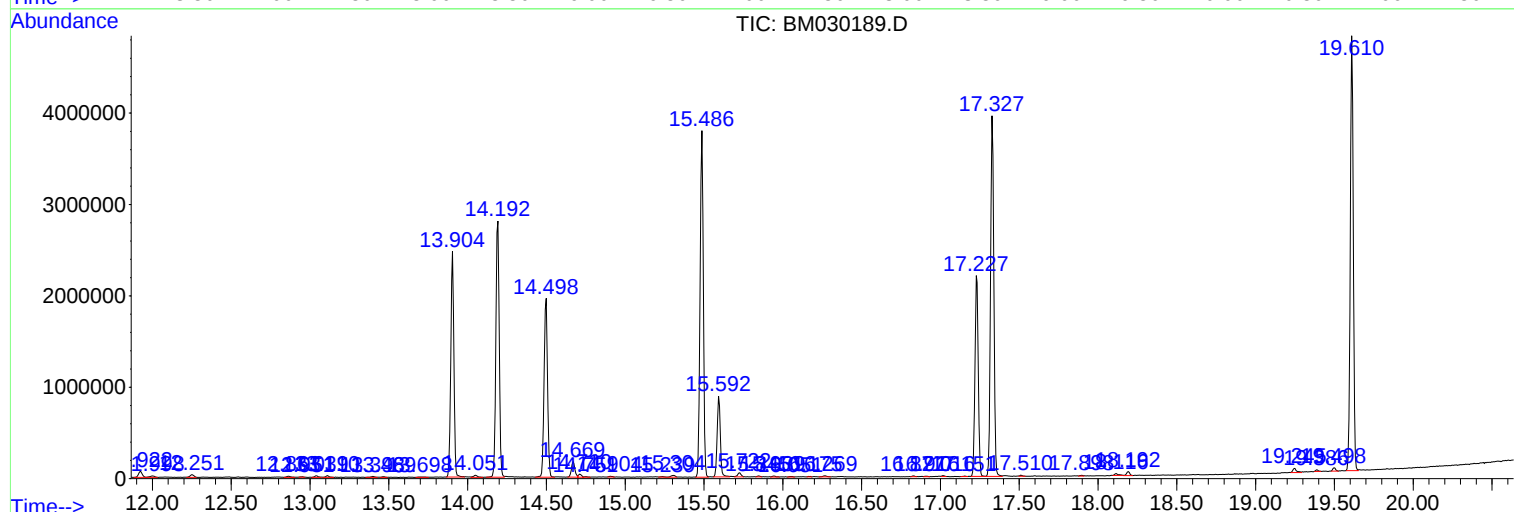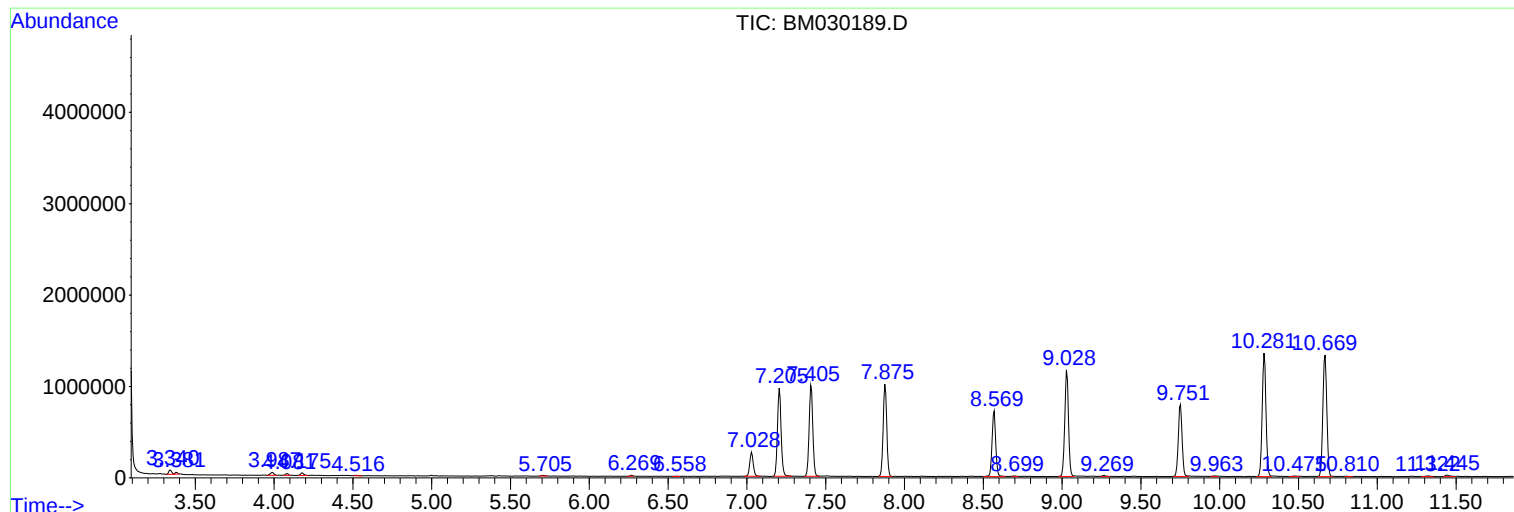

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030189.D
Acq On : 27 May 2021 03:58
Operator : CG/JU
Sample : M2495-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB459

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
Data File : BM030189.D
Acq On : 27 May 2021 03:58
Operator : CG/JU
Sample : M2495-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB459

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
