
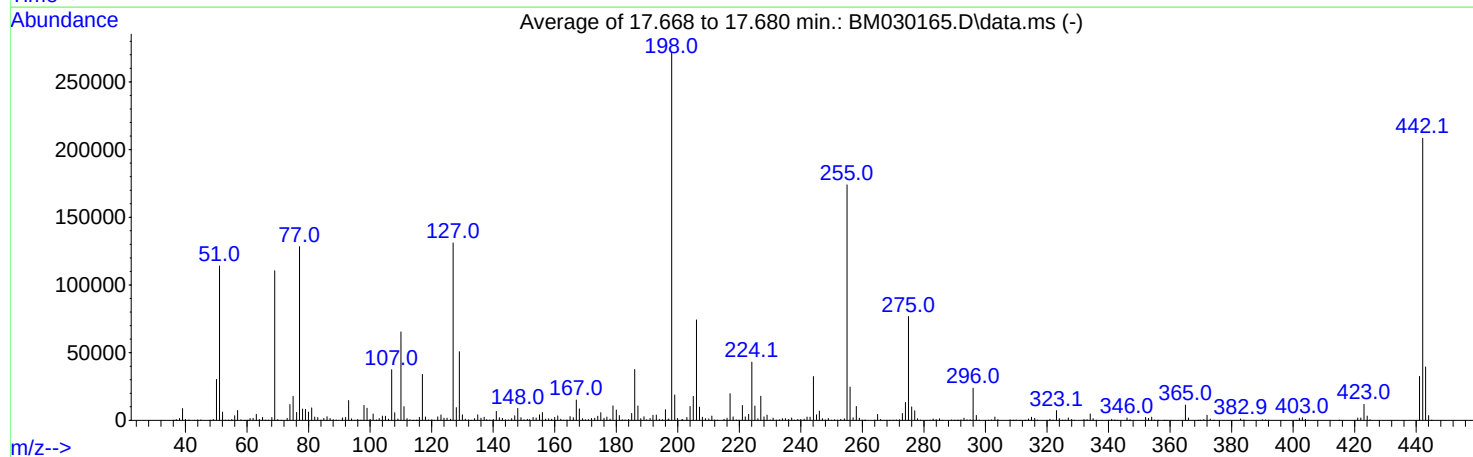


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052621\
 Data File : BM030165.D
 Acq On : 26 May 2021 11:12
 Operator : CG/JU
 Sample : DFTPP14
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP014

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION
 Last Update : Thu May 27 10:27:00 2021

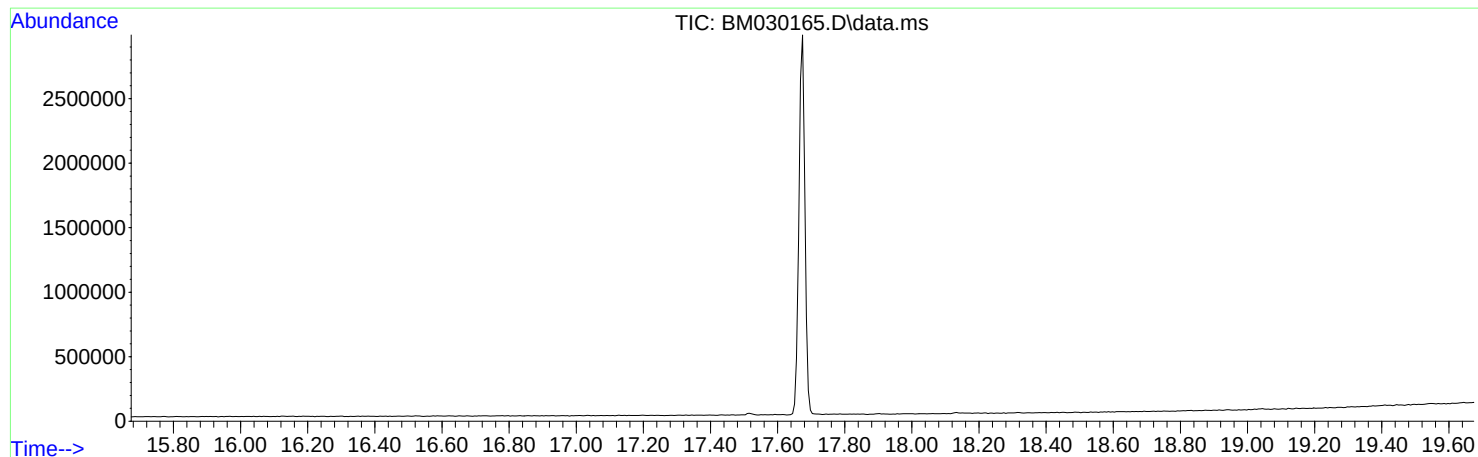

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	114106	PASS
68	69	0.00	2	1.9	2102	PASS
69	198	0.00	100	40.7	110509	PASS
70	69	0.00	2	0.5	571	PASS
127	198	10	80	48.2	131083	PASS
197	198	0.00	2	0.4	1104	PASS
198	198	100	100	100.0	271701	PASS
199	198	5	9	6.9	18749	PASS
275	198	10	60	28.2	76752	PASS
365	198	1	100	4.2	11394	PASS
441	198	0.01	100	12.0	32475	PASS
442	198	50	100	76.7	208341	PASS
443	442	15	24	19.0	39493	PASS

m/z	Abundance
36.00	293.0
37.00	529.0
38.10	1903.0
39.10	10660.0
40.00	1909.0
41.10	1257.0
42.10	240.0
43.00	832.0
44.10	9014.0
45.00	638.0
47.90	165.0
49.00	1531.0
50.10	35352.0
51.10	134400.0
52.10	7313.0
52.90	486.0
54.00	300.0
55.10	1634.0
56.00	4558.0
57.00	8867.0
58.00	422.0
59.00	313.0
61.00	1791.0
62.00	1856.0
63.00	5693.0
64.00	791.0
65.00	2517.0
66.00	236.0
67.00	540.0
68.00	2175.0
69.00	130248.0
70.00	1070.0
71.10	329.0
73.10	3868.0
74.00	13776.0
75.10	19920.0
76.10	7047.0
77.10	149248.0
78.10	10391.0
79.00	9248.0
80.00	6923.0
81.00	11056.0
82.00	2757.0
83.00	2514.0
84.00	720.0
84.90	1550.0
86.00	3188.0
87.00	1499.0
88.10	399.0
89.00	321.0
91.00	2560.0
92.00	2184.0
93.00	17616.0
94.00	1323.0
95.10	351.0
96.00	1182.0
96.90	510.0
98.00	12942.0
99.00	10307.0
100.00	1024.0
101.00	4993.0
102.10	407.0
102.90	1783.0
104.00	3468.0
105.00	3428.0
106.00	1107.0
107.00	42936.0
108.00	6152.0
109.00	1302.0
110.00	73712.0
111.00	10824.0
112.00	1313.0
112.90	464.0
115.00	392.0
116.00	2606.0
117.00	37000.0
118.00	2920.0
119.00	658.0
120.00	618.0
121.00	359.0
122.00	2848.0
123.00	4407.0
124.00	1827.0
125.00	1846.0
126.10	810.0
127.00	143232.0
128.00	10327.0
129.00	55592.0
130.00	4902.0
131.00	796.0
132.00	511.0
133.00	967.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

134.00	1703.0
135.00	5474.0
136.00	1974.0
137.00	2382.0
137.90	680.0
138.90	278.0
140.00	735.0
141.00	6849.0
142.00	2316.0
143.00	1708.0
144.00	670.0
144.90	480.0
146.00	1199.0
147.00	4579.0
148.00	9684.0
149.00	2228.0
150.00	541.0
151.10	915.0
151.90	655.0
153.00	2061.0
154.00	1796.0
155.00	4549.0
156.00	6116.0
157.10	1073.0
158.00	1284.0
159.00	959.0
160.00	2504.0
161.00	3520.0
162.00	1108.0
163.00	397.0
164.00	368.0
165.00	2981.0
166.00	2172.0
167.00	15388.0
168.00	9224.0
169.10	1512.0
169.90	469.0
170.90	507.0
171.90	1314.0
173.00	1843.0
174.00	3027.0
175.00	6190.0
176.00	1857.0
177.00	3116.0
178.00	1030.0
179.00	11872.0
180.00	8644.0
181.00	4321.0
181.90	423.0
182.90	332.0
184.00	846.0
185.00	5542.0
186.00	39656.0
187.00	11472.0
188.00	1605.0
189.00	2718.0
190.00	579.0
191.00	2337.0
192.00	4289.0
193.00	5306.0
194.00	1084.0
195.00	563.0
196.00	8020.0
196.80	1339.0
197.10	1406.0
198.00	283712.0
199.00	20224.0
199.90	1629.0
201.40	1374.0
202.90	2070.0
204.00	10668.0
205.10	18400.0
206.10	75520.0
207.10	19688.0
208.00	4093.0
209.10	2073.0
210.10	1144.0
211.00	3449.0
213.00	184.0
215.00	998.0
216.00	1845.0
217.00	19752.0
218.00	2825.0
219.10	401.0
219.90	263.0
221.10	12357.0
222.00	2766.0
223.00	4788.0
224.00	44512.0
225.10	11324.0
226.00	1372.0
227.00	17384.0
228.00	2873.0
229.00	3916.0
230.00	433.0
231.00	1726.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

232.00	317.0
233.00	591.0
234.00	1217.0
235.00	1490.0
236.00	770.0
237.00	1925.0
238.00	404.0
239.00	689.0
240.00	519.0
241.10	975.0
242.00	2593.0
243.00	2534.0
244.10	33224.0
245.00	4187.0
246.00	6742.0
247.00	1410.0
248.00	319.0
248.90	1754.0
249.90	288.0
250.90	477.0
251.90	255.0
253.00	1005.0
254.10	947.0
255.00	174080.0
256.00	25424.0
257.00	2212.0
258.00	10118.0
259.00	1609.0
260.00	228.0
260.80	245.0
264.10	356.0
265.00	4618.0
266.00	692.0
267.00	398.0
269.10	158.0
270.10	169.0
270.90	282.0
272.10	546.0
273.00	5150.0
274.00	13137.0
275.00	74368.0
276.00	10167.0
277.00	6743.0
278.00	1123.0
278.90	155.0
281.00	2031.0
282.00	756.0
283.10	1434.0
284.00	562.0
285.10	1085.0
286.00	280.0
289.00	424.0
290.00	183.0
290.90	173.0
292.10	363.0
293.00	1654.0
294.00	594.0
295.10	701.0
296.00	22560.0
297.00	3297.0
298.00	241.0
300.90	336.0
302.00	257.0
303.10	2347.0
304.10	420.0
308.00	588.0
308.90	164.0
309.90	317.0
311.00	158.0
312.80	172.0
314.00	984.0
315.00	2325.0
316.00	1428.0
316.90	181.0
321.00	721.0
322.00	290.0
323.10	6900.0
324.00	1307.0
325.10	204.0
325.90	204.0
327.00	1649.0
328.00	624.0
328.90	165.0
332.00	674.0
333.10	551.0
334.00	4089.0
335.00	1270.0
341.10	1064.0
342.10	340.0
343.00	203.0
346.00	1566.0
346.80	311.0
347.10	298.0
352.10	1969.0
353.00	1494.0
354.00	2175.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

355.10	659.0
356.10	193.0
365.00	10007.0
366.00	1629.0
369.90	242.0
370.90	495.0
372.00	3413.0
373.00	826.0
382.90	908.0
383.80	372.0
390.00	457.0
391.10	336.0
392.00	197.0
401.10	351.0
402.00	1150.0
403.00	1621.0
404.00	652.0
415.00	172.0
421.00	1343.0
422.00	1685.0
423.00	10210.0
424.00	3022.0
424.90	394.0
441.00	27656.0
442.10	170624.0
443.00	33504.0
444.00	2986.0
445.10	261.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

m/z	Abundance
36.00	408.0
37.00	632.0
38.10	1887.0
39.10	11330.0
40.00	1852.0
41.10	1118.0
42.00	512.0
43.10	838.0
44.00	9233.0
45.00	778.0
46.90	167.0
49.00	1546.0
50.10	36272.0
51.10	132416.0
52.00	7204.0
53.00	509.0
54.00	180.0
55.10	1445.0
56.00	4423.0
57.00	8667.0
58.00	762.0
59.10	267.0
61.00	1680.0
62.00	1759.0
63.00	4545.0
64.00	702.0
65.10	2547.0
66.00	325.0
67.10	506.0
68.10	2516.0
69.00	127736.0
70.00	626.0
71.10	287.0
73.10	4764.0
74.00	13758.0
75.00	21552.0
76.10	6718.0
77.10	148672.0
78.10	10438.0
79.00	10015.0
80.00	7701.0
81.00	10790.0
82.00	2868.0
83.00	2663.0
84.00	589.0
85.00	1841.0
86.00	3371.0
87.00	1673.0
88.00	494.0
88.90	326.0
91.00	2426.0
92.00	2767.0
93.00	16137.0
93.90	1435.0
95.00	474.0
96.00	1581.0
97.00	503.0
98.00	12911.0
99.00	10399.0
100.00	1005.0
101.00	5503.0
102.00	340.0
103.00	2076.0
104.00	3818.0
105.00	3863.0
106.00	990.0
107.00	44248.0
108.00	6803.0
109.10	1189.0
110.00	76904.0
111.00	12432.0
112.00	1798.0
113.00	507.0
113.90	152.0
115.20	381.0
116.00	2303.0
117.00	39520.0
118.00	3034.0
119.00	626.0
120.10	506.0
121.00	361.0
122.00	2854.0
123.00	4396.0
124.00	2116.0
125.00	2079.0
126.20	1036.0
127.00	156160.0
128.00	11467.0
129.00	60496.0
130.00	4691.0
131.00	1108.0
132.00	636.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

133.00	705.0
134.00	1737.0
135.00	4972.0
136.00	1898.0
137.00	2765.0
137.90	656.0
139.00	448.0
140.10	1000.0
141.00	8182.0
142.00	2321.0
143.00	1867.0
144.00	621.0
145.00	411.0
146.00	1503.0
147.00	5157.0
148.00	10334.0
149.00	2873.0
150.00	526.0
151.00	1178.0
151.80	718.0
153.00	2737.0
154.00	2133.0
155.10	4735.0
156.00	7209.0
157.10	1093.0
158.00	1506.0
159.00	1243.0
160.00	2657.0
161.00	3774.0
162.00	1058.0
162.90	454.0
163.90	587.0
165.00	3595.0
166.10	2466.0
167.00	17416.0
168.00	10009.0
169.00	1433.0
170.00	677.0
171.00	668.0
172.00	1844.0
173.00	1811.0
174.00	3769.0
175.00	6827.0
176.00	1810.0
177.00	3462.0
178.00	1130.0
179.00	12926.0
180.00	8974.0
181.00	4041.0
182.00	701.0
182.90	446.0
184.00	881.0
185.00	6101.0
186.00	44512.0
187.00	12438.0
188.00	1551.0
189.00	3150.0
189.90	698.0
191.00	2533.0
192.00	4887.0
193.00	5385.0
194.00	1173.0
195.00	786.0
196.00	9795.0
197.10	1907.0
198.00	321152.0
199.00	22096.0
200.00	1792.0
201.60	1342.0
203.00	2452.0
204.00	12088.0
205.00	20776.0
206.10	90016.0
207.00	20576.0
208.00	5088.0
209.00	2038.0
210.10	1409.0
211.00	3512.0
212.10	639.0
213.00	396.0
215.00	1010.0
216.00	1873.0
217.00	23544.0
218.00	3174.0
219.00	314.0
219.90	512.0
221.00	13986.0
221.90	3494.0
223.00	5515.0
224.10	51352.0
225.00	11983.0
226.10	1907.0
227.00	21320.0
228.00	2926.0
229.00	4332.0
230.10	415.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

231.00	2208.0
232.00	333.0
232.90	414.0
234.00	1769.0
235.00	1599.0
236.00	902.0
237.00	2174.0
237.90	243.0
239.00	973.0
240.00	1067.0
241.00	1443.0
242.00	3139.0
243.00	2530.0
244.10	38592.0
245.10	5089.0
246.00	8196.0
247.00	1547.0
248.00	305.0
249.00	1718.0
250.00	374.0
251.00	673.0
251.90	642.0
253.00	955.0
254.10	1610.0
255.00	206336.0
256.00	28296.0
257.00	2098.0
258.00	12396.0
259.00	2253.0
259.90	257.0
261.00	345.0
264.00	349.0
265.00	5279.0
265.90	769.0
266.90	502.0
267.90	211.0
268.80	204.0
270.00	310.0
271.00	358.0
272.10	548.0
273.00	6141.0
274.00	15980.0
275.00	91368.0
276.00	11689.0
277.00	8483.0
278.00	1456.0
279.00	344.0
281.00	2328.0
282.10	810.0
283.10	1737.0
284.00	659.0
285.00	1529.0
286.00	223.0
289.00	329.0
290.10	230.0
291.10	229.0
292.10	248.0
293.00	1777.0
294.00	550.0
295.10	651.0
296.00	28960.0
297.00	4221.0
298.00	455.0
301.10	304.0
302.00	680.0
303.00	2754.0
304.10	863.0
308.00	457.0
309.10	304.0
309.90	236.0
312.90	290.0
314.00	1488.0
315.00	2721.0
316.00	1959.0
317.00	229.0
320.90	922.0
322.00	365.0
323.10	8556.0
324.00	1694.0
325.10	439.0
325.90	199.0
327.00	2022.0
328.00	778.0
328.90	223.0
332.00	679.0
332.90	821.0
334.00	6217.0
335.00	1766.0
336.00	223.0
340.10	214.0
341.00	1425.0
342.00	309.0
346.00	2165.0
347.10	271.0
352.00	2783.0
353.00	1952.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

354.00	2706.0
355.10	915.0
356.10	173.0
358.00	156.0
358.90	255.0
365.00	14001.0
366.00	1864.0
369.10	161.0
369.90	298.0
371.00	760.0
372.00	4621.0
373.10	1020.0
374.10	167.0
383.00	1141.0
384.00	349.0
390.00	391.0
391.00	362.0
392.00	305.0
401.00	402.0
402.00	2049.0
403.00	2391.0
404.00	1127.0
404.90	210.0
415.10	317.0
421.00	2427.0
422.00	1980.0
423.00	13743.0
424.00	3613.0
425.00	530.0
429.10	173.0
441.10	39240.0
442.10	247680.0
443.10	47040.0
444.10	4417.0
445.10	225.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

m/z	Abundance
36.00	250.0
37.00	507.0
38.10	1069.0
39.10	6719.0
40.00	1611.0
41.10	1043.0
42.00	395.0
43.00	836.0
44.00	9162.0
45.00	553.0
49.00	1078.0
50.10	19792.0
51.10	76368.0
52.10	4280.0
53.00	308.0
54.10	246.0
55.10	991.0
56.00	2550.0
57.00	5422.0
58.00	342.0
59.00	327.0
60.10	190.0
61.00	976.0
62.00	1096.0
63.00	3239.0
64.00	645.0
65.00	1550.0
65.90	259.0
67.00	453.0
68.10	1616.0
69.00	74256.0
70.00	509.0
71.00	260.0
73.00	4063.0
74.00	8253.0
75.00	13040.0
76.10	4073.0
77.10	88464.0
78.10	5516.0
79.00	6133.0
80.00	4359.0
81.00	6437.0
82.00	1773.0
83.10	1726.0
84.00	648.0
84.90	944.0
86.00	2333.0
87.00	1041.0
88.00	663.0
89.10	415.0
91.00	1943.0
92.10	1822.0
93.00	10608.0
94.00	774.0
94.90	274.0
96.10	1197.0
97.00	434.0
98.00	7920.0
99.00	6322.0
100.00	431.0
101.00	3738.0
102.00	255.0
103.00	1210.0
103.90	2161.0
105.00	1928.0
105.90	720.0
107.00	25200.0
108.00	4064.0
109.00	834.0
110.00	45512.0
111.00	7192.0
111.90	807.0
113.00	469.0
115.00	320.0
116.00	1782.0
117.00	25304.0
118.00	1536.0
119.00	569.0
120.10	425.0
122.00	2020.0
123.00	3112.0
124.00	1238.0
125.00	987.0
126.10	663.0
127.00	93856.0
128.00	6506.0
129.00	36176.0
130.00	2863.0
130.90	785.0
132.00	367.0
132.90	871.0
134.00	1107.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

135.00	3326.0
136.00	1083.0
137.10	1880.0
137.90	424.0
138.90	215.0
140.00	475.0
141.00	4784.0
142.00	1440.0
143.00	1180.0
143.90	320.0
145.00	358.0
146.00	1125.0
147.00	3816.0
148.00	6961.0
149.00	1611.0
150.00	350.0
151.20	490.0
151.80	349.0
153.00	1564.0
153.90	1325.0
155.00	3258.0
156.00	3978.0
157.00	899.0
158.10	747.0
159.00	710.0
160.00	1578.0
161.00	2751.0
162.00	687.0
162.90	306.0
163.90	321.0
165.00	2088.0
166.00	1401.0
167.00	12149.0
168.00	6413.0
169.00	933.0
170.10	339.0
170.90	503.0
171.90	1096.0
173.00	1183.0
174.00	2346.0
175.00	3953.0
176.00	1051.0
177.00	2109.0
178.00	744.0
179.00	8008.0
180.00	5567.0
181.00	2428.0
182.00	475.0
182.80	158.0
184.00	616.0
185.00	3599.0
186.00	28688.0
187.10	7971.0
187.90	966.0
189.00	2348.0
189.80	328.0
191.00	1832.0
192.00	2631.0
193.00	3954.0
194.00	813.0
195.10	299.0
196.00	5998.0
198.00	210240.0
199.00	13926.0
200.00	1022.0
201.40	893.0
203.00	1792.0
204.00	8268.0
205.10	13882.0
206.00	57136.0
207.00	15588.0
208.00	3808.0
209.00	2029.0
210.00	810.0
211.10	2448.0
211.90	421.0
212.90	254.0
214.90	516.0
216.00	1312.0
217.00	16061.0
218.00	1972.0
218.90	261.0
221.00	9108.0
222.00	2225.0
223.00	3867.0
224.00	33192.0
225.00	8757.0
226.00	791.0
227.00	14784.0
228.00	2002.0
229.00	3367.0
230.00	321.0
231.00	1033.0
232.00	230.0
233.10	350.0
234.00	947.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

235.10	909.0
236.00	562.0
237.00	1360.0
237.90	232.0
239.00	425.0
239.90	472.0
241.00	650.0
242.00	1848.0
243.00	1916.0
244.10	25496.0
245.00	3065.0
246.00	5515.0
247.00	1042.0
247.90	398.0
249.00	1193.0
250.10	191.0
251.00	255.0
253.00	681.0
254.10	862.0
255.00	141568.0
256.00	20216.0
257.00	1492.0
258.00	8391.0
259.00	1134.0
260.00	223.0
260.90	235.0
265.00	3633.0
266.00	539.0
267.00	492.0
269.10	242.0
269.90	278.0
271.10	347.0
272.00	403.0
273.00	4151.0
274.00	10543.0
275.00	64520.0
276.00	8045.0
277.00	5968.0
277.90	1224.0
279.00	226.0
281.10	2066.0
282.00	516.0
283.00	1294.0
283.90	544.0
285.10	1108.0
288.90	217.0
290.00	226.0
291.90	345.0
293.00	1518.0
294.00	378.0
295.00	724.0
296.00	19616.0
297.00	3402.0
298.00	150.0
301.00	195.0
301.90	347.0
303.10	2381.0
303.90	545.0
307.90	261.0
309.00	194.0
310.00	383.0
313.10	208.0
314.00	770.0
314.90	2210.0
316.00	1142.0
317.00	286.0
321.00	730.0
321.90	169.0
323.10	6133.0
324.00	1011.0
325.00	172.0
326.00	180.0
326.90	1522.0
328.00	711.0
332.00	764.0
333.00	473.0
334.10	3890.0
334.90	820.0
341.00	1074.0
342.10	441.0
342.90	233.0
346.00	1777.0
347.00	363.0
352.00	2123.0
353.00	1301.0
354.00	2087.0
355.00	742.0
356.10	194.0
359.00	230.0
365.00	10174.0
366.00	1692.0
370.00	194.0
371.00	662.0
372.00	3513.0
373.00	913.0
383.00	1215.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

384.00	336.0
390.00	516.0
391.00	231.0
392.00	212.0
401.00	364.0
402.00	1412.0
403.00	2186.0
404.00	645.0
404.90	189.0
414.90	325.0
421.00	1601.0
422.00	1815.0
423.00	11638.0
424.10	2931.0
425.10	407.0
429.10	157.0
441.00	30528.0
442.10	206720.0
443.00	37936.0
444.00	3269.0
445.00	287.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

m/z	Abundance
36.00	261.0
38.00	207.0
39.00	767.0
40.00	1092.0
41.10	714.0
42.10	482.0
43.00	726.0
44.00	8825.0
44.90	301.0
46.80	195.0
49.00	673.0
50.00	230.0
51.00	289.0
52.10	150.0
53.10	197.0
55.00	809.0
56.00	434.0
56.90	314.0
59.10	270.0
67.00	264.0
69.10	238.0
70.00	164.0
71.10	150.0
73.10	2653.0
73.90	260.0
75.00	429.0
77.00	479.0
78.00	404.0
79.10	256.0
79.90	154.0
81.00	221.0
83.00	185.0
84.00	363.0
86.00	221.0
89.00	162.0
91.00	403.0
93.00	177.0
95.00	208.0
96.00	656.0
96.70	246.0
97.10	290.0
98.00	169.0
103.00	325.0
118.90	241.0
121.10	163.0
133.00	767.0
133.90	194.0
135.10	483.0
147.00	1021.0
148.00	167.0
149.00	204.0
162.90	187.0
176.90	436.0
178.90	153.0
191.00	844.0
191.80	186.0
193.10	921.0
194.10	226.0
207.10	8822.0
208.10	1906.0
209.00	766.0
221.00	854.0
222.00	230.0
223.10	239.0
248.80	157.0
264.90	175.0
267.10	374.0
281.00	1999.0
282.00	435.0
283.00	359.0
295.00	221.0
341.00	322.0
355.00	525.0
356.00	151.0
401.00	198.0
429.00	163.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014