


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052819\
 Data File : BM020572.D
 Acq On : 28 May 2019 08:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 16:07:05 2019

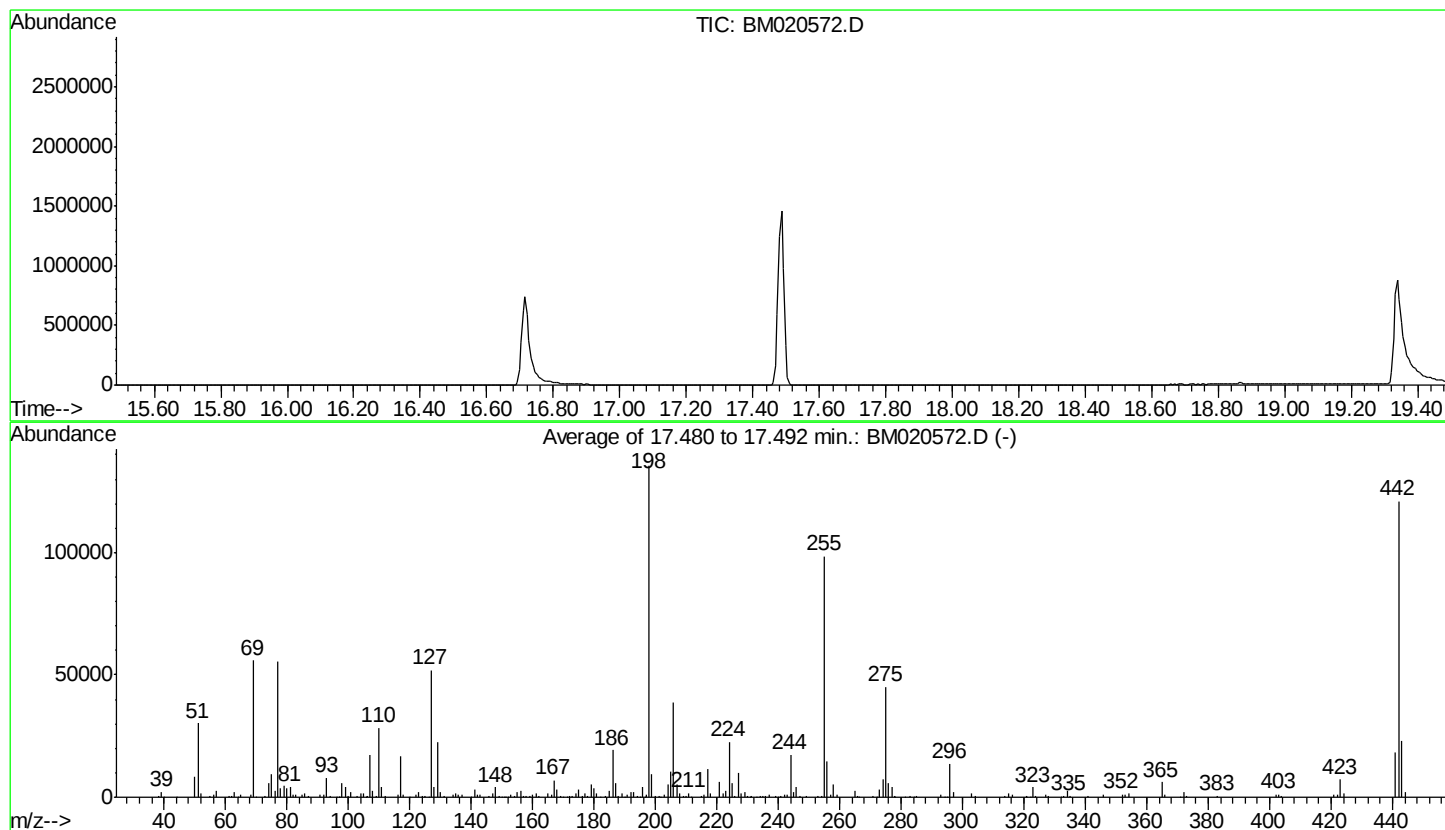

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	30317	PASS
68	69	0.00	2	1.9	1048	PASS
69	198	0.00	100	41.1	55762	PASS
70	69	0.00	2	0.4	248	PASS
127	198	10	80	38.3	51898	PASS
197	198	0.00	2	0.8	1034	PASS
198	198	100	100	100.0	135554	PASS
199	198	5	9	6.9	9350	PASS
275	198	10	60	33.3	45189	PASS
365	198	1	100	4.5	6094	PASS
441	198	0.01	100	13.4	18126	PASS
442	198	50	100	89.3	121112	PASS
443	442	15	24	18.8	22808	PASS