


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM053019\
 Data File : BM020596.D
 Acq On : 29 May 2019 11:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 30 02:15:06 2019

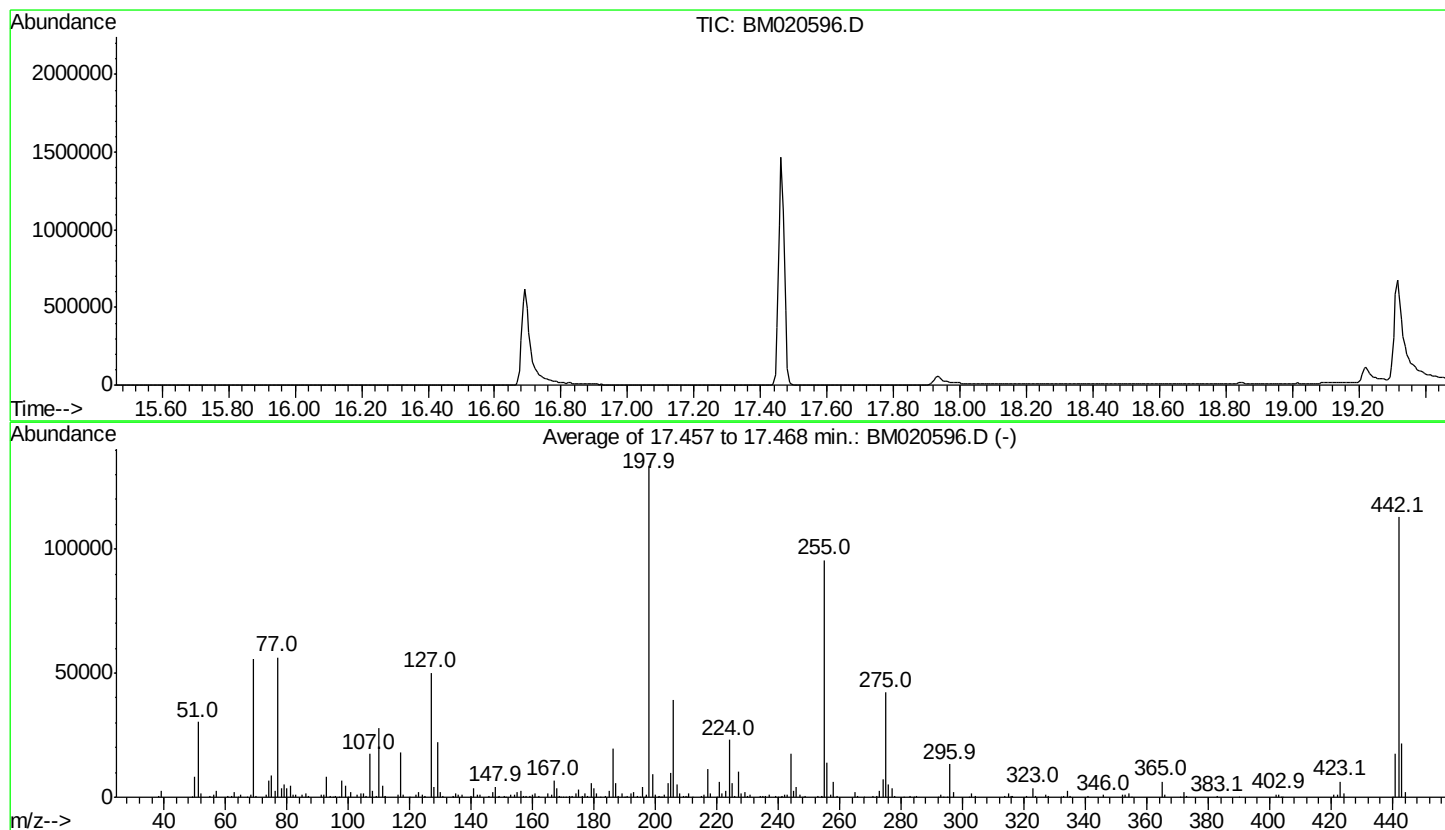

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	30229	PASS
68	69	0.00	2	1.9	1065	PASS
69	198	0.00	100	41.9	55981	PASS
70	69	0.00	2	0.7	375	PASS
127	198	10	80	37.6	50274	PASS
197	198	0.00	2	0.7	895	PASS
198	198	100	100	100.0	133634	PASS
199	198	5	9	6.8	9076	PASS
275	198	10	60	31.5	42128	PASS
365	198	1	100	4.8	6351	PASS
441	198	0.01	100	13.3	17713	PASS
442	198	50	100	84.5	112906	PASS
443	442	15	24	19.3	21808	PASS