


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM053019\
 Data File : BM020613.D
 Acq On : 30 May 2019 00:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 30 02:15:06 2019

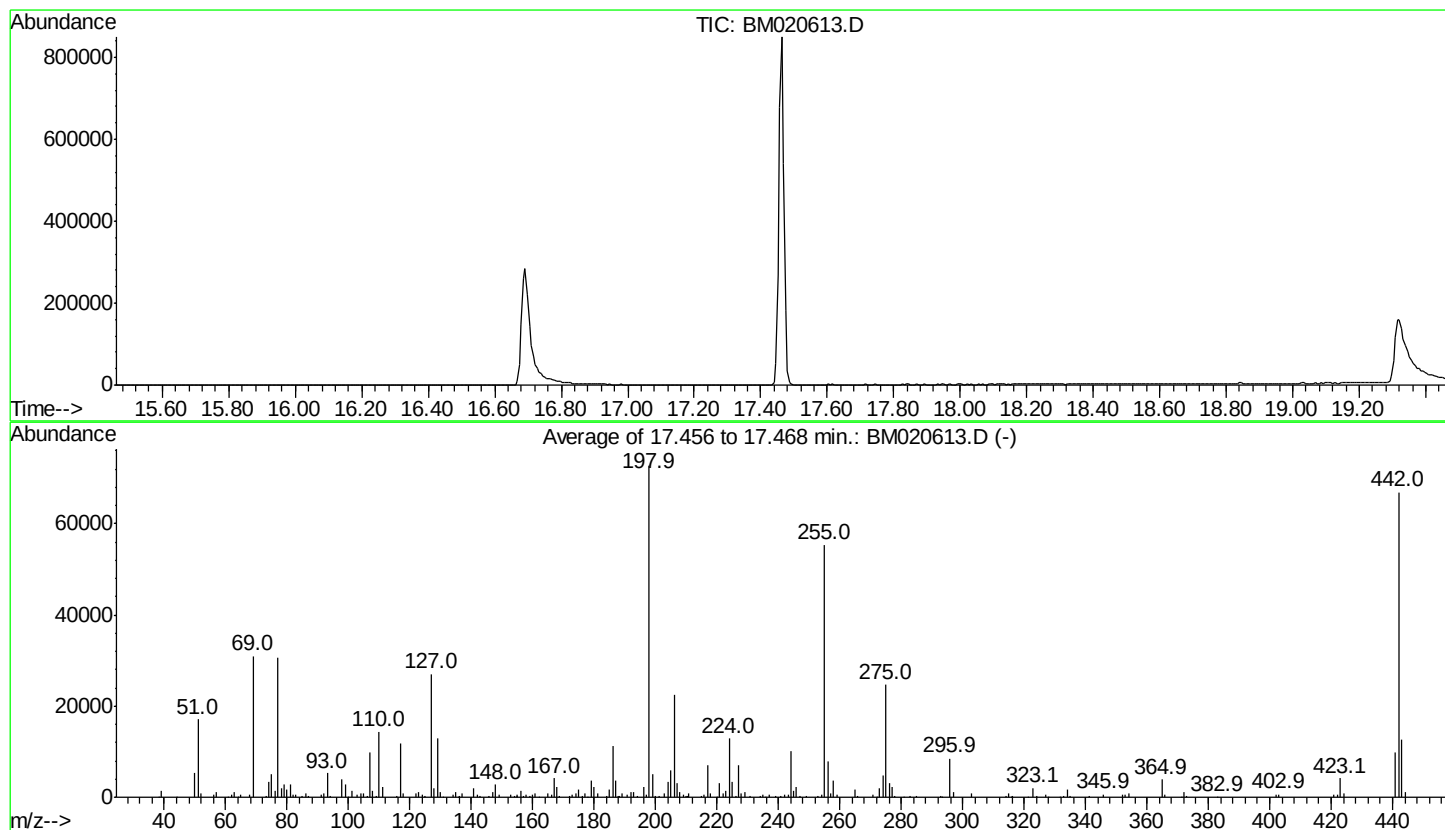

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	17033	PASS
68	69	0.00	2	1.5	473	PASS
69	198	0.00	100	42.6	30970	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.1	26976	PASS
197	198	0.00	2	0.7	535	PASS
198	198	100	100	100.0	72733	PASS
199	198	5	9	6.8	4933	PASS
275	198	10	60	33.9	24653	PASS
365	198	1	100	5.3	3857	PASS
441	198	0.01	100	13.6	9896	PASS
442	198	50	100	92.0	66912	PASS
443	442	15	24	19.0	12705	PASS