

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040053.D
 Acq On : 30 May 2023 13:13
 Operator : CG/JU
 Sample : PB153102BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK102

Quant Time: May 31 02:02:07 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	6658	0.400	ng/ul	0.00
4) Naphthalene-d8	10.826	136	22366	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.645	164	10441	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.390	188	17685	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.572	240	7795	0.400	ng/ul	0.00
23) Perylene-d12	24.018	264	7563	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.379	96	56656	7.308	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.410	152	10303	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.415	212	12399	0.528	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.778	202	3390	0.095	ng/ul#	1
26) Benzo(a)pyrene	23.861	252	4403	0.175	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
Data File : BM040053.D
Acq On : 30 May 2023 13:13
Operator : CG/JU
Sample : PB153102BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK102

Quant Time: May 31 02:02:07 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 14:54:33 2023
Response via : Initial Calibration




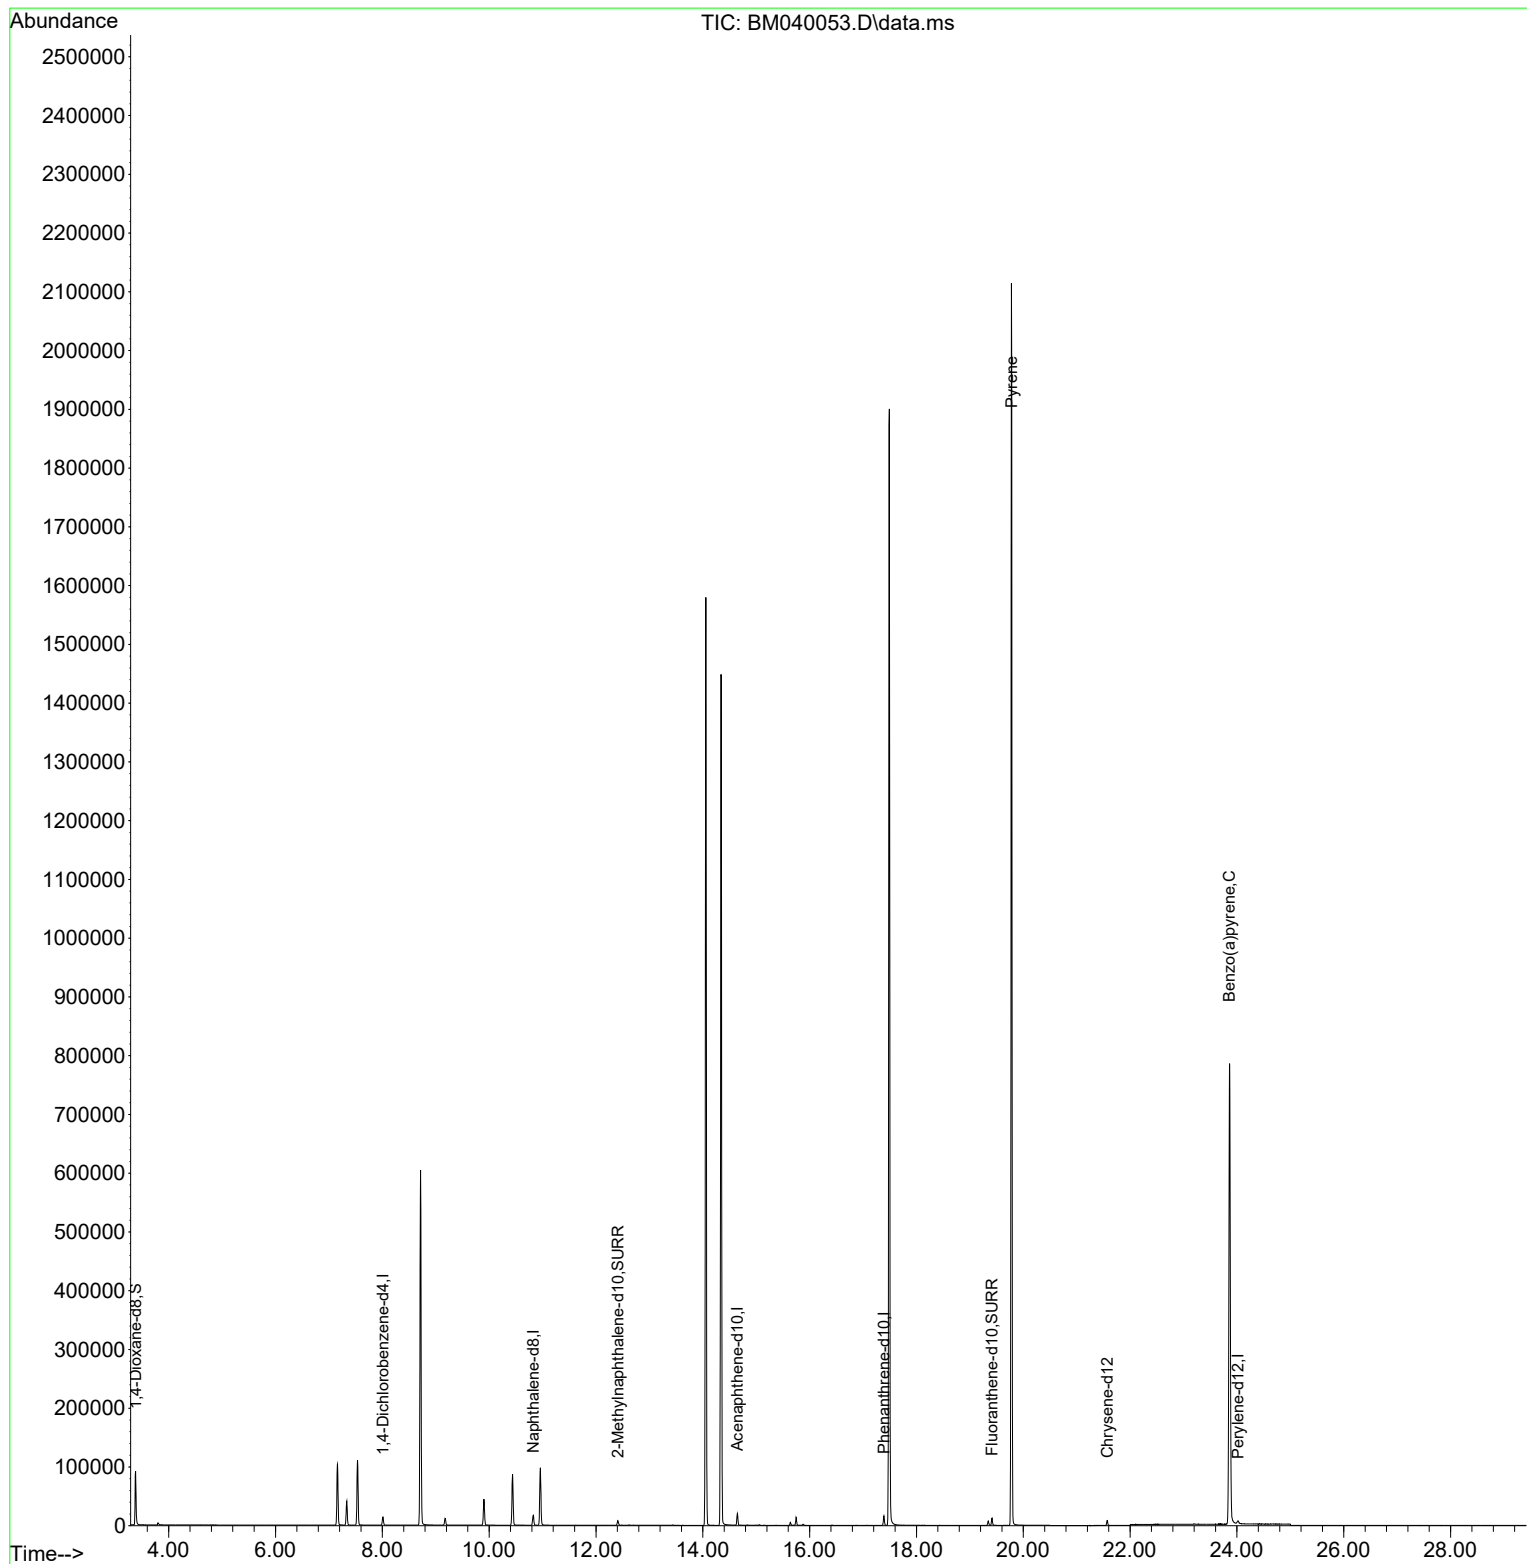


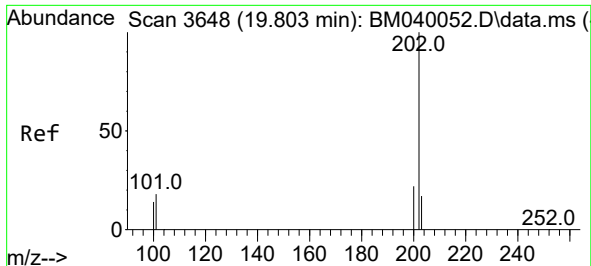

#20
Pyrene
Concen: 0.095 ng/ul
RT: 19.778 min Scan# 30
Delta R.T. -0.025 min
Lab File: BM040053.D
Acq: 30 May 2023 13:13

Instrument :
BNA_M
ClientSampleId :
SBLK102

Tgt Ion:202 Resp: 3390
Ion Ratio Lower Upper
202 100
101 155.3 13.3 19.9#
100 1158.8 10.9 16.3#

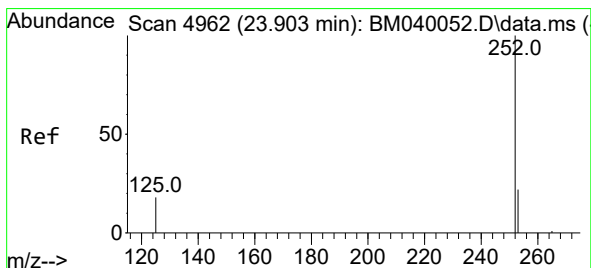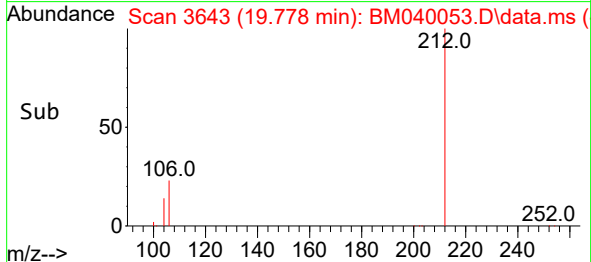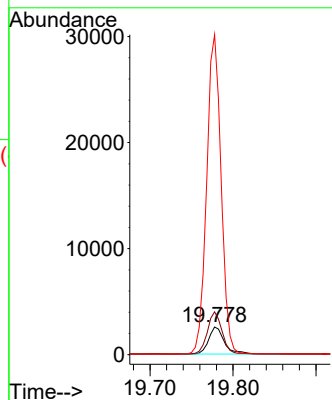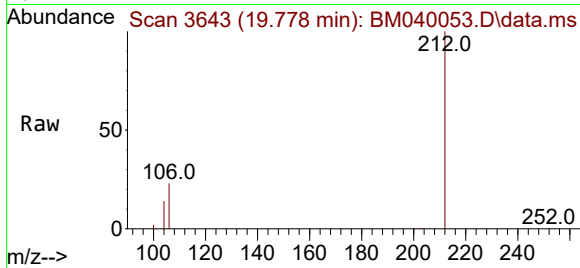

#26
Benzo(a)pyrene
Concen: 0.175 ng/ul
RT: 23.861 min Scan# 4948
Delta R.T. -0.042 min
Lab File: BM040053.D
Acq: 30 May 2023 13:13

Tgt Ion:252 Resp: 4403
Ion Ratio Lower Upper
252 100
253 41.8 20.6 31.0#
125 42.2 19.1 28.7#

