

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040054.D
 Acq On : 30 May 2023 13:49
 Operator : CG/JU
 Sample : PB153104BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK104

Quant Time: May 31 02:02:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	6663	0.400	ng/ul	0.00
4) Naphthalene-d8	10.821	136	22807	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.645	164	10516	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.390	188	17548	0.400	ng/ul	0.00
17) Chrysene-d12	21.566	240	7427	0.400	ng/ul	0.00
23) Perylene-d12	24.010	264	7676	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	61375	7.911	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.410	152	11454	0.411	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	13066	0.584	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.778	202	3500	0.103	ng/ul#	1
26) Benzo(a)pyrene	23.855	252	5110	0.200	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
Data File : BM040054.D
Acq On : 30 May 2023 13:49
Operator : CG/JU
Sample : PB153104BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK104

Quant Time: May 31 02:02:13 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 14:54:33 2023
Response via : Initial Calibration




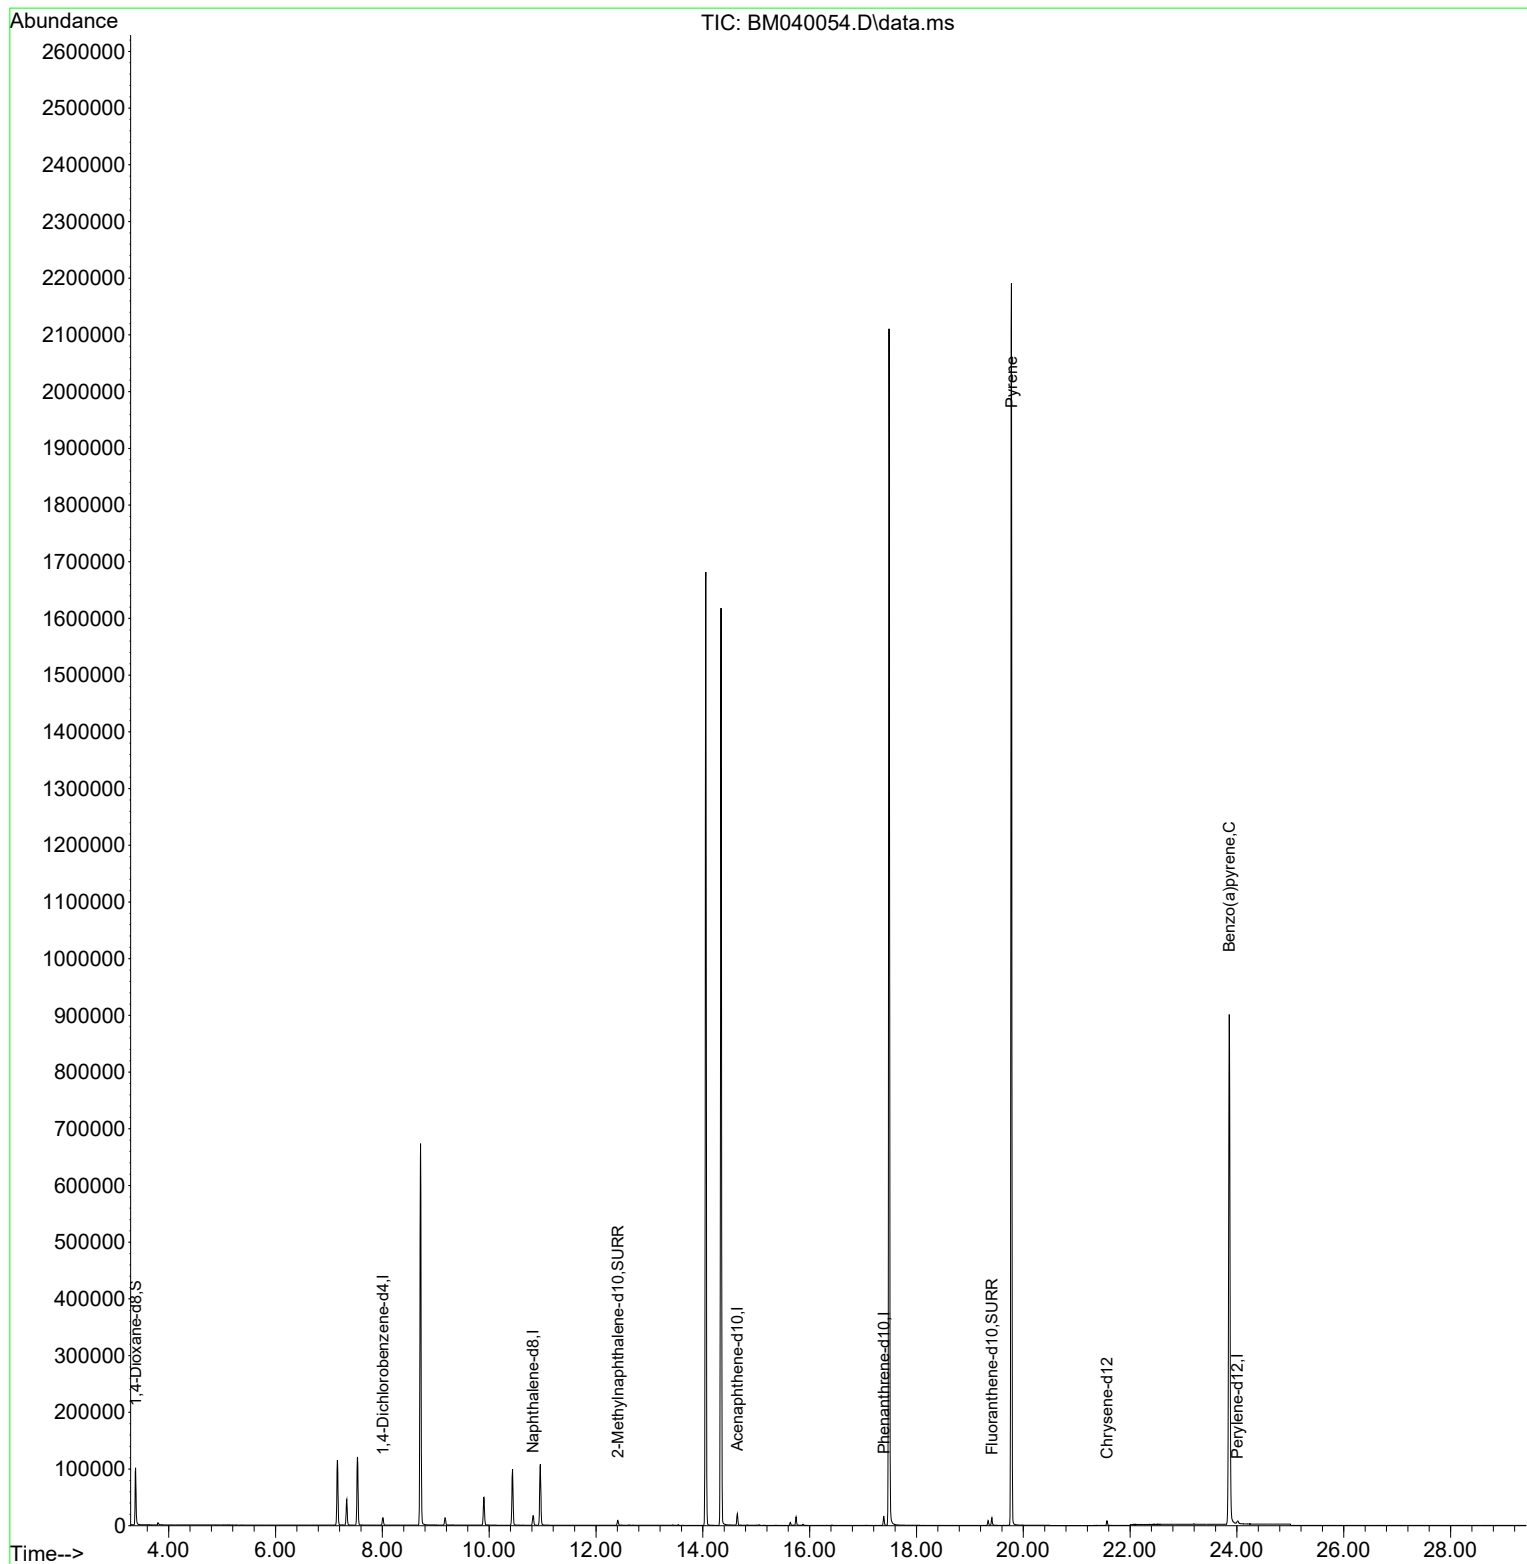


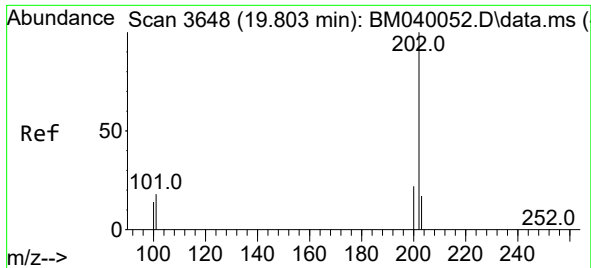

#20
Pyrene
Concen: 0.103 ng/ul
RT: 19.778 min Scan# 3643
Delta R.T. -0.025 min
Lab File: BM040054.D
Acq: 30 May 2023 13:49

Instrument :
BNA_M
ClientSampleId :
SBLK104

Tgt Ion:202 Resp: 3500
Ion Ratio Lower Upper
202 100
101 148.3 13.3 19.9#
100 1060.2 10.9 16.3#

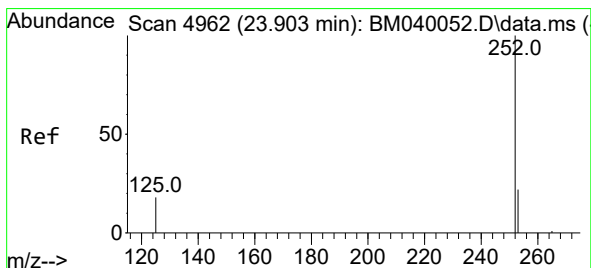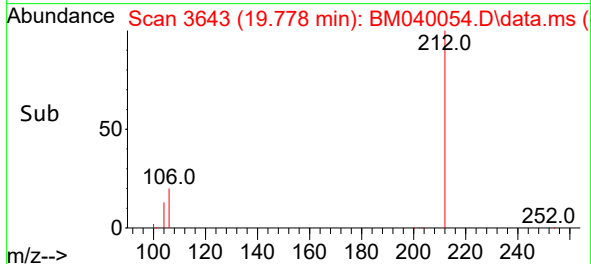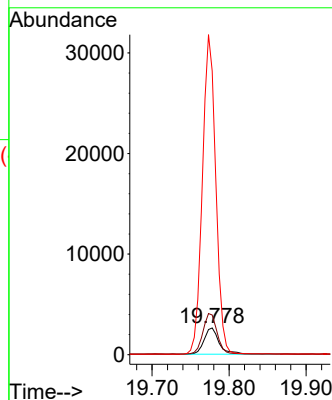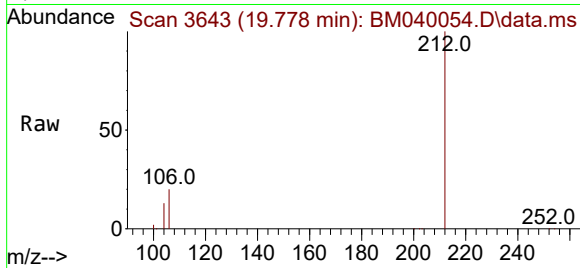

#26
Benzo(a)pyrene
Concen: 0.200 ng/ul
RT: 23.855 min Scan# 4946
Delta R.T. -0.048 min
Lab File: BM040054.D
Acq: 30 May 2023 13:49

Tgt Ion:252 Resp: 5110
Ion Ratio Lower Upper
252 100
253 39.2 20.6 31.0#
125 38.0 19.1 28.7#

