

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040060.D
 Acq On : 30 May 2023 17:29
 Operator : CG/JU
 Sample : 02961-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FP2

Quant Time: May 31 02:02:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	6030	0.400	ng/ul	0.00
4) Naphthalene-d8	10.822	136	20071	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	9371	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.387	188	15313	0.400	ng/ul	0.00
17) Chrysene-d12	21.564	240	7160	0.400	ng/ul	0.00
23) Perylene-d12	24.011	264	7485	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	33582	4.783	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.406	152	5830	0.238	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	7935	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.775	202	2294	0.070	ng/ul#	1
26) Benzo(a)pyrene	23.853	252	3017	0.121	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
Data File : BM040060.D
Acq On : 30 May 2023 17:29
Operator : CG/JU
Sample : 02961-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FP2

Quant Time: May 31 02:02:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 14:54:33 2023
Response via : Initial Calibration

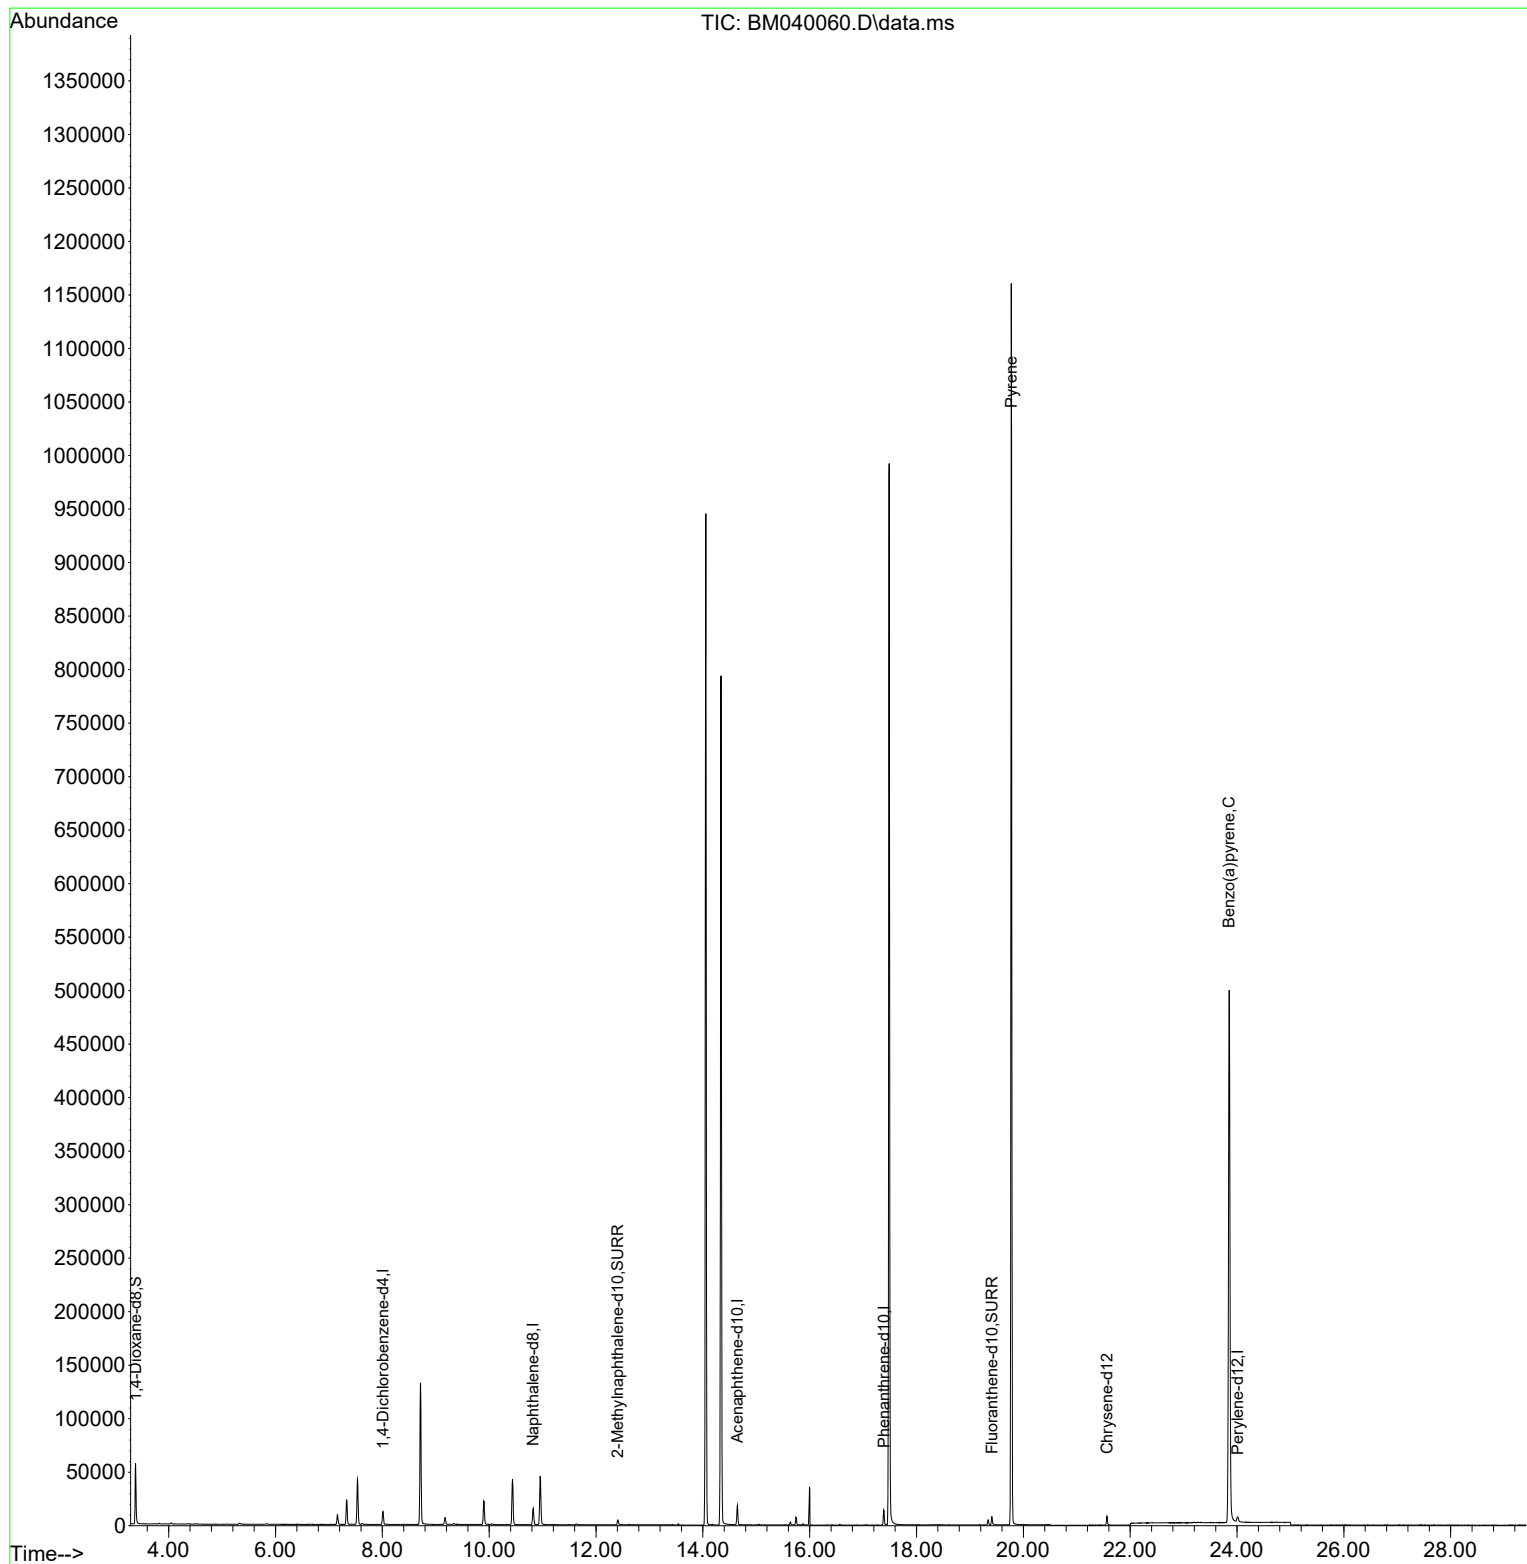

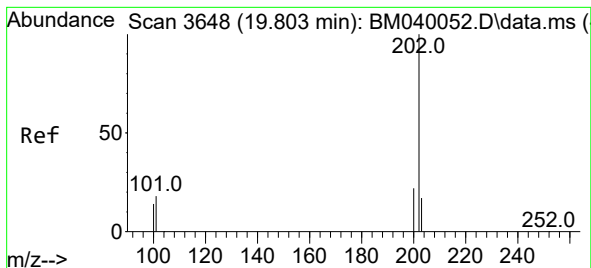

#20

Pyrene

Concen: 0.070 ng/ul

RT: 19.775 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM040060.D

Acq: 30 May 2023 17:29

Instrument :

BNA_M

ClientSampleId :

H0FP2





Tgt Ion:202 Resp: 2294

Ion Ratio Lower Upper

202 100

101 151.2 13.3 19.9#

100 1104.3 10.9 16.3#

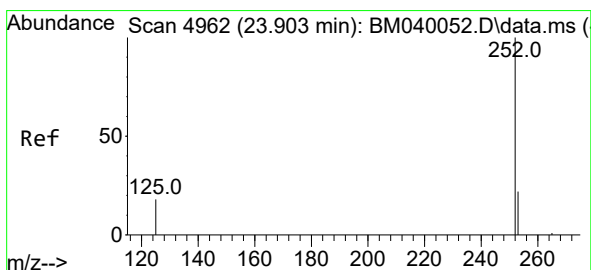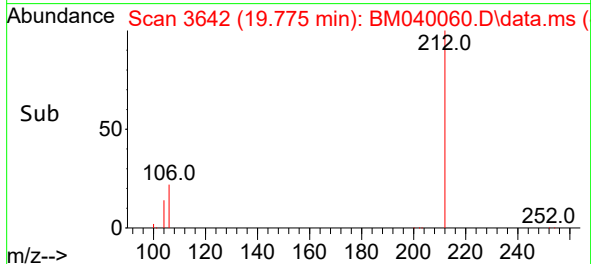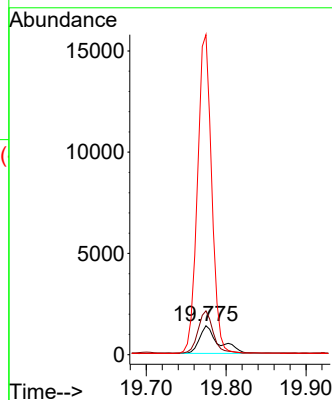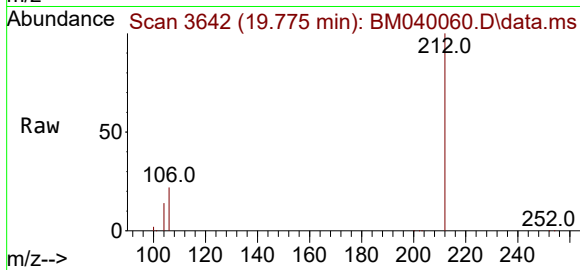

#26

Benzo(a)pyrene

Concen: 0.121 ng/ul

RT: 23.853 min Scan# 4945

Delta R.T. -0.050 min

Lab File: BM040060.D

Acq: 30 May 2023 17:29

Tgt Ion:252 Resp: 3017

Ion Ratio Lower Upper

252 100

253 47.4 20.6 31.0#

125 51.6 19.1 28.7#

