

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040063.D
 Acq On : 30 May 2023 19:19
 Operator : CG/JU
 Sample : 02961-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FP5

Quant Time: May 31 02:03:09 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	5997	0.400	ng/ul	0.00
4) Naphthalene-d8	10.822	136	20372	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	9343	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.387	188	14920	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.564	240	6923	0.400	ng/ul	0.00
23) Perylene-d12	24.011	264	7990	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	39819	5.702	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.406	152	9688	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	12591	0.604	ng/ul	0.00
Target Compounds						
12) Fluorene	15.637	166	3908	0.124	ng/ul#	13
20) Pyrene	19.775	202	3064	0.097	ng/ul#	1
26) Benzo(a)pyrene	23.853	252	5364	0.202	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040063.D
 Acq On : 30 May 2023 19:19
 Operator : CG/JU
 Sample : 02961-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FP5

Quant Time: May 31 02:03:09 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration

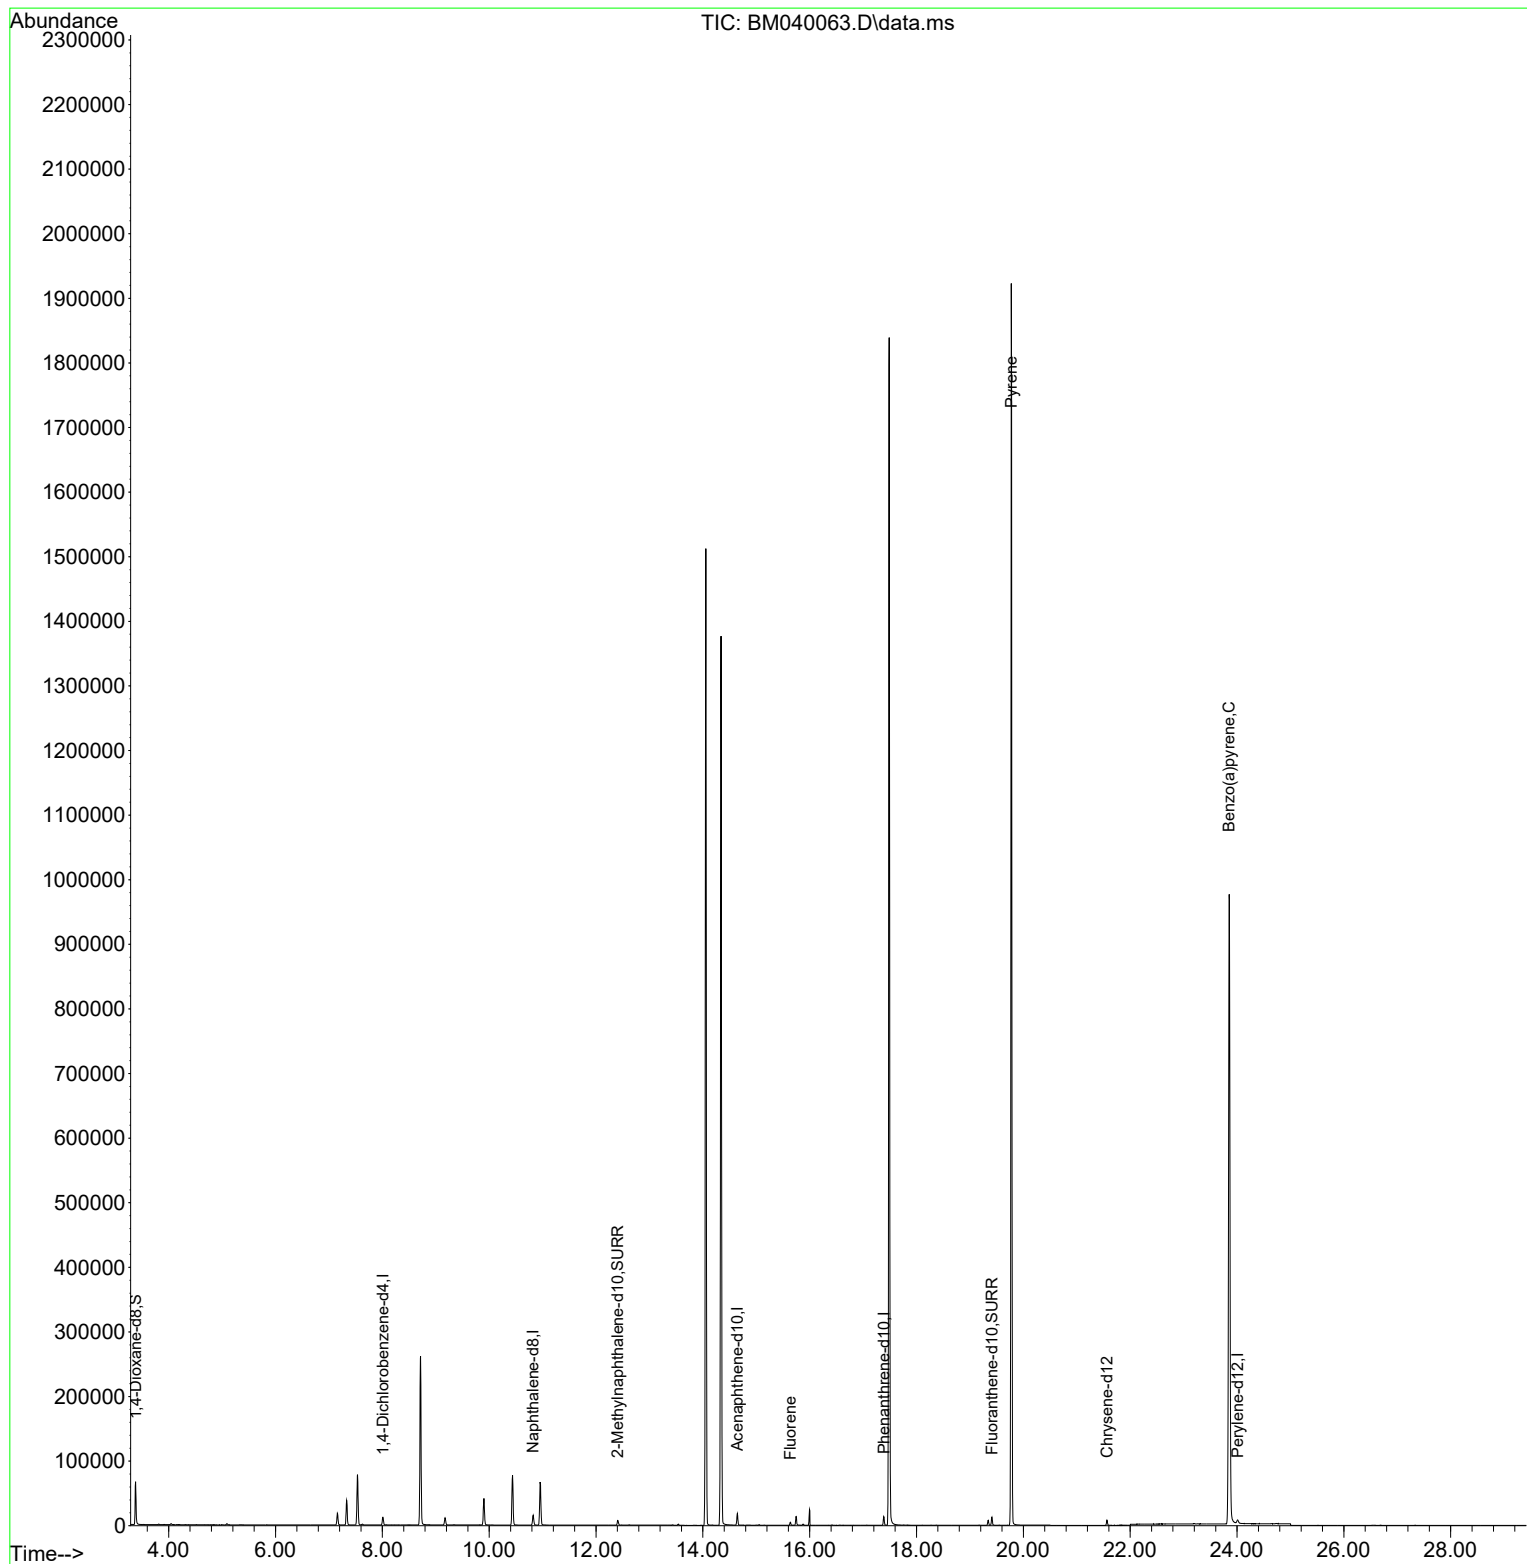




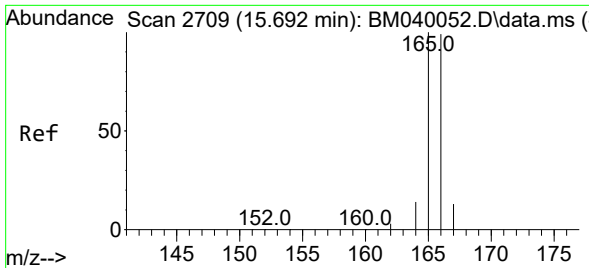


#12
 Fluorene
 Concen: 0.124 ng/u1
 RT: 15.637 min Scan# 2697
 Delta R.T. -0.056 min
 Lab File: BM040063.D
 Acq: 30 May 2023 19:19

Instrument :
 BNA_M
 ClientSampleId :
 H0FP5

Tgt Ion:166 Resp: 3908




Ion	Ratio	Lower	Upper
166	100		
165	7.1	79.3	118.9#
167	31.3	10.8	16.2#

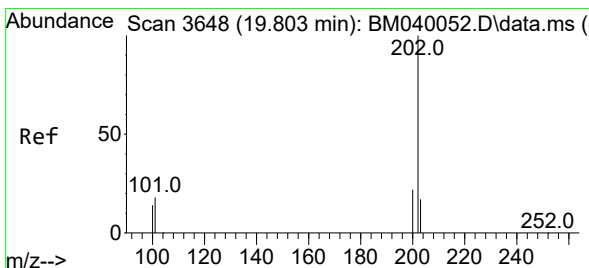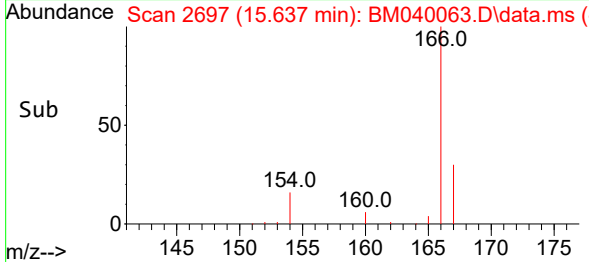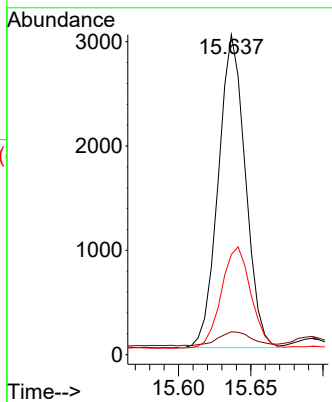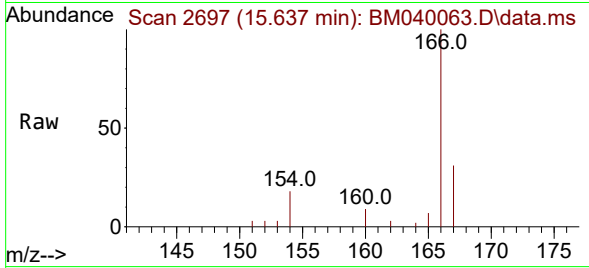


#20
 Pyrene
 Concen: 0.097 ng/u1
 RT: 19.775 min Scan# 3642
 Delta R.T. -0.028 min
 Lab File: BM040063.D
 Acq: 30 May 2023 19:19

Tgt Ion:202 Resp: 3064


Ion	Ratio	Lower	Upper
202	100		
101	157.6	13.3	19.9#
100	1174.9	10.9	16.3#

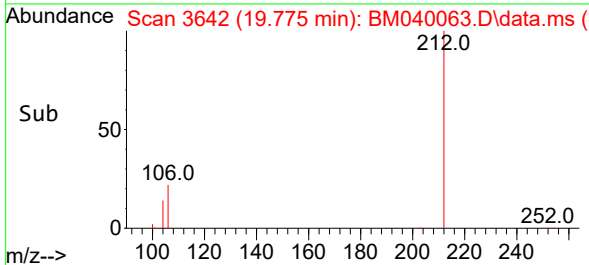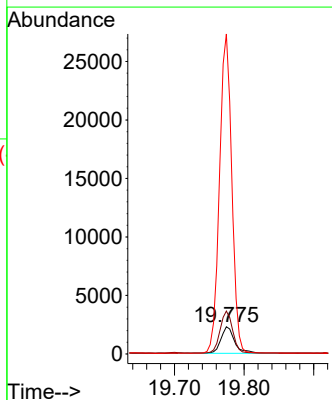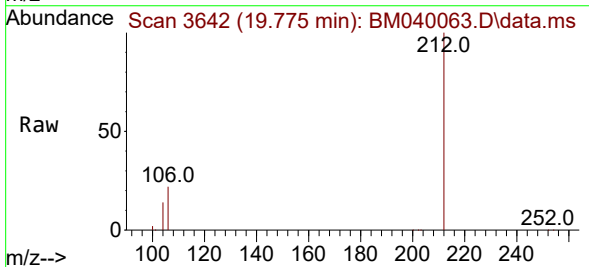

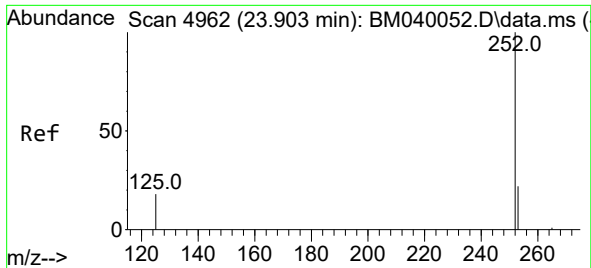

#26
 Benzo(a)pyrene
 Concen: 0.202 ng/ul
 RT: 23.853 min Scan# 4962
 Delta R.T. -0.050 min
 Lab File: BM040063.D
 Acq: 30 May 2023 19:19

Instrument :
 BNA_M
 ClientSampleId :
 H0FP5

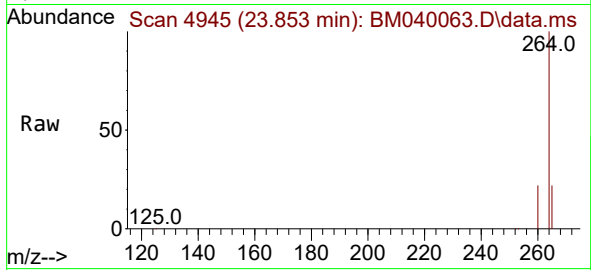

Tgt Ion:252 Resp: 5364
 Ion Ratio Lower Upper
 252 100
 253 39.6 20.6 31.0#
 125 38.3 19.1 28.7#

