

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
 Data File : BM040055.D
 Acq On : 30 May 2023 14:26
 Operator : CG/JU
 Sample : 02961-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FP8

Quant Time: May 31 02:02:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 14:54:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	6448	0.400	ng/ul	0.00
4) Naphthalene-d8	10.822	136	21932	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.646	164	10807	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.387	188	18894	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.567	240	8566	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264	8639	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	38851	5.175	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.406	152	9043	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	13549	0.525	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.037	266	97	0.025	ng/ul	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM053023\
Data File : BM040055.D
Acq On : 30 May 2023 14:26
Operator : CG/JU
Sample : 02961-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FP8


Quant Time: May 31 02:02:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 14:54:33 2023
Response via : Initial Calibration

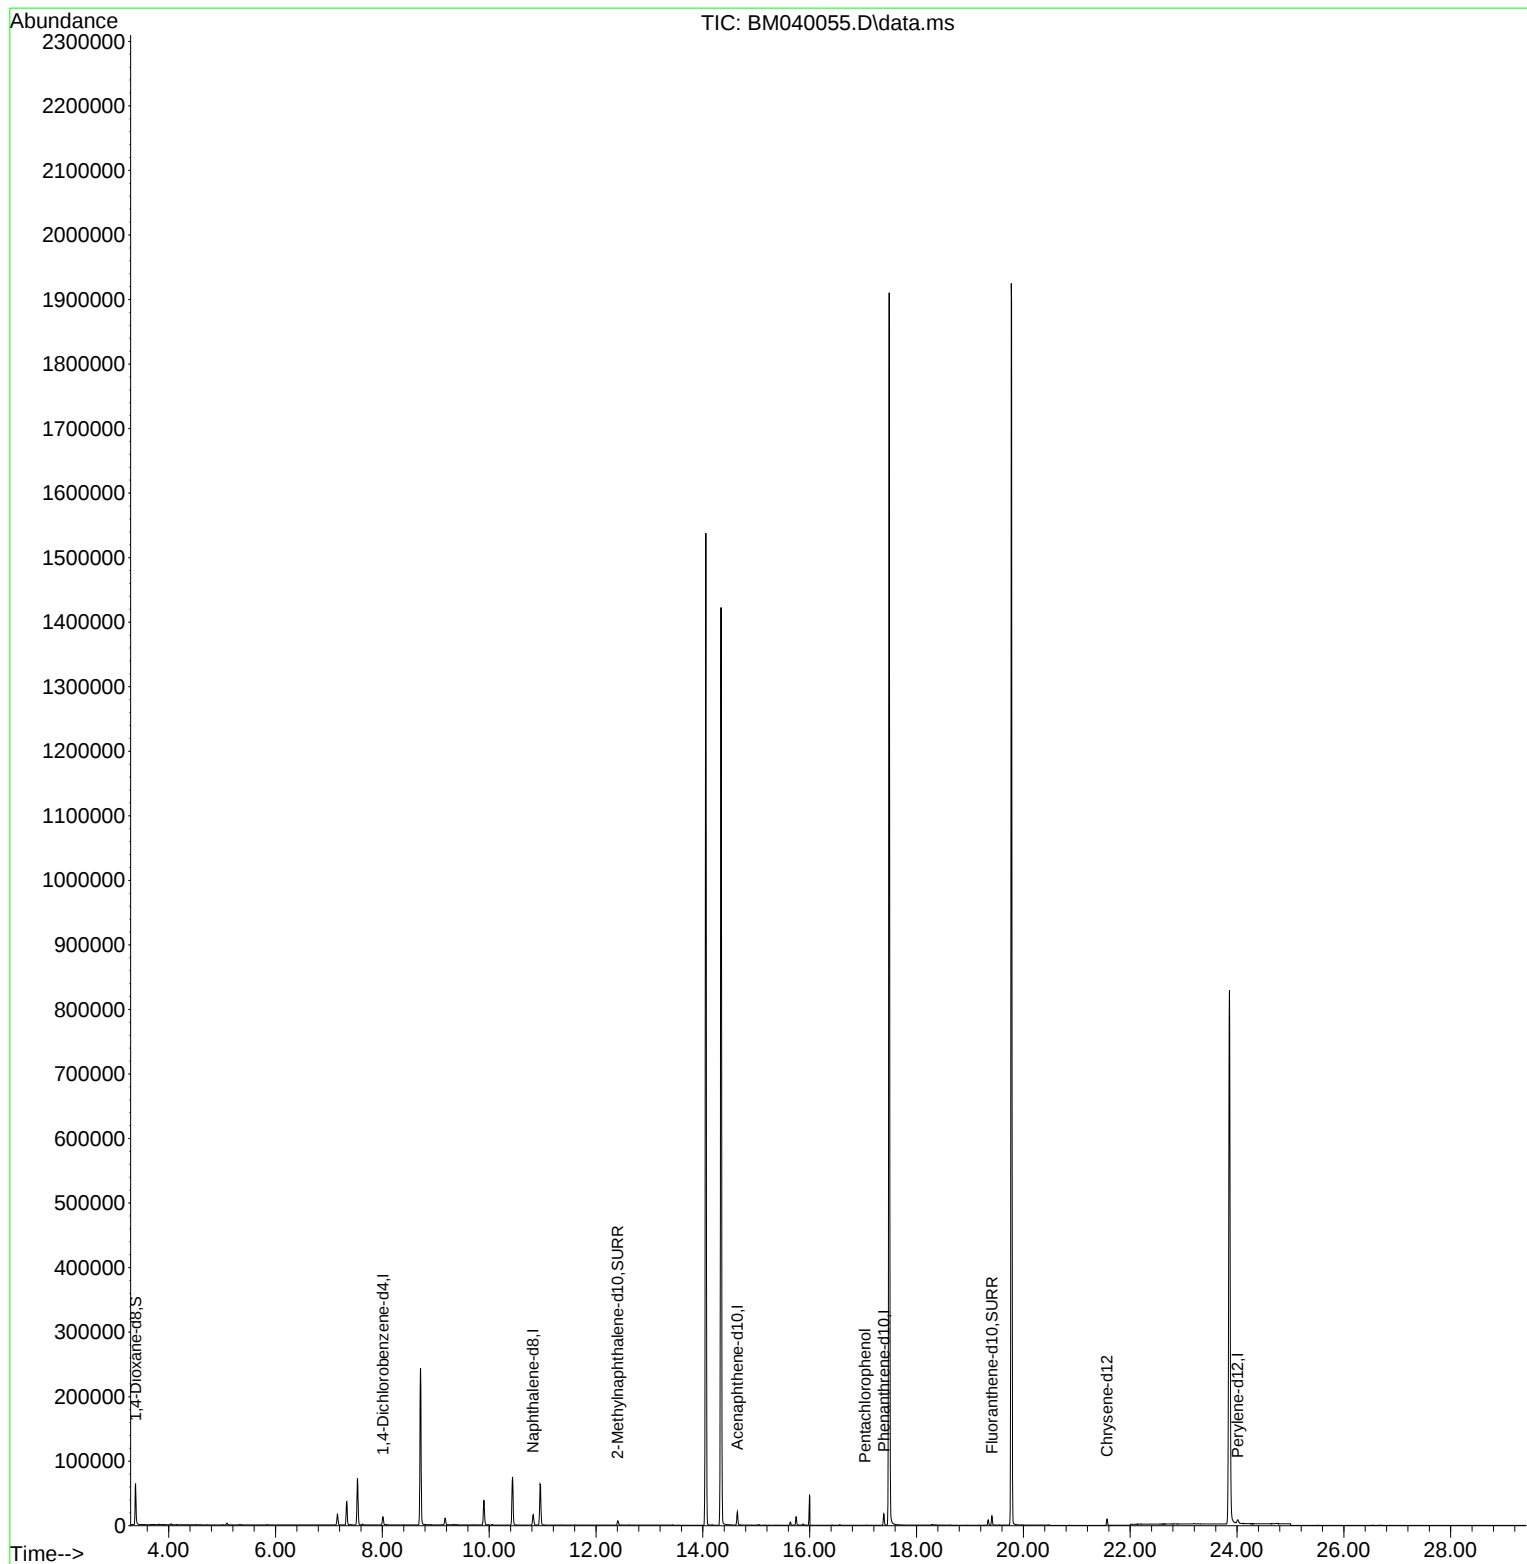

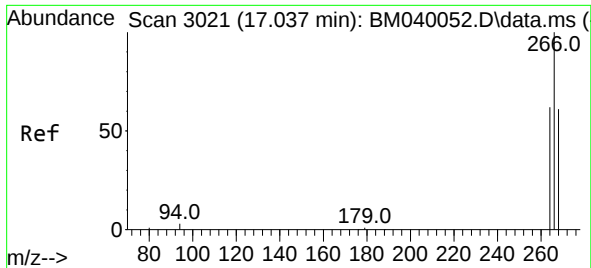

#14
 Pentachlorophenol
 Concen: 0.025 ng/ul
 RT: 17.037 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BM040055.D
 Acq: 30 May 2023 14:26

Instrument :
 BNA_M
 ClientSampleId :
 H0FP8

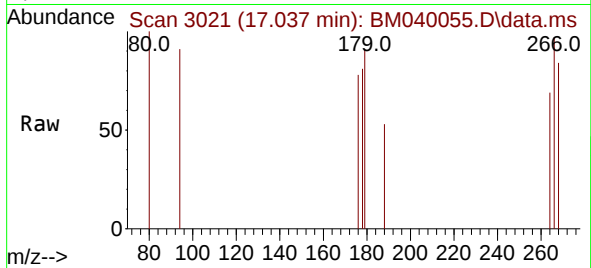

Tgt Ion:266	Resp:	97	
Ion	Ratio	Lower	Upper
266	100		
264	49.5	49.2	73.8
268	59.8	51.9	77.9

