


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM053119\
 Data File : BM020624.D
 Acq On : 31 May 2019 08:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 15:48:49 2019

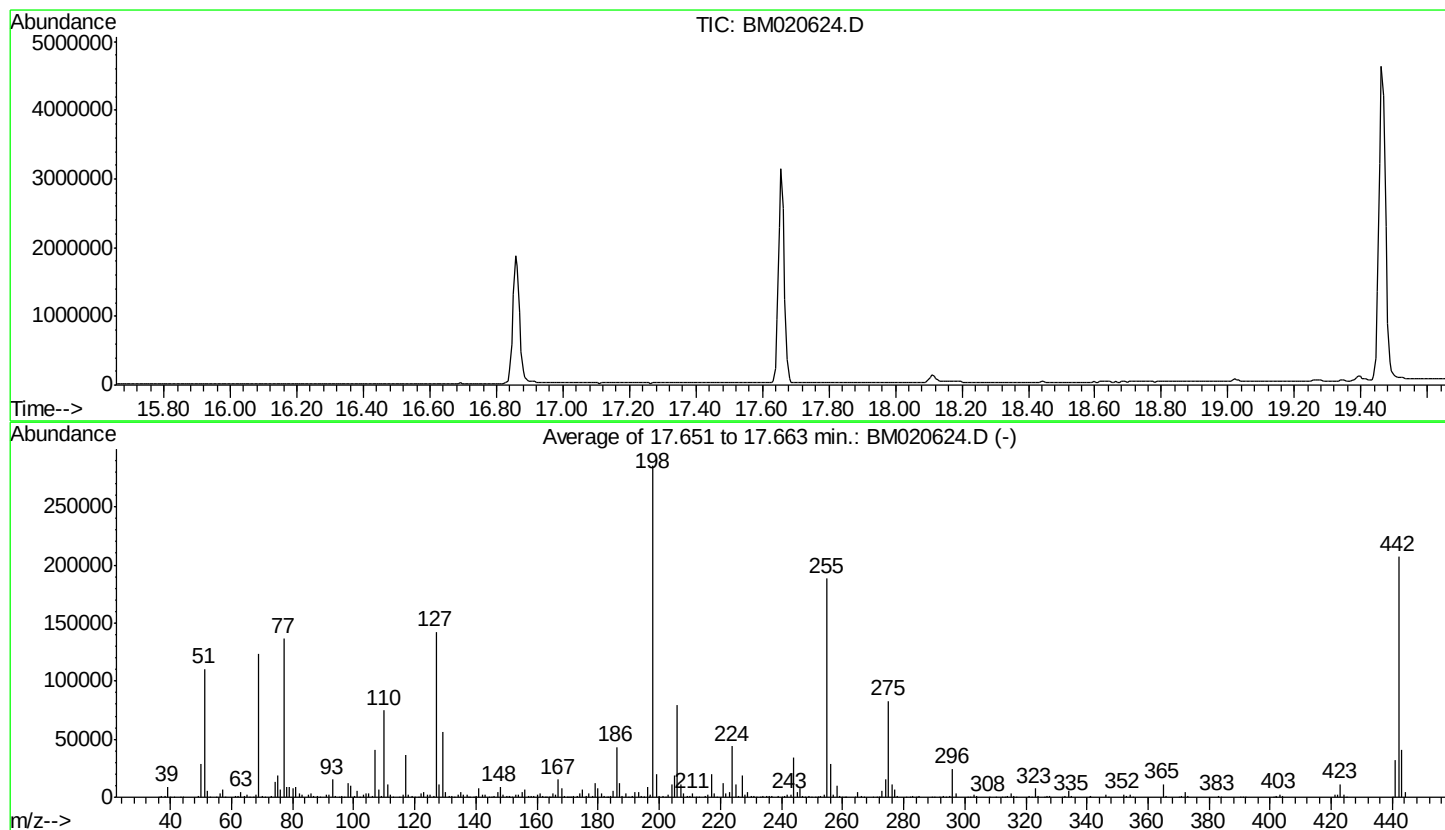

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	110363	PASS
68	69	0.00	2	2.0	2479	PASS
69	198	0.00	100	43.3	123504	PASS
70	69	0.00	2	0.7	865	PASS
127	198	10	80	50.0	142744	PASS
197	198	0.00	2	0.6	1726	PASS
198	198	100	100	100.0	285482	PASS
199	198	5	9	6.9	19642	PASS
275	198	10	60	29.1	83109	PASS
365	198	1	100	4.1	11567	PASS
441	198	0.01	100	11.2	32072	PASS
442	198	50	100	72.5	206933	PASS
443	442	15	24	19.5	40442	PASS