


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM053119\  
 Data File : BM020638.D  
 Acq On : 31 May 2019 20:11  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM053119.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 31 15:48:49 2019

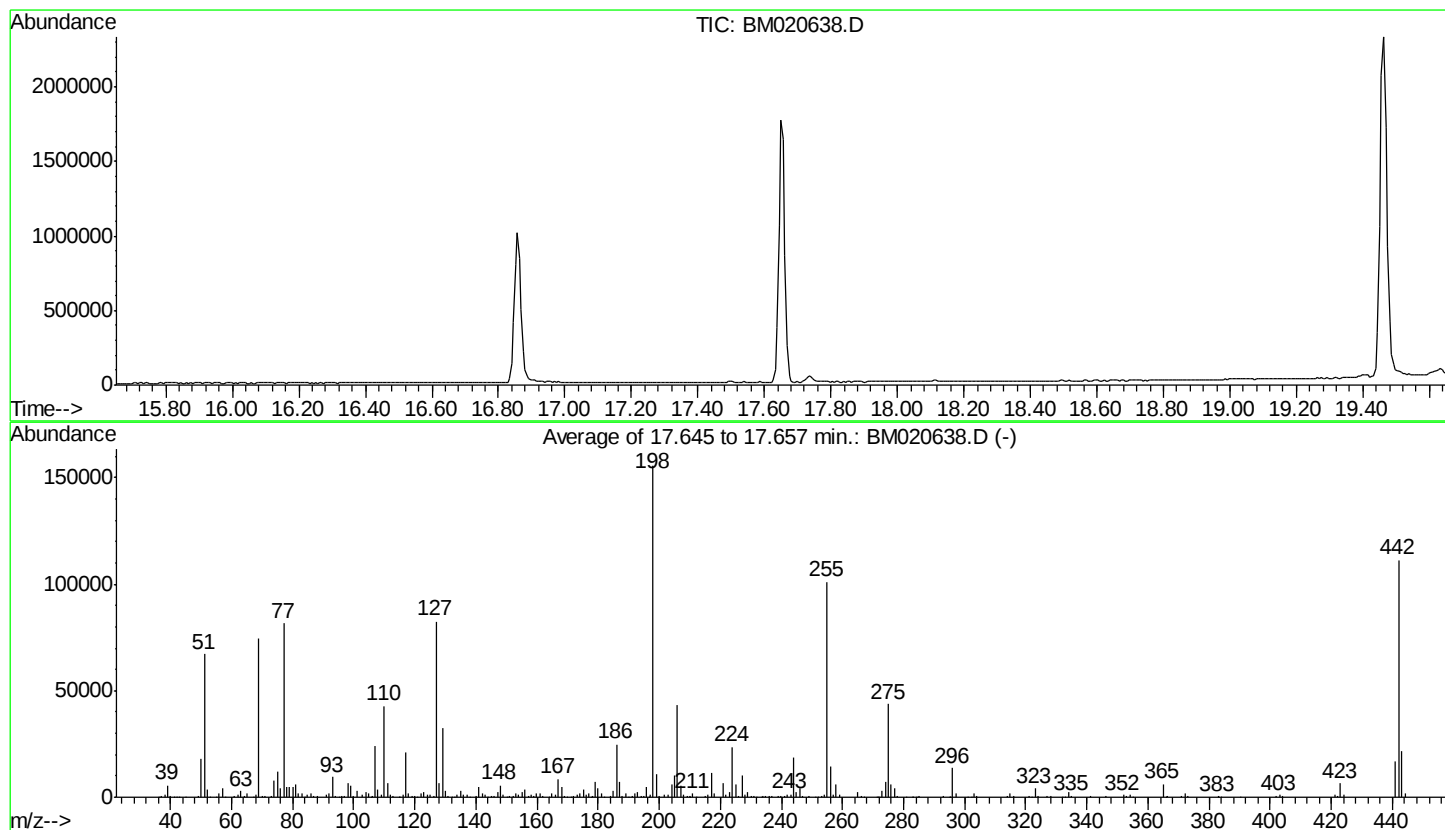

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 43.1      | 67160   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 1293    | PASS             |
| 69          | 198          | 0.00         | 100          | 47.9      | 74587   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 572     | PASS             |
| 127         | 198          | 10           | 80           | 53.0      | 82482   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 1114    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 155656  | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 10854   | PASS             |
| 275         | 198          | 10           | 60           | 28.1      | 43672   | PASS             |
| 365         | 198          | 1            | 100          | 4.1       | 6315    | PASS             |
| 441         | 198          | 0.01         | 100          | 10.9      | 16913   | PASS             |
| 442         | 198          | 50           | 100          | 71.6      | 111445  | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 21719   | PASS             |