

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060119\
 Data File : BM020658.D
 Acq On : 01 Jun 2019 19:45
 Operator : HP/JU
 Sample : K3105-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 66-67-TRACK

Quant Time: Jun 03 03:24:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 31 15:48:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	299516	20.00	ng	0.00
21) Naphthalene-d8	10.62	136	1271213	20.00	ng	0.00
39) Acenaphthene-d10	14.46	164	759974	20.00	ng	-0.01
64) Phenanthrene-d10	17.21	188	1688878	20.00	ng	0.00
76) Chrysene-d12	21.39	240	1336656	20.00	ng	-0.01
87) Perylene-d12	23.67	264	1290557	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	2518623	147.92	ng	0.00
7) Phenol-d6	7.00	99	3628120	144.71	ng	0.00
23) Nitrobenzene-d5	8.99	82	2248897	91.66	ng	0.00
42) 2,4,6-Tribromophenol	15.96	330	1485630	157.78	ng	0.00
45) 2-Fluorobiphenyl	13.09	172	4706727	82.34	ng	0.00
79) Terphenyl-d14	19.83	244	6969250	87.21	ng	-0.01
Target Compounds						
50) Dimethylphthalate	13.92	163	613617	9.451	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060119\
Data File : BM020658.D
Acq On : 01 Jun 2019 19:45
Operator : HP/JU
Sample : K3105-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
66-67-TRACK

Quant Time: Jun 03 03:24:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 31 15:48:49 2019
Response via : Initial Calibration

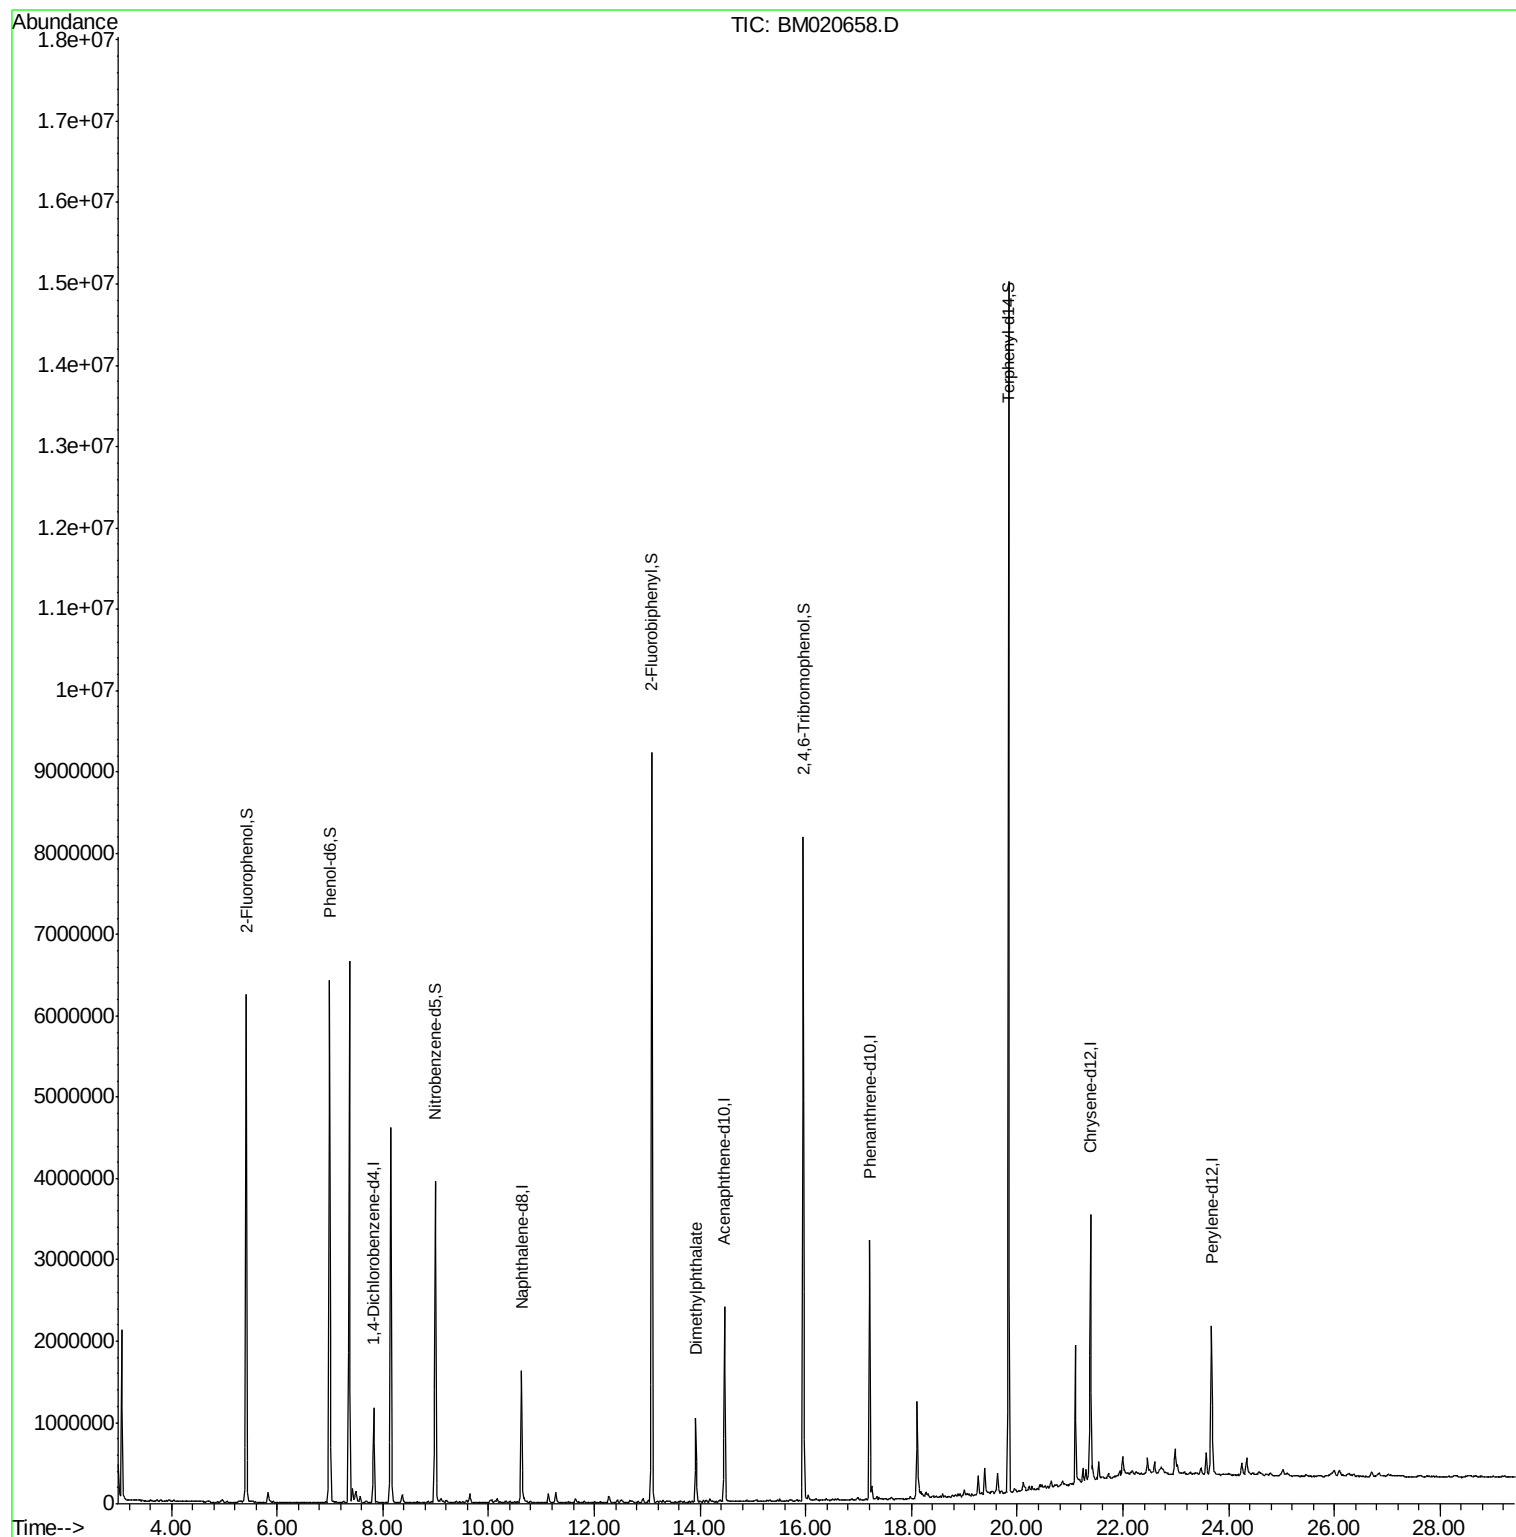

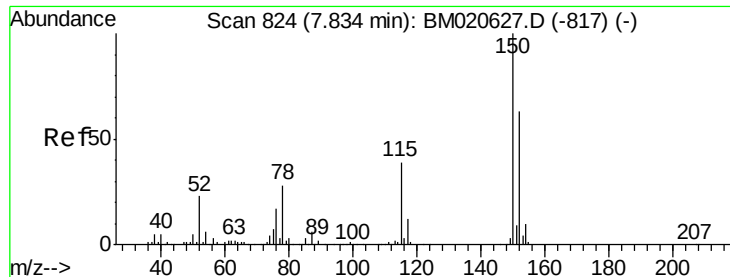


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.83 min Scan# 823
Delta R.T. -0.01 min
Lab File: BM020658.D
Acq: 01 Jun 2019 19:45

Instrument :
BNA_M
ClientSampleId :
66-67-TRACK

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.5	126.0	189.0
115	62.1	49.6	74.4



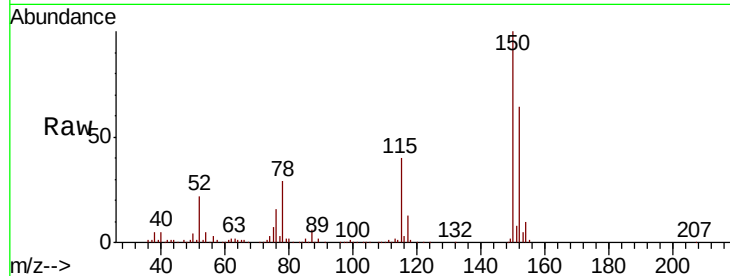


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

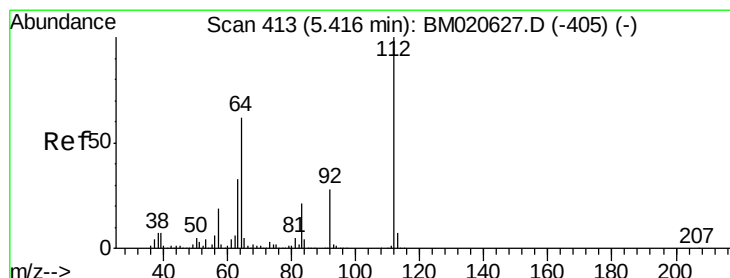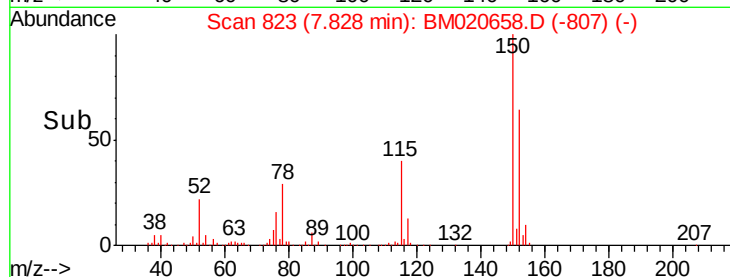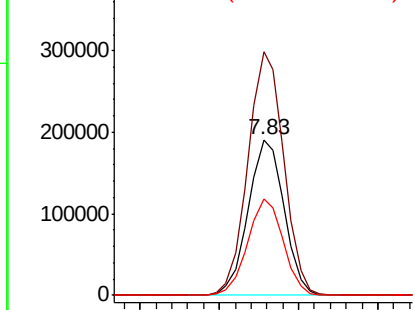

#5

2-Fluorophenol
Concen: 147.919 ng
RT: 5.42 min Scan# 413
Delta R.T. -0.00 min
Lab File: BM020658.D
Acq: 01 Jun 2019 19:45

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.5	49.7	74.5
63	33.0	26.4	39.6


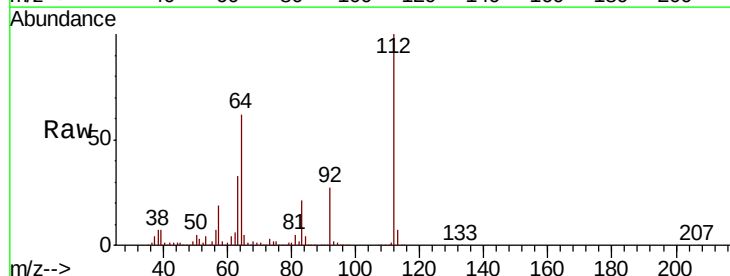



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

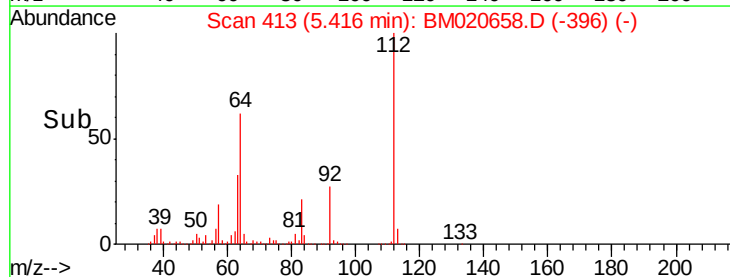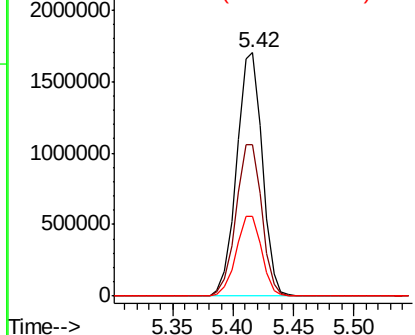

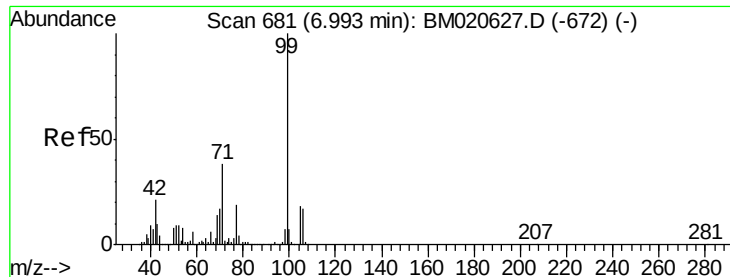

#7

Phenol-d6

Concen: 144.710 ng

RT: 7.00 min Scan# 682

Delta R.T. 0.01 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45

Instrument :


BNA_M

ClientSampleId :

66-67-TRACK

Tot Ion: 99 Resp: 3628120

Ion	Ratio	Lower	Upper
99	100		
42	19.0	16.5	24.7
71	37.3	30.7	46.1



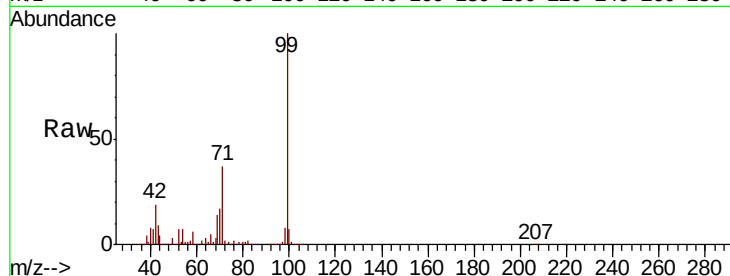


Abundance

Ion 99.00 (98.70 to 99.70): BM020627.D (-672) (-)

Ion 42.00 (41.70 to 42.70): BM020627.D (-672) (-)

Ion 71.00 (70.70 to 71.70): BM020627.D (-672) (-)

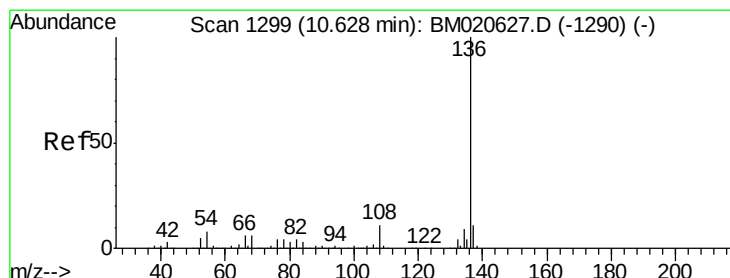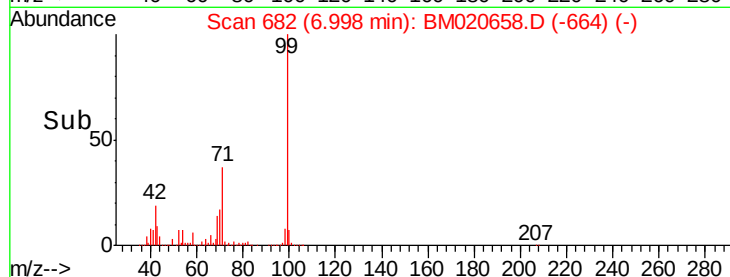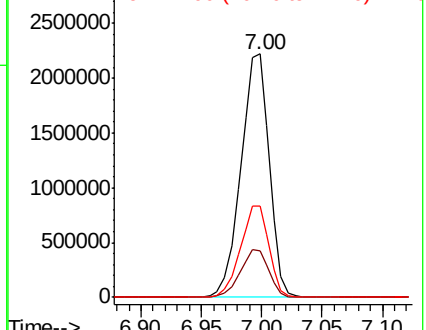

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.62 min Scan# 1298


Delta R.T. -0.01 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45

Tgt Ion: 136 Resp: 1271213

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	8.0	6.6	10.0
68	6.0	5.1	7.7

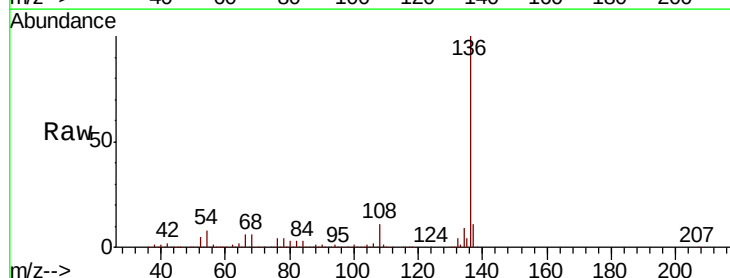



Abundance


Ion 136.00 (135.70 to 136.70): BM020627.D (-1290) (-)

Ion 137.00 (136.70 to 137.70): BM020627.D (-1290) (-)

Ion 54.00 (53.70 to 54.70): BM020627.D (-1290) (-)

Ion 68.00 (67.70 to 68.70): BM020627.D (-1290) (-)

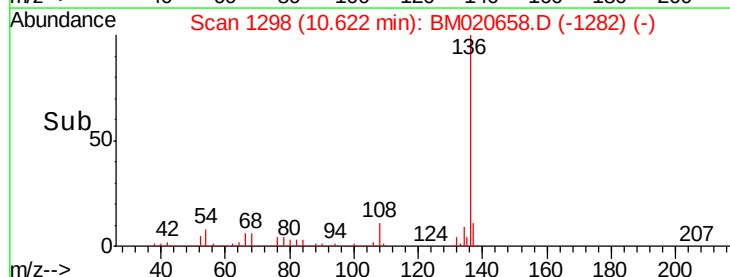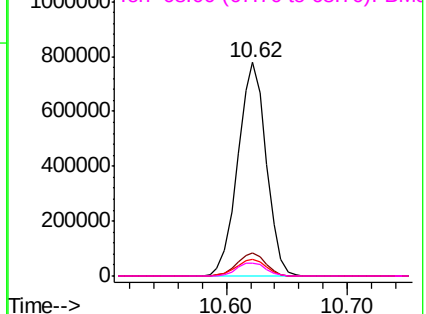


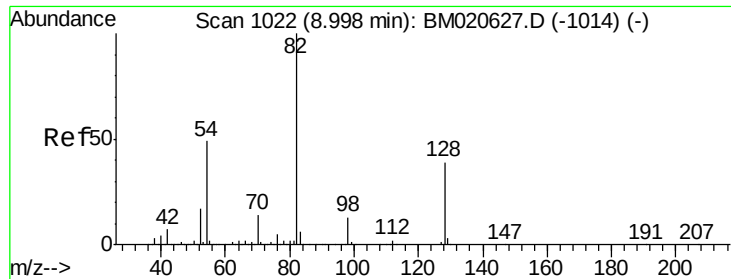




#23
Nitrobenzene-d5
Concen: 91.660 ng
RT: 8.99 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BM020658.D
Acq: 01 Jun 2019 19:45

Instrument :
BNA_M
ClientSampleId :
66-67-TRACK

Tot Ion: 82 Resp: 2248897
Ion Ratio Lower Upper
82 100
128 41.1 31.5 47.3
54 48.6 39.4 59.0

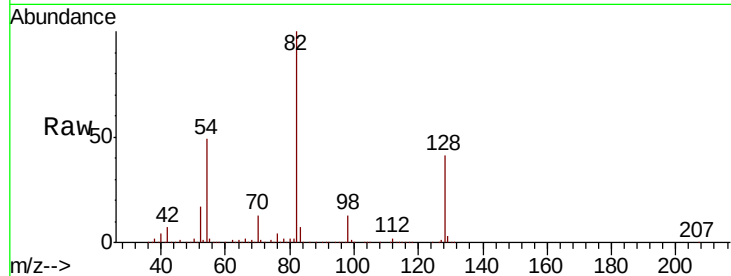


Abundance Ion 82.00 (81.70 to 82.70): BM020627.D (-1014) (-)
Ion 128.00 (127.70 to 128.70): BM020627.D (-1014) (-)
Ion 54.00 (53.70 to 54.70): BM020627.D (-1014) (-)

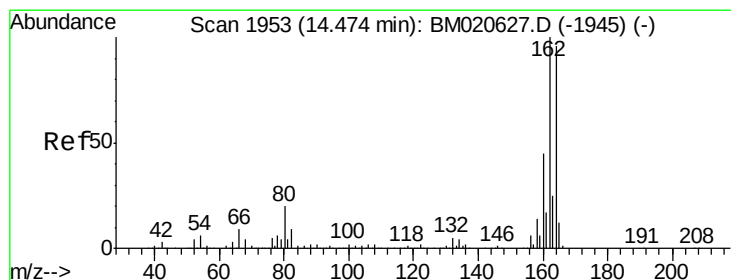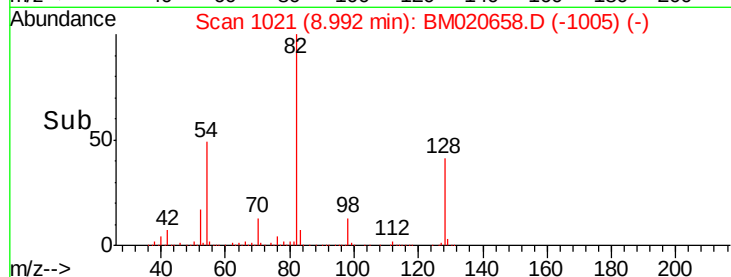
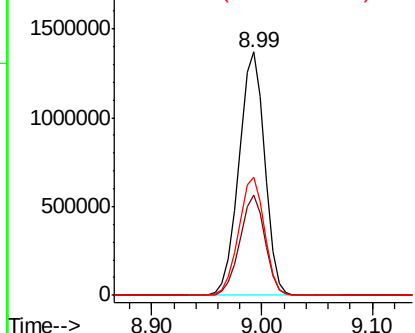



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.46 min Scan# 1951
Delta R.T. -0.01 min
Lab File: BM020658.D
Acq: 01 Jun 2019 19:45

Tgt Ion:164 Resp: 759974
Ion Ratio Lower Upper
164 100
162 102.3 83.2 124.8
160 45.8 37.5 56.3

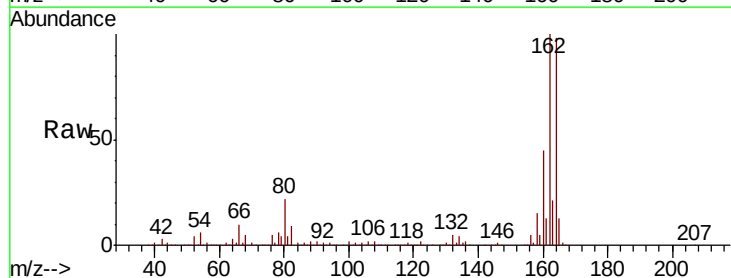

Abundance Ion 164.00 (163.70 to 164.70): BM020627.D (-1945) (-)
Ion 162.00 (161.70 to 162.70): BM020627.D (-1945) (-)
Ion 160.00 (159.70 to 160.70): BM020627.D (-1945) (-)

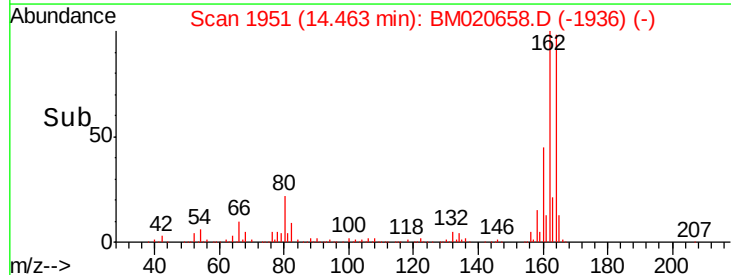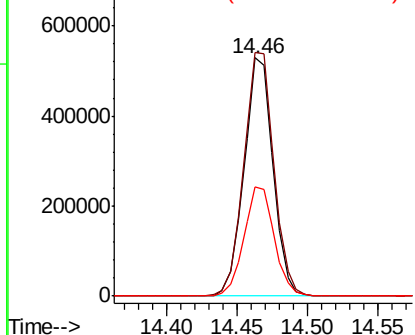

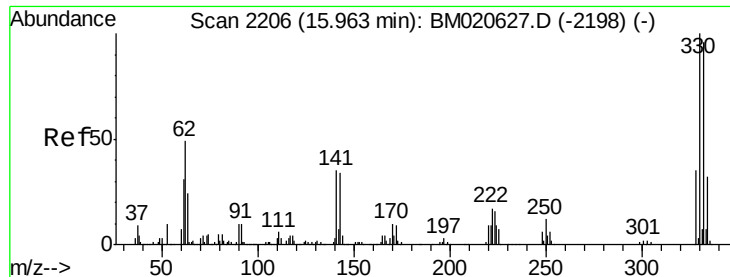

#42

2,4,6-Tribromophenol

Concen: 157.777 ng

RT: 15.96 min Scan# 2205

Delta R.T. -0.01 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45

Instrument :

BNA_M

ClientSampleId :

66-67-TRACK


Tot Ion:330 Resp: 1485630

Ion Ratio Lower Upper

330 100

332 96.6 77.4 116.0

141 35.9 30.4 45.6



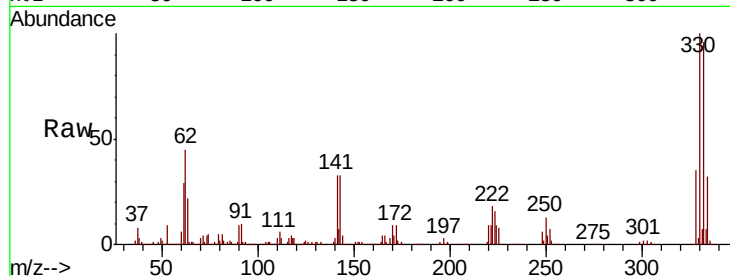


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

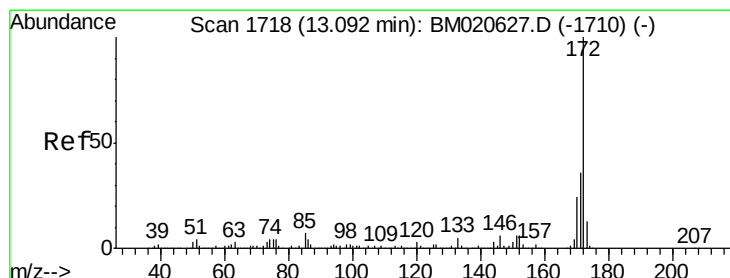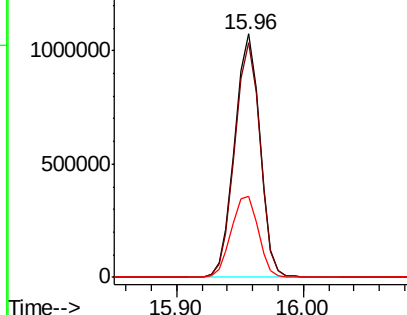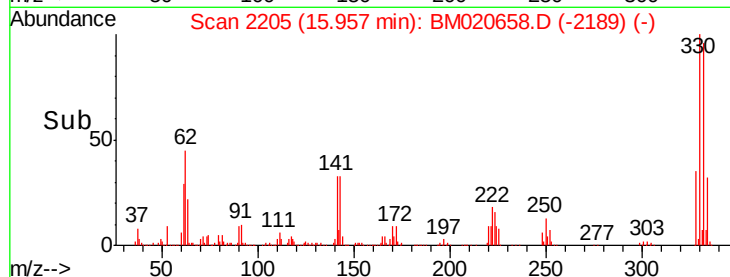

#45

2-Fluorobiphenyl

Concen: 82.337 ng

RT: 13.09 min Scan# 1717

Delta R.T. -0.01 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45


Tgt Ion:172 Resp: 4706727

Ion Ratio Lower Upper

172 100

171 36.1 28.6 43.0

170 23.6 18.9 28.3


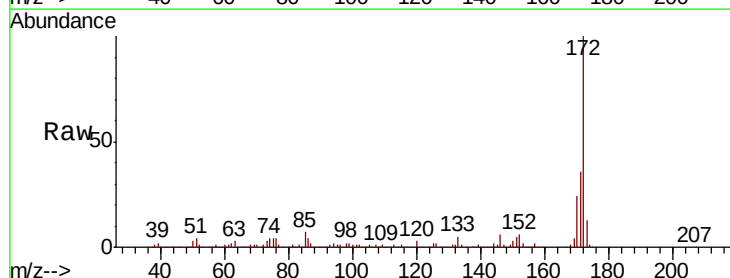



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

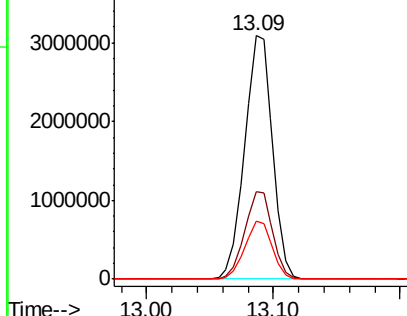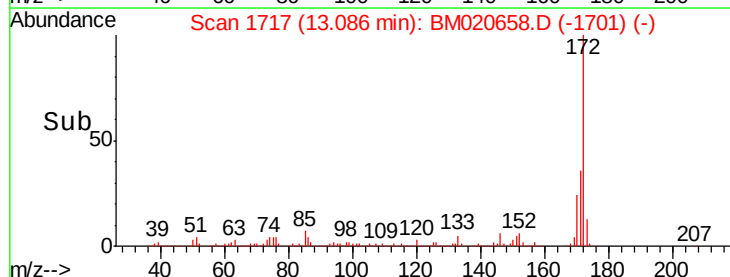

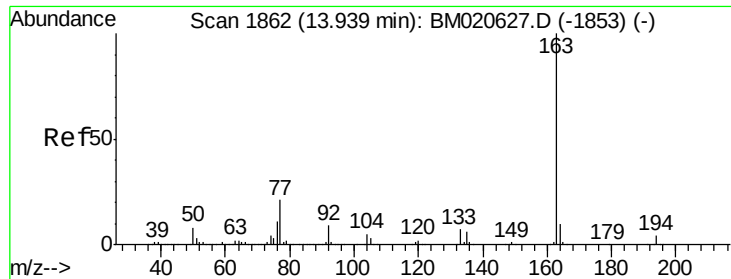

#50

Dimethylphthalate

Concen: 9.451 ng

RT: 13.92 min Scan# 1859

Delta R.T. -0.02 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45

Instrument :

BNA_M

ClientSampleId :

66-67-TRACK


Tot Ion:163 Resp: 613617

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8




164 9.9 7.9 11.9

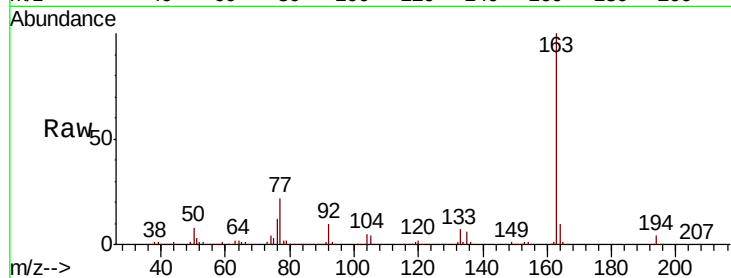

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

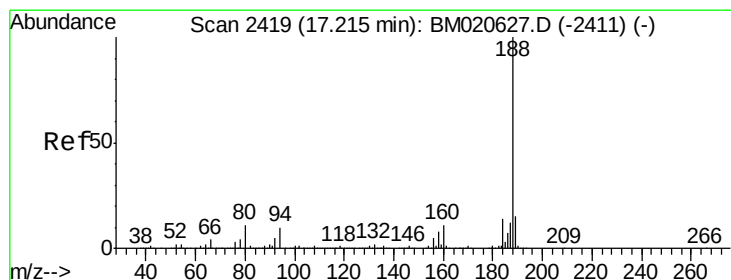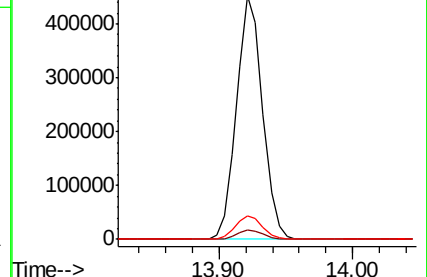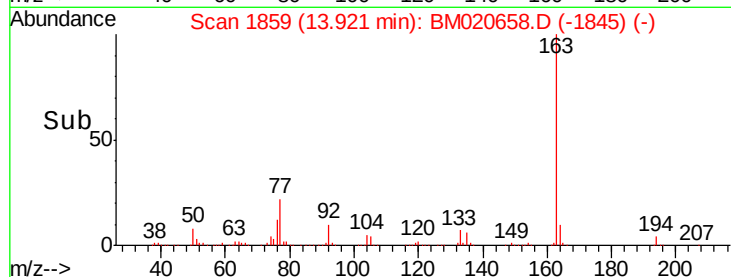

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.21 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BM020658.D

Acq: 01 Jun 2019 19:45


Tgt Ion:188 Resp: 1688878

Ion Ratio Lower Upper

188 100

94 9.6 7.8 11.8



80 11.4 9.0 13.6

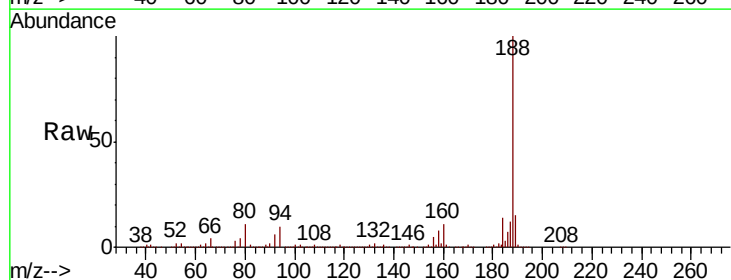


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

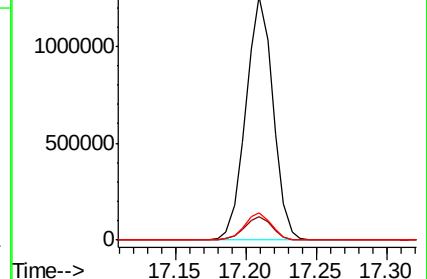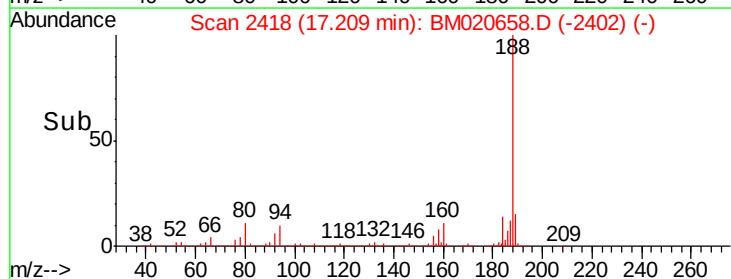


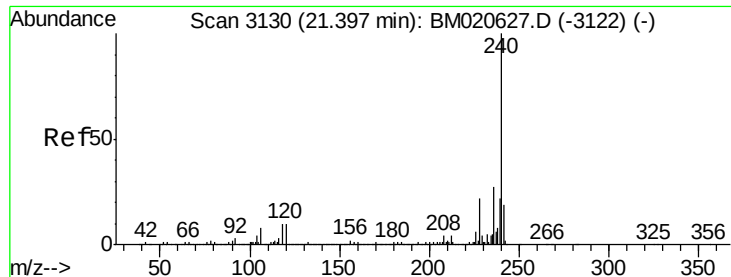




#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.39 min Scan# 3128
 Delta R.T. -0.01 min
 Lab File: BM020658.D
 Acq: 01 Jun 2019 19:45

Instrument :
 BNA_M
 ClientSampleId :
 66-67-TRACK

Tot Ion:240 Resp: 1336656
 Ion Ratio Lower Upper
 240 100
 120 10.9 8.2 12.2
 236 26.6 21.2 31.8

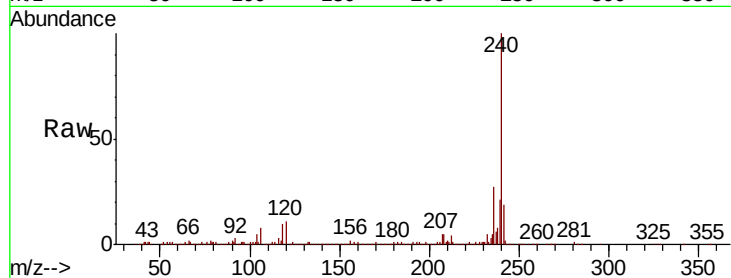


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

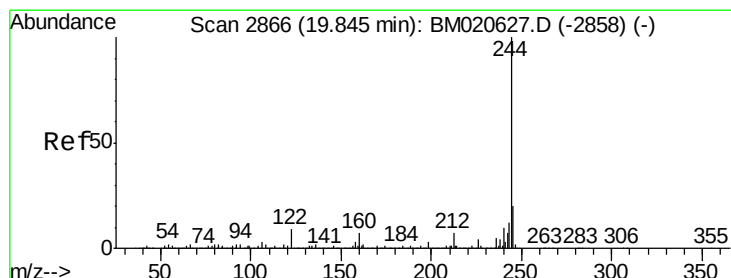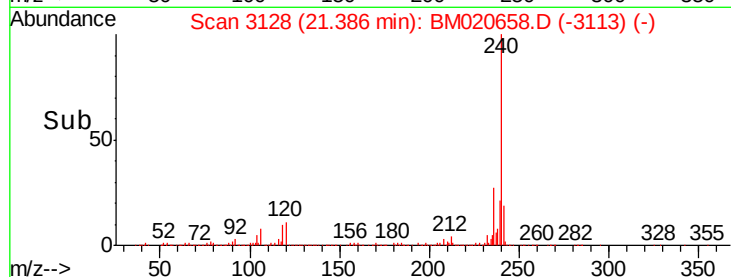
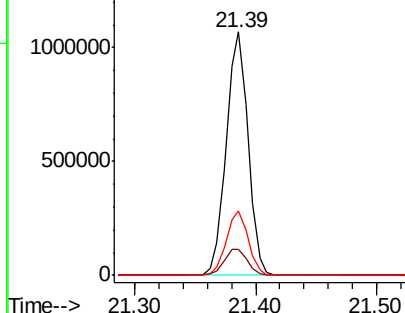



#79
 Terphenyl-d14
 Concen: 87.211 ng
 RT: 19.83 min Scan# 2864
 Delta R.T. -0.01 min
 Lab File: BM020658.D
 Acq: 01 Jun 2019 19:45

Tgt Ion:244 Resp: 6969250
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.7 8.5
 122 10.4 7.2 10.8

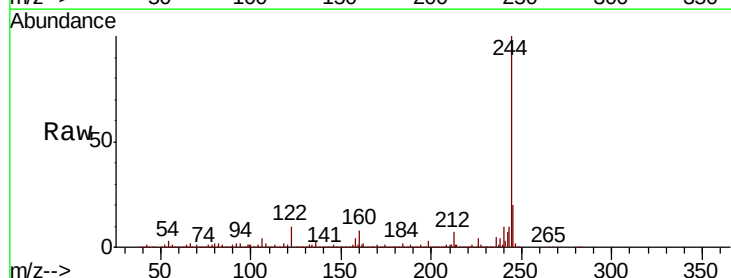

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

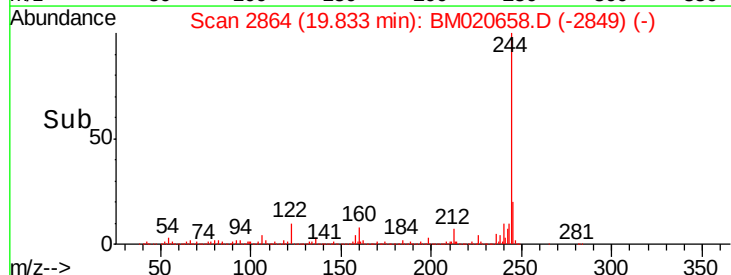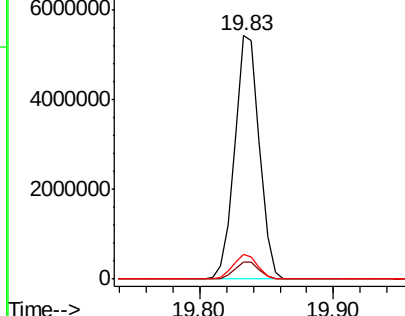

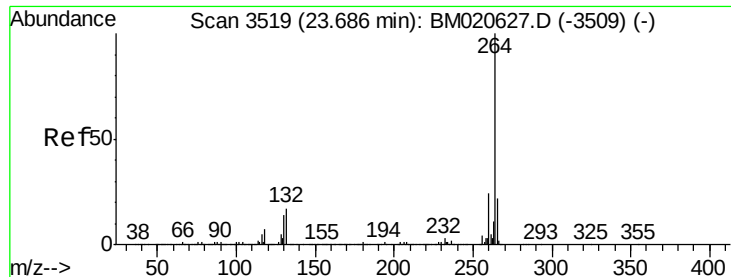

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.67 min Scan# 3517
Delta R.T. -0.01 min
Lab File: BM020658.D
Acq: 01 Jun 2019 19:45

Instrument :
BNA_M
ClientSampleId :
66-67-TRACK

Tot Ion: 264 Resp: 1290557

Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.2	28.8
265	22.0	17.6	26.4

