


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060119\
Data File : BM020643.D
Acq On : 01 Jun 2019 10:10
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 31 15:48:49 2019

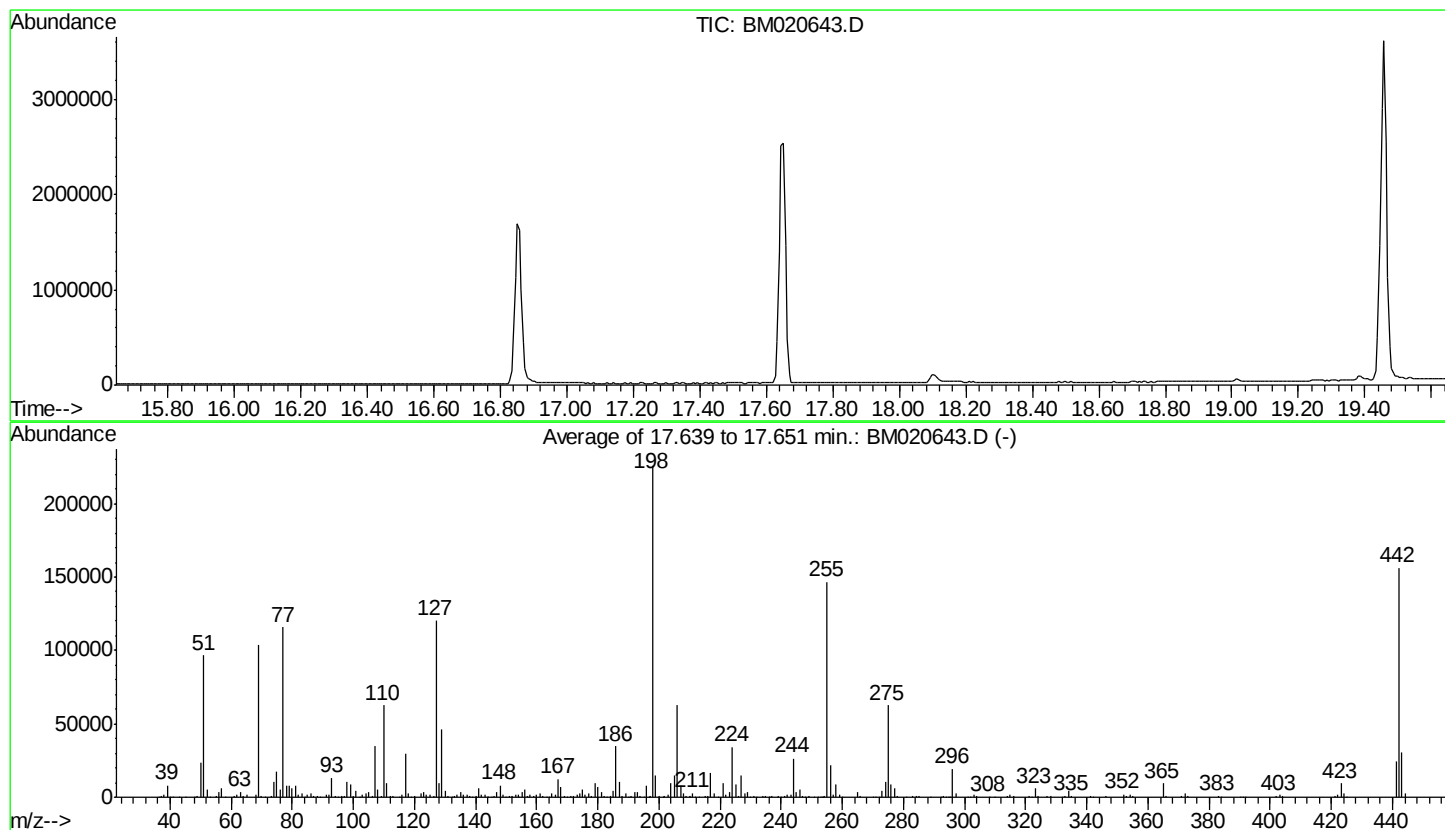

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	96420	PASS
68	69	0.00	2	1.9	2021	PASS
69	198	0.00	100	46.1	104143	PASS
70	69	0.00	2	0.6	676	PASS
127	198	10	80	53.1	119944	PASS
197	198	0.00	2	0.5	1202	PASS
198	198	100	100	100.0	225877	PASS
199	198	5	9	6.6	15017	PASS
275	198	10	60	27.8	62738	PASS
365	198	1	100	4.2	9498	PASS
441	198	0.01	100	10.8	24387	PASS
442	198	50	100	69.2	156258	PASS
443	442	15	24	19.3	30158	PASS