

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
 Data File : BM026212.D
 Acq On : 02 Jun 2020 00:17
 Operator : JU/CG
 Sample : L2829-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CE3

Manual Integrations
 APPROVED

mohammad
 6/2/2020 3:22:00 PM

Quant Time: Jun 02 11:01:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 01 16:59:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	166347	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	668910	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	448801	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.91	188	850996	20.00	ng/ul	0.04
78) Chrysene-d12	21.07	240	841448	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	827225	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	26500	4.81	ng/uL	0.00
5) Phenol-d5	6.67	99	126321	8.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	317529	30.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	303667	25.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	221403	19.47	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	194769	35.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	218347	40.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	360003	33.24	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.55	166	1208709	33.58	ng/ul	0.00
47) Acenaphthylene-d8	13.81	160	1466800	34.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	57243m	8.98	ng/ul	0.02
58) Fluorene-d10	15.13	176	1055910	33.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	227637m	45.88	ng/ul	0.00
71) Anthracene-d10	17.00	188	1632030	38.92	ng/ul	0.03
79) Pyrene-d10	19.28	212	1687251	39.04	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.06	264	1418860	32.22	ng/ul	0.00

Target Compounds

						Qvalue
16) 4-Methylphenol	8.26	108	19544	1.54	ng/ul	98
27) 2,4-Dichlorophenol	9.89	162	12339	1.10	ng/ul#	51
39) 2,4,6-Trichlorophenol	12.54	196	15612	1.67	ng/ul	97
40) 2,4,5-Trichlorophenol	12.62	196	26551	2.57	ng/ul	92
45) Dimethylphthalate	13.60	163	97574	2.58	ng/ul#	94
56) 2,3,4,6-Tetrachlorophenol	14.79	232	5966538	687.01	ng/ul	95
69) Pentachlorophenol	16.62	266	49057300m	7994.06	ng/ul	
77) Fluoranthene	18.94	202	71570	1.27	ng/ul#	83
80) Pyrene	19.31	202	163718	2.77	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026212.D
Acq On : 02 Jun 2020 00:17
Operator : JU/CG
Sample : L2829-10
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C5CE3

Quant Time: Jun 02 11:01:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 01 16:59:35 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/2/2020 3:22:00 PM

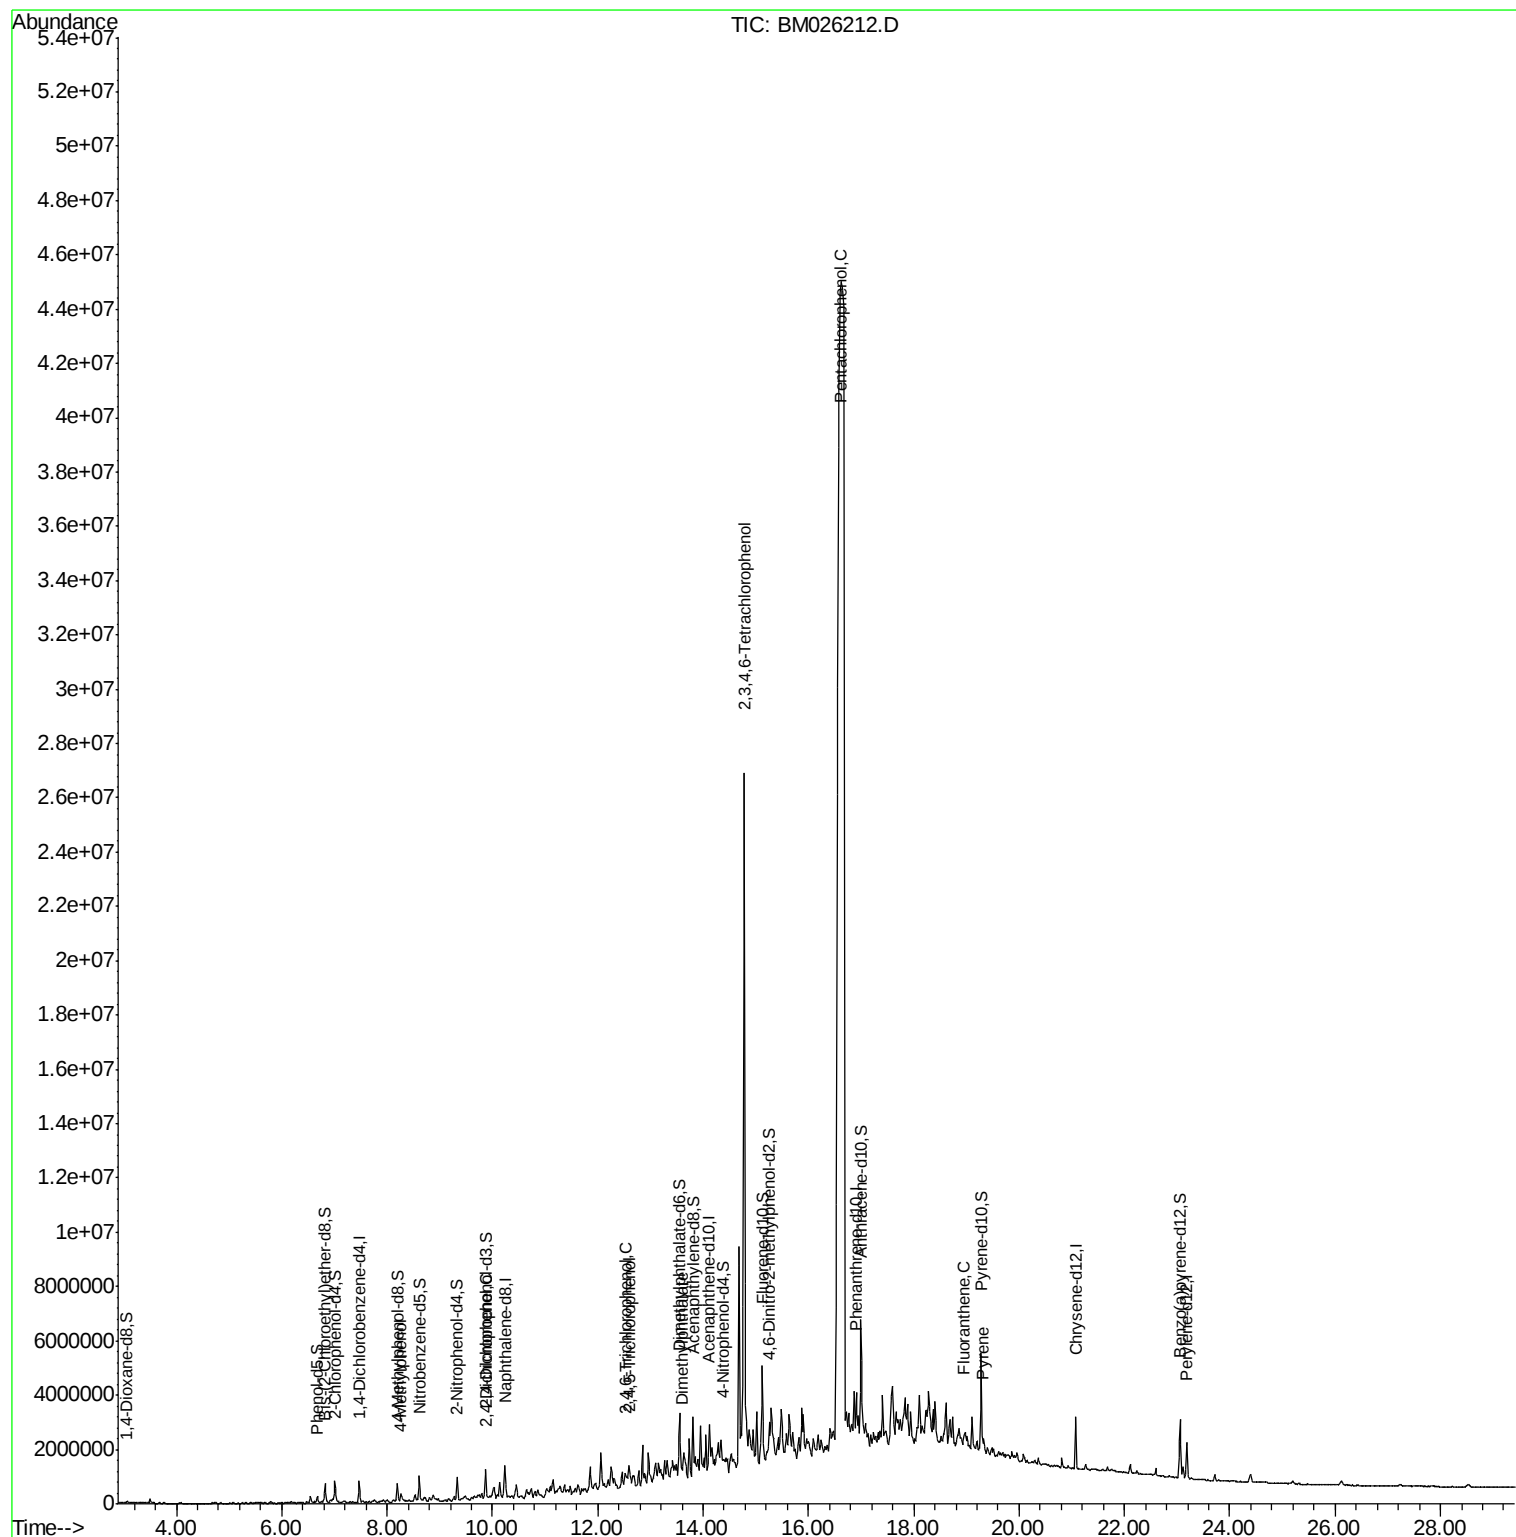

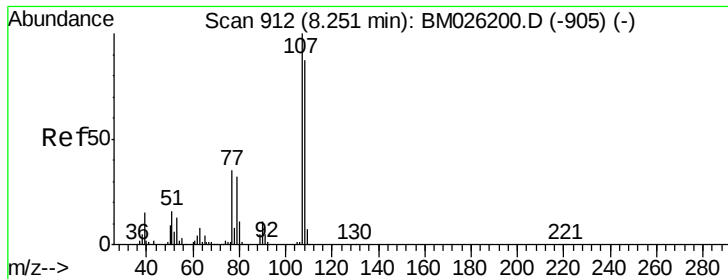





#16
4-Methylphenol
Concen: 1.54 ng/ul
RT: 8.26 min Scan# 913
Delta R.T. 0.01 min
Lab File: BM026212.D
Acq: 02 Jun 2020 00:17

Instrument :
BNA_M
ClientSampleId :
C5CE3

Tgt Ion	Ratio	Resp	Lower	Upper
108	100	19544		
107	113.2	88.6	132.8	




Manual Integrations
APPROVED


mohammad
6/2/2020 3:22:00 PM

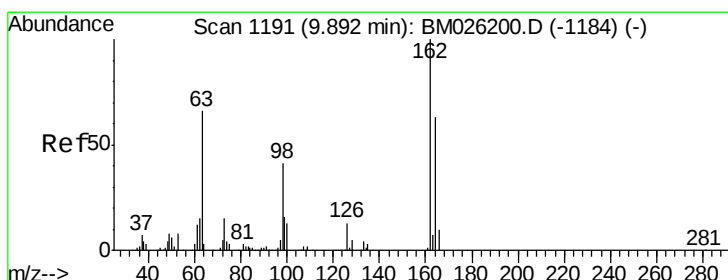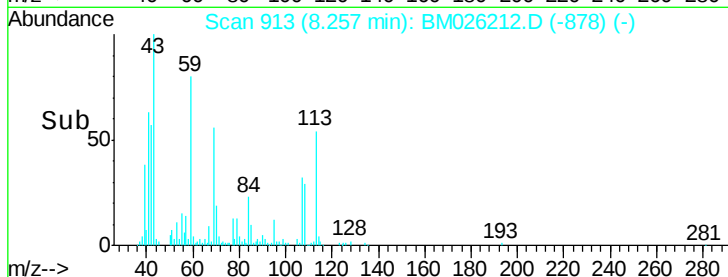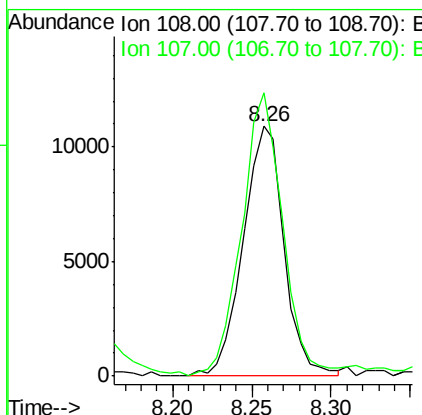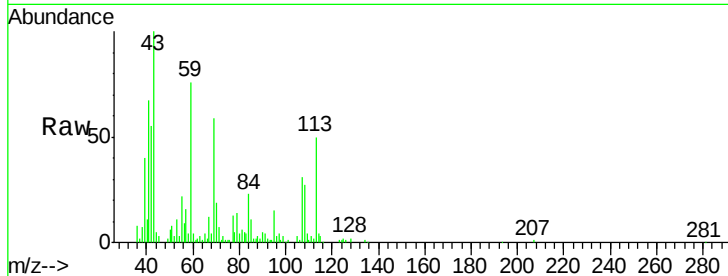

#27
2,4-Dichlorophenol
Concen: 1.10 ng/ul
RT: 9.89 min Scan# 1191
Delta R.T. 0.00 min
Lab File: BM026212.D
Acq: 02 Jun 2020 00:17

Tgt Ion	Ratio	Resp	Lower	Upper
162	100	12339		
164	114.2	51.0	76.4#	
98	55.3	32.1	48.1#	

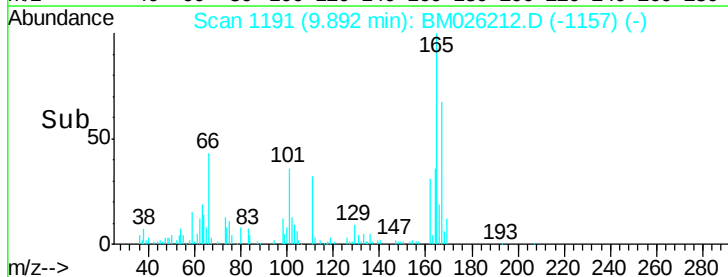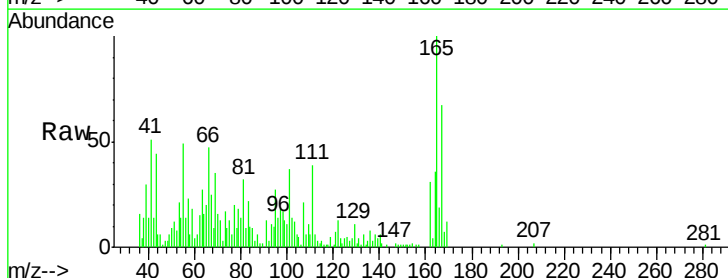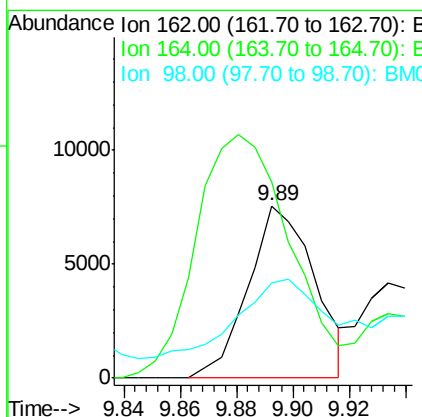

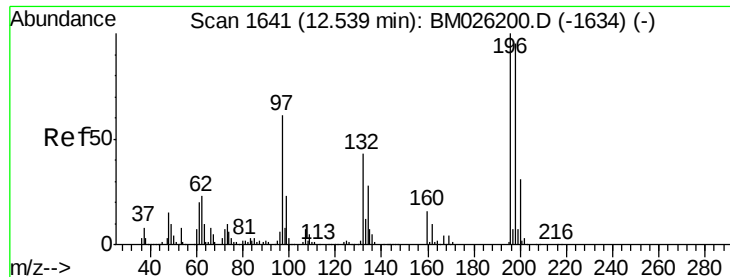





#39
 2,4,6-Trichlorophenol
 Concen: 1.67 ng/ul
 RT: 12.54 min Scan# 1641
 Delta R.T. 0.00 min
 Lab File: BM026212.D
 Acq: 02 Jun 2020 00:17

Instrument :
 BNA_M
 ClientSampleId :
 C5CE3

Tgt Ion:	196	Resp:	15612
Ion Ratio	Lower	Upper	
196	100		
198	93.3	76.0	114.0
200	34.1	24.5	36.7




Manual Integrations
 APPROVED


mohammad
 6/2/2020 3:22:00 PM

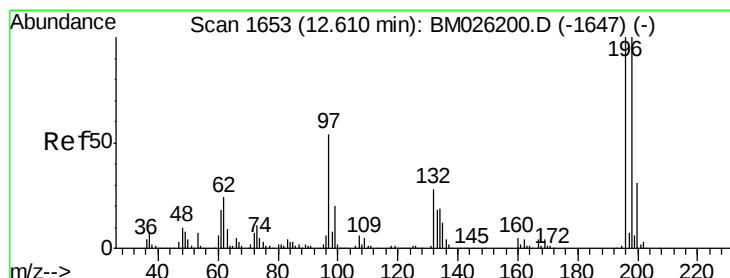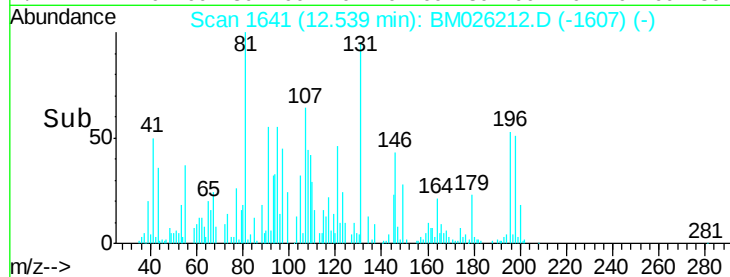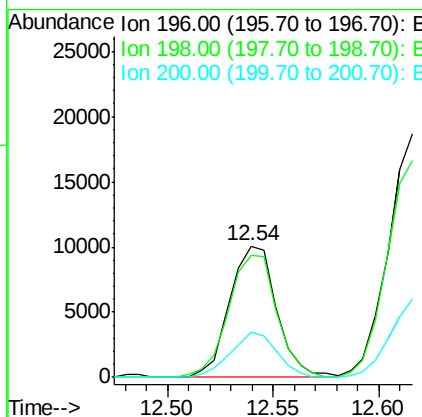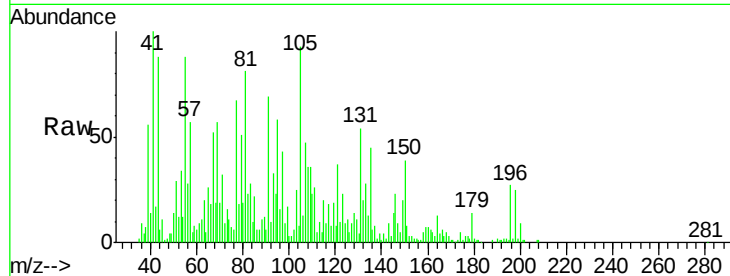

#40
 2,4,5-Trichlorophenol
 Concen: 2.57 ng/ul
 RT: 12.62 min Scan# 1654
 Delta R.T. 0.01 min
 Lab File: BM026212.D
 Acq: 02 Jun 2020 00:17

Tgt Ion:	196	Resp:	26551
Ion Ratio	Lower	Upper	
196	100		
198	88.8	79.0	118.6
200	32.2	25.0	37.4

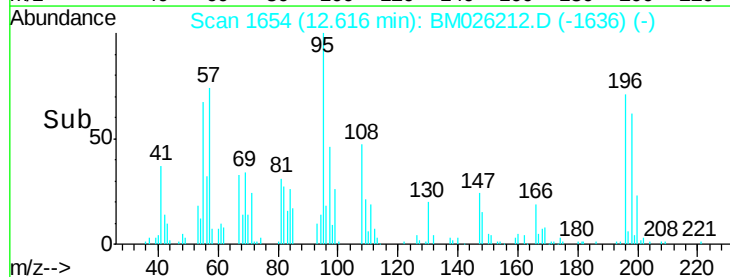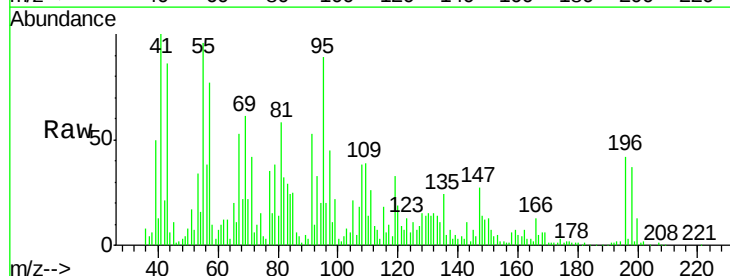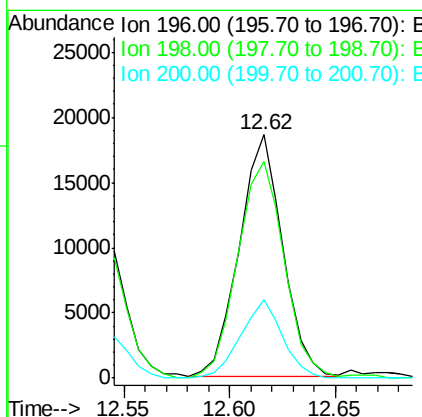

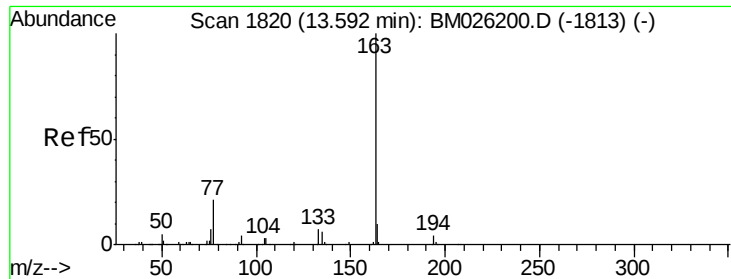





#45
Dimethylphthalate
Concen: 2.58 ng/ul
RT: 13.60 min Scan# 1821
Delta R.T. 0.01 min
Lab File: BM026212.D
Acq: 02 Jun 2020 00:17

Instrument :
BNA_M
ClientSampleId :
C5CE3

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	97574		
194	3.7		3.2	4.8
164	13.0		8.0	12.0#




Manual Integrations
APPROVED


mohammad
6/2/2020 3:22:00 PM

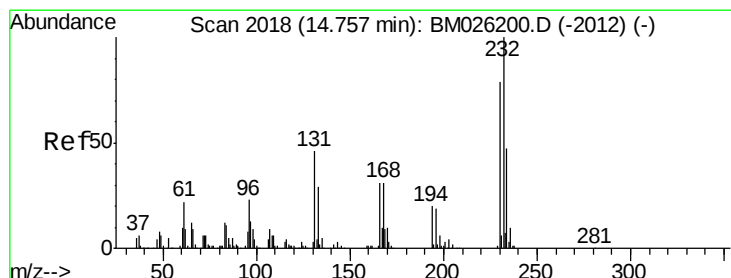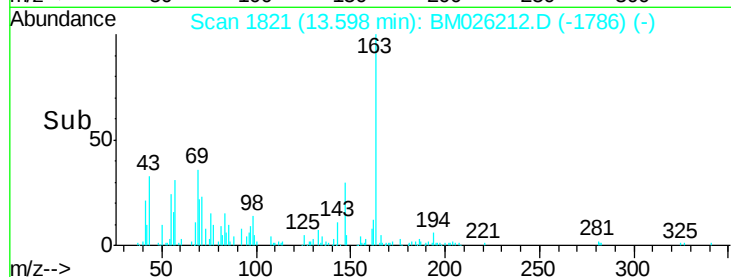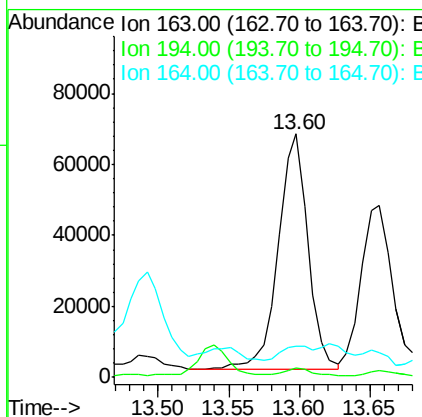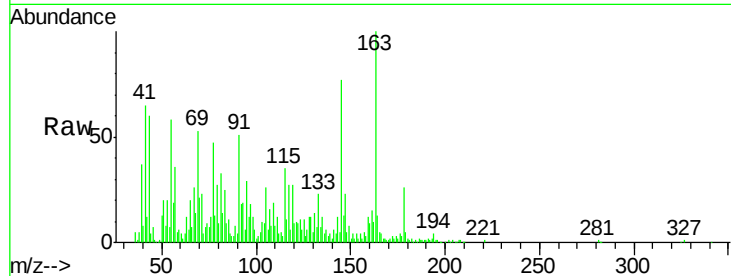

#56
2,3,4,6-Tetrachlorophenol
Concen: 687.01 ng/ul
RT: 14.79 min Scan# 2023
Delta R.T. 0.03 min
Lab File: BM026212.D
Acq: 02 Jun 2020 00:17

Tgt Ion	Ratio	Resp	Lower	Upper
232	100	5966538		
131	41.5		37.0	55.4
130	2.4		1.8	2.8
166	29.7		25.4	38.0

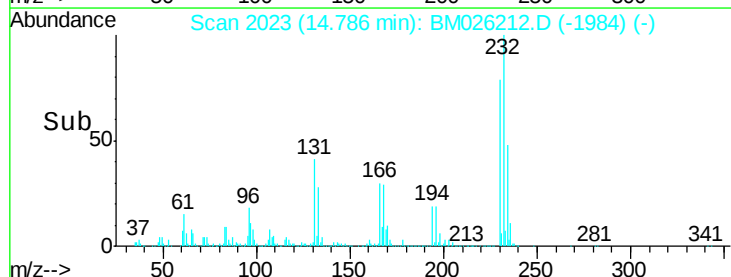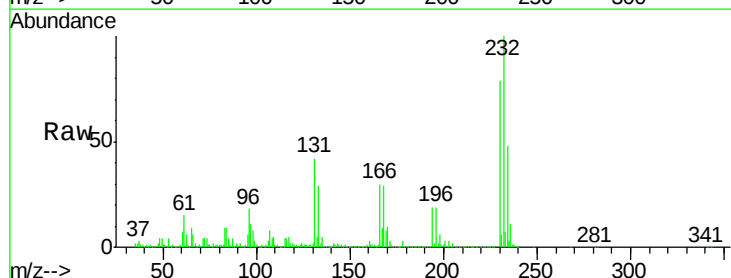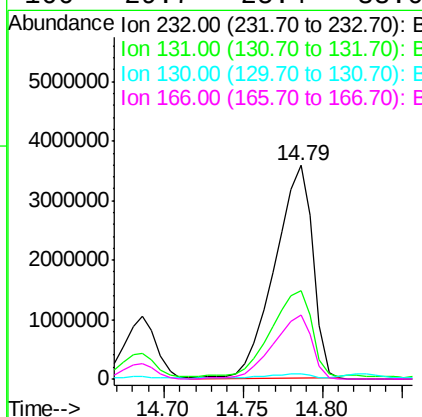

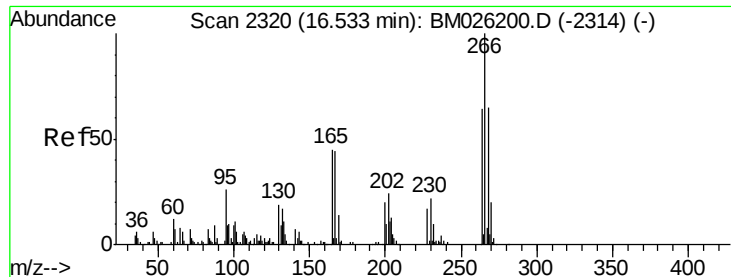





#69
 Pentachlorophenol
 Concen: 7994.06 ng/ul m
 RT: 16.62 min Scan# 2335
 Delta R.T. 0.09 min
 Lab File: BM026212.D
 Acq: 02 Jun 2020 00:17

Instrument :
 BNA_M
 ClientSampleId :
 C5CE3

Tgt Ion:266 Resp:49057300
 Ion Ratio Lower Upper
 266 100
 264 65.0 49.3 73.9
 268 65.5 52.4 78.6




Manual Integrations
 APPROVED


mohammad
 6/2/2020 3:22:00 PM

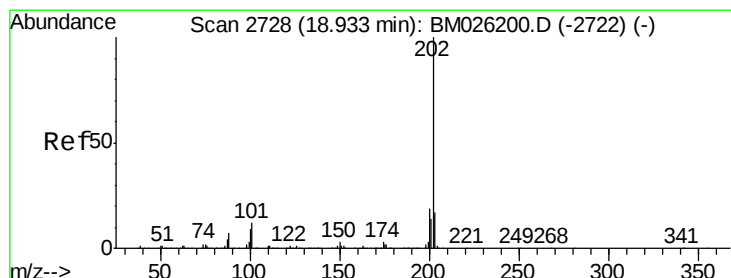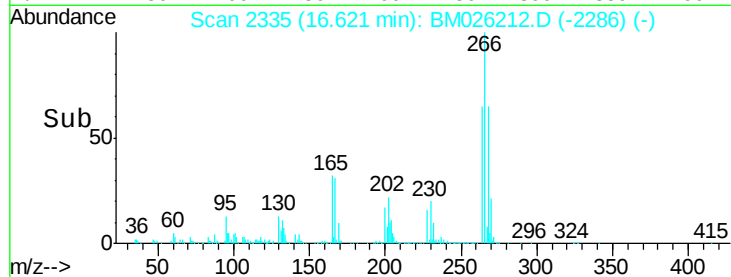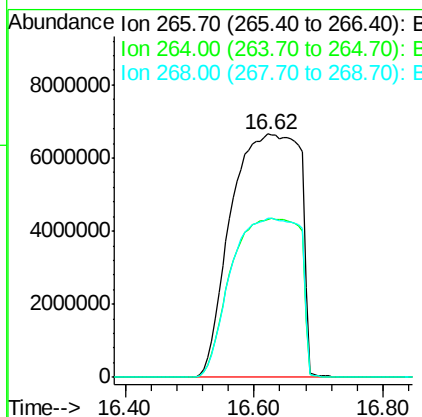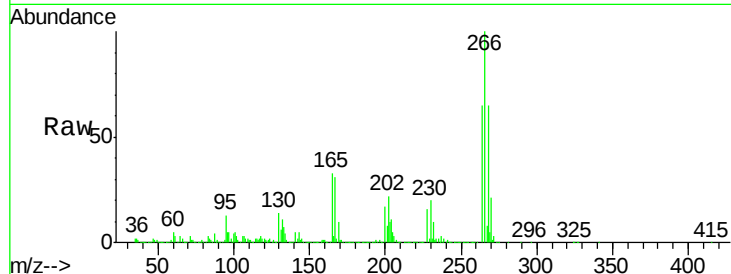

#77
 Fluoranthene
 Concen: 1.27 ng/ul
 RT: 18.94 min Scan# 2730
 Delta R.T. 0.01 min
 Lab File: BM026212.D
 Acq: 02 Jun 2020 00:17

Tgt Ion:202 Resp: 71570
 Ion Ratio Lower Upper
 202 100
 101 21.2 9.5 14.3#
 100 12.9 7.6 11.4#

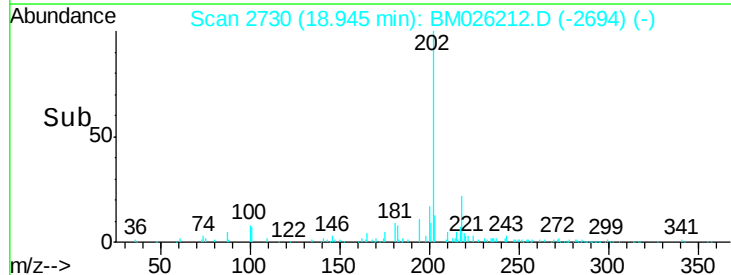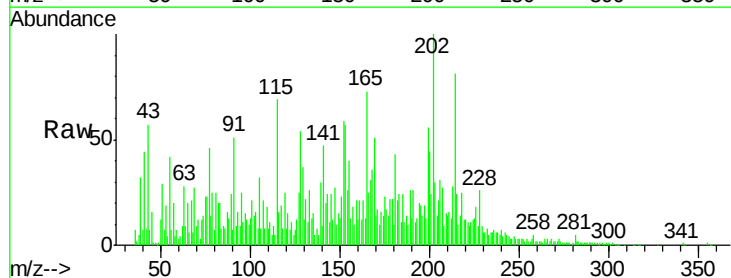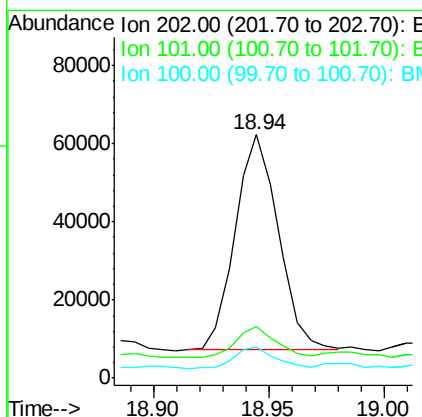

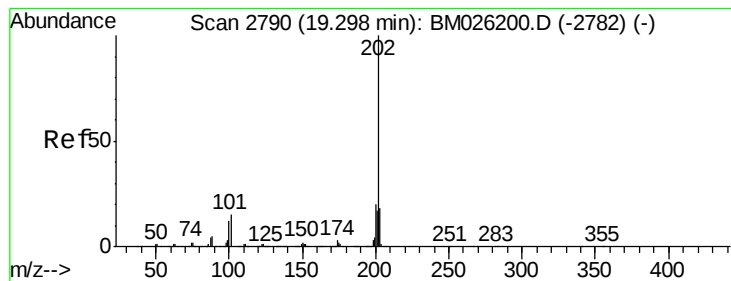

#80

Pyrene

Concen: 2.77 ng/ul

RT: 19.31 min Scan# 2792

Delta R.T. 0.01 min

Lab File: BM026212.D


Acq: 02 Jun 2020 00:17

Instrument :

BNA_M

ClientSampleId :

C5CE3

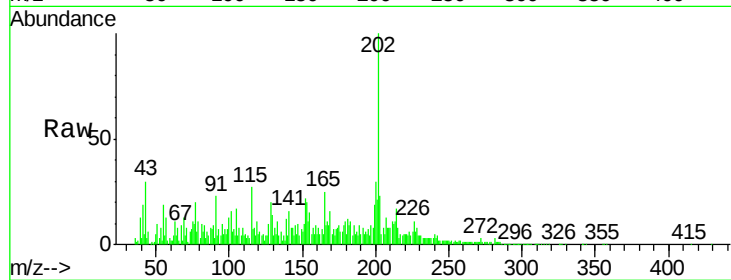

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		163718		
101	16.5	12.2	18.4		
100	13.1	10.2	15.4		

Manual Integrations
APPROVED

mohammad
6/2/2020 3:22:00 PM

