

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
 Data File : BM026217.D
 Acq On : 02 Jun 2020 08:30
 Operator : JU/CG
 Sample : L2829-01DL 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.752	144	147	153	rVB2	12469	17458	0.61%	0.101%
2	5.522	444	448	452	rBV6	1589	2855	0.10%	0.016%
3	6.675	639	644	651	rBV	14680	25617	0.90%	0.148%
4	6.828	664	670	677	rVB	48454	78741	2.76%	0.455%
5	7.010	696	701	708	rBV	52419	86548	3.04%	0.500%
6	7.469	773	779	788	rBV	802065	1212484	42.54%	7.001%
7	8.193	896	902	913	rVB2	38889	62507	2.19%	0.361%
8	8.616	968	974	983	rBV	58201	95092	3.34%	0.549%
9	9.334	1089	1096	1101	rBV2	41644	69532	2.44%	0.402%
10	9.875	1181	1188	1195	rBV	62105	110971	3.89%	0.641%
11	10.234	1241	1249	1260	rBV	1039569	1661483	58.29%	9.594%
12	10.398	1274	1277	1286	rVB7	4774	7105	0.25%	0.041%
13	10.863	1351	1356	1360	rVB7	2283	4115	0.14%	0.024%
14	11.792	1512	1514	1518	rVB4	2928	3848	0.14%	0.022%
15	11.833	1518	1521	1525	rVB5	2894	2908	0.10%	0.017%
16	11.922	1532	1536	1542	rBV7	2148	4741	0.17%	0.027%
17	12.257	1588	1593	1595	rBV5	2357	3507	0.12%	0.020%
18	12.539	1638	1641	1646	rVB4	4287	6784	0.24%	0.039%
19	12.616	1648	1654	1660	rVB5	16469	29774	1.04%	0.172%
20	12.851	1690	1694	1700	rVV4	10159	16363	0.57%	0.094%
21	13.416	1787	1790	1791	rBV2	3586	3841	0.13%	0.022%
22	13.539	1805	1811	1817	rBV	128915	191878	6.73%	1.108%
23	13.586	1817	1819	1823	rVB3	9707	11916	0.42%	0.069%
24	13.804	1849	1856	1863	rBV	150808	219308	7.69%	1.266%
25	13.945	1877	1880	1882	rBV4	3706	4737	0.17%	0.027%
26	14.051	1894	1898	1901	rBV5	3446	4169	0.15%	0.024%
27	14.116	1902	1909	1920	rBV	1417272	2052895	72.02%	11.854%
28	14.374	1947	1953	1958	rBV9	7173	16039	0.56%	0.093%
29	14.621	1993	1995	1998	rVB3	2779	3086	0.11%	0.018%
30	14.674	1998	2004	2010	rBV	91576	142033	4.98%	0.820%
31	14.721	2010	2012	2013	rVV2	9561	7794	0.27%	0.045%
32	14.757	2015	2018	2024	rVB2	30374	43542	1.53%	0.251%
33	14.886	2033	2040	2043	rBV7	5708	11757	0.41%	0.068%
34	14.951	2049	2051	2056	rVB5	4166	6401	0.22%	0.037%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
 Data File : BM026217.D
 Acq On : 02 Jun 2020 08:30
 Operator : JU/CG
 Sample : L2829-01DL 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	15.116	2072	2079	2085	rBV	197176	291198	10.22%	1.682%
36	15.257	2098	2103	2104	rBV2	35642	47733	1.67%	0.276%
37	15.280	2104	2107	2116	rVV	116360	179346	6.29%	1.036%
38	15.357	2118	2120	2123	rVB4	5942	6740	0.24%	0.039%
39	15.421	2129	2131	2136	rVB5	5720	7369	0.26%	0.043%
40	15.469	2136	2139	2142	rBV4	5494	6059	0.21%	0.035%
41	15.574	2151	2157	2158	rBV6	7990	12600	0.44%	0.073%
42	15.639	2164	2168	2171	rBV6	6573	9211	0.32%	0.053%
43	15.733	2181	2184	2185	rBV3	3026	3341	0.12%	0.019%
44	15.827	2196	2200	2201	rBV4	4712	5620	0.20%	0.032%
45	15.845	2201	2203	2205	rBV3	3452	3119	0.11%	0.018%
46	15.898	2210	2212	2213	rBV2	4813	3607	0.13%	0.021%
47	16.068	2239	2241	2243	rVB3	4317	3849	0.14%	0.022%
48	16.445	2302	2305	2308	rBV5	3838	4976	0.17%	0.029%
49	16.527	2312	2319	2337	rBV	1144794	1762808	61.85%	10.179%
50	16.821	2367	2369	2371	rBV2	5285	4272	0.15%	0.025%
51	16.868	2371	2377	2388	rVV	1734465	2416813	84.79%	13.956%
52	16.963	2388	2393	2404	rVB	208996	318217	11.16%	1.838%
53	19.268	2780	2785	2792	rBV	276663	357515	12.54%	2.064%
54	21.068	3086	3091	3099	rBV	2301598	2801138	98.27%	16.175%
55	23.186	3445	3451	3464	rVB	1669079	2850312	100.00%	16.459%


Sum of corrected areas: 17317672

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026217.D
Acq On : 02 Jun 2020 08:30
Operator : JU/CG
Sample : L2829-01DL 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC5DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

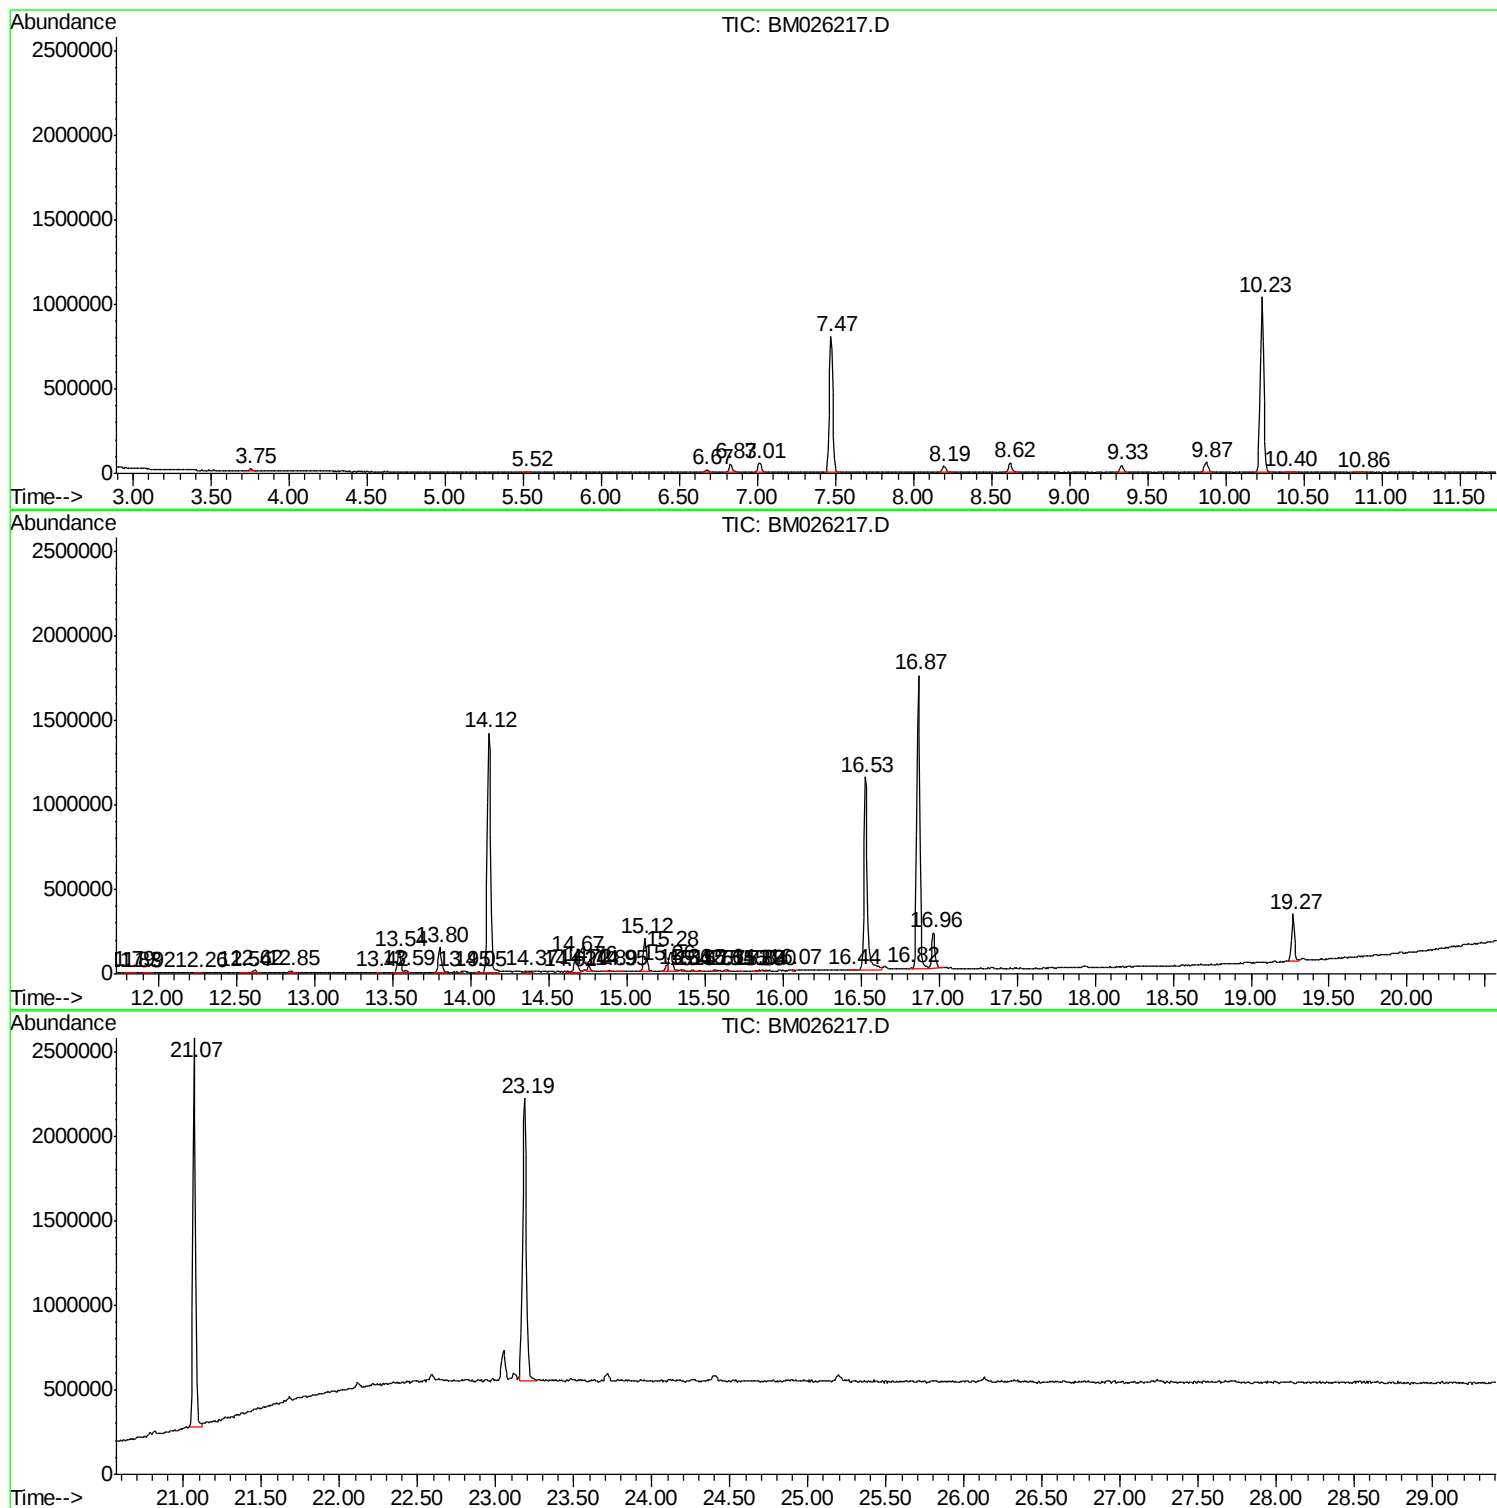

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026217.D
Acq On : 02 Jun 2020 08:30
Operator : JU/CG
Sample : L2829-01DL 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC5DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026217.D
Acq On : 02 Jun 2020 08:30
Operator : JU/CG
Sample : L2829-01DL 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CC5DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc