

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
 Data File : BM026234.D
 Acq On : 02 Jun 2020 19:05
 Operator : JU/CG
 Sample : L2829-07DL2 100X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	88	90	93	rBV3	2780	2428	0.12%	0.021%
2	3.752	143	147	152	rVB2	9019	12370	0.59%	0.105%
3	3.981	182	186	192	rVB9	3956	6769	0.32%	0.058%
4	5.516	442	447	450	rBV6	2514	4140	0.20%	0.035%
5	5.593	458	460	465	rVB6	1659	2424	0.12%	0.021%
6	6.358	586	590	592	rVB3	1863	2399	0.11%	0.020%
7	6.681	639	645	648	rBV4	2099	3554	0.17%	0.030%
8	6.834	665	671	675	rBV7	3885	7642	0.37%	0.065%
9	7.010	696	701	706	rBV6	4537	6873	0.33%	0.059%
10	7.128	713	721	727	rVB3	7616	11295	0.54%	0.096%
11	7.469	772	779	788	rBV	569850	879010	42.02%	7.486%
12	7.593	794	800	802	rBV3	5864	8311	0.40%	0.071%
13	7.716	818	821	825	rBV5	1889	3002	0.14%	0.026%
14	7.834	837	841	845	rVB6	2722	3899	0.19%	0.033%
15	8.210	899	905	907	rBV5	3303	4691	0.22%	0.040%
16	8.634	972	977	986	rBV8	3635	8927	0.43%	0.076%
17	8.946	1028	1030	1037	rBV7	1376	3071	0.15%	0.026%
18	9.093	1051	1055	1057	rVB4	2128	2515	0.12%	0.021%
19	9.334	1092	1096	1099	rBV5	2681	3740	0.18%	0.032%
20	9.651	1143	1150	1152	rBV5	2590	4525	0.22%	0.039%
21	9.704	1154	1159	1161	rVB4	1578	2460	0.12%	0.021%
22	9.740	1161	1165	1170	rVB3	1484	2902	0.14%	0.025%
23	9.893	1186	1191	1192	rBV4	3634	4733	0.23%	0.040%
24	10.228	1241	1248	1254	rBV	748109	1215369	58.10%	10.351%
25	10.275	1254	1256	1266	rVB	37843	58627	2.80%	0.499%
26	10.657	1314	1321	1322	rBV2	2120	2517	0.12%	0.021%
27	10.869	1354	1357	1360	rBV4	1478	2120	0.10%	0.018%
28	11.910	1529	1534	1543	rVB2	10412	22173	1.06%	0.189%
29	12.063	1551	1560	1563	rBV8	3454	7255	0.35%	0.062%
30	12.098	1563	1566	1567	rVV3	2000	2599	0.12%	0.022%
31	12.128	1567	1571	1576	rVB3	9954	16632	0.80%	0.142%
32	12.245	1590	1591	1594	rBV3	2092	2205	0.11%	0.019%
33	12.457	1623	1627	1631	rBV4	1668	2405	0.11%	0.020%
34	12.504	1631	1635	1640	rVV7	1408	2310	0.11%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
 Data File : BM026234.D
 Acq On : 02 Jun 2020 19:05
 Operator : JU/CG
 Sample : L2829-07DL2 100X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	12.563	1640	1645	1649	rVB4	1532	3085	0.15%	0.026%
36	12.745	1670	1676	1677	rVB5	1783	3303	0.16%	0.028%
37	12.857	1689	1695	1699	rBV7	3041	6047	0.29%	0.051%
38	13.192	1749	1752	1756	rVB4	1801	2438	0.12%	0.021%
39	13.275	1762	1766	1768	rBV5	2793	3703	0.18%	0.032%
40	13.434	1789	1793	1799	rBV4	4432	7482	0.36%	0.064%
41	13.545	1808	1812	1816	rBV	9784	14928	0.71%	0.127%
42	13.669	1830	1833	1838	rBV6	2870	3770	0.18%	0.032%
43	13.704	1838	1839	1844	rVB5	2211	2435	0.12%	0.021%
44	13.804	1848	1856	1860	rBV	12376	18305	0.87%	0.156%
45	13.916	1870	1875	1879	rBV4	1776	3990	0.19%	0.034%
46	14.057	1895	1899	1901	rBV4	1819	2646	0.13%	0.023%
47	14.116	1902	1909	1922	rBV	1014661	1521301	72.72%	12.956%
48	14.639	1995	1998	1999	rBV3	2367	2503	0.12%	0.021%
49	14.675	2001	2004	2008	rVB5	6474	8459	0.40%	0.072%
50	14.757	2013	2018	2031	rVB3	44128	80681	3.86%	0.687%
51	15.075	2068	2072	2075	rBV6	3002	3547	0.17%	0.030%
52	15.122	2075	2080	2087	rBV2	16442	23993	1.15%	0.204%
53	15.281	2101	2107	2116	rVB2	6485	15413	0.74%	0.131%
54	15.351	2116	2119	2122	rBV3	1745	2357	0.11%	0.020%
55	15.469	2135	2139	2144	rBV6	4955	8360	0.40%	0.071%
56	15.598	2160	2161	2164	rVB2	2950	2310	0.11%	0.020%
57	15.992	2226	2228	2230	rBV3	2729	2113	0.10%	0.018%
58	16.033	2234	2235	2237	rBV2	2924	2222	0.11%	0.019%
59	16.228	2262	2268	2269	rBV5	2667	3772	0.18%	0.032%
60	16.304	2278	2281	2284	rBV5	1610	2199	0.11%	0.019%
61	16.333	2284	2286	2290	rVB5	1965	2482	0.12%	0.021%
62	16.528	2313	2319	2338	rBV	1015796	1569508	75.02%	13.367%
63	16.651	2338	2340	2348	rVB6	12464	22315	1.07%	0.190%
64	16.869	2370	2377	2389	rBV	1212584	1814284	86.72%	15.451%
65	16.963	2389	2393	2399	rVV	25153	44396	2.12%	0.378%
66	17.022	2401	2403	2409	rVB7	3723	5460	0.26%	0.046%
67	17.151	2421	2425	2428	rBV5	2228	3002	0.14%	0.026%
68	17.239	2438	2440	2442	rBV3	2824	2254	0.11%	0.019%
69	17.339	2454	2457	2459	rBV4	3364	3680	0.18%	0.031%
70	17.651	2508	2510	2513	rBV4	2102	2253	0.11%	0.019%
71	17.692	2513	2517	2518	rBV3	2363	2578	0.12%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026234.D
Acq On : 02 Jun 2020 19:05
Operator : JU/CG
Sample : L2829-07DL2 100X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CD2DL2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Title : SVOA CALIBRATION

72	18.292	2617	2619	2622	rBV4	4032	3517	0.17%	0.030%
73	18.322	2622	2624	2626	rBV3	3266	2993	0.14%	0.025%
74	19.263	2781	2784	2791	rVB3	20209	30245	1.45%	0.258%
75	21.068	3086	3091	3099	rBV	1687832	2063807	98.65%	17.576%
76	23.180	3444	3450	3460	rVB	1163304	2092021	100.00%	17.816%


Sum of corrected areas: 11742049

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026234.D
Acq On : 02 Jun 2020 19:05
Operator : JU/CG
Sample : L2829-07DL2 100X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

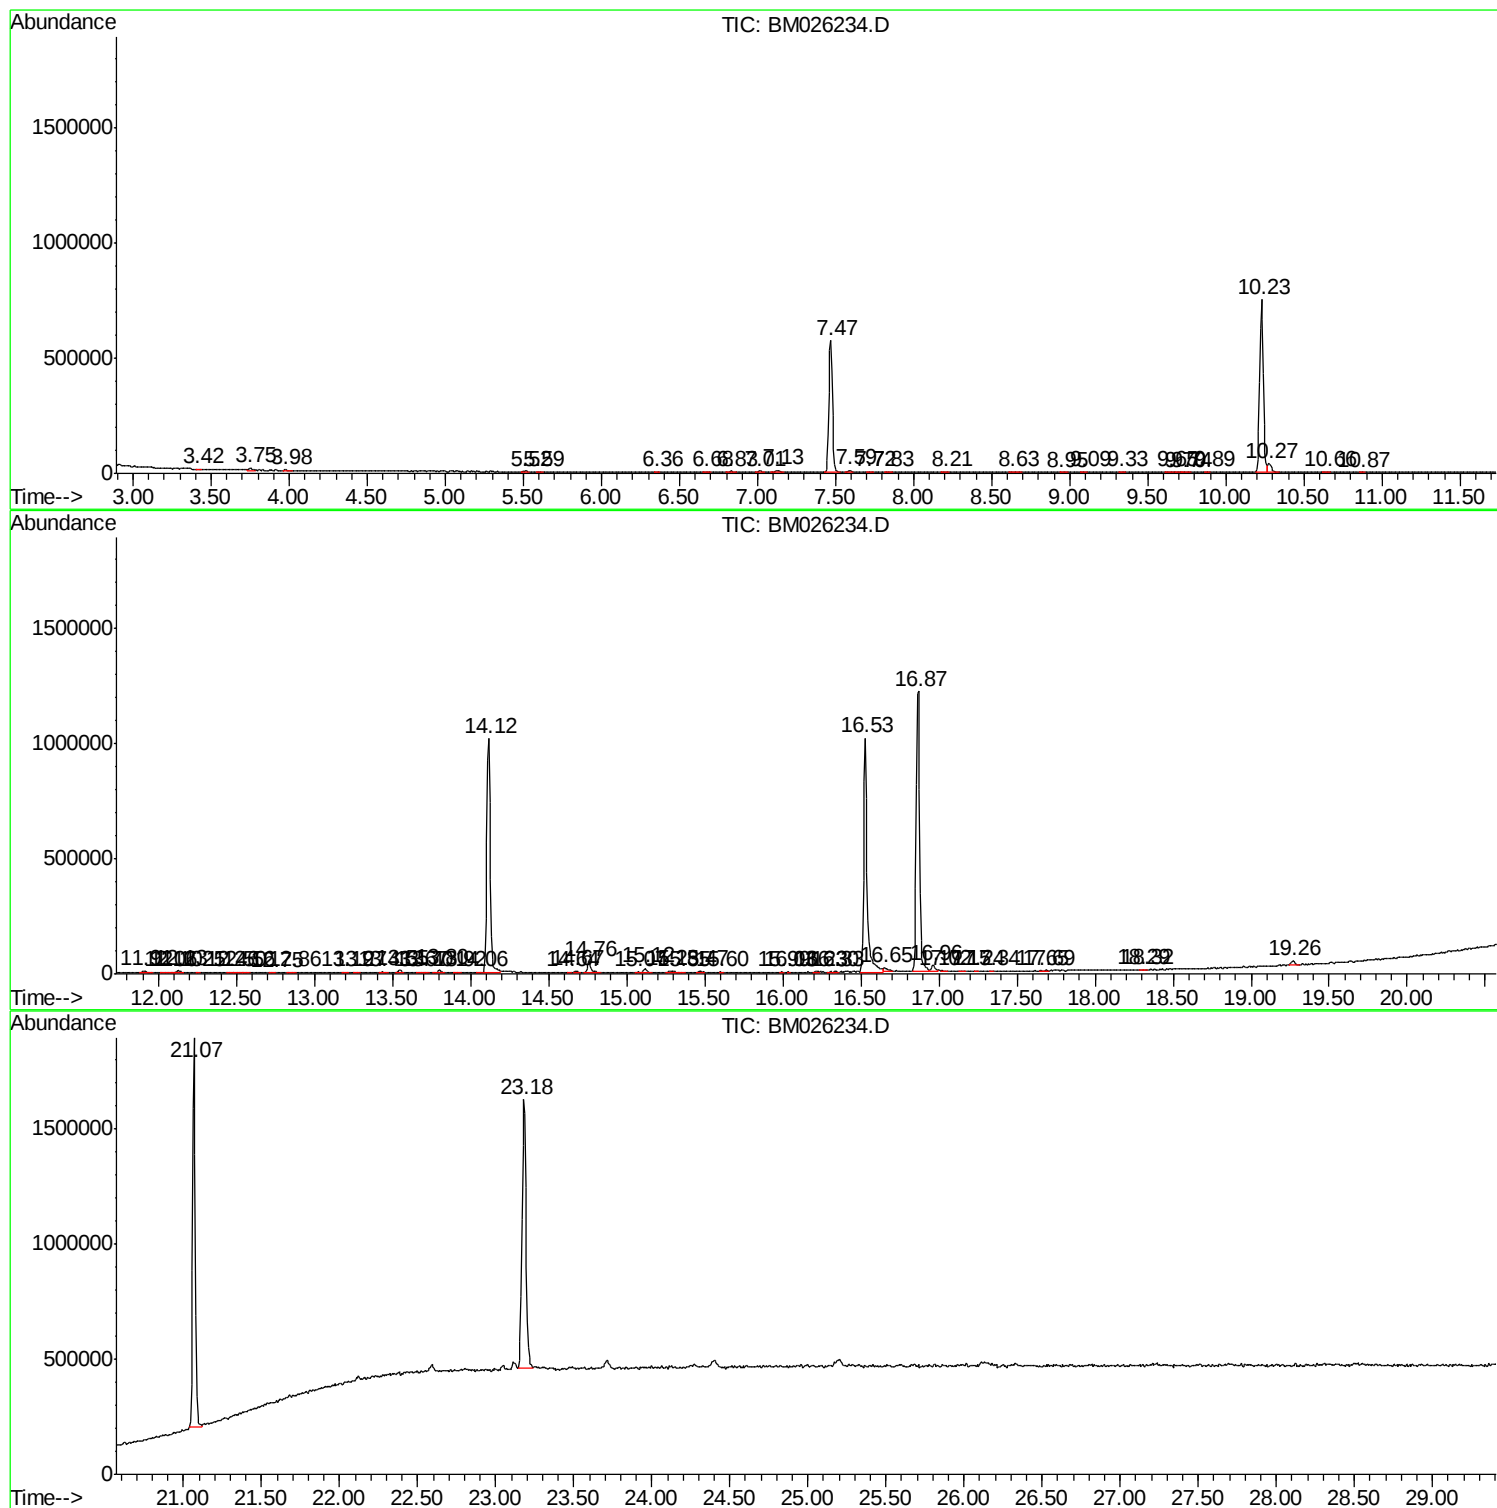

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026234.D
Acq On : 02 Jun 2020 19:05
Operator : JU/CG
Sample : L2829-07DL2 100X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060120\
Data File : BM026234.D
Acq On : 02 Jun 2020 19:05
Operator : JU/CG
Sample : L2829-07DL2 100X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CD2DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc