

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020695.D
 Acq On : 04 Jun 2019 08:18
 Operator : HP/JU
 Sample : K3036-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FESB-26(2.5-3)

Quant Time: Jun 04 13:03:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 31 15:48:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	588092	20.00	ng	-0.01
21) Naphthalene-d8	10.62	136	2416906	20.00	ng	-0.01
39) Acenaphthene-d10	14.46	164	1312435	20.00	ng	-0.01
64) Phenanthrene-d10	17.20	188	2663022	20.00	ng	-0.01
76) Chrysene-d12	21.38	240	2258943	20.00	ng	-0.02
87) Perylene-d12	23.67	264	2649884	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	2252342	67.37	ng	0.00
7) Phenol-d6	6.99	99	3164781	64.29	ng	0.00
23) Nitrobenzene-d5	8.99	82	1905443	40.85	ng	-0.01
42) 2,4,6-Tribromophenol	15.95	330	1008172	62.00	ng	-0.01
45) 2-Fluorobiphenyl	13.08	172	3530185	35.76	ng	-0.01
79) Terphenyl-d14	19.83	244	4200238	31.10	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.92	163	347047	3.095	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020695.D
Acq On : 04 Jun 2019 08:18
Operator : HP/JU
Sample : K3036-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FESB-26(2.5-3)

Quant Time: Jun 04 13:03:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 31 15:48:49 2019
Response via : Initial Calibration

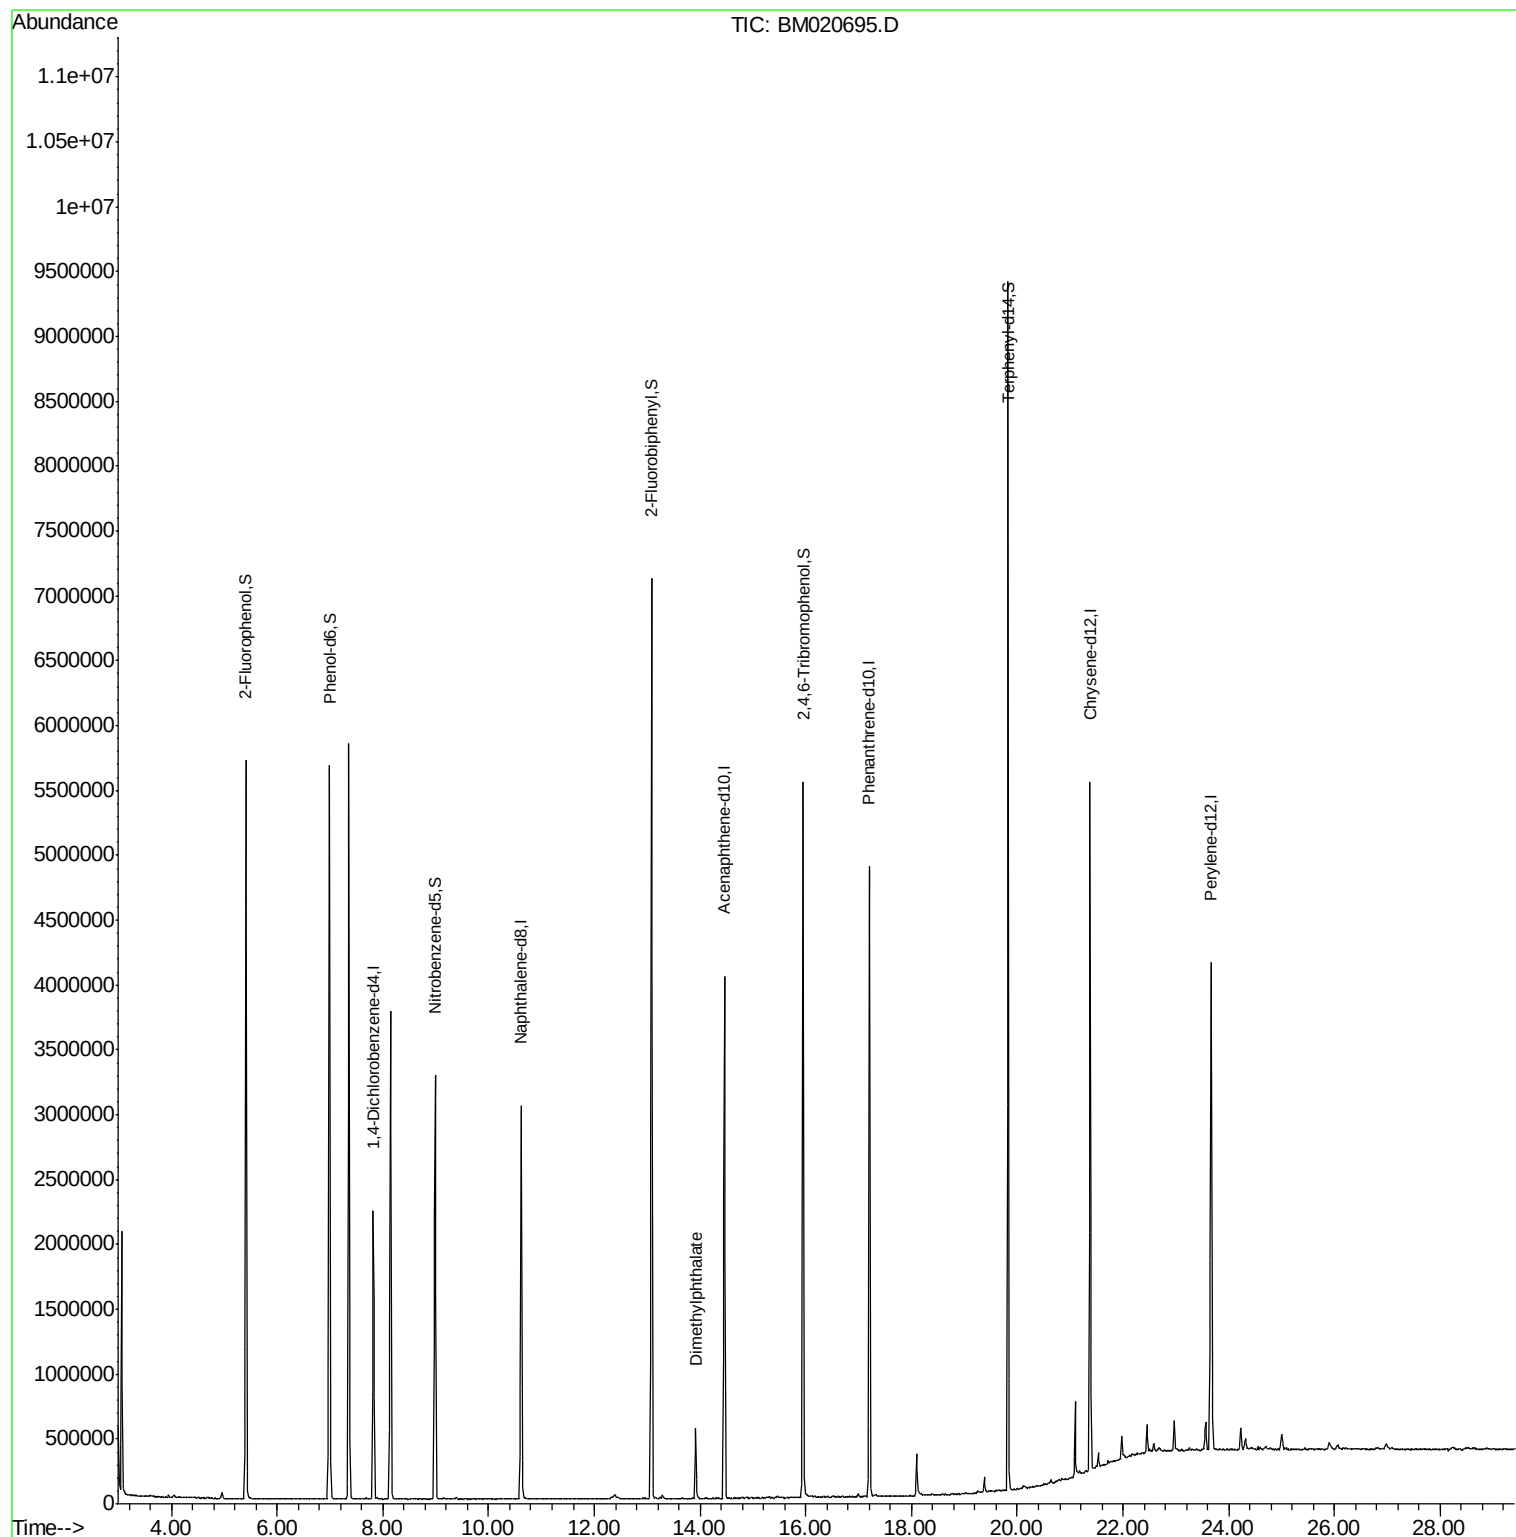




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.82 min Scan# 822
Delta R.T. -0.01 min
Lab File: BM020695.D
Acq: 04 Jun 2019 08:18

Instrument :
BNA_M
ClientSampleId :
FESB-26(2.5-3)

Tot Ion	152	Resp	588092
Ion	Ratio	Lower	Upper
152	100		
150	155.5	126.0	189.0
115	60.9	49.6	74.4



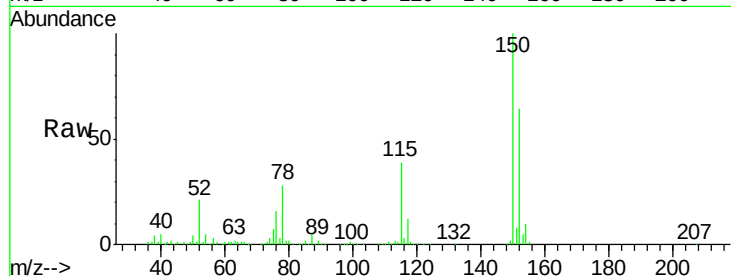


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

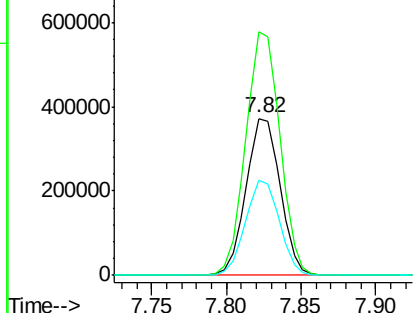

#5

2-Fluorophenol
Concen: 67.371 ng
RT: 5.41 min Scan# 412
Delta R.T. -0.01 min
Lab File: BM020695.D
Acq: 04 Jun 2019 08:18

Tgt Ion	112	Resp	2252342
Ion	Ratio	Lower	Upper
112	100		
64	60.7	49.7	74.5
63	31.8	26.4	39.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

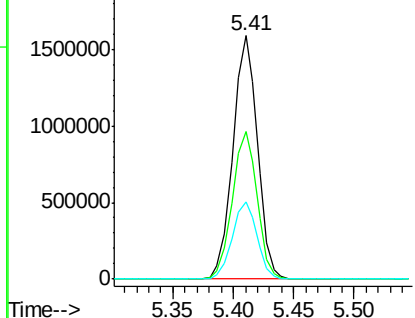

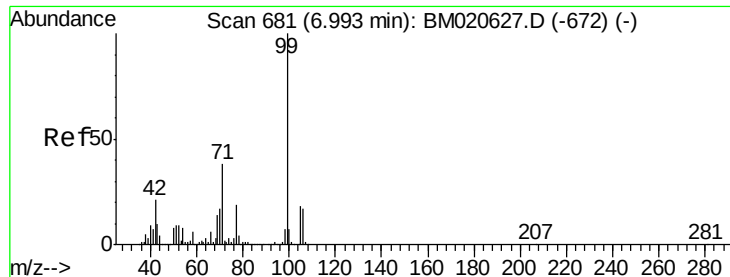

#7

Phenol-d6

Concen: 64.289 ng

RT: 6.99 min Scan# 681

Delta R.T. -0.00 min

Lab File: BM020695.D

Acq: 04 Jun 2019 08:18

Instrument :

BNA_M

ClientSampleId :

FESB-26(2.5-3)


Tot Ion: 99 Resp: 3164781

Ion Ratio Lower Upper

99 100

42 18.7 16.5 24.7




71 37.0 30.7 46.1

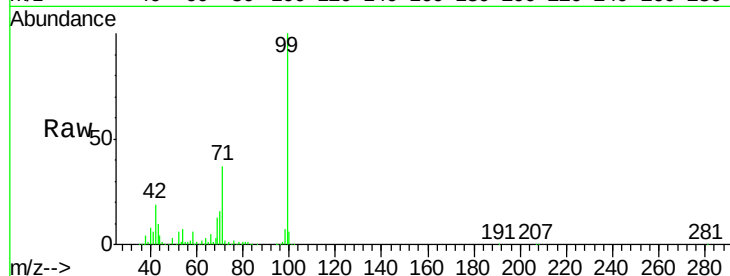

Abundance Ion 99.00 (98.70 to 99.70): BM020627.D (-672) (-)

Ion 42.00 (41.70 to 42.70): BM020627.D (-672) (-)

Ion 71.00 (70.70 to 71.70): BM020627.D (-672) (-)

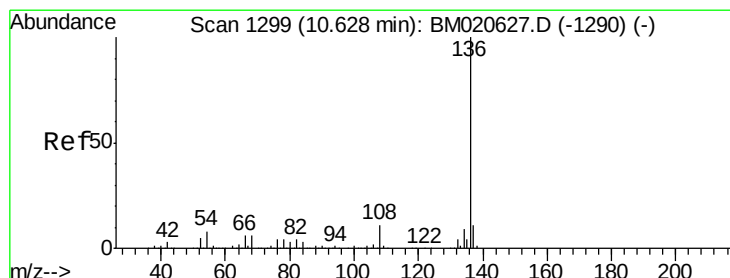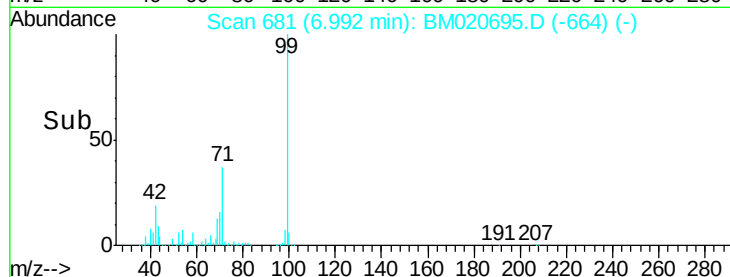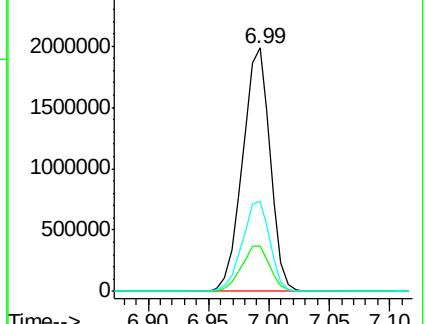

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.62 min Scan# 1297

Delta R.T. -0.01 min

Lab File: BM020695.D

Acq: 04 Jun 2019 08:18

Tgt Ion: 136 Resp: 2416906


Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2

54 7.9 6.6 10.0

68 6.2 5.1 7.7


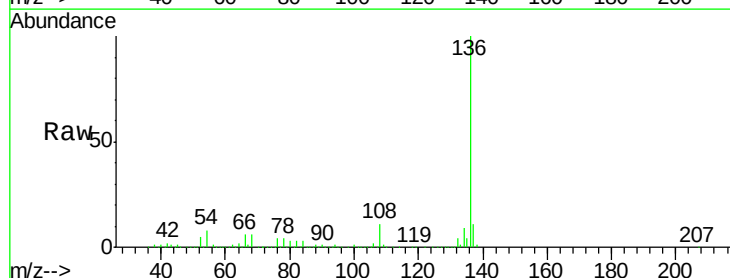



Abundance Ion 136.00 (135.70 to 136.70): BM020627.D (-1290) (-)

Ion 137.00 (136.70 to 137.70): BM020627.D (-1290) (-)

Ion 54.00 (53.70 to 54.70): BM020627.D (-1290) (-)

Ion 68.00 (67.70 to 68.70): BM020627.D (-1290) (-)

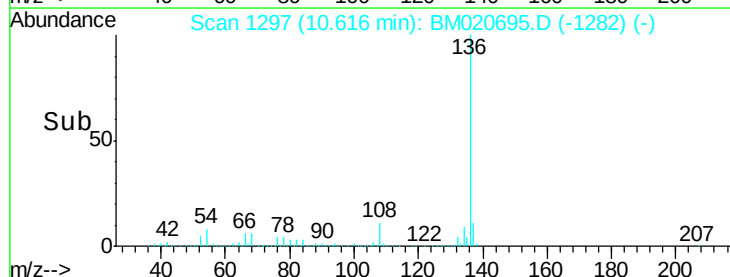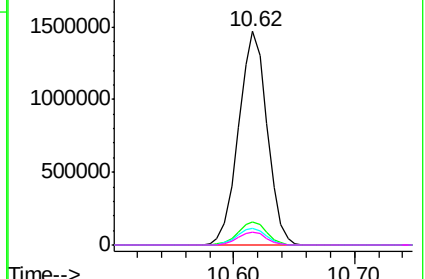


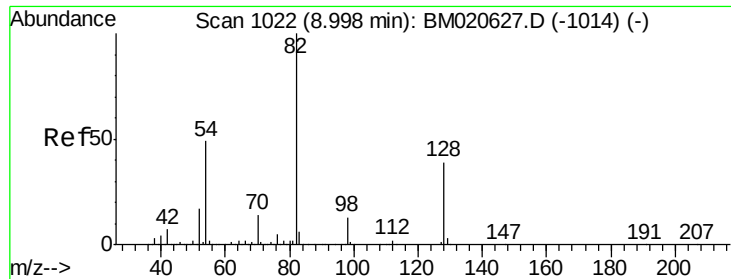




#23
 Nitrobenzene-d5
 Concen: 40.847 ng
 RT: 8.99 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Instrument :
 BNA_M
 ClientSampleId :
 FESB-26(2.5-3)

Tot Ion: 82 Resp: 1905443
 Ion Ratio Lower Upper
 82 100
 128 41.5 31.5 47.3
 54 47.2 39.4 59.0

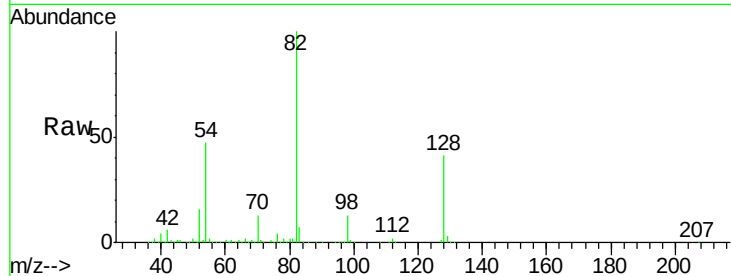


Abundance Ion 82.00 (81.70 to 82.70): BM020627.D (-1014) (-)
 Ion 128.00 (127.70 to 128.70): BM020627.D (-1014) (-)
 Ion 54.00 (53.70 to 54.70): BM020627.D (-1014) (-)

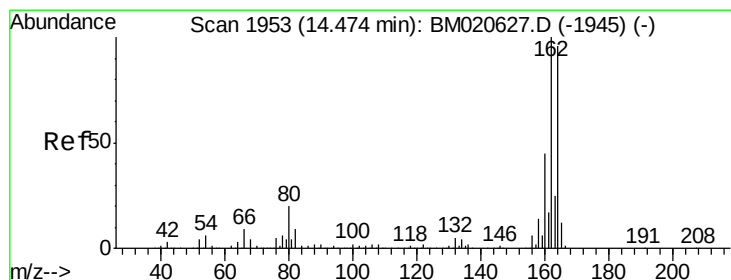
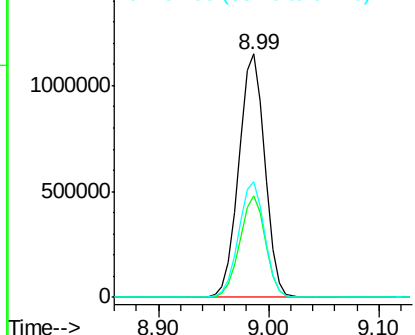



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.46 min Scan# 1951
 Delta R.T. -0.01 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Tgt Ion:164 Resp: 1312435
 Ion Ratio Lower Upper
 164 100
 162 104.5 83.2 124.8
 160 47.1 37.5 56.3



Abundance Ion 164.00 (163.70 to 164.70): BM020627.D (-1945) (-)
 Ion 162.00 (161.70 to 162.70): BM020627.D (-1945) (-)
 Ion 160.00 (159.70 to 160.70): BM020627.D (-1945) (-)

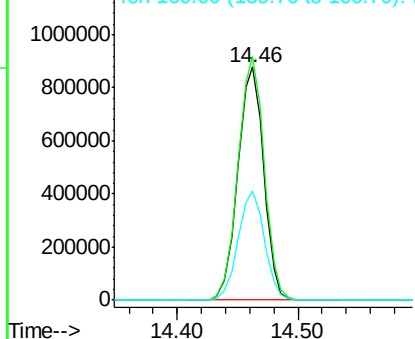


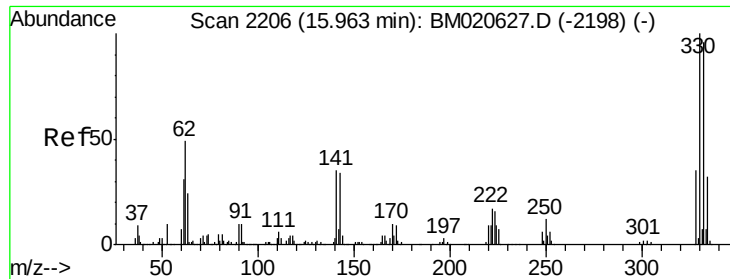




#42
 2,4,6-Tribromophenol
 Concen: 62.000 ng
 RT: 15.95 min Scan# 2204
 Delta R.T. -0.01 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Instrument :
 BNA_M
 ClientSampleId :
 FESB-26(2.5-3)

Tot Ion:330 Resp: 1008172
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.4 116.0
 141 35.2 30.4 45.6

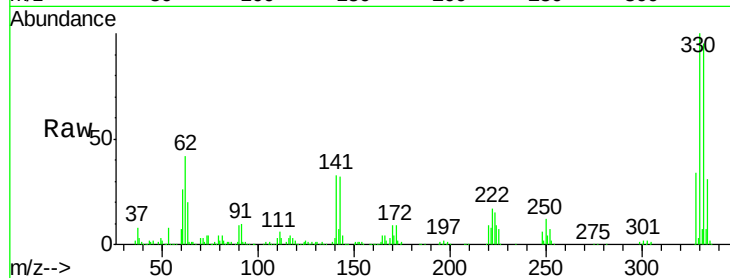


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

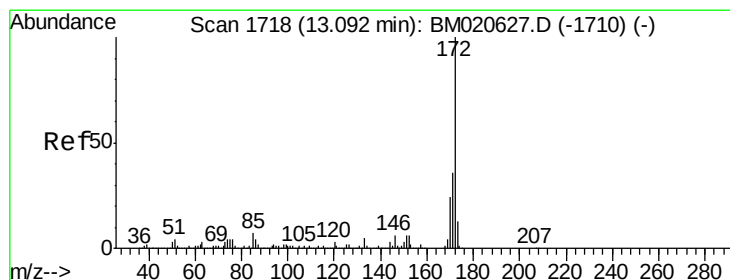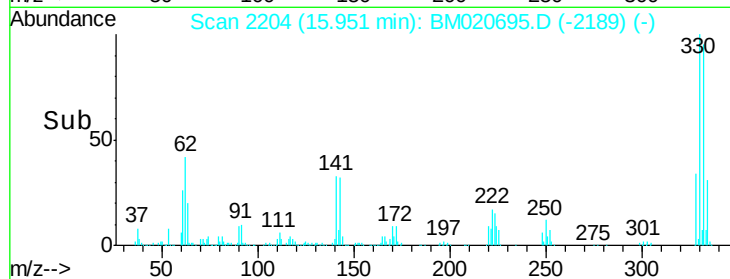
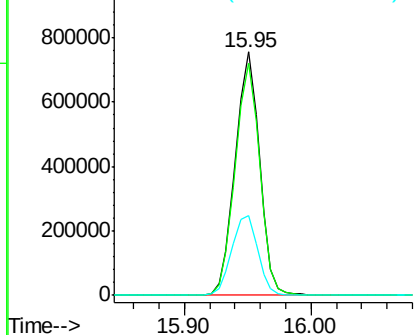



#45
 2-Fluorobiphenyl
 Concen: 35.760 ng
 RT: 13.08 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Tgt Ion:172 Resp: 3530185
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.6 43.0
 170 23.7 18.9 28.3

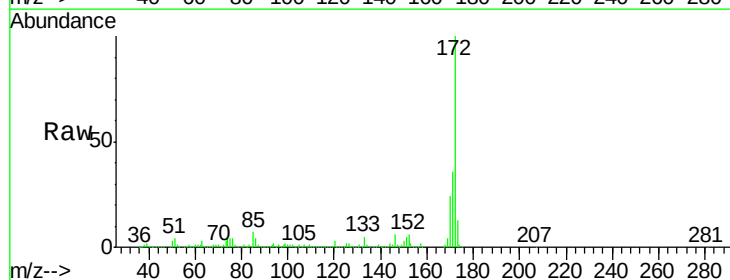

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

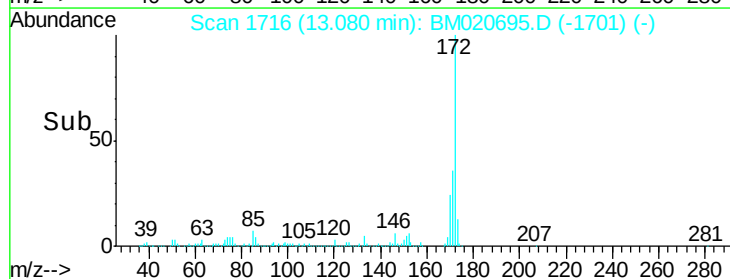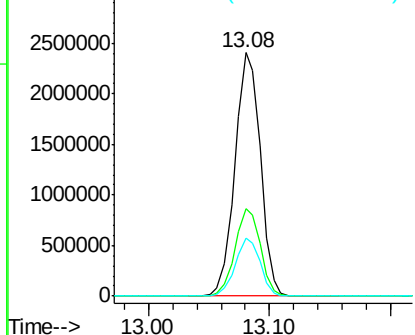

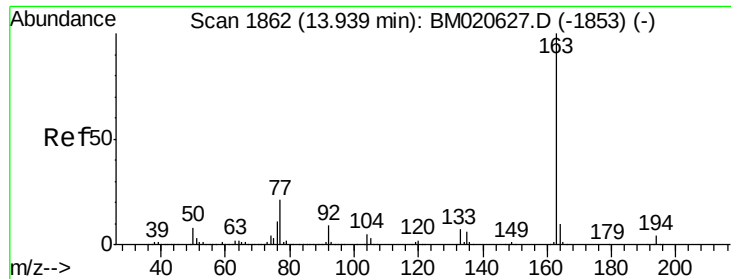

#50

Dimethylphthalate

Concen: 3.095 ng

RT: 13.92 min Scan# 1858

Delta R.T. -0.02 min

Lab File: BM020695.D

Acq: 04 Jun 2019 08:18

Instrument :

BNA_M

ClientSampleId :

FESB-26(2.5-3)


Tot Ion:163 Resp: 347047

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8




164 10.0 7.9 11.9



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

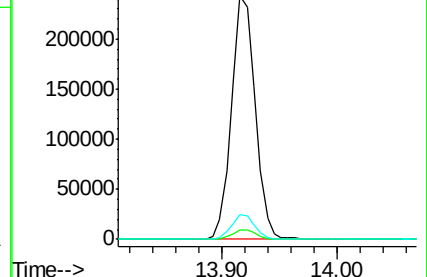

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.20 min Scan# 2417

Delta R.T. -0.01 min

Lab File: BM020695.D

Acq: 04 Jun 2019 08:18


Tgt Ion:188 Resp: 2663022

Ion Ratio Lower Upper

188 100

94 9.3 7.8 11.8



80 10.7 9.0 13.6




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

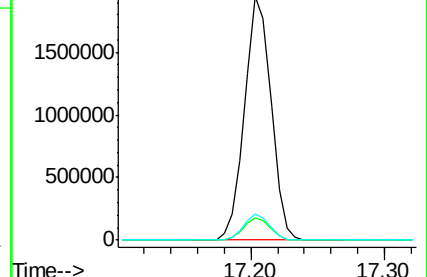







#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.38 min Scan# 3127
 Delta R.T. -0.02 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Instrument :
 BNA_M
 ClientSampleId :
 FESB-26(2.5-3)

Tot Ion:240 Resp: 2258943
 Ion Ratio Lower Upper
 240 100
 120 10.6 8.2 12.2
 236 26.1 21.2 31.8




Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E


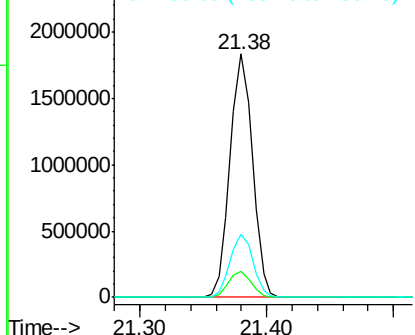



#79
 Terphenyl-d14
 Concen: 31.101 ng
 RT: 19.83 min Scan# 2863
 Delta R.T. -0.02 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Tgt Ion:244 Resp: 4200238
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.7 8.5
 122 10.1 7.2 10.8



Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

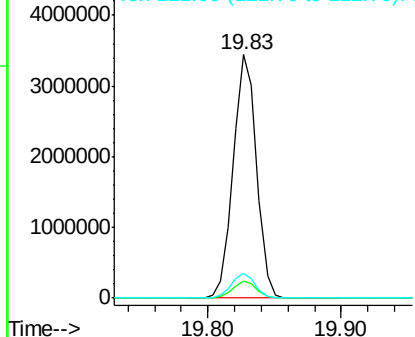


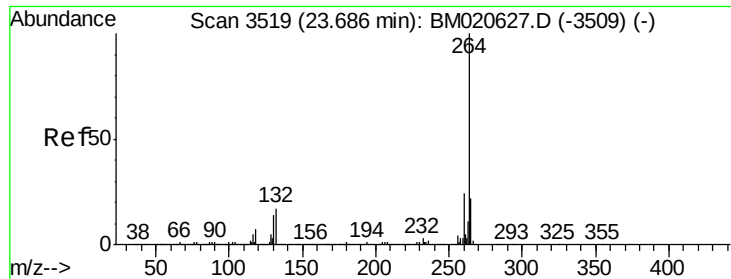

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.67 min Scan# 3516
 Delta R.T. -0.02 min
 Lab File: BM020695.D
 Acq: 04 Jun 2019 08:18

Instrument :
 BNA_M
 ClientSampleId :
 FESB-26(2.5-3)

Tot Ion:264 Resp: 2649884
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 21.6 17.6 26.4



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

