

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020663.D
 Acq On : 03 Jun 2019 10:28
 Operator : HP/JU
 Sample : PB120182BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120182BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	9	13	20	rVB	151770	177908	1.11%	0.195%
2	5.416	406	413	424	rBV	5351932	7642088	47.86%	8.376%
3	6.998	673	682	692	rBV	5238151	8545533	53.52%	9.366%
4	7.363	736	744	757	rBV	5544624	8557486	53.59%	9.380%
5	7.828	817	823	832	rVB	1088124	1724220	10.80%	1.890%
6	8.151	870	878	885	rBV	3986124	6310265	39.52%	6.916%
7	8.992	1013	1021	1035	rBV	3183747	5145518	32.22%	5.640%
8	10.622	1290	1298	1307	rBV	1423816	2378648	14.90%	2.607%
9	13.086	1710	1717	1725	rBV	8237722	12316939	77.13%	13.500%
10	14.468	1945	1952	1961	rVB2	2117482	3243664	20.31%	3.555%
11	15.957	2198	2205	2224	rBV	6008479	8727740	54.66%	9.566%
12	17.209	2411	2418	2428	rBV2	2706288	3797597	23.78%	4.162%
13	19.839	2859	2865	2871	rBV	12797931	15968133	100.00%	17.502%
14	21.386	3123	3128	3137	rBV	2670179	3417207	21.40%	3.745%
15	23.680	3511	3518	3529	rVB	1711245	3282719	20.56%	3.598%


Sum of corrected areas: 91235665

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020663.D
Acq On : 03 Jun 2019 10:28
Operator : HP/JU
Sample : PB120182BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120182BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

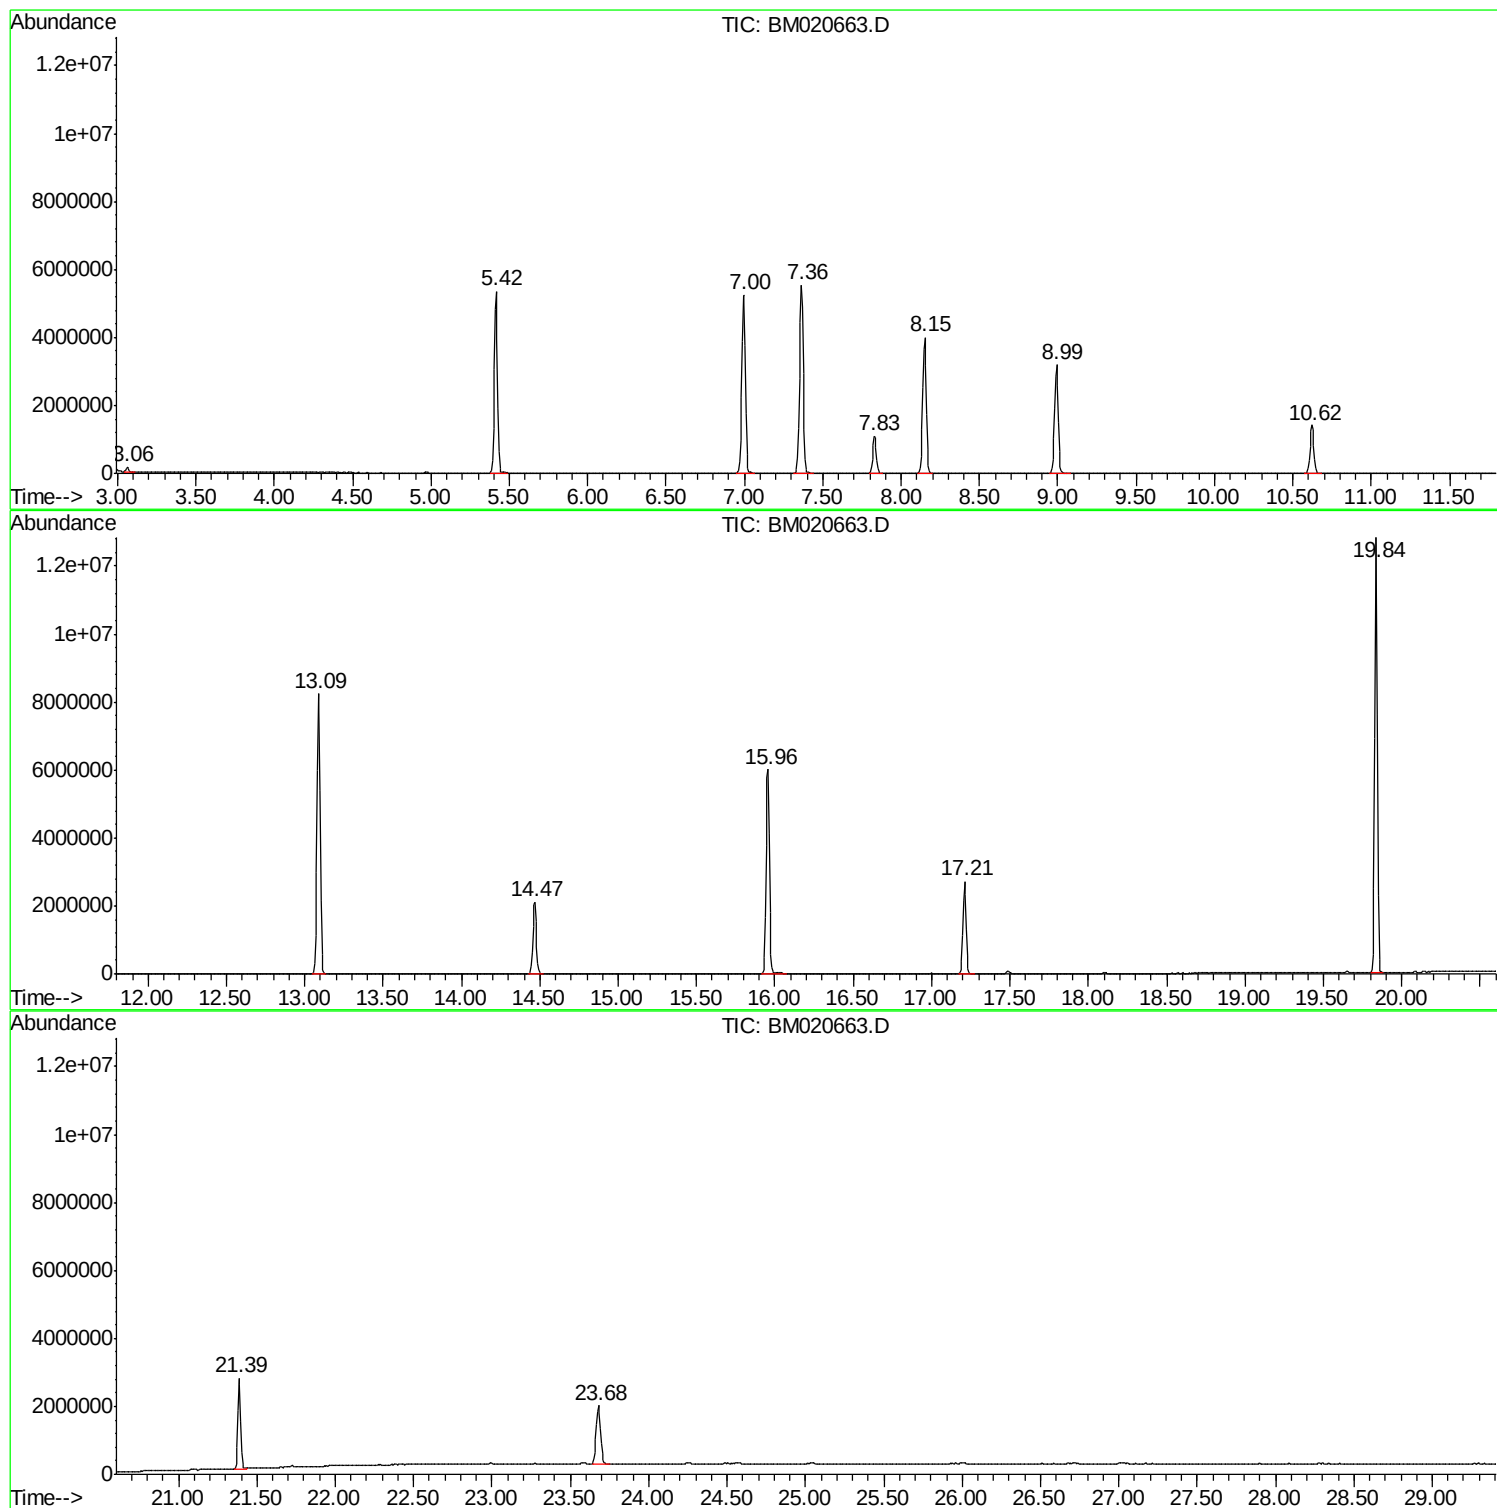

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020663.D
Acq On : 03 Jun 2019 10:28
Operator : HP/JU
Sample : PB120182BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120182BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	2.06 ng	177908	1,4-Dichlorobenzene-d4	7.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	56
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

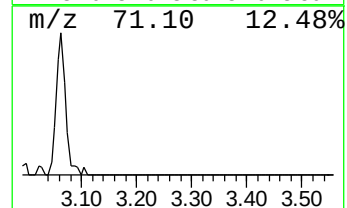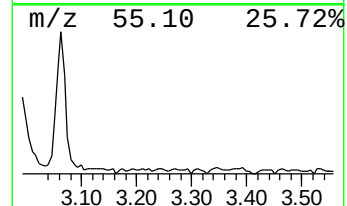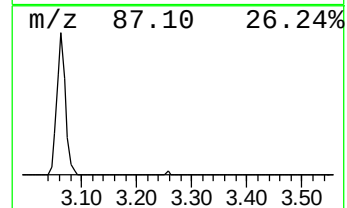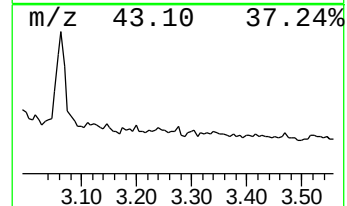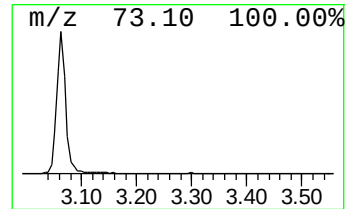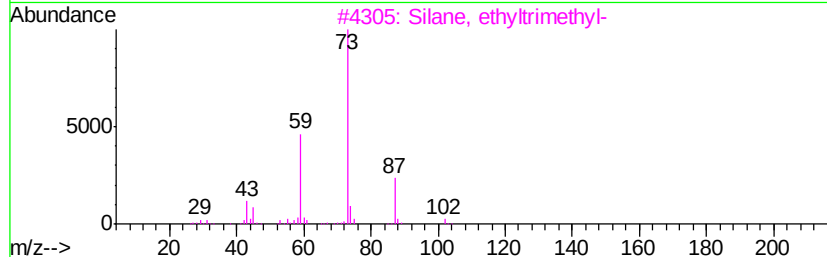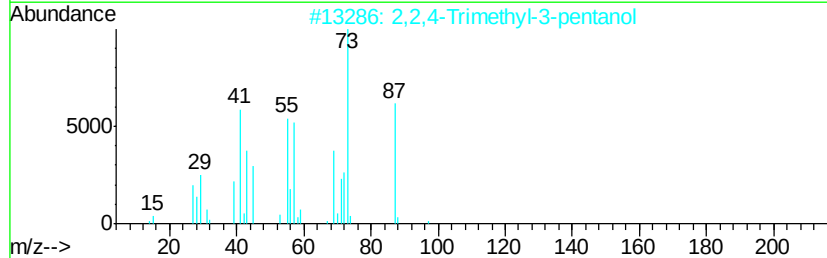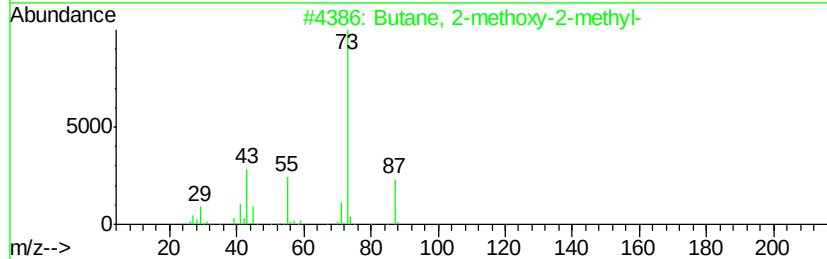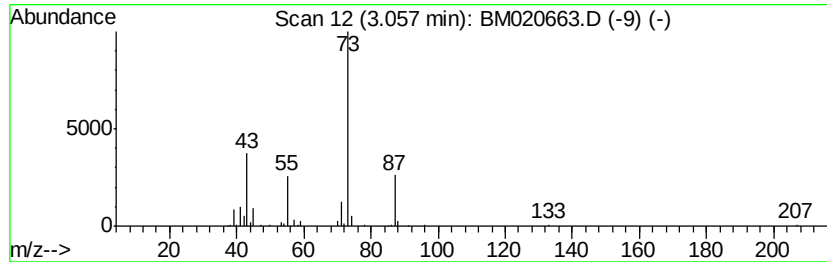

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020663.D
Acq On : 03 Jun 2019 10:28
Operator : HP/JU
Sample : PB120182BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120182BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	99.26 ng	8557490	1,4-Dichlorobenzene-d4	7.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
4		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

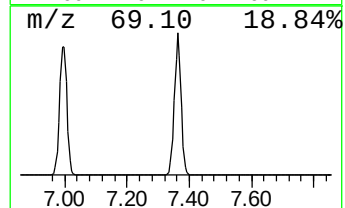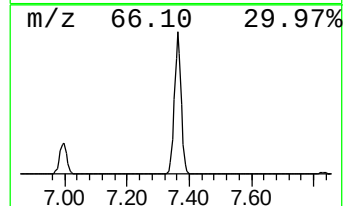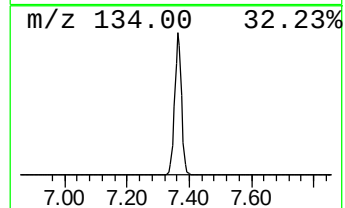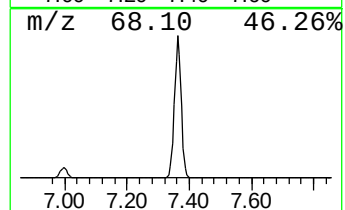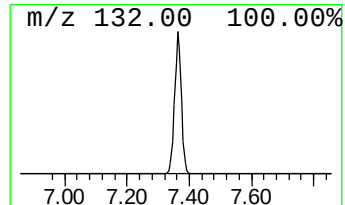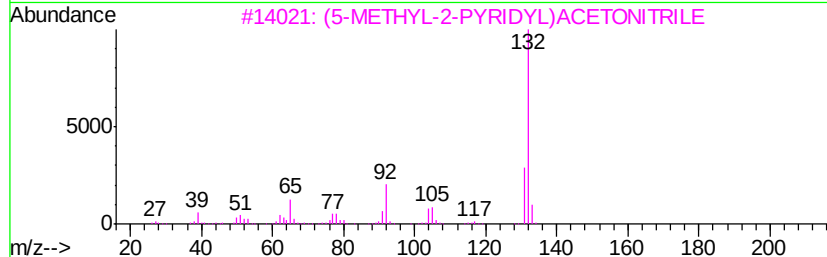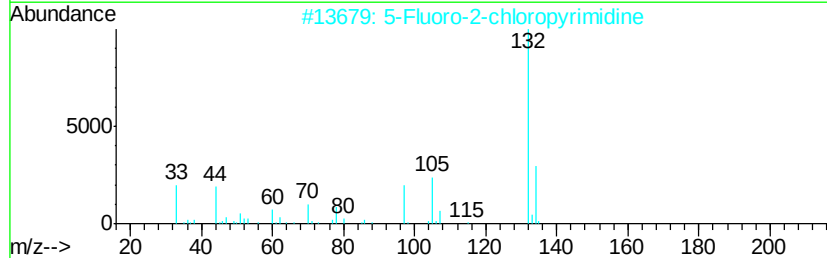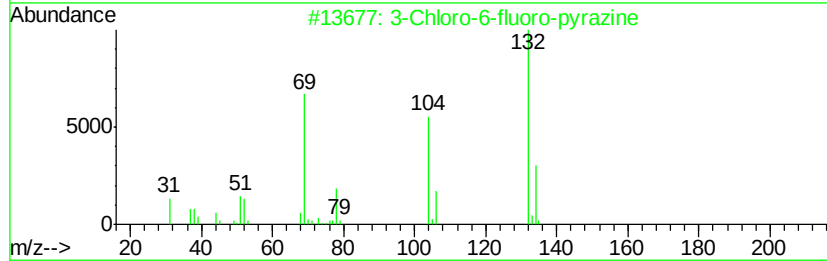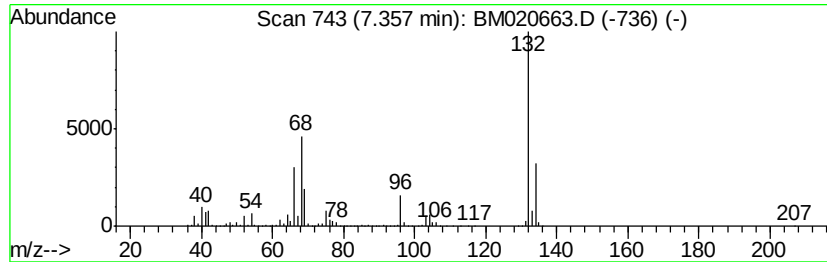

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060319\
Data File : BM020663.D
Acq On : 03 Jun 2019 10:28
Operator : HP/JU
Sample : PB120182BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120182BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	2.1	ng	177908	1	7.83	1724220	20.0
unknown7.36	7.36	99.3	ng	8557490	1	7.83	1724220	20.0