

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020670.D
 Acq On : 03 Jun 2019 14:40
 Operator : HP/JU
 Sample : PB120211BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120211BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	8	13	22	rVB	253261	316765	2.72%	0.411%
2	5.410	405	412	428	rBV	4953800	7130687	61.31%	9.245%
3	6.992	673	681	693	rBV	4880836	7698844	66.20%	9.982%
4	7.357	735	743	757	rBV	4837589	7862094	67.60%	10.194%
5	7.828	816	823	831	rBV	1063244	1664327	14.31%	2.158%
6	8.145	869	877	885	rBV	3789211	6043033	51.96%	7.835%
7	8.986	1012	1020	1033	rBV	2864774	4682068	40.26%	6.071%
8	10.616	1290	1297	1306	rBV	1267595	2159355	18.57%	2.800%
9	13.086	1710	1717	1724	rBV	7302848	10178979	87.52%	13.198%
10	14.462	1945	1951	1959	rBV2	1731010	2569831	22.10%	3.332%
11	15.951	2197	2204	2217	rBV	4545769	6276397	53.97%	8.138%
12	17.209	2411	2418	2424	rBV2	1930733	2761052	23.74%	3.580%
13	19.833	2858	2864	2869	rBV	9597591	11630472	100.00%	15.080%
14	21.386	3122	3128	3137	rBV	2175725	2920901	25.11%	3.787%
15	23.674	3510	3517	3530	rVB2	1673118	3231778	27.79%	4.190%


Sum of corrected areas: 77126583

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020670.D
Acq On : 03 Jun 2019 14:40
Operator : HP/JU
Sample : PB120211BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120211BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

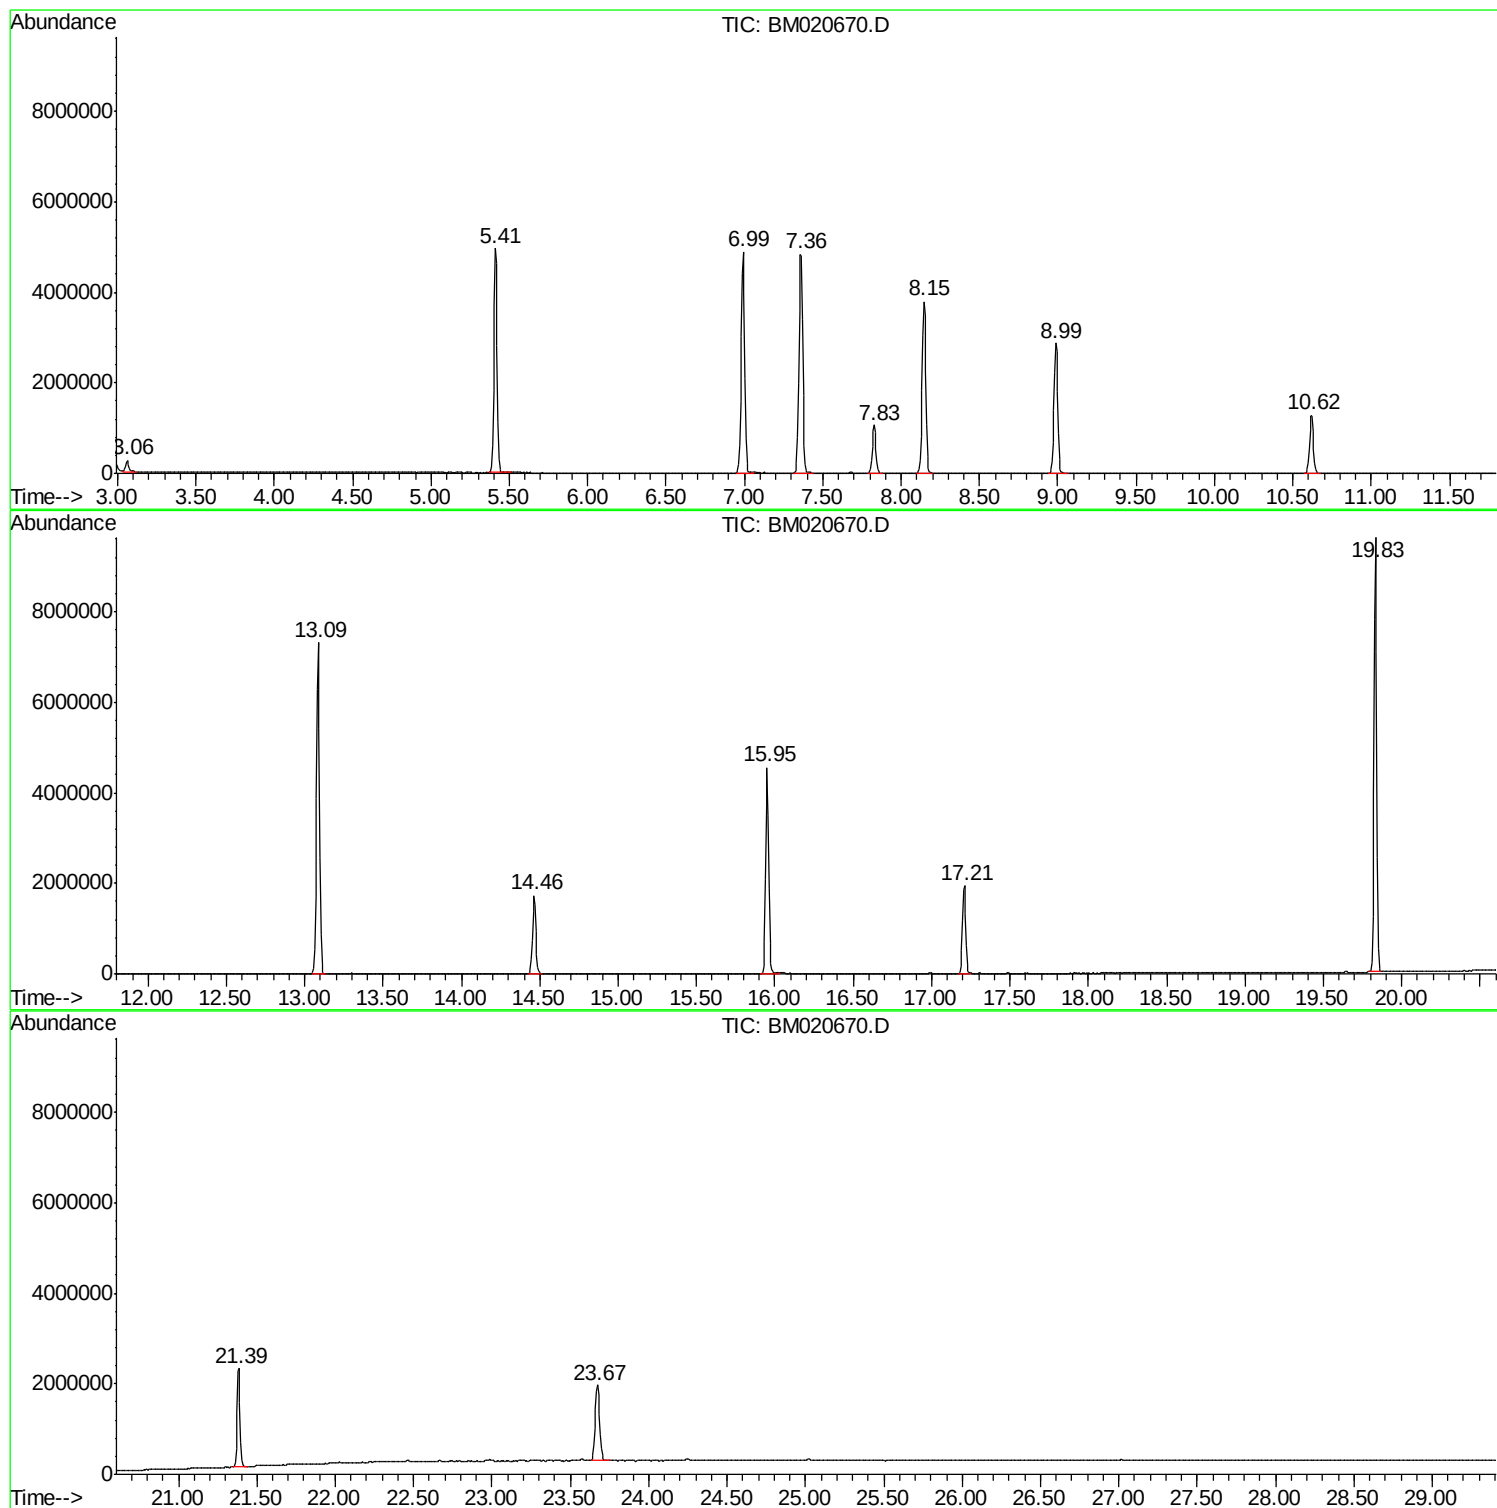

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020670.D
Acq On : 03 Jun 2019 14:40
Operator : HP/JU
Sample : PB120211BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120211BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	3.81 ng	316765	1,4-Dichlorobenzene-d4	7.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	56
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

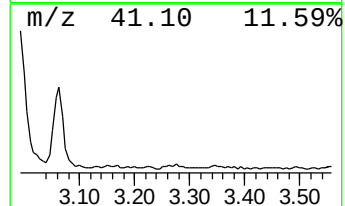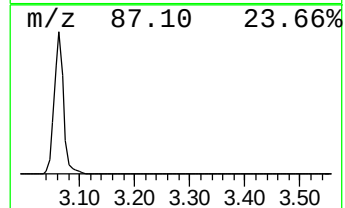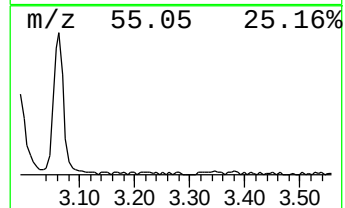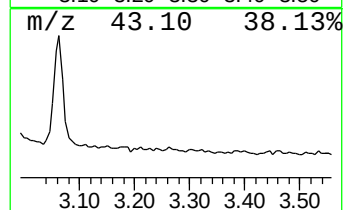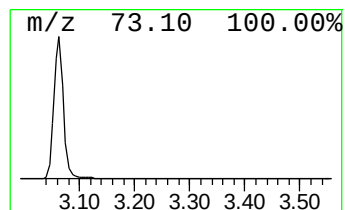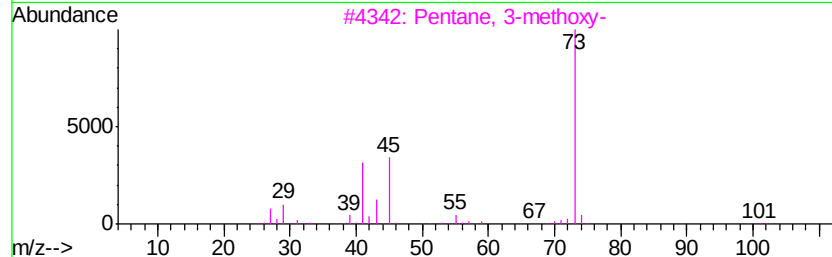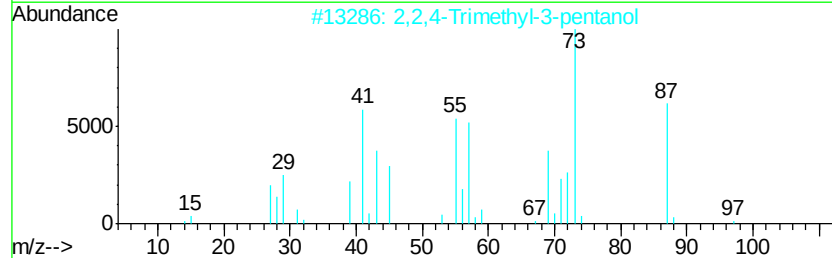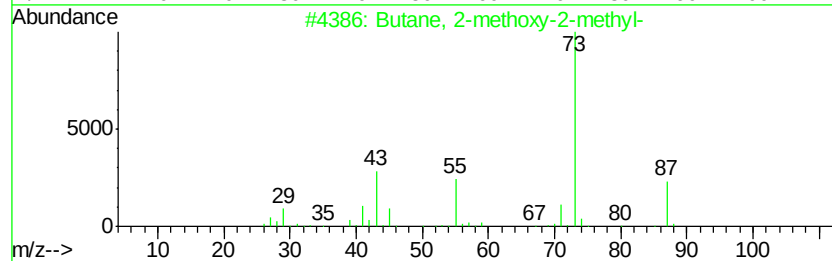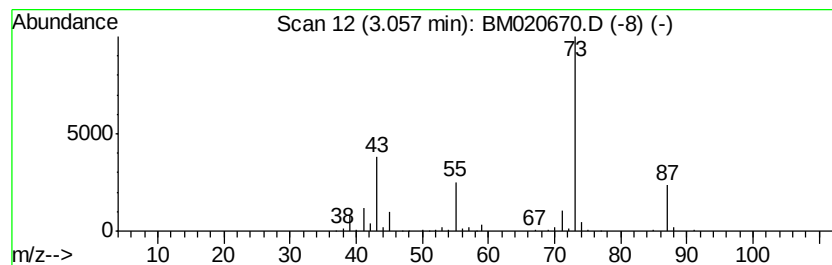

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020670.D
Acq On : 03 Jun 2019 14:40
Operator : HP/JU
Sample : PB120211BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120211BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	94.48 ng	7862090	1,4-Dichlorobenzene-d4	7.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

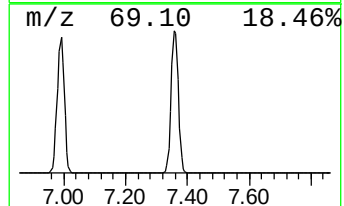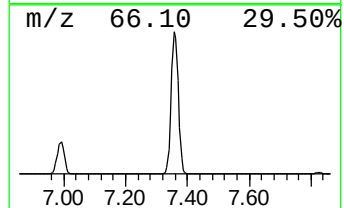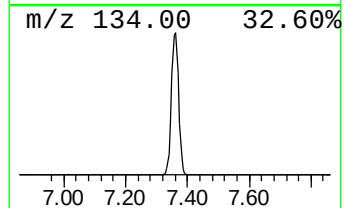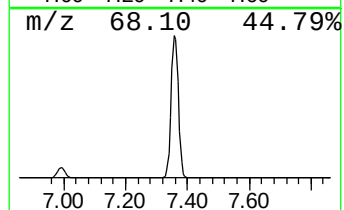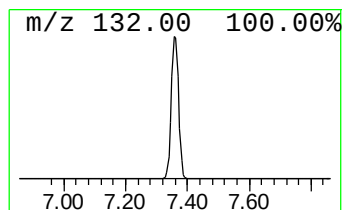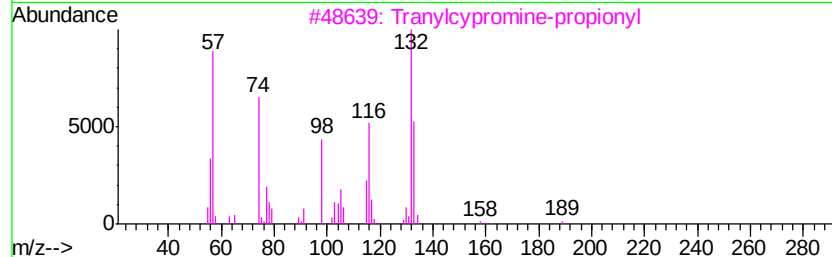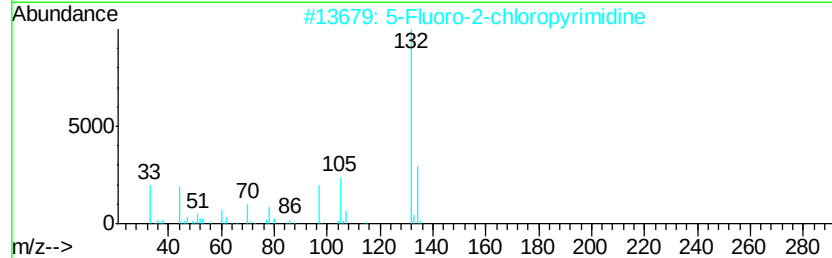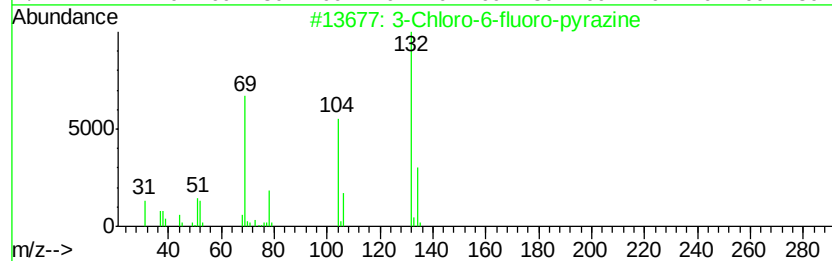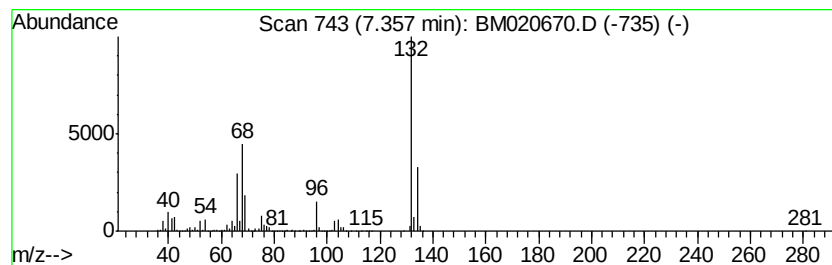

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060319\
Data File : BM020670.D
Acq On : 03 Jun 2019 14:40
Operator : HP/JU
Sample : PB120211BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120211BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	3.8	ng	316765	1	7.83	1664330	20.0
unknown7.36	7.36	94.5	ng	7862090	1	7.83	1664330	20.0