

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020680.D
 Acq On : 03 Jun 2019 20:42
 Operator : HP/JU
 Sample : PB120232BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120232BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	8	13	21	rVB	159710	199499	2.13%	0.320%
2	5.410	405	412	424	rBV	3961327	5540594	59.22%	8.897%
3	6.987	672	680	698	rBV	3737722	5980573	63.92%	9.603%
4	7.357	734	743	753	rBV	3905598	6111162	65.31%	9.813%
5	7.828	816	823	830	rVB	940422	1495436	15.98%	2.401%
6	8.146	869	877	884	rBV	3004811	4711267	50.35%	7.565%
7	8.987	1011	1020	1028	rBV	2207195	3620765	38.70%	5.814%
8	10.616	1290	1297	1305	rVB	1169978	1947303	20.81%	3.127%
9	13.086	1709	1717	1726	rBV	5312530	7970888	85.19%	12.799%
10	14.463	1944	1951	1959	rBV2	1562808	2333792	24.94%	3.747%
11	15.951	2197	2204	2216	rBV	3434674	4824617	51.56%	7.747%
12	17.204	2411	2417	2425	rBV2	1743671	2533611	27.08%	4.068%
13	19.827	2858	2863	2869	rBV	7244284	9356587	100.00%	15.024%
14	21.380	3122	3127	3133	rBV	2107102	2726650	29.14%	4.378%
15	23.674	3510	3517	3527	rVB2	1470253	2924341	31.25%	4.696%


Sum of corrected areas: 62277085

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020680.D
Acq On : 03 Jun 2019 20:42
Operator : HP/JU
Sample : PB120232BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120232BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

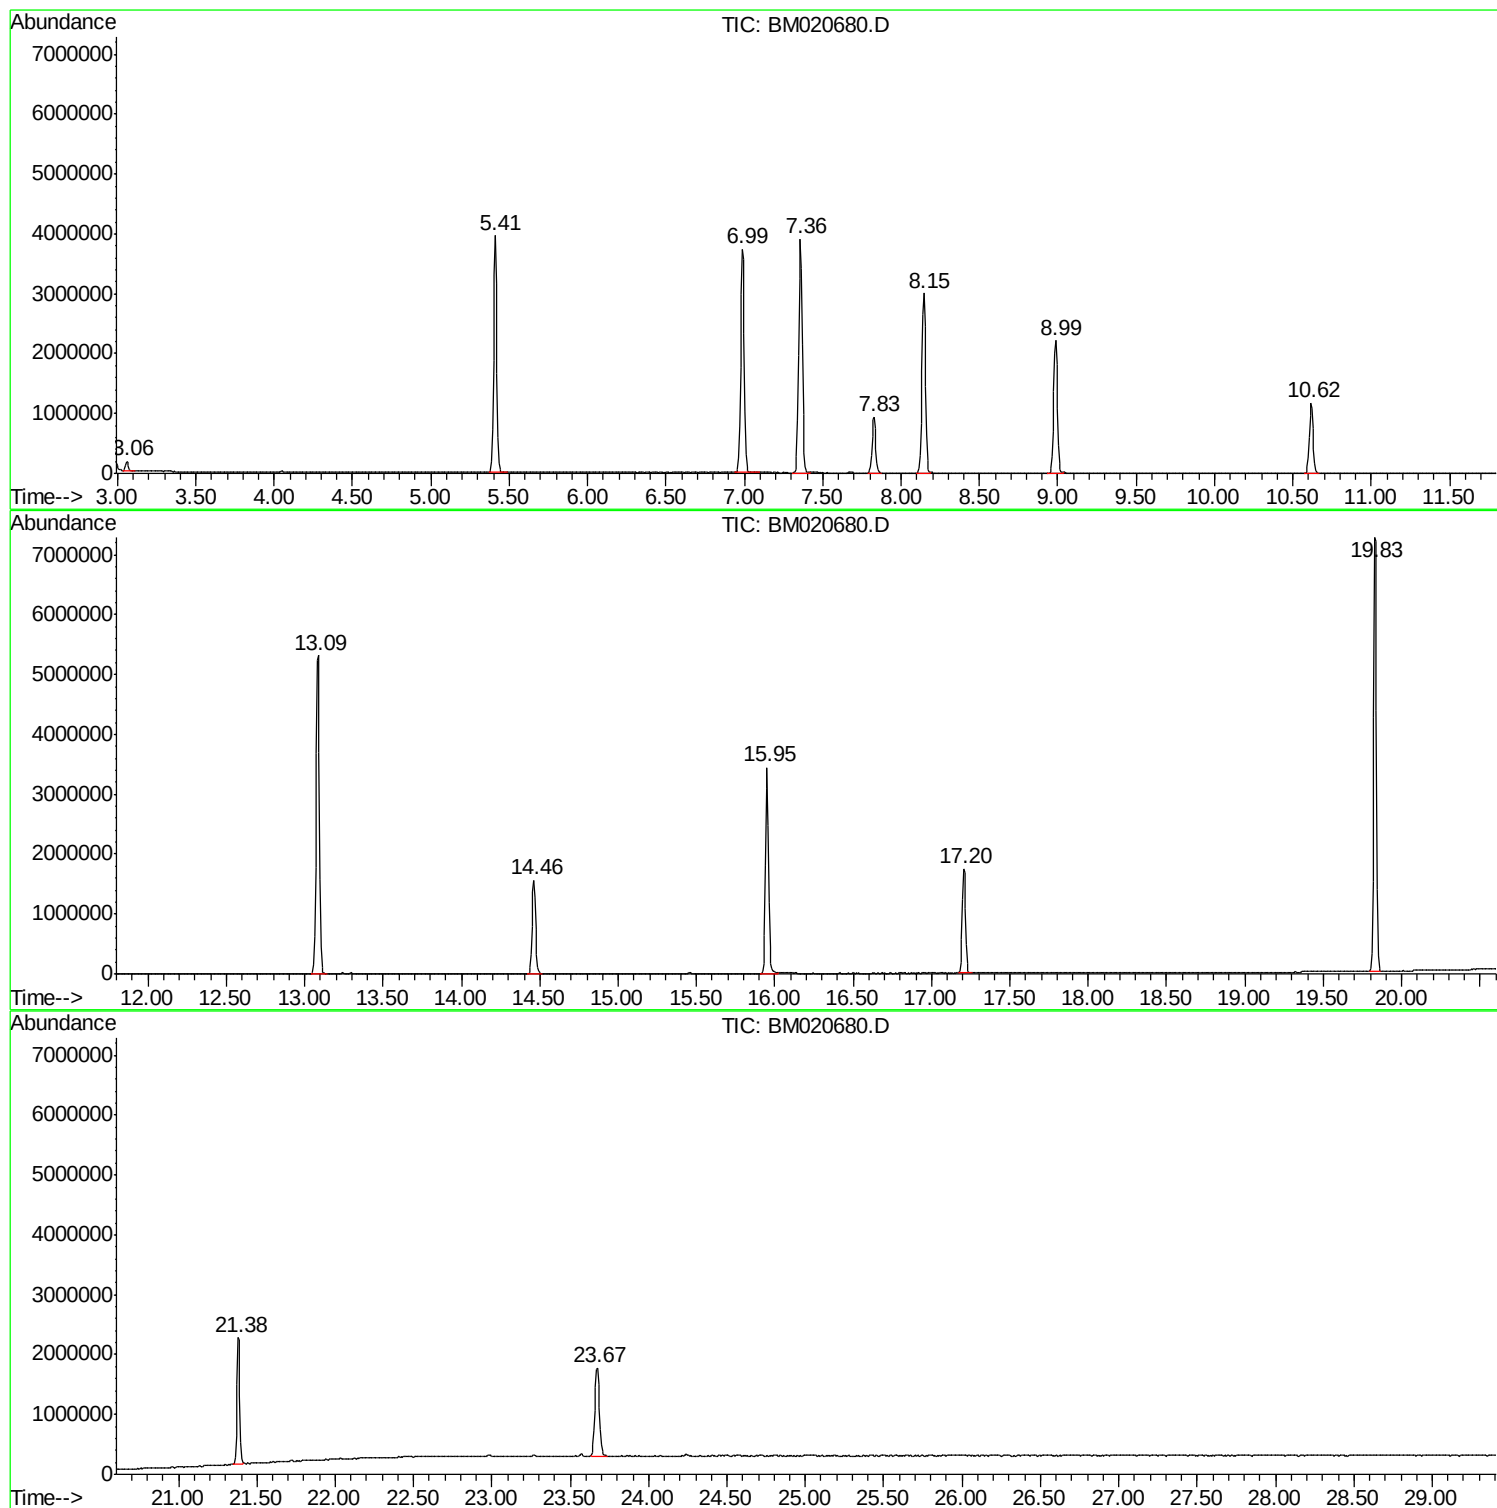

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020680.D
Acq On : 03 Jun 2019 20:42
Operator : HP/JU
Sample : PB120232BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120232BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	2.67 ng	199499	1,4-Dichlorobenzene-d4	7.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	27
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	9

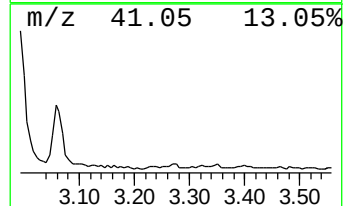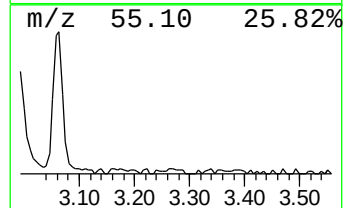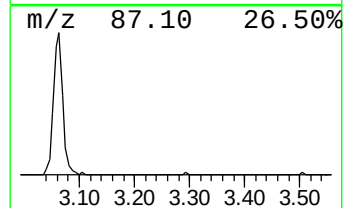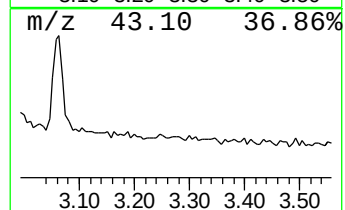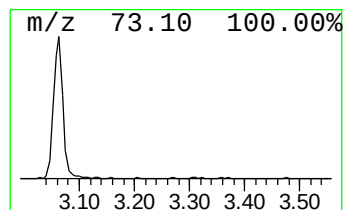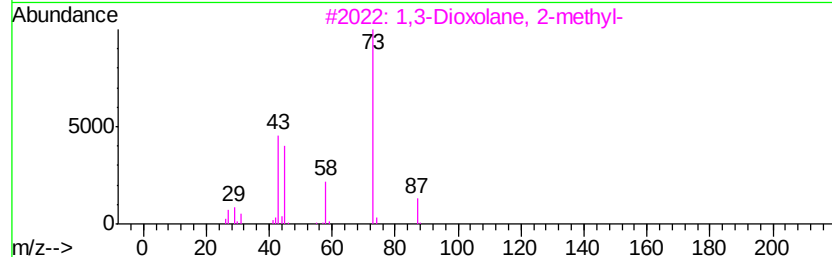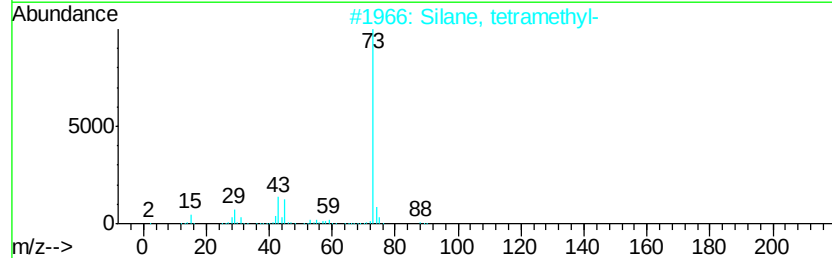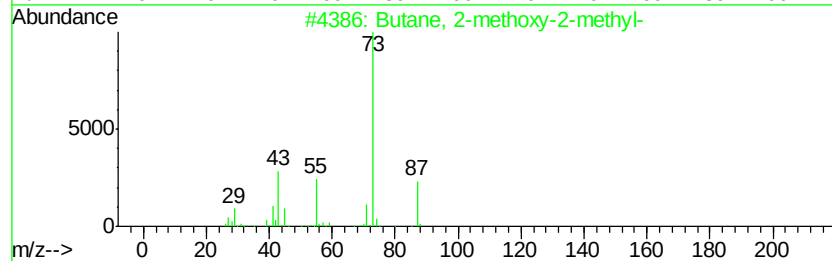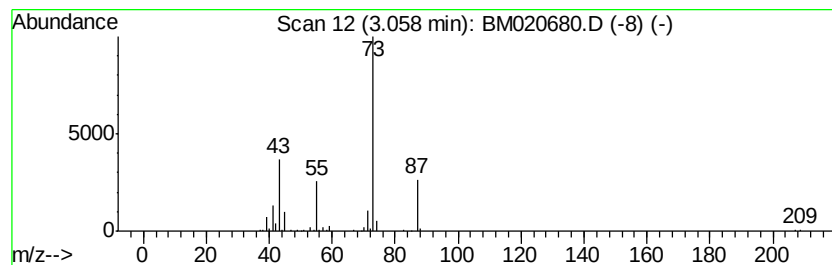

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
Data File : BM020680.D
Acq On : 03 Jun 2019 20:42
Operator : HP/JU
Sample : PB120232BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120232BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	81.73 ng	6111160	1,4-Dichlorobenzene-d4	7.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Xenon	132	Xe	007440-63-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

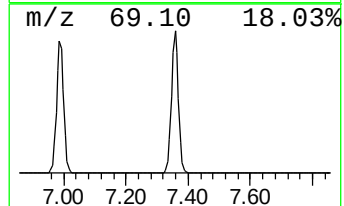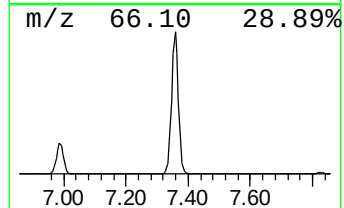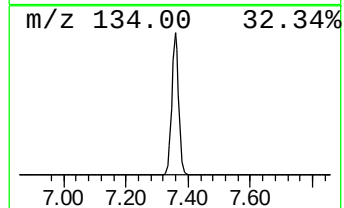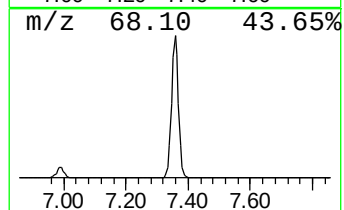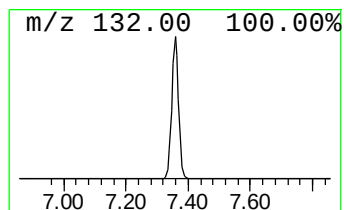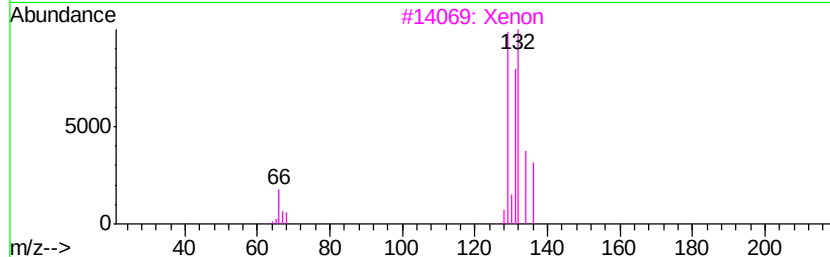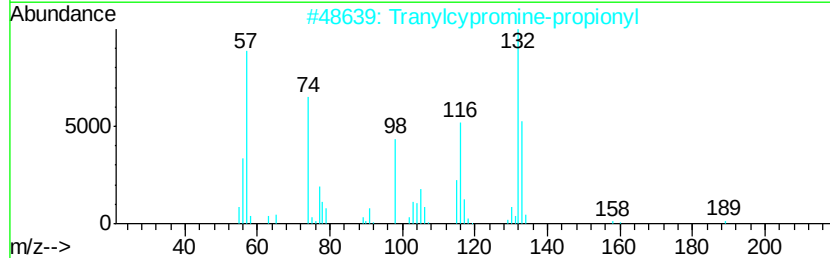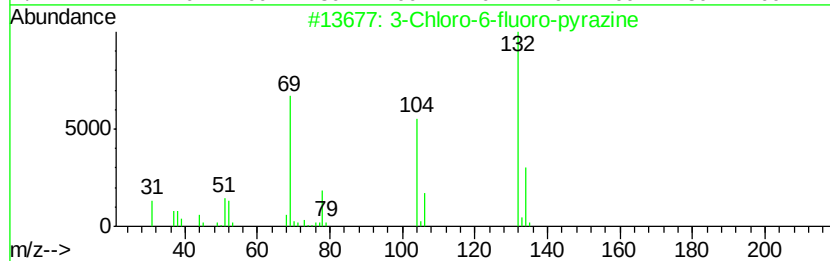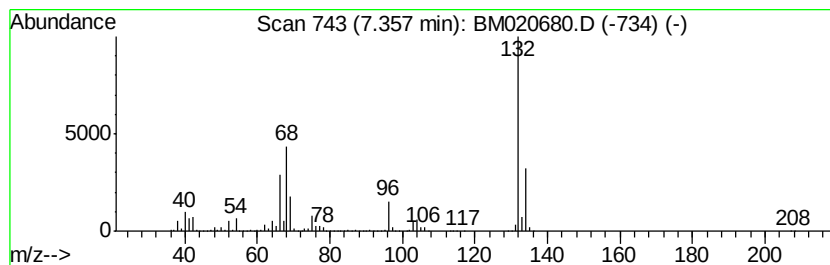

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060319\
Data File : BM020680.D
Acq On : 03 Jun 2019 20:42
Operator : HP/JU
Sample : PB120232BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120232BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	2.7	ng	199499	1	7.83	1495440	20.0
unknown7.36	7.36	81.7	ng	6111160	1	7.83	1495440	20.0