

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060319\
 Data File : BM020694.D
 Acq On : 04 Jun 2019 07:42
 Operator : HP/JU
 Sample : K3015-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OUTFALL001-WK-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	29	rVB	6954429	8646526	55.73%	7.532%
2	5.410	405	412	420	rBV	2448574	3600858	23.21%	3.137%
3	6.987	672	680	689	rBV	1447989	2309698	14.89%	2.012%
4	7.357	735	743	753	rBV	4831740	7661979	49.39%	6.675%
5	7.822	814	822	829	rBV	2130239	3430269	22.11%	2.988%
6	8.146	869	877	886	rBV	4171646	6875955	44.32%	5.990%
7	8.987	1011	1020	1029	rBV	3587299	6008271	38.73%	5.234%
8	10.616	1287	1297	1304	rBV	2780573	4665996	30.07%	4.065%
9	13.081	1709	1716	1728	rBV	8494491	12586508	81.13%	10.964%
10	14.463	1943	1951	1966	rVB2	3815277	5694094	36.70%	4.960%
11	15.951	2197	2204	2219	rBV	5992163	8723230	56.23%	7.599%
12	17.204	2410	2417	2428	rBV2	4332877	6243048	40.24%	5.438%
13	19.827	2857	2863	2870	rBV	12429426	15514784	100.00%	13.515%
14	21.098	3076	3079	3083	rVB	176653	174866	1.13%	0.152%
15	21.380	3121	3127	3133	rBV	5393152	6632350	42.75%	5.778%
16	21.533	3149	3153	3157	rBV	494612	548334	3.53%	0.478%
17	21.980	3224	3229	3233	rBV	875409	1057685	6.82%	0.921%
18	22.451	3305	3309	3317	rVB	1223461	1596451	10.29%	1.391%
19	22.974	3393	3398	3404	rBV	1177105	1737095	11.20%	1.513%
20	23.562	3492	3498	3506	rVB	1037218	1761665	11.35%	1.535%
21	23.668	3509	3516	3528	rVB2	3742283	7228542	46.59%	6.297%
22	24.227	3606	3611	3620	rVB	687991	1329380	8.57%	1.158%
23	25.003	3738	3743	3754	rVB	343917	766663	4.94%	0.668%


Sum of corrected areas: 114794247

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060319\
Data File : BM020694.D
Acq On : 04 Jun 2019 07:42
Operator : HP/JU
Sample : K3015-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OUTFALL001-WK-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

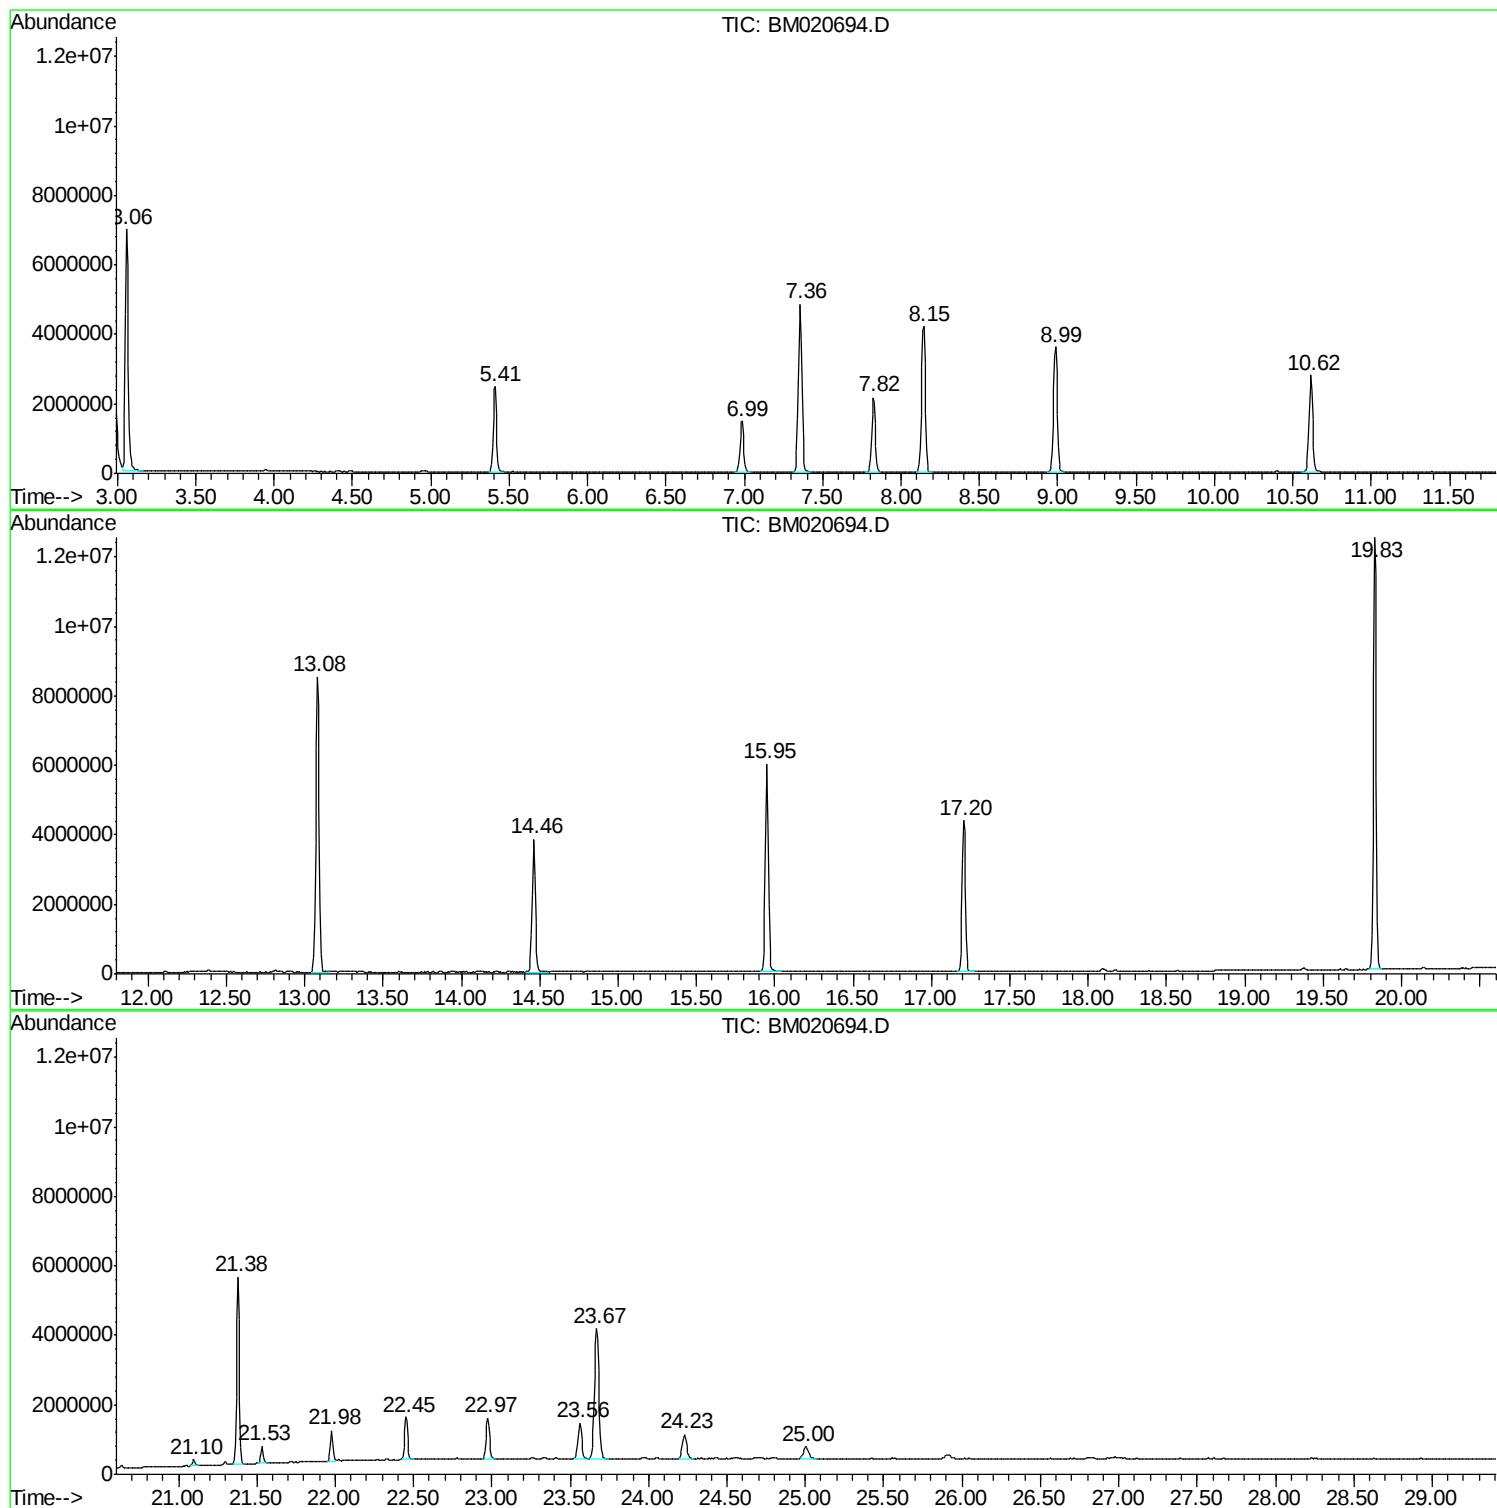

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060319\
Data File : BM020694.D
Acq On : 04 Jun 2019 07:42
Operator : HP/JU
Sample : K3015-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OUTFALL001-WK-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060319\
Data File : BM020694.D
Acq On : 04 Jun 2019 07:42
Operator : HP/JU
Sample : K3015-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OUTFALL001-WK-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc