


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020671.D
 Acq On : 03 Jun 2019 15:16
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 15:48:49 2019

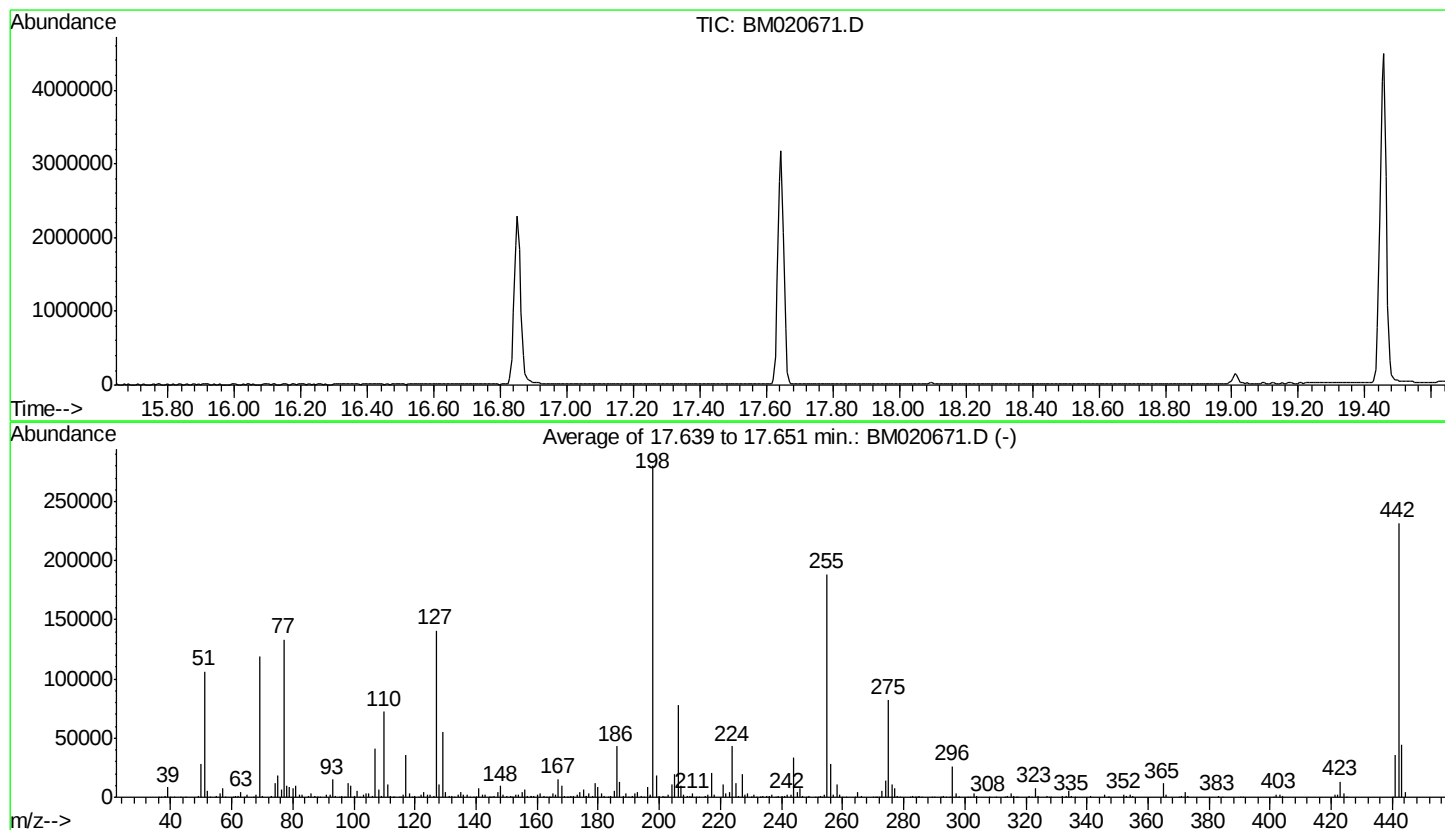

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	106490	PASS
68	69	0.00	2	1.8	2190	PASS
69	198	0.00	100	42.3	118650	PASS
70	69	0.00	2	0.6	655	PASS
127	198	10	80	50.2	140768	PASS
197	198	0.00	2	0.6	1737	PASS
198	198	100	100	100.0	280384	PASS
199	198	5	9	6.8	18956	PASS
275	198	10	60	29.4	82341	PASS
365	198	1	100	4.2	11772	PASS
441	198	0.01	100	12.8	36026	PASS
442	198	50	100	82.8	232149	PASS
443	442	15	24	19.1	44389	PASS