


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060319\
 Data File : BM020689.D
 Acq On : 04 Jun 2019 03:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 15:48:49 2019

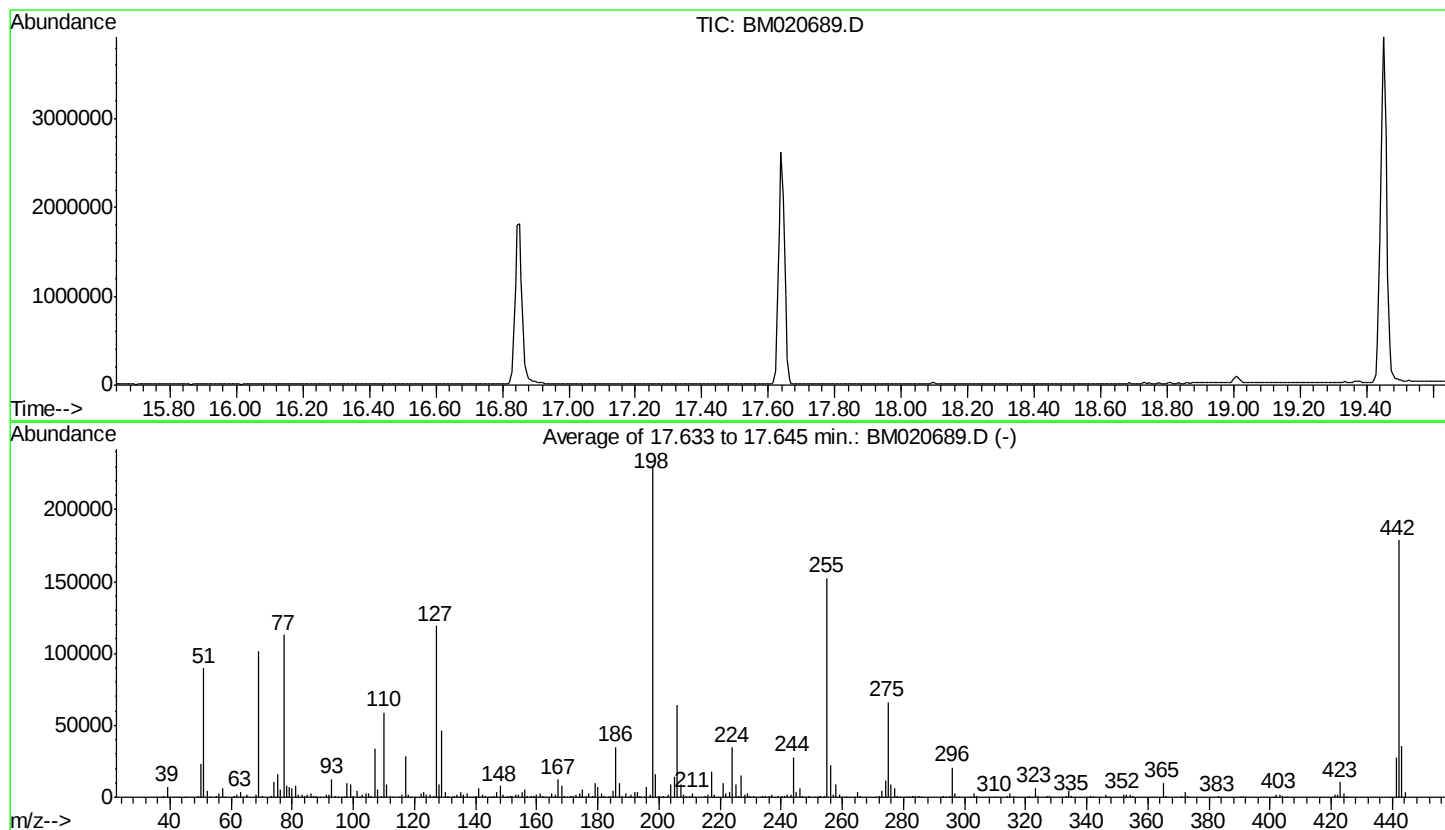

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	89522	PASS
68	69	0.00	2	1.9	1886	PASS
69	198	0.00	100	44.0	101581	PASS
70	69	0.00	2	0.6	602	PASS
127	198	10	80	51.6	118978	PASS
197	198	0.00	2	0.7	1677	PASS
198	198	100	100	100.0	230634	PASS
199	198	5	9	6.9	15895	PASS
275	198	10	60	28.8	66330	PASS
365	198	1	100	4.3	9898	PASS
441	198	0.01	100	11.9	27341	PASS
442	198	50	100	77.5	178645	PASS
443	442	15	24	19.8	35437	PASS