

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060419\
 Data File : BM020723.D
 Acq On : 05 Jun 2019 05:07
 Operator : HP/JU
 Sample : K2641-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D

Quant Time: Jun 05 06:49:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 31 15:48:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	304484	20.00	ng	-0.01
21) Naphthalene-d8	10.61	136	1150731	20.00	ng	-0.02
39) Acenaphthene-d10	14.46	164	600809	20.00	ng	-0.02
64) Phenanthrene-d10	17.20	188	1277644	20.00	ng	-0.01
76) Chrysene-d12	21.37	240	1193251	20.00	ng	-0.02
87) Perylene-d12	23.66	264	1374446	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	2086304	120.53	ng	0.00
7) Phenol-d6	6.99	99	2448869	96.08	ng	0.00
23) Nitrobenzene-d5	8.99	82	2025739	91.21	ng	-0.01
42) 2,4,6-Tribromophenol	15.94	330	1101484	147.97	ng	-0.02
45) 2-Fluorobiphenyl	13.08	172	4263499	94.34	ng	-0.01
79) Terphenyl-d14	19.83	244	6142777	86.11	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.99	77	5395	Below Cal	Qvalue #	11
32) Benzoic acid	9.92	122	118	5.145 ng	#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060419\
Data File : BM020723.D
Acq On : 05 Jun 2019 05:07
Operator : HP/JU
Sample : K2641-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-053119-D

Quant Time: Jun 05 06:49:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 31 15:48:49 2019
Response via : Initial Calibration

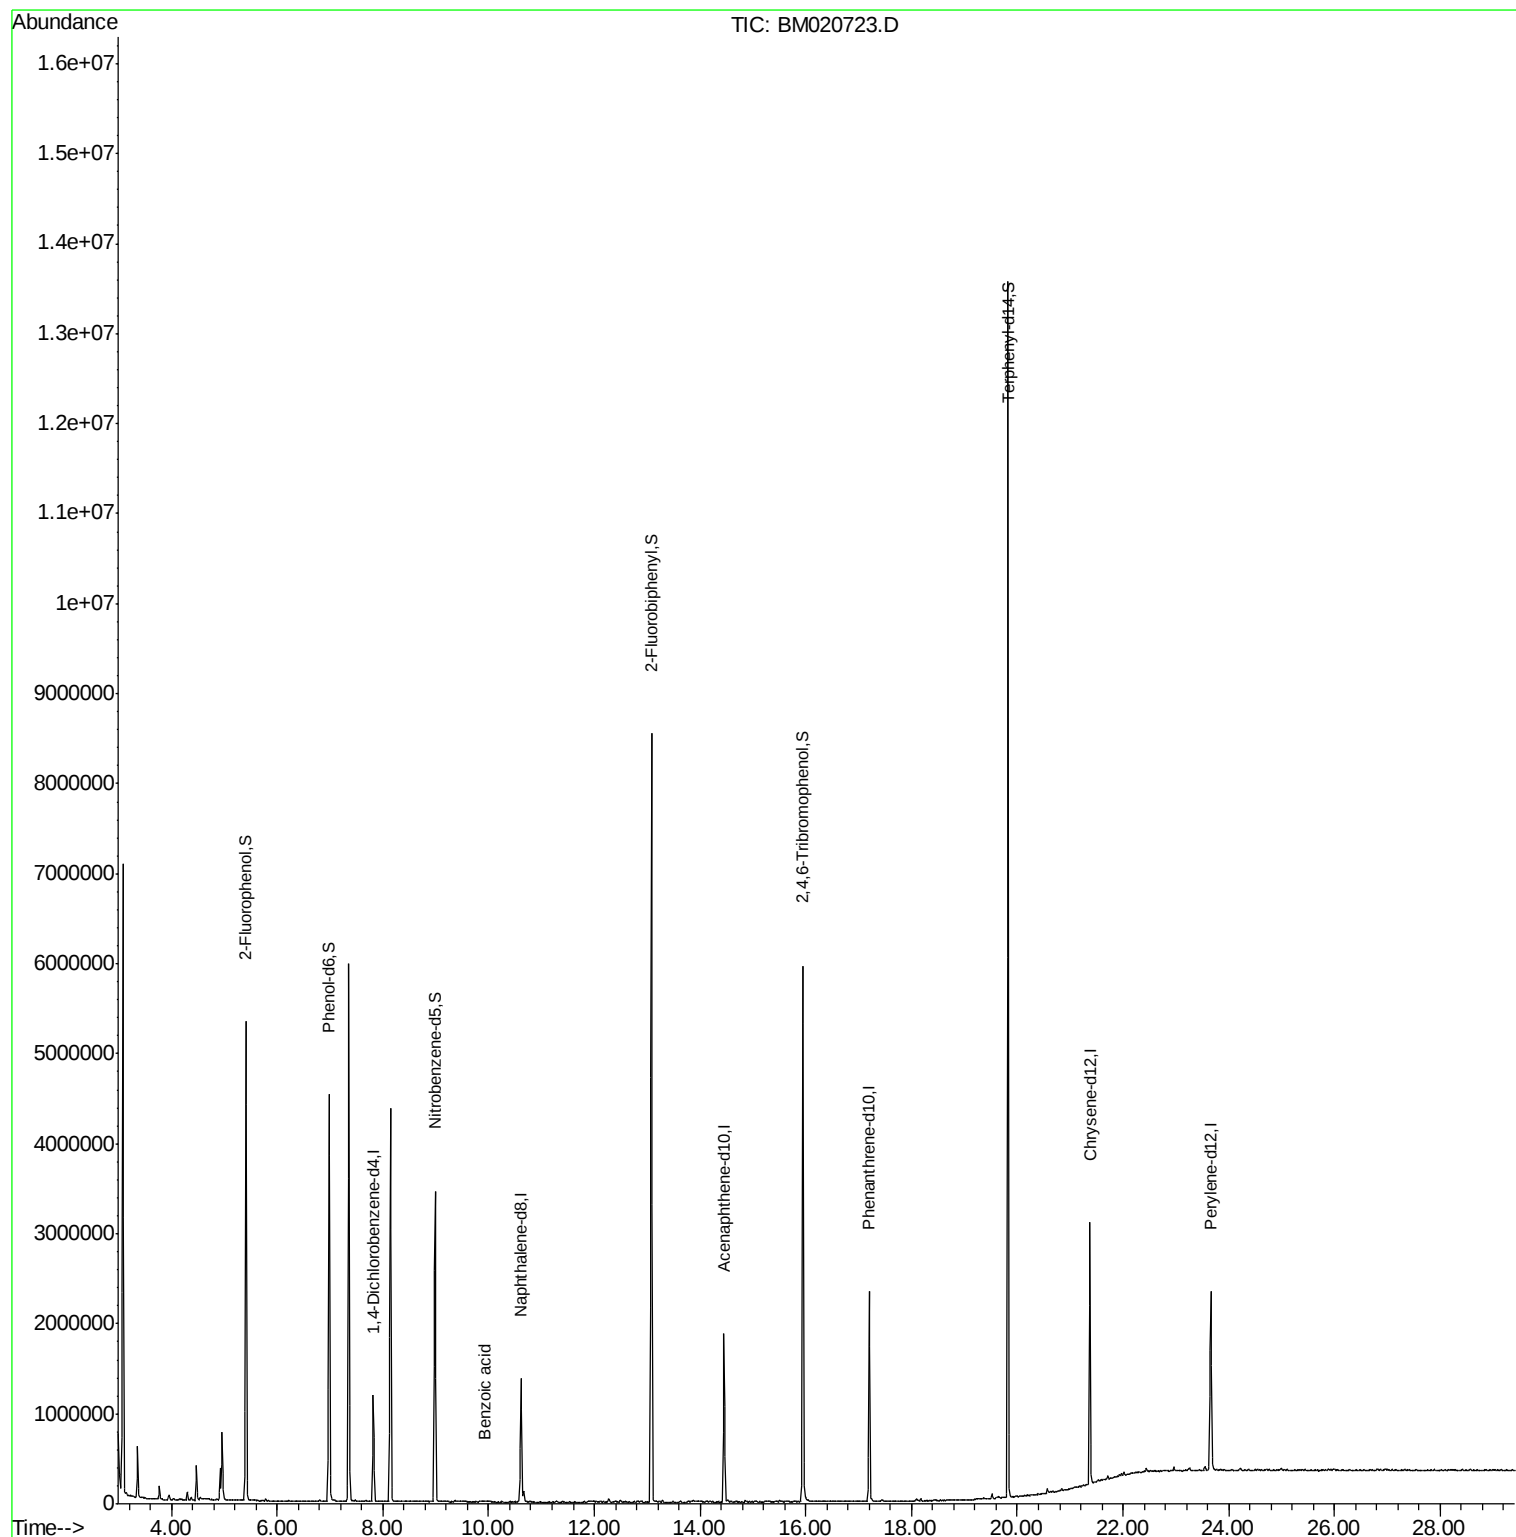

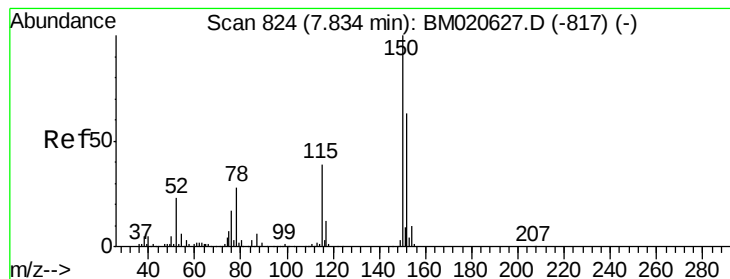


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.82 min Scan# 822
Delta R.T. -0.01 min
Lab File: BM020723.D
Acq: 05 Jun 2019 05:07

Instrument :
BNA_M
ClientSampleId :
CL-02-053119-D

Tgt Ion:152 Resp: 304484
Ion Ratio Lower Upper
152 100
150 155.9 126.0 189.0
115 59.9 49.6 74.4

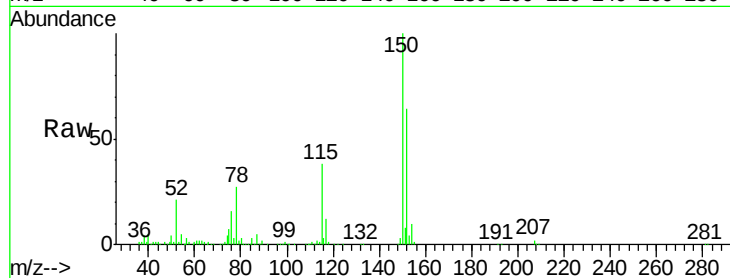


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

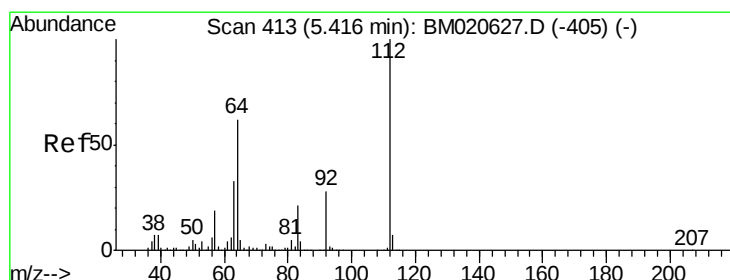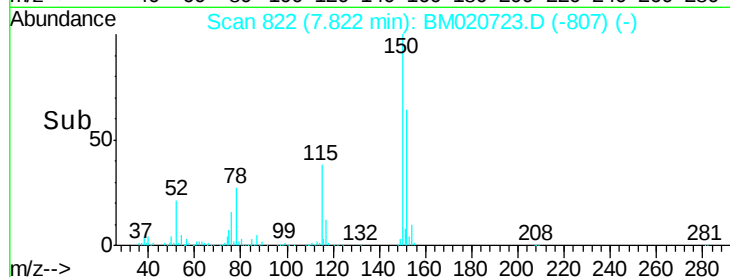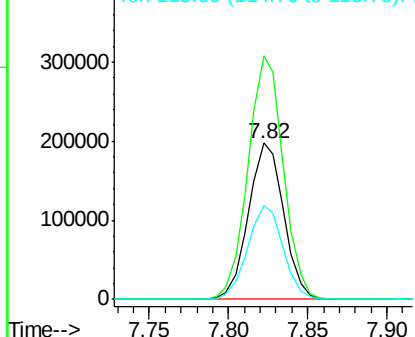



#5


2-Fluorophenol
Concen: 120.530 ng
RT: 5.41 min Scan# 412
Delta R.T. -0.01 min
Lab File: BM020723.D
Acq: 05 Jun 2019 05:07

Tgt Ion:112 Resp: 2086304
Ion Ratio Lower Upper
112 100
64 61.1 49.7 74.5
63 32.2 26.4 39.6

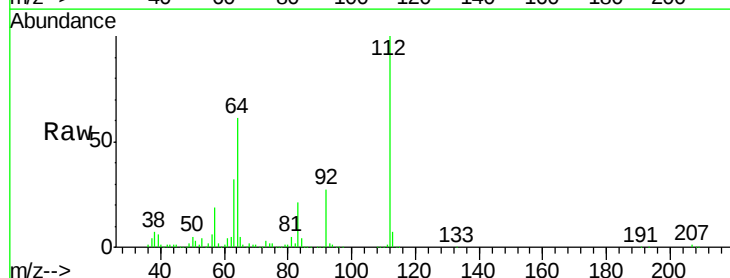

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

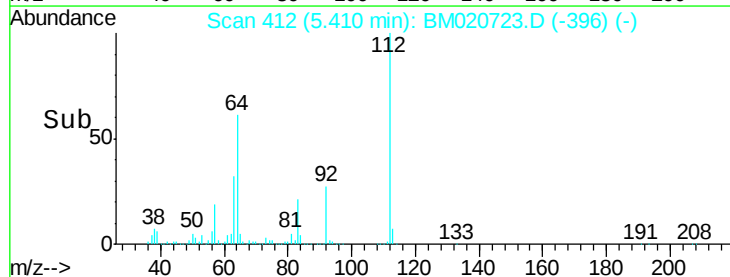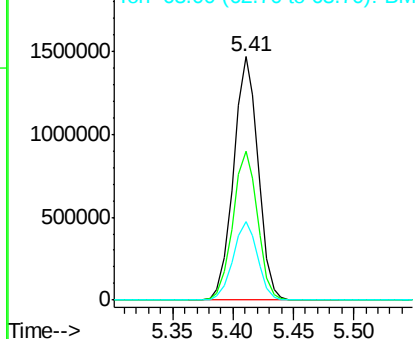

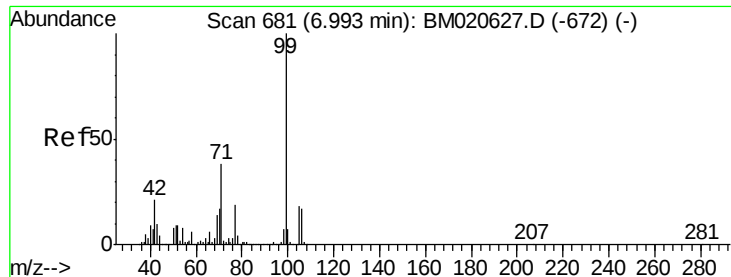

#7

Phenol-d6

Concen: 96.081 ng

RT: 6.99 min Scan# 680

Delta R.T. -0.01 min

Lab File: BM020723.D

Acq: 05 Jun 2019 05:07

Instrument :

BNA_M

ClientSampleId :

CL-02-053119-D


Tgt Ion: 99 Resp: 2448869

Ion Ratio Lower Upper




99 100

42 18.9 16.5 24.7

71 37.3 30.7 46.1

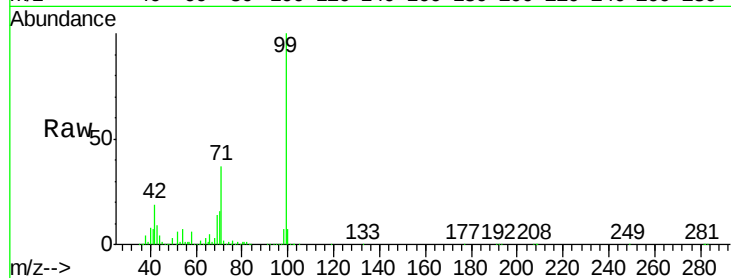

Abundance Ion 99.00 (98.70 to 99.70): BM020723.D (-664) (-)

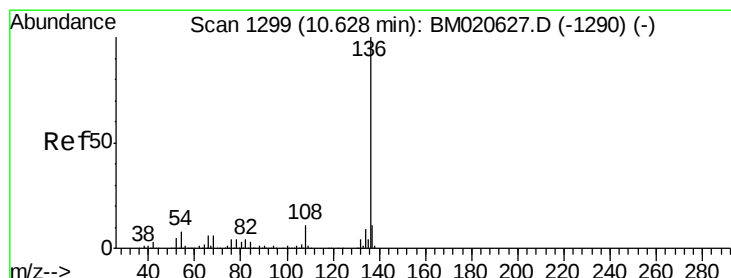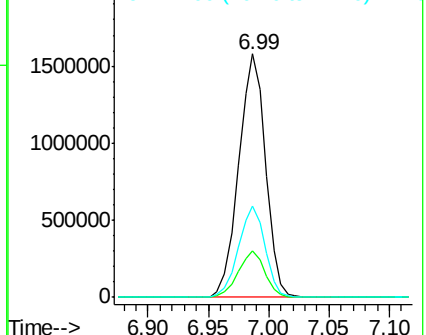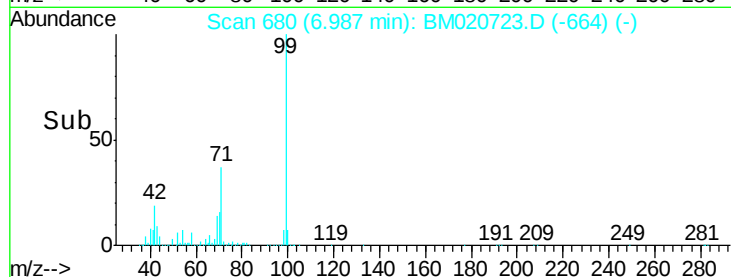

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1296

Delta R.T. -0.02 min

Lab File: BM020723.D

Acq: 05 Jun 2019 05:07

Tgt Ion: 136 Resp: 1150731


Ion Ratio Lower Upper

136 100



137 10.8 8.8 13.2


54 7.8 6.6 10.0

68 6.1 5.1 7.7

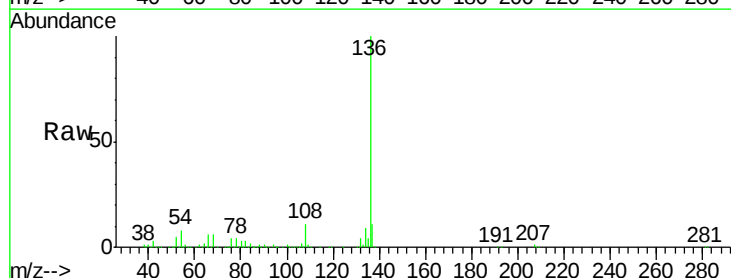

Abundance Ion 136.00 (135.70 to 136.70): BM020723.D (-1282) (-)



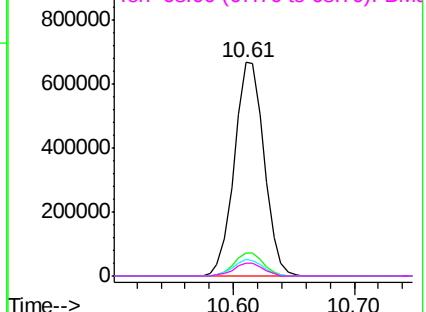
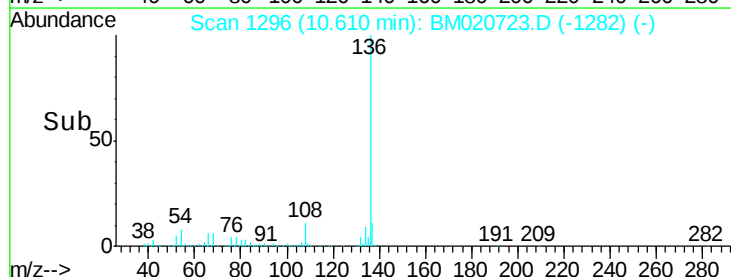




#23
 Nitrobenzene-d5
 Concen: 91.209 ng
 RT: 8.99 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07




Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D


Tgt Ion: 82 Resp: 2025739
 Ion Ratio Lower Upper
 82 100
 128 42.0 31.5 47.3
 54 46.8 39.4 59.0

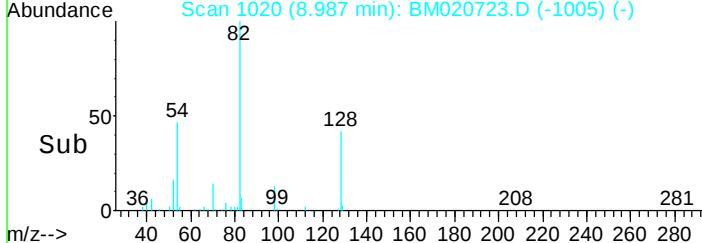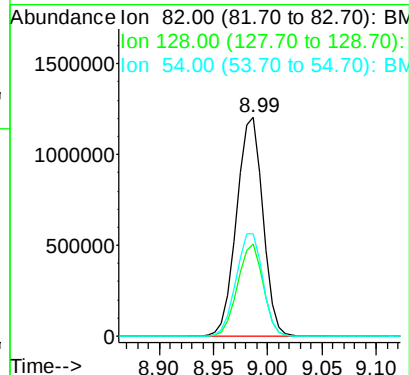

#32
 Benzoic acid
 Concen: 5.145 ng
 RT: 9.92 min Scan# 1179
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Tgt Ion:122 Resp: 118
 Ion Ratio Lower Upper
 122 100

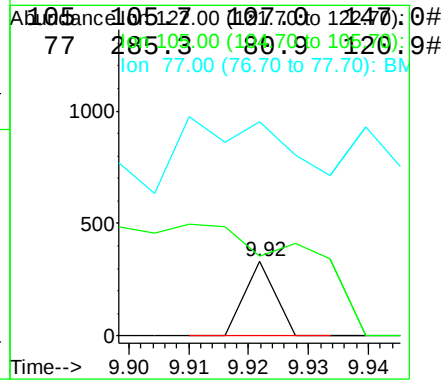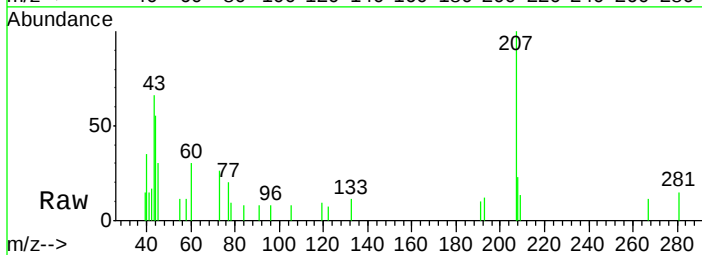







#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.46 min Scan# 1950
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D

Tgt Ion:164 Resp: 600809
 Ion Ratio Lower Upper
 164 100
 162 101.8 83.2 124.8
 160 46.8 37.5 56.3




Abundance Ion 164.00 (163.70 to 164.70):
 Ion 162.00 (161.70 to 162.70):
 Ion 160.00 (159.70 to 160.70):

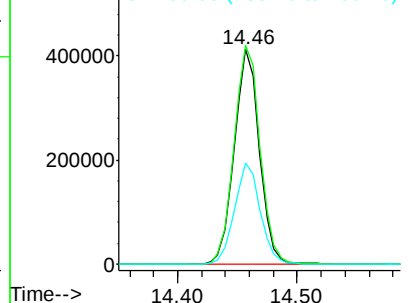
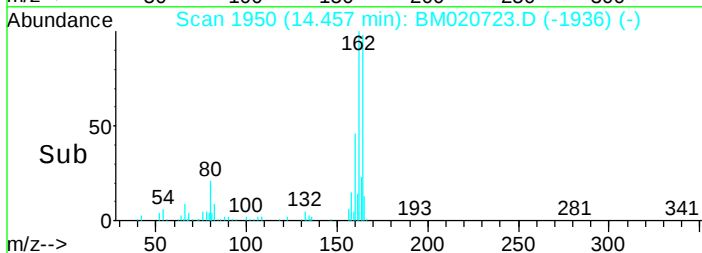



#42
 2,4,6-Tribromophenol
 Concen: 147.970 ng
 RT: 15.94 min Scan# 2203
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Tgt Ion:330 Resp: 1101484
 Ion Ratio Lower Upper
 330 100

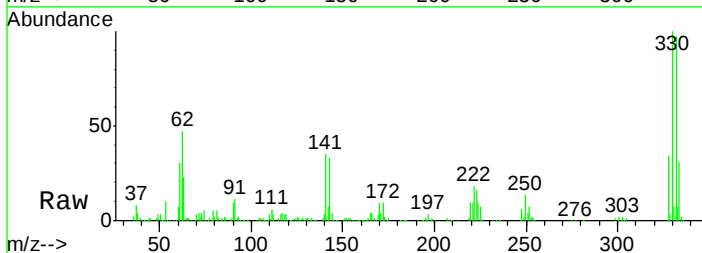

Abundance Ion 330.80 (329.50 to 331.10):
 Ion 330.80 (329.50 to 332.10):
 Ion 141.00 (140.70 to 141.70):



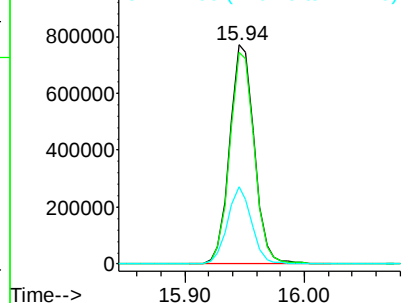





#45
 2-Fluorobiphenyl
 Concen: 94.341 ng
 RT: 13.08 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07




Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D


Tgt Ion:172 Resp: 4263499
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 43.0
 170 23.1 18.9 28.3

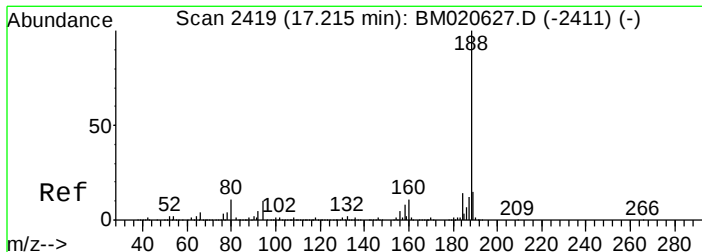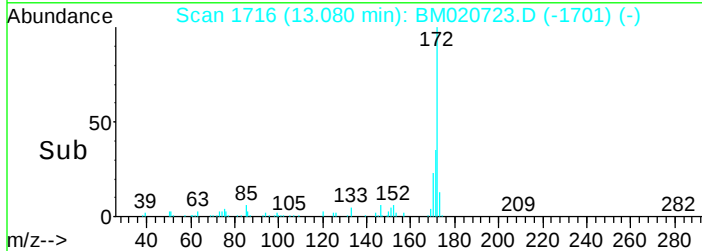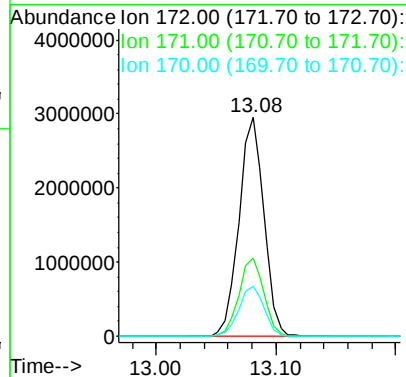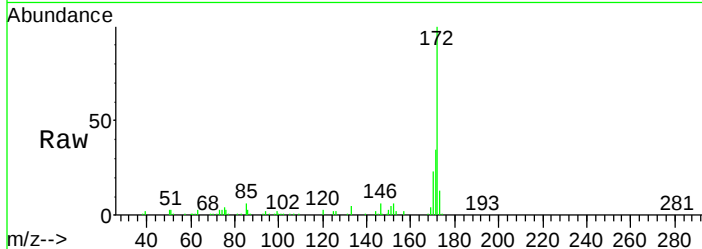

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.20 min Scan# 2417
 Delta R.T. -0.01 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Tgt Ion:188 Resp: 1277644
 Ion Ratio Lower Upper
 188 100

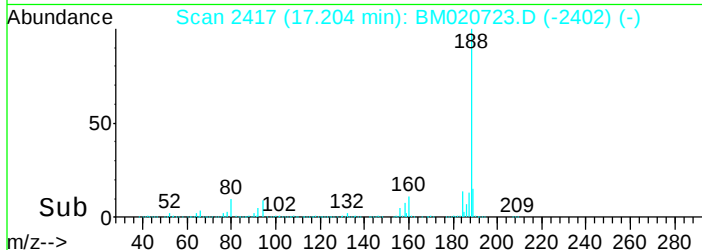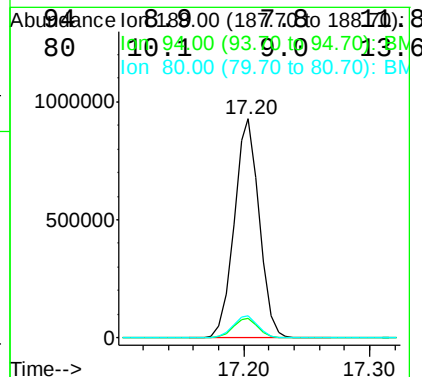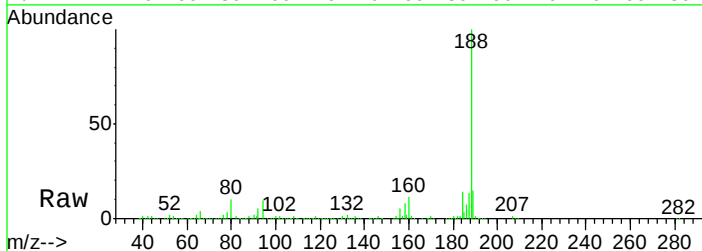







#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.37 min Scan# 3126
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D

Tgt Ion:240 Resp: 1193251
 Ion Ratio Lower Upper
 240 100
 120 10.5 8.2 12.2
 236 26.5 21.2 31.8

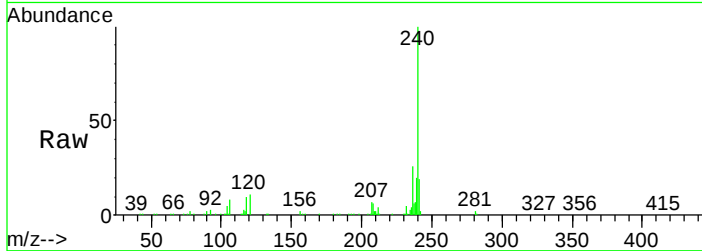


Abundance Ion 240.00 (239.70 to 240.70):
 Ion 120.00 (119.70 to 120.70):
 Ion 236.00 (235.70 to 236.70):

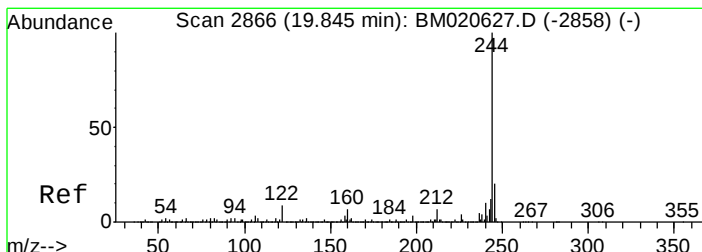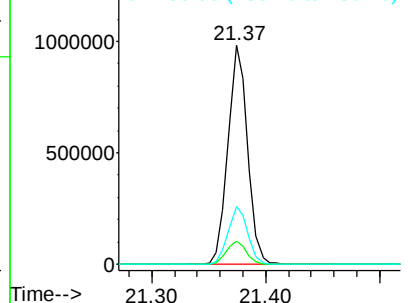
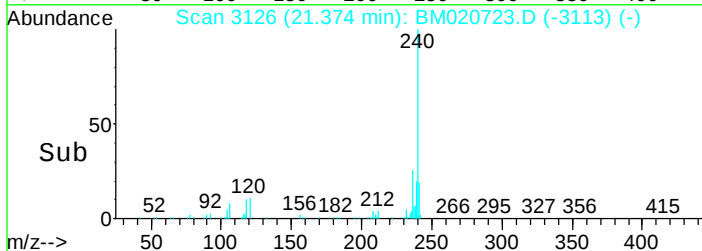





#79
 Terphenyl-d14
 Concen: 86.107 ng
 RT: 19.83 min Scan# 2863
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Tgt Ion:244 Resp: 6142777
 Ion Ratio Lower Upper
 244 100
 122 9.2 7.2 10.8

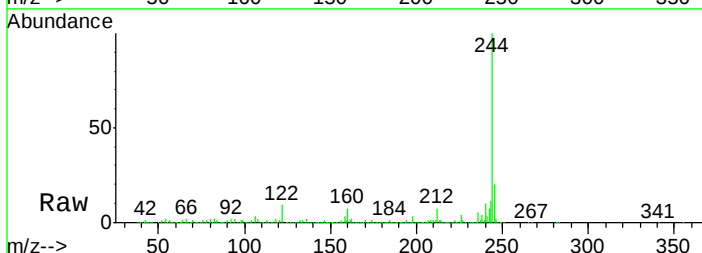

Abundance Ion 244.00 (243.70 to 244.70):
 Ion 122.00 (121.70 to 122.70):

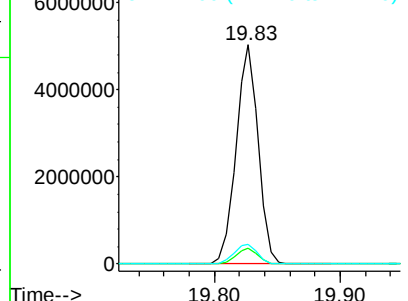

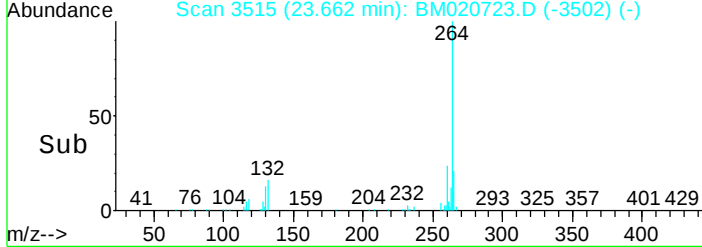

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.66 min Scan# 3515
 Delta R.T. -0.02 min
 Lab File: BM020723.D
 Acq: 05 Jun 2019 05:07

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-053119-D

Tgt Ion:264 Resp: 1374446
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.2 28.8
 265 21.4 17.6 26.4

