

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
 Data File : BM020710.D
 Acq On : 04 Jun 2019 19:25
 Operator : HP/JU
 Sample : PB120137BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120137BL

Quant Time: Jun 05 03:52:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 31 15:48:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	313092	20.00	ng	-0.01
21) Naphthalene-d8	10.62	136	1225800	20.00	ng	-0.01
39) Acenaphthene-d10	14.46	164	669172	20.00	ng	-0.02
64) Phenanthrene-d10	17.20	188	1389565	20.00	ng	-0.01
76) Chrysene-d12	21.38	240	1125215	20.00	ng	-0.02
87) Perylene-d12	23.66	264	1274054	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	2264596	127.23	ng	0.00
7) Phenol-d6	6.99	99	3083921	117.67	ng	0.00
23) Nitrobenzene-d5	8.99	82	1879208	79.43	ng	-0.01
42) 2,4,6-Tribromophenol	15.95	330	1047205	126.31	ng	-0.01
45) 2-Fluorobiphenyl	13.08	172	4314273	85.71	ng	-0.01
79) Terphenyl-d14	19.83	244	5346671	79.48	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020710.D
Acq On : 04 Jun 2019 19:25
Operator : HP/JU
Sample : PB120137BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120137BL

Quant Time: Jun 05 03:52:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 31 15:48:49 2019
Response via : Initial Calibration

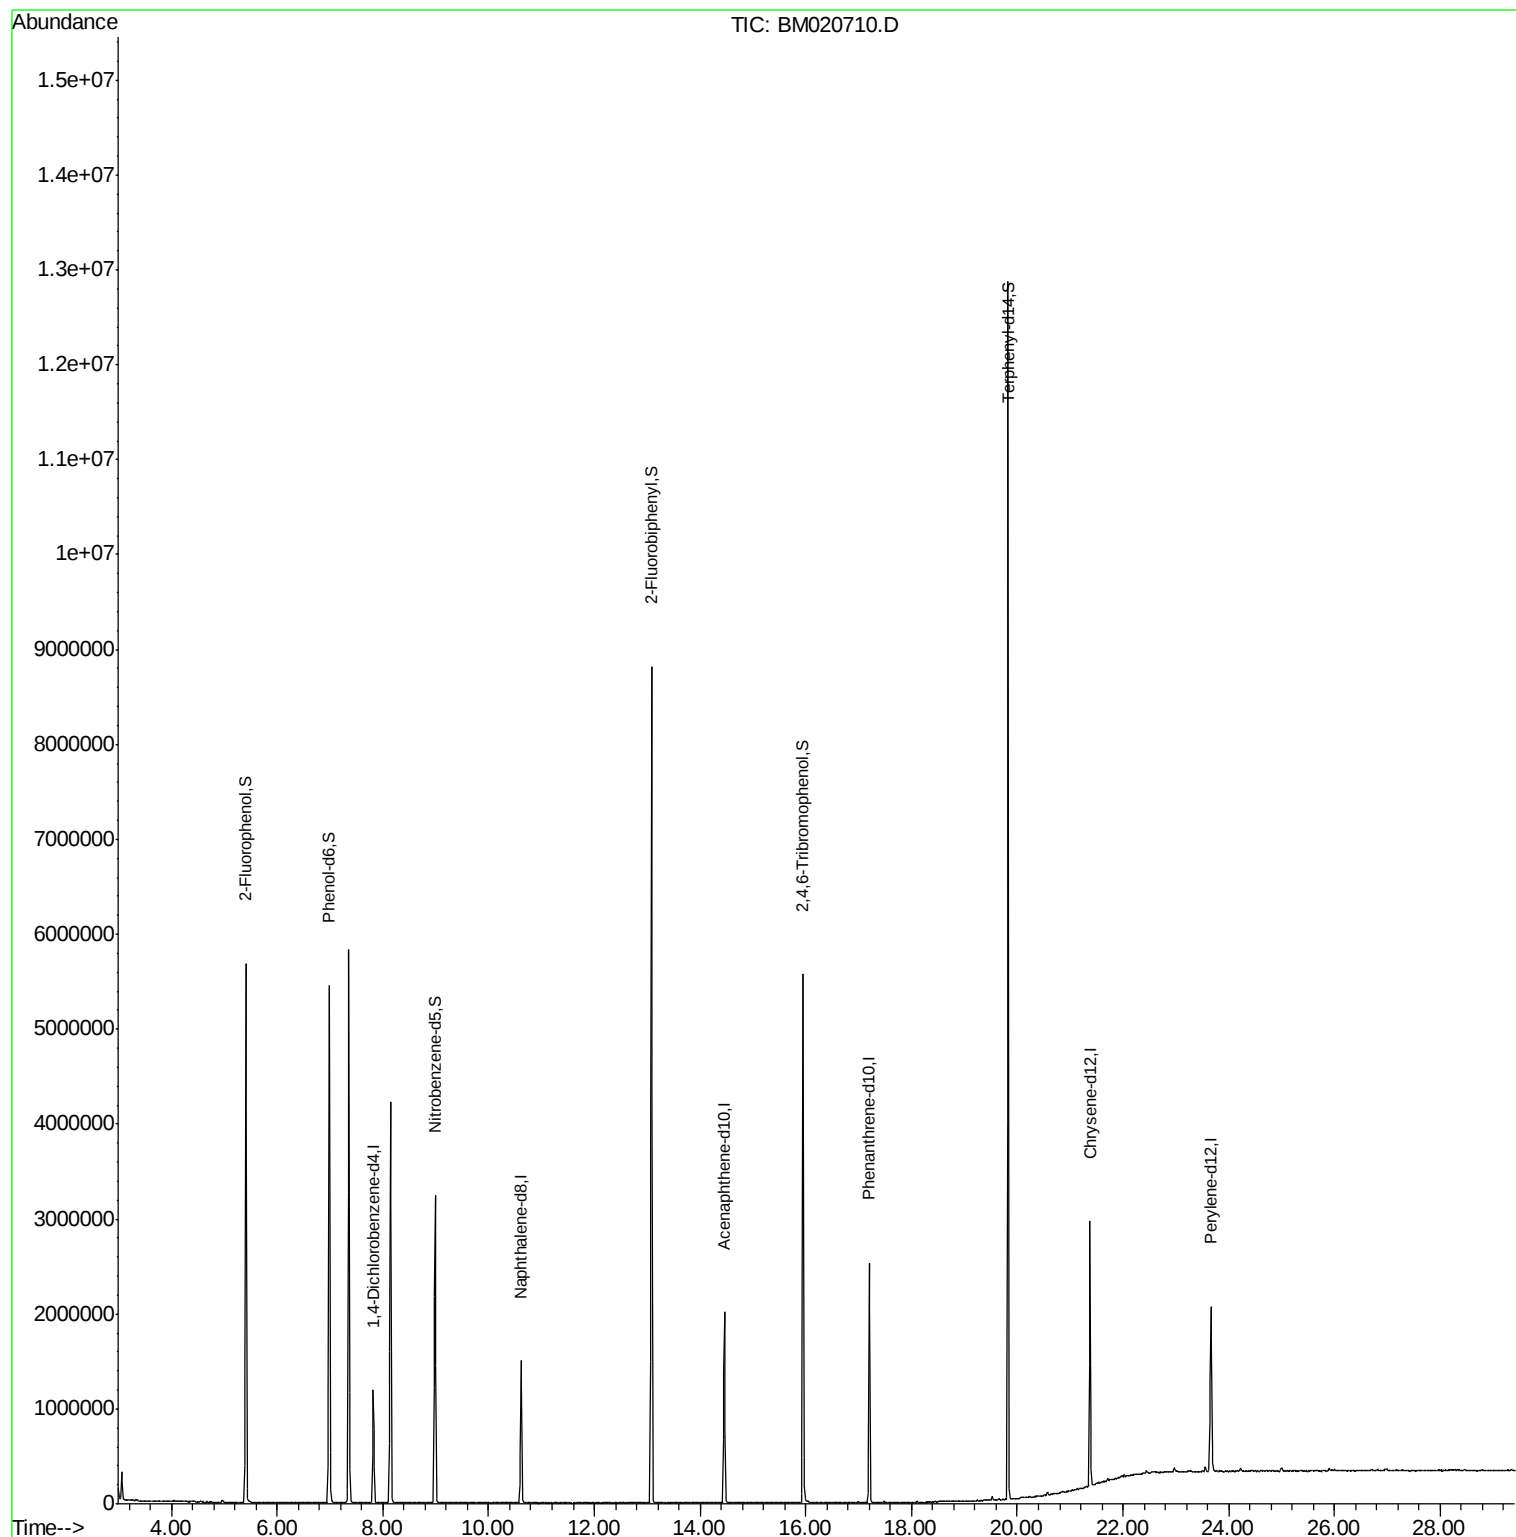

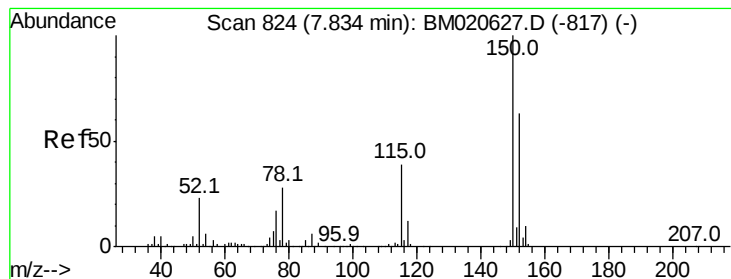


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.82 min Scan# 822
Delta R.T. -0.01 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25

Instrument :
BNA_M
ClientSampleId :
PB120137BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.4	126.0	189.0
115	60.6	49.6	74.4



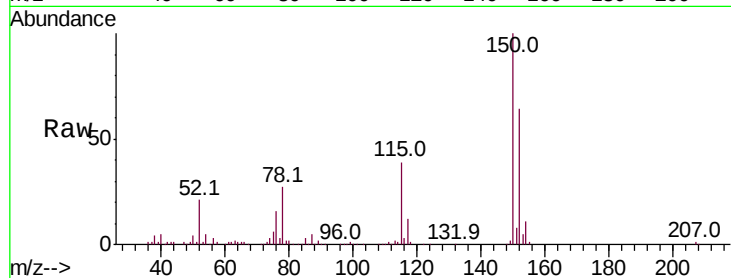


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

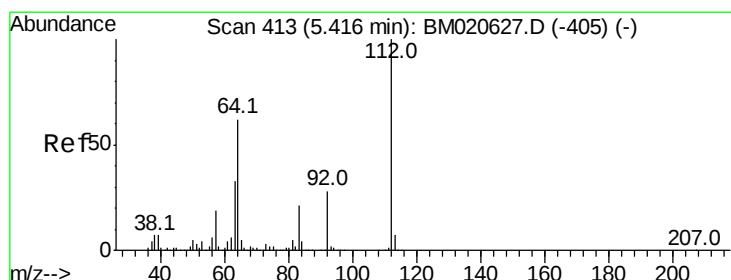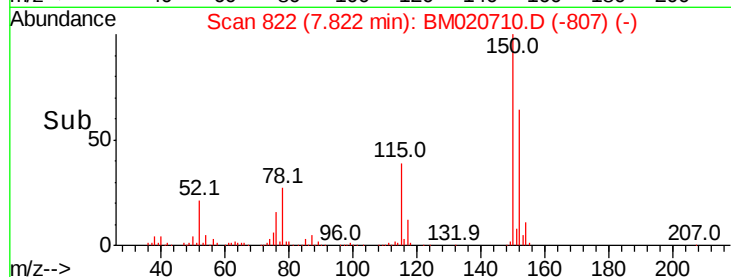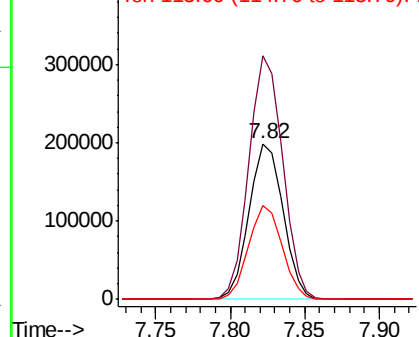

#5

2-Fluorophenol
Concen: 127.233 ng
RT: 5.41 min Scan# 412
Delta R.T. -0.01 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.2	49.7	74.5
63	31.3	26.4	39.6


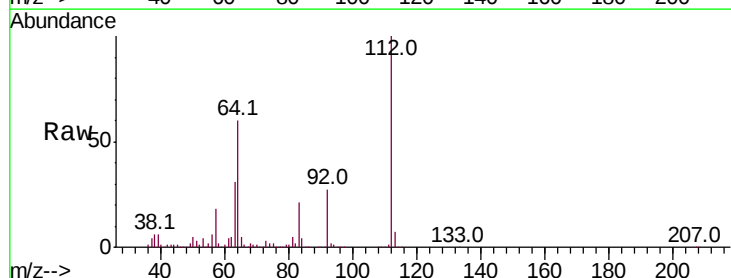



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

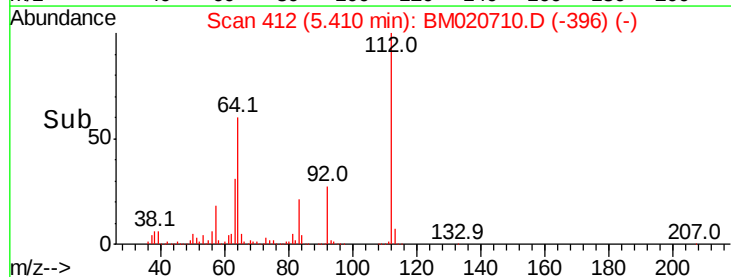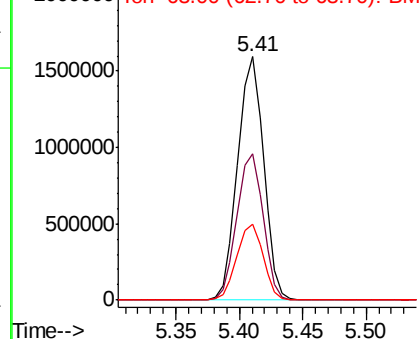

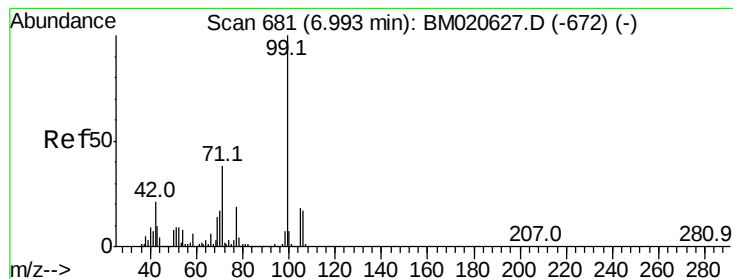

#7

Phenol-d6

Concen: 117.671 ng

RT: 6.99 min Scan# 680

Delta R.T. -0.01 min

Lab File: BM020710.D

Acq: 04 Jun 2019 19:25

Instrument :


BNA_M

ClientSampleId :

PB120137BL

Tot Ion: 99 Resp: 3083921

Ion	Ratio	Lower	Upper
99	100		
42	19.1	16.5	24.7
71	38.1	30.7	46.1



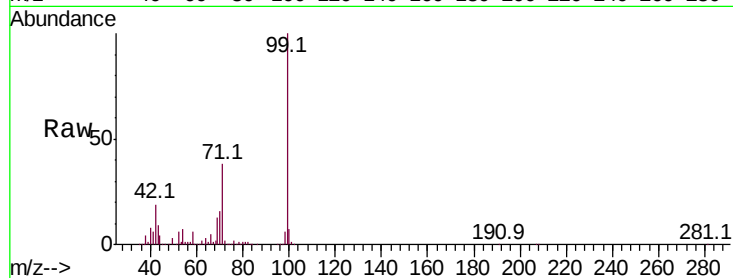


Abundance

Ion 99.00 (98.70 to 99.70): BM020627.D (-672) (-)

Ion 42.00 (41.70 to 42.70): BM020627.D (-672) (-)

Ion 71.00 (70.70 to 71.70): BM020627.D (-672) (-)

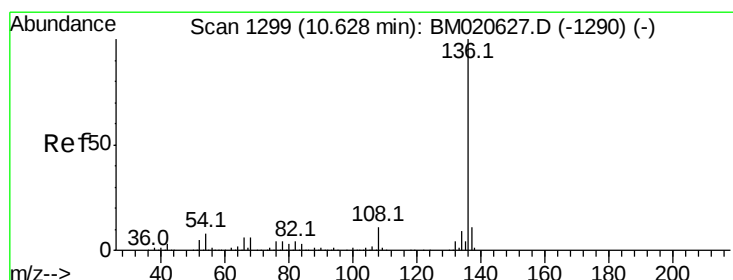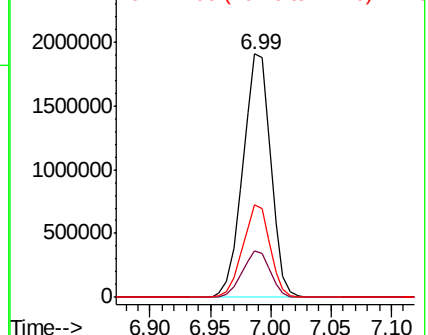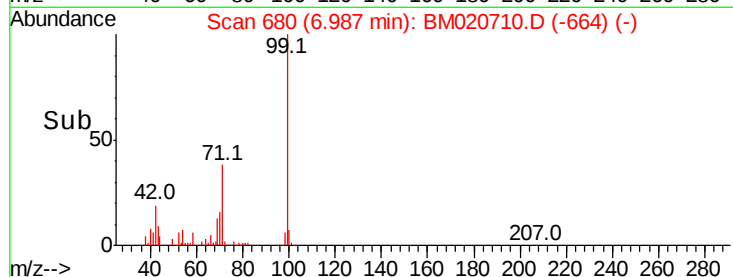

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.62 min Scan# 1297


Delta R.T. -0.01 min

Lab File: BM020710.D

Acq: 04 Jun 2019 19:25

Tgt Ion: 136 Resp: 1225800

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.8	13.2
54	7.4	6.6	10.0
68	6.2	5.1	7.7

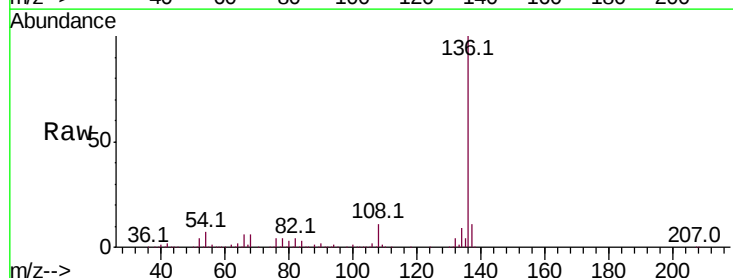



Abundance


Ion 136.00 (135.70 to 136.70): BM020627.D (-1290) (-)

Ion 137.00 (136.70 to 137.70): BM020627.D (-1290) (-)

Ion 54.00 (53.70 to 54.70): BM020627.D (-1290) (-)

Ion 68.00 (67.70 to 68.70): BM020627.D (-1290) (-)

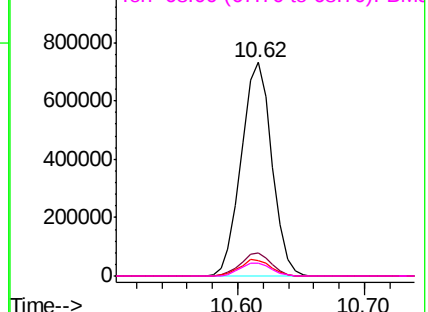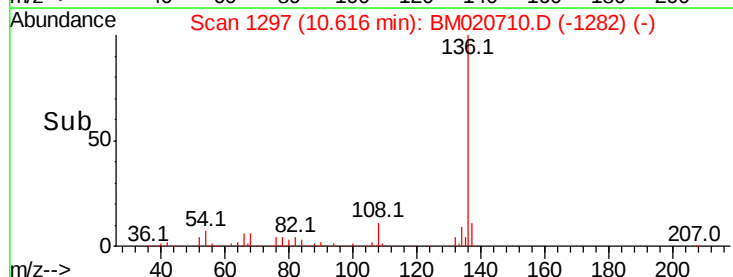


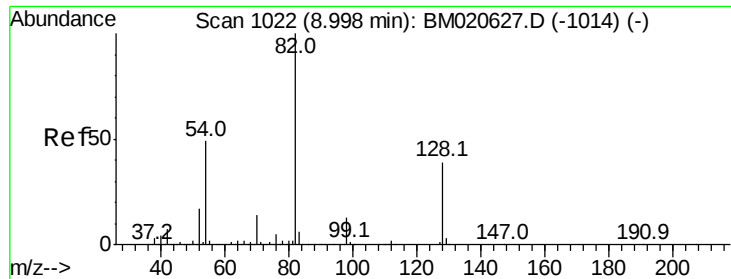




#23
Nitrobenzene-d5
Concen: 79.430 ng
RT: 8.99 min Scan# 1020
Delta R.T. -0.01 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25

Instrument :
BNA_M
ClientSampleId :
PB120137BL

Tot Ion: 82 Resp: 1879208
Ion Ratio Lower Upper
82 100
128 41.6 31.5 47.3
54 47.7 39.4 59.0

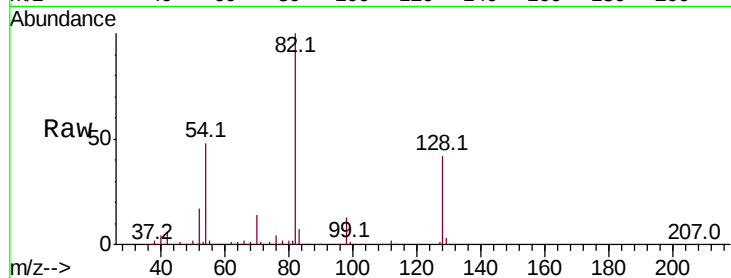


Abundance Ion 82.00 (81.70 to 82.70): BM020627.D (-1014) (-)
Ion 128.00 (127.70 to 128.70): BM020627.D (-1014) (-)
Ion 54.00 (53.70 to 54.70): BM020627.D (-1014) (-)

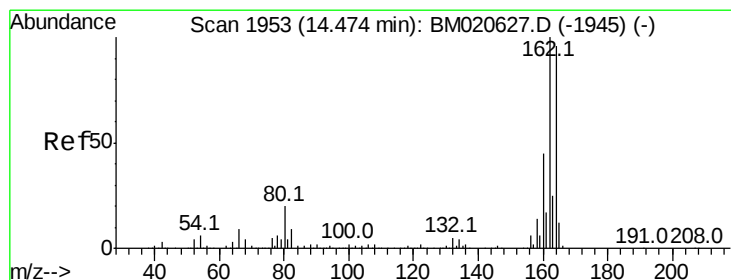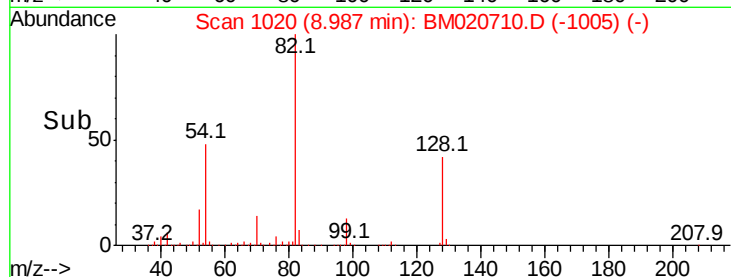
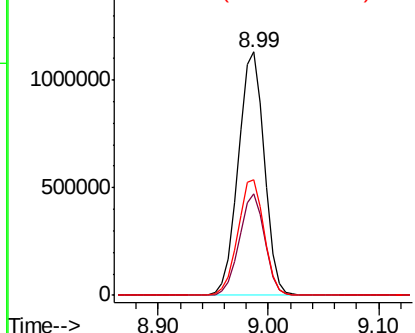



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.46 min Scan# 1950
Delta R.T. -0.02 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25

Tgt Ion:164 Resp: 669172
Ion Ratio Lower Upper
164 100
162 104.2 83.2 124.8
160 46.4 37.5 56.3

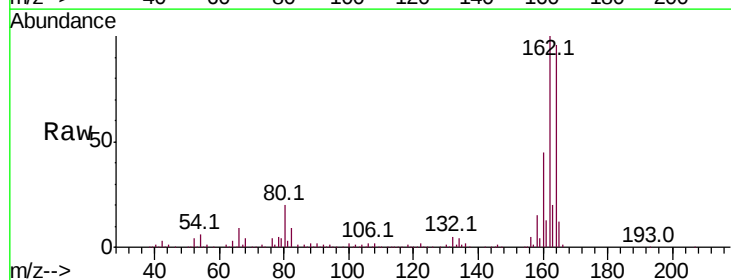

Abundance Ion 164.00 (163.70 to 164.70): BM020627.D (-1945) (-)
Ion 162.00 (161.70 to 162.70): BM020627.D (-1945) (-)
Ion 160.00 (159.70 to 160.70): BM020627.D (-1945) (-)

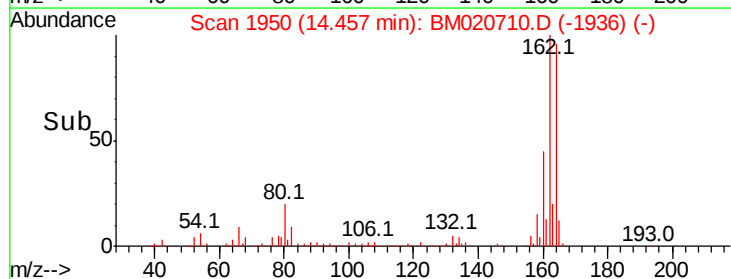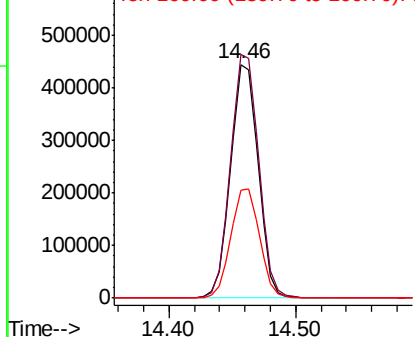


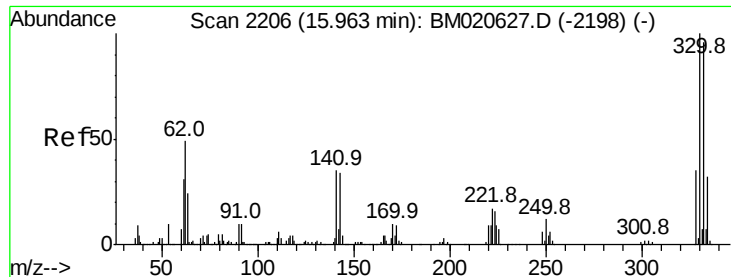




#42
 2,4,6-Tribromophenol
 Concen: 126.306 ng
 RT: 15.95 min Scan# 2204
 Delta R.T. -0.01 min
 Lab File: BM020710.D
 Acq: 04 Jun 2019 19:25

Instrument :
 BNA_M
 ClientSampleId :
 PB120137BL

Tot Ion:330 Resp: 1047205
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.4 116.0
 141 35.0 30.4 45.6

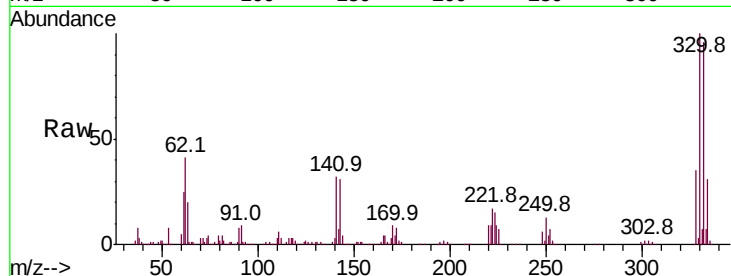


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

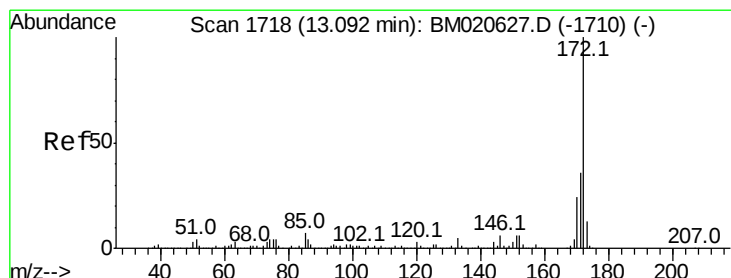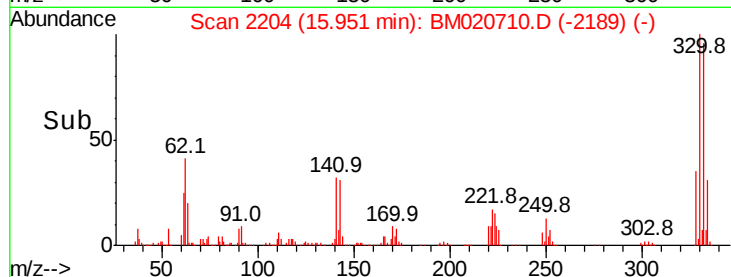
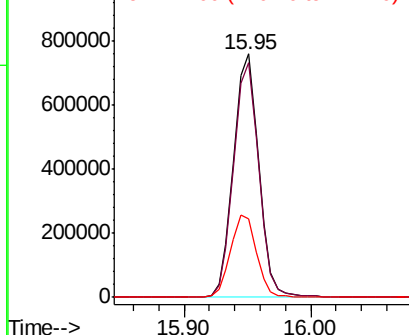



#45
 2-Fluorobiphenyl
 Concen: 85.712 ng
 RT: 13.08 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BM020710.D
 Acq: 04 Jun 2019 19:25

Tgt Ion:172 Resp: 4314273
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 43.0
 170 23.1 18.9 28.3

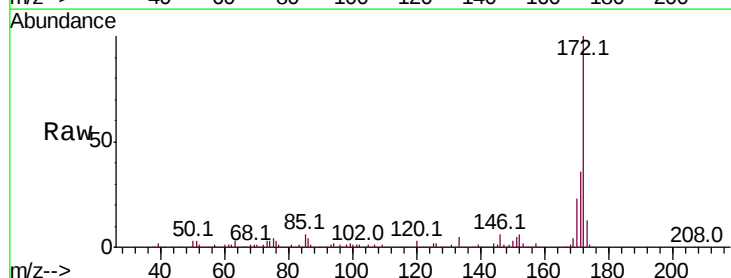

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



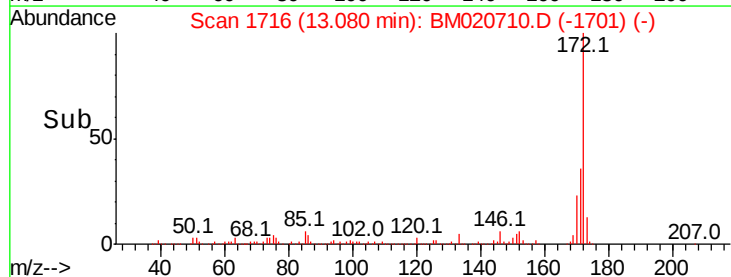
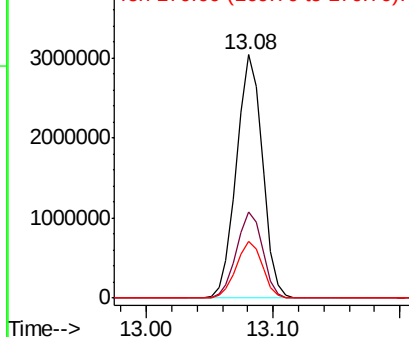


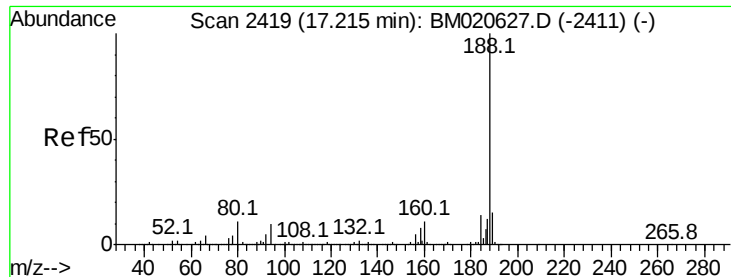

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.20 min Scan# 2417
Delta R.T. -0.01 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25




Instrument :
BNA_M
ClientSampleId :
PB120137BL


Tot Ion:188 Resp: 1389565
Ion Ratio Lower Upper
188 100
94 9.1 7.8 11.8
80 10.3 9.0 13.6

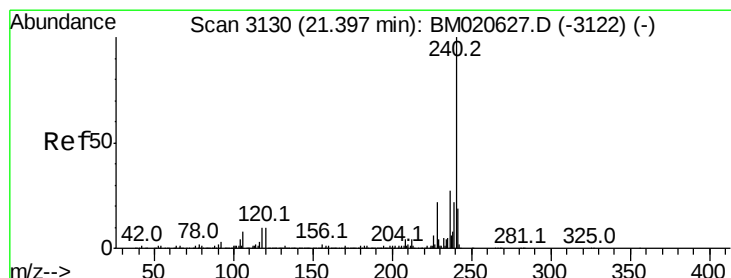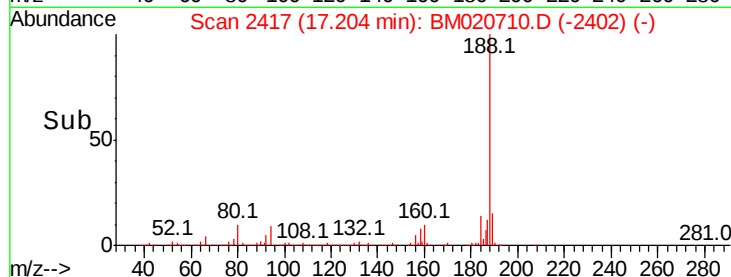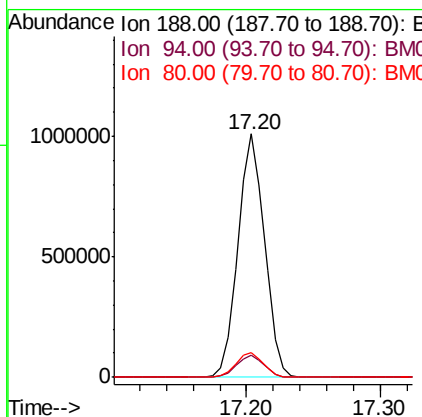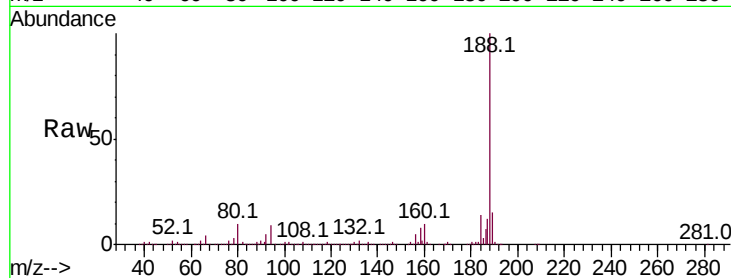

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.38 min Scan# 3127
Delta R.T. -0.02 min
Lab File: BM020710.D
Acq: 04 Jun 2019 19:25

Tgt Ion:240 Resp: 1125215
Ion Ratio Lower Upper
240 100
120 10.5 8.2 12.2
236 26.5 21.2 31.8

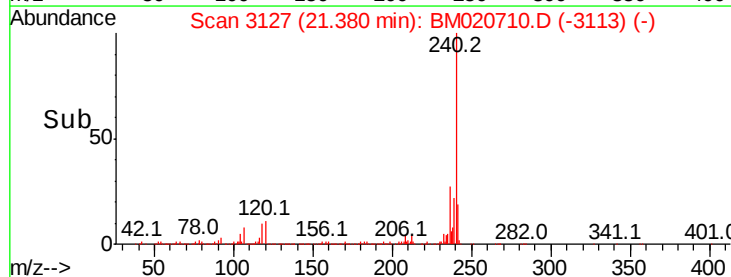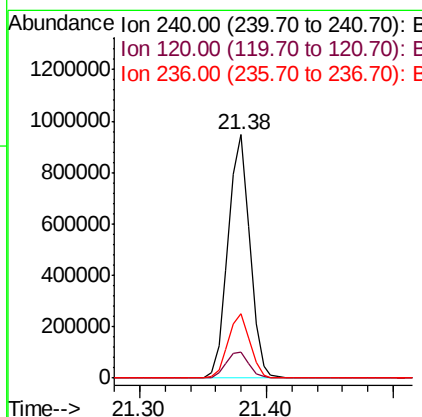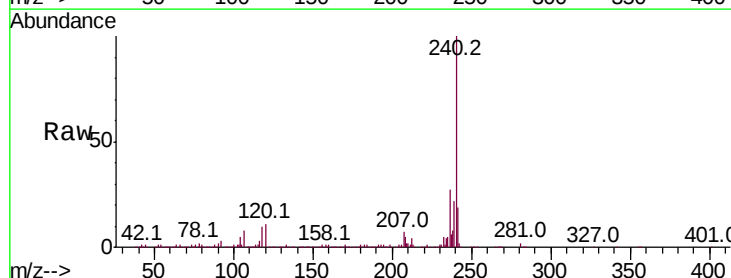

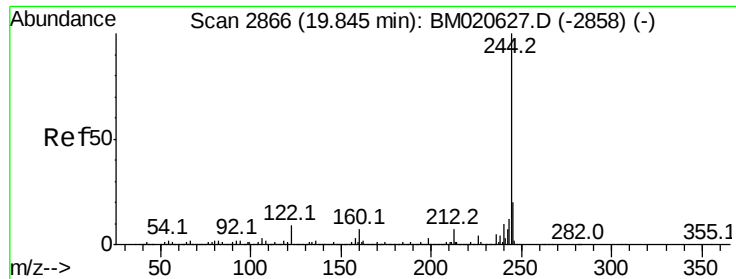

#79

Terphenyl-d14

Concen: 79.479 ng

RT: 19.83 min Scan# 2863

Delta R.T. -0.02 min

Lab File: BM020710.D

Acq: 04 Jun 2019 19:25

Instrument :

BNA_M

ClientSampleId :

PB120137BL


Tot Ion:244 Resp: 5346671

Ion Ratio Lower Upper

244 100

212 6.9 5.7 8.5




122 9.5 7.2 10.8

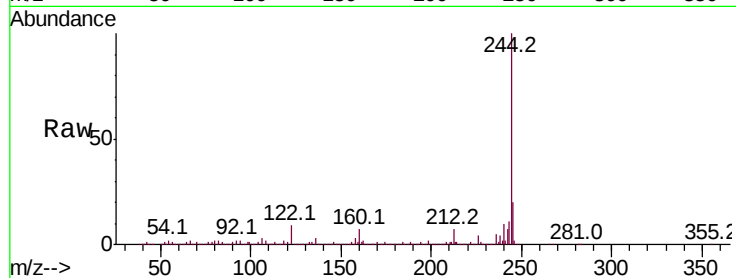

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

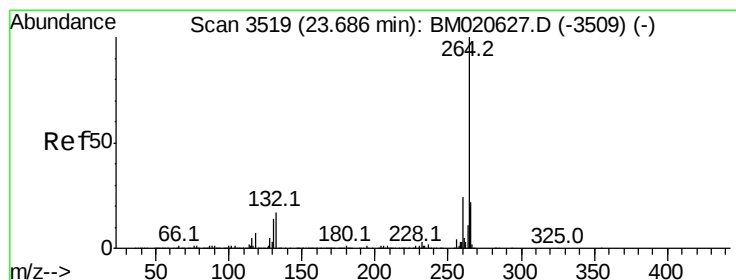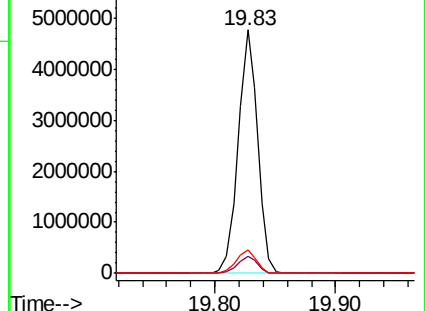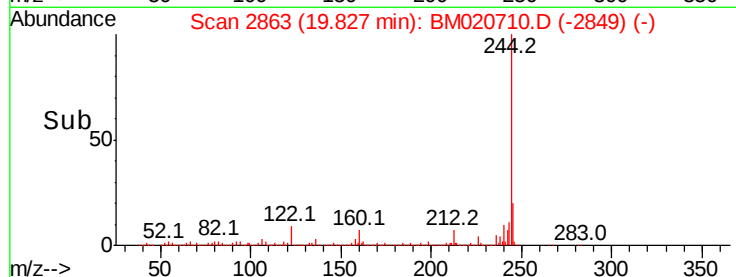

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.66 min Scan# 3515

Delta R.T. -0.02 min

Lab File: BM020710.D

Acq: 04 Jun 2019 19:25


Tgt Ion:264 Resp: 1274054

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 22.1 17.6 26.4

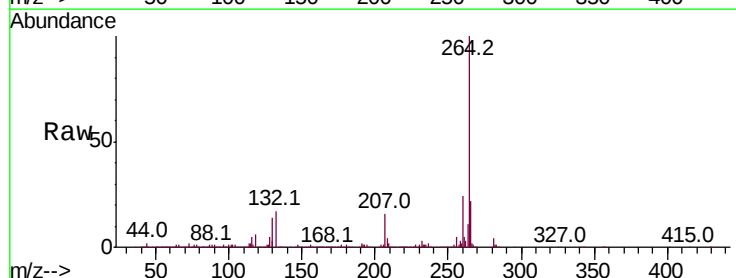

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

