

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
 Data File : BM020710.D
 Acq On : 04 Jun 2019 19:25
 Operator : HP/JU
 Sample : PB120137BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120137BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	9	13	19	rVB	287242	315683	2.17%	0.344%
2	5.410	405	412	421	rBV	5680090	8122800	55.77%	8.839%
3	6.987	670	680	700	rBV	5453112	8916312	61.21%	9.703%
4	7.357	735	743	755	rBV	5830090	9043283	62.08%	9.841%
5	7.822	815	822	831	rVB	1191850	1894120	13.00%	2.061%
6	8.145	869	877	885	rBV	4230404	6863851	47.12%	7.469%
7	8.987	1011	1020	1030	rBV	3245115	5389220	37.00%	5.864%
8	10.616	1289	1297	1305	rVB	1500692	2506944	17.21%	2.728%
9	13.080	1708	1716	1729	rBV	8818618	12554127	86.19%	13.661%
10	14.463	1943	1951	1961	rBV2	2010624	3189436	21.90%	3.471%
11	15.945	2197	2203	2223	rBV	5576114	8162928	56.04%	8.883%
12	17.204	2410	2417	2430	rBV2	2526337	3532968	24.25%	3.845%
13	19.827	2857	2863	2869	rBV	12830891	14566071	100.00%	15.850%
14	21.380	3121	3127	3133	rBV	2796125	3401062	23.35%	3.701%
15	23.662	3509	3515	3527	rVB2	1734673	3437852	23.60%	3.741%


Sum of corrected areas: 91896657

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020710.D
Acq On : 04 Jun 2019 19:25
Operator : HP/JU
Sample : PB120137BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120137BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

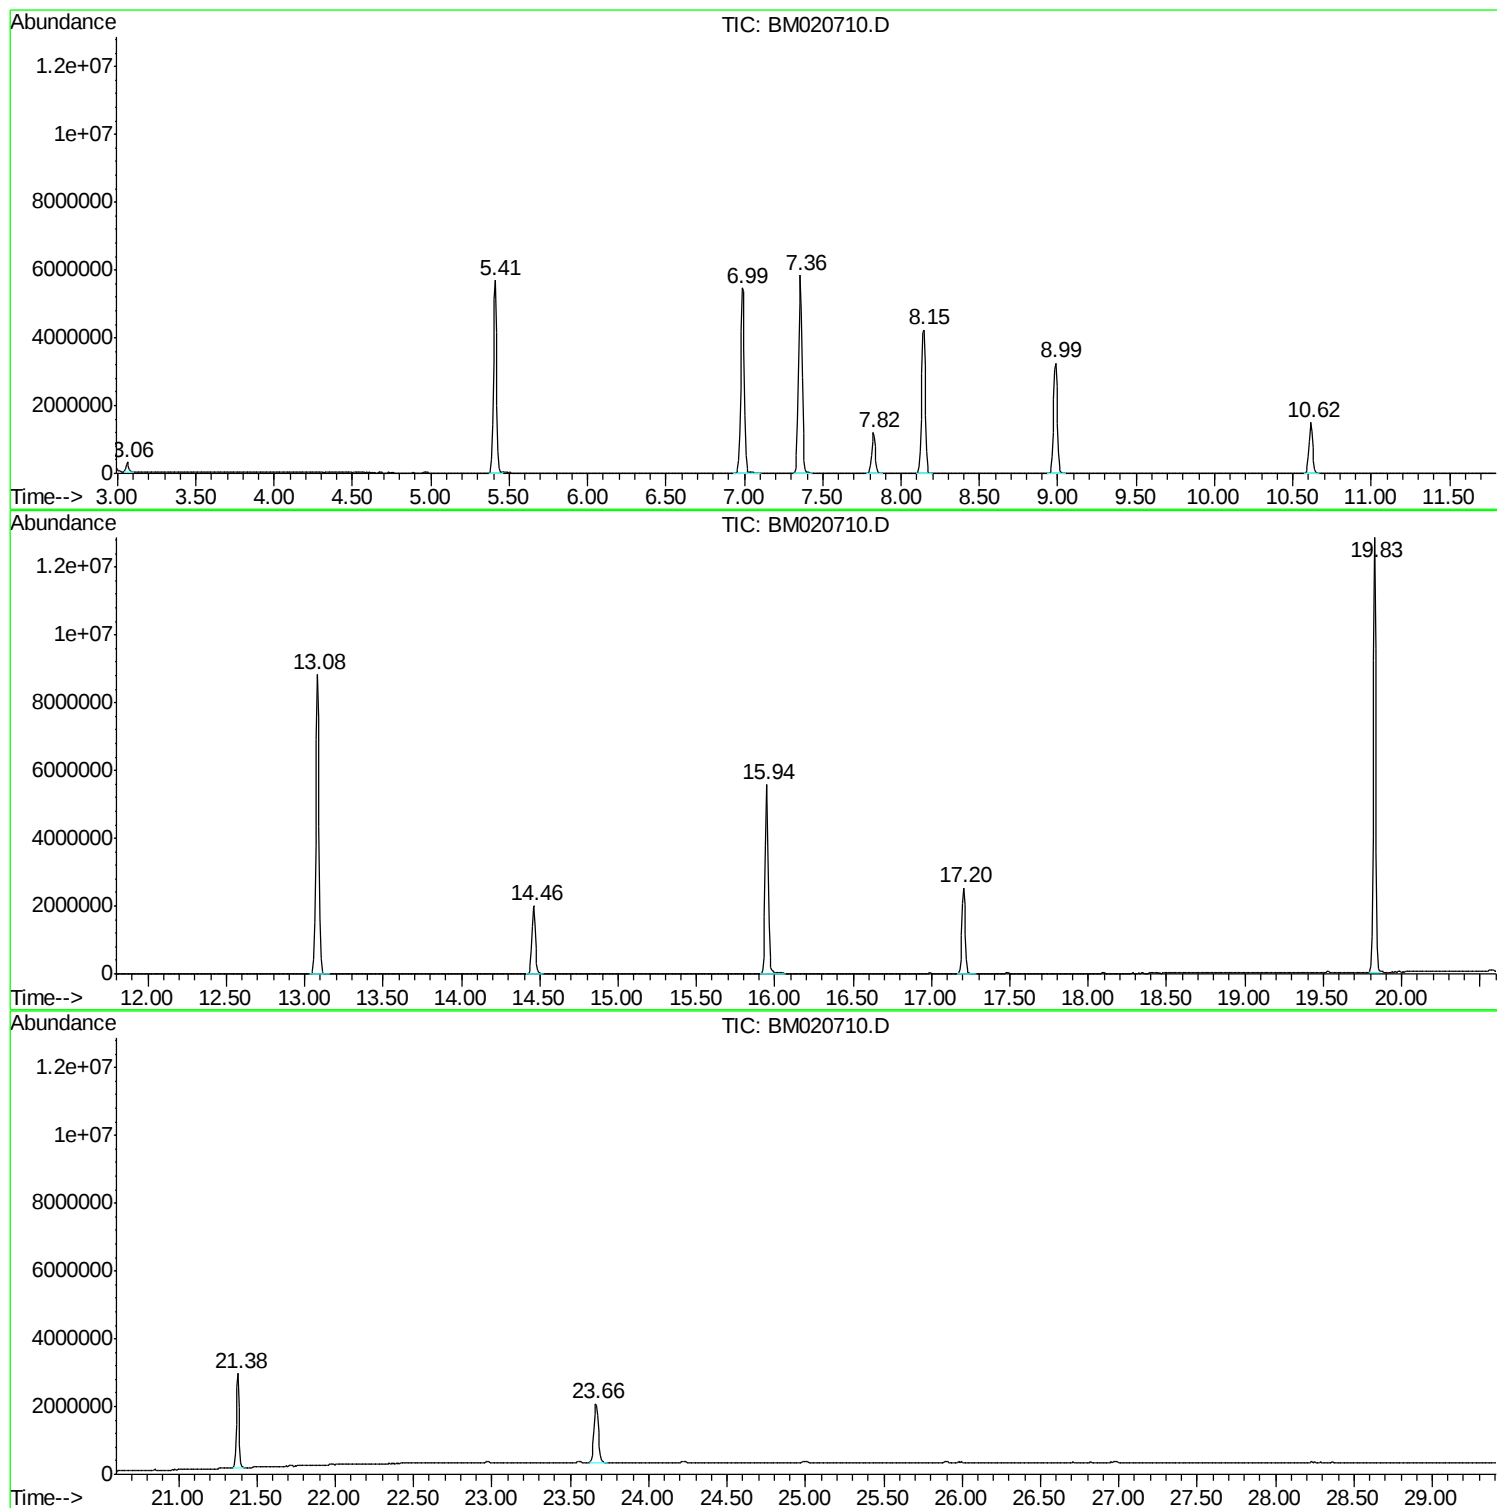

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020710.D
Acq On : 04 Jun 2019 19:25
Operator : HP/JU
Sample : PB120137BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120137BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	3.33 ng	315683	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5		N-Ethylformamide	73	C3H7NO	000627-45-2	9

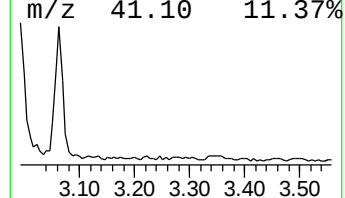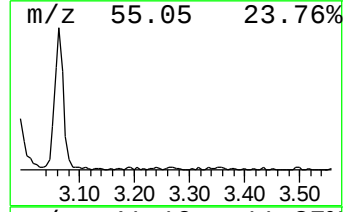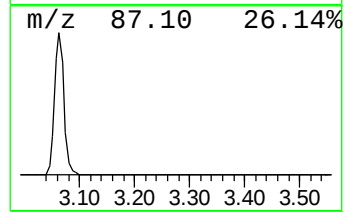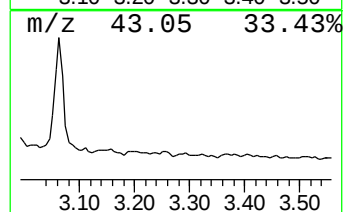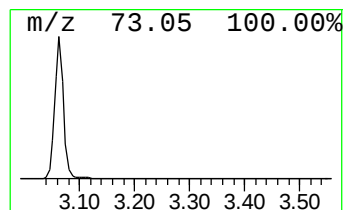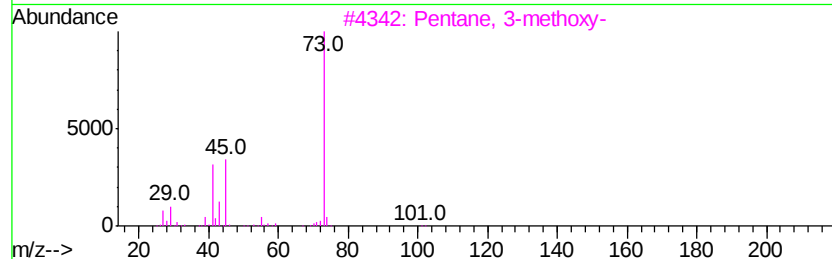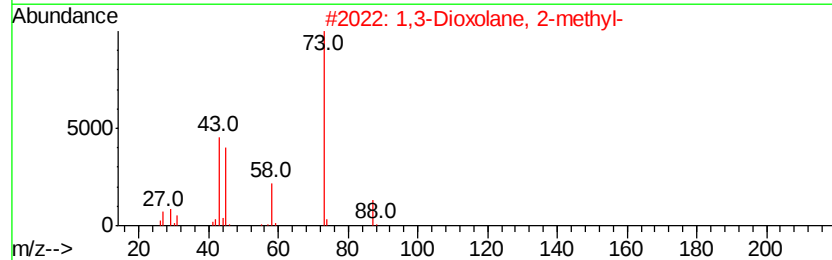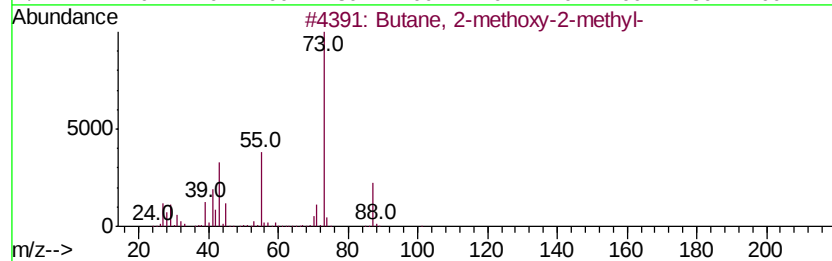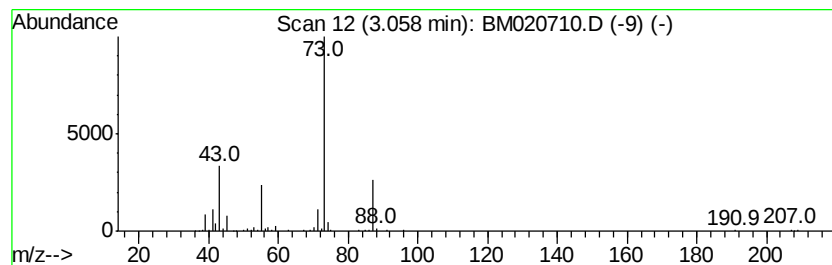

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020710.D
Acq On : 04 Jun 2019 19:25
Operator : HP/JU
Sample : PB120137BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120137BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	95.49 ng	9043280	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Xenon	132	Xe	007440-63-3	9

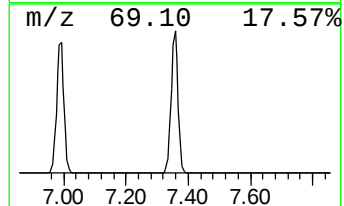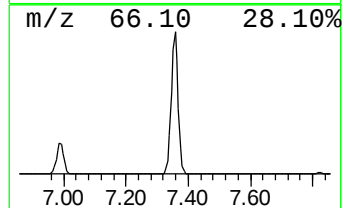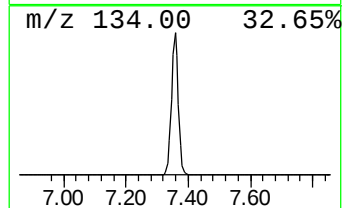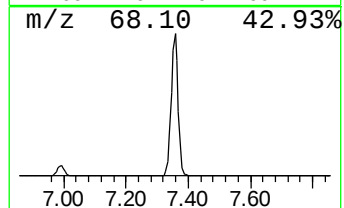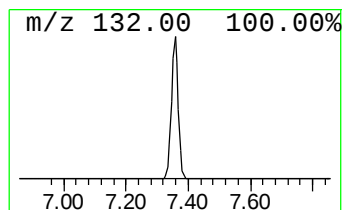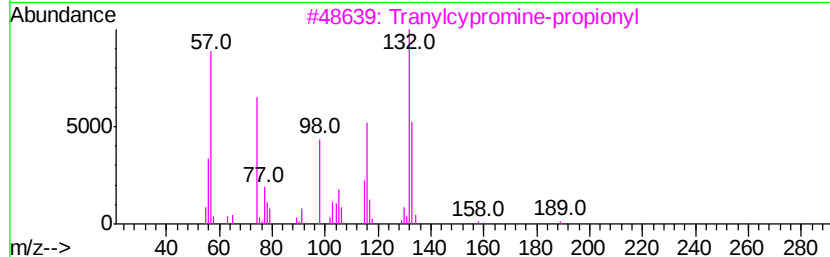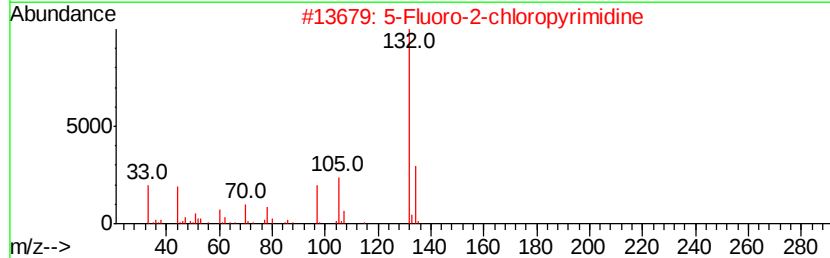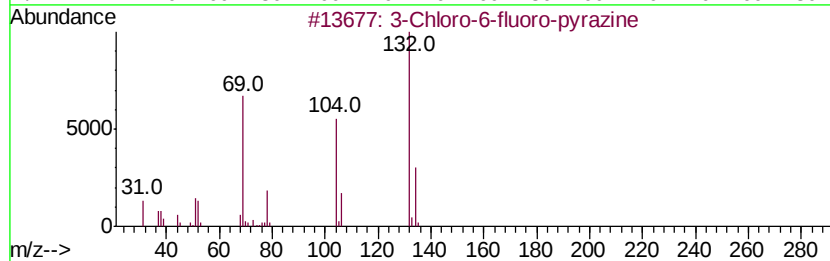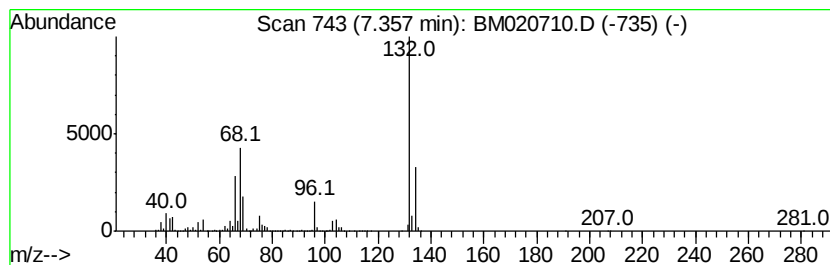

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060419\
Data File : BM020710.D
Acq On : 04 Jun 2019 19:25
Operator : HP/JU
Sample : PB120137BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120137BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	3.3	ng	315683	1	7.82	1894120	20.0
unknown7.36	7.36	95.5	ng	9043280	1	7.82	1894120	20.0