

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
 Data File : BM020718.D
 Acq On : 05 Jun 2019 02:05
 Operator : HP/JU
 Sample : PB120308BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120308BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	9	13	20	rVB	133181	159742	1.26%	0.189%
2	5.410	405	412	425	rBV	5460170	7770160	61.39%	9.178%
3	6.987	672	680	692	rBV	5311354	8414335	66.48%	9.938%
4	7.357	735	743	757	rBV	5422869	8561851	67.65%	10.113%
5	7.822	815	822	831	rVB	1173568	1845298	14.58%	2.180%
6	8.139	867	876	884	rBV	4000096	6569195	51.90%	7.759%
7	8.986	1012	1020	1032	rBV	3001720	5087019	40.19%	6.008%
8	10.616	1289	1297	1306	rBV	1443266	2424832	19.16%	2.864%
9	13.080	1709	1716	1728	rBV	7947303	11374645	89.87%	13.435%
10	14.457	1943	1950	1962	rBV2	1889059	2949133	23.30%	3.483%
11	15.945	2197	2203	2228	rBV	4744713	7071167	55.87%	8.352%
12	17.204	2410	2417	2431	rBV2	2234287	3178432	25.11%	3.754%
13	19.827	2857	2863	2868	rBV	10584234	12656928	100.00%	14.949%
14	21.374	3121	3126	3136	rBV	2431964	3205061	25.32%	3.786%
15	23.662	3508	3515	3524	rBV2	1780623	3397110	26.84%	4.012%


Sum of corrected areas: 84664908

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020718.D
Acq On : 05 Jun 2019 02:05
Operator : HP/JU
Sample : PB120308BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120308BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

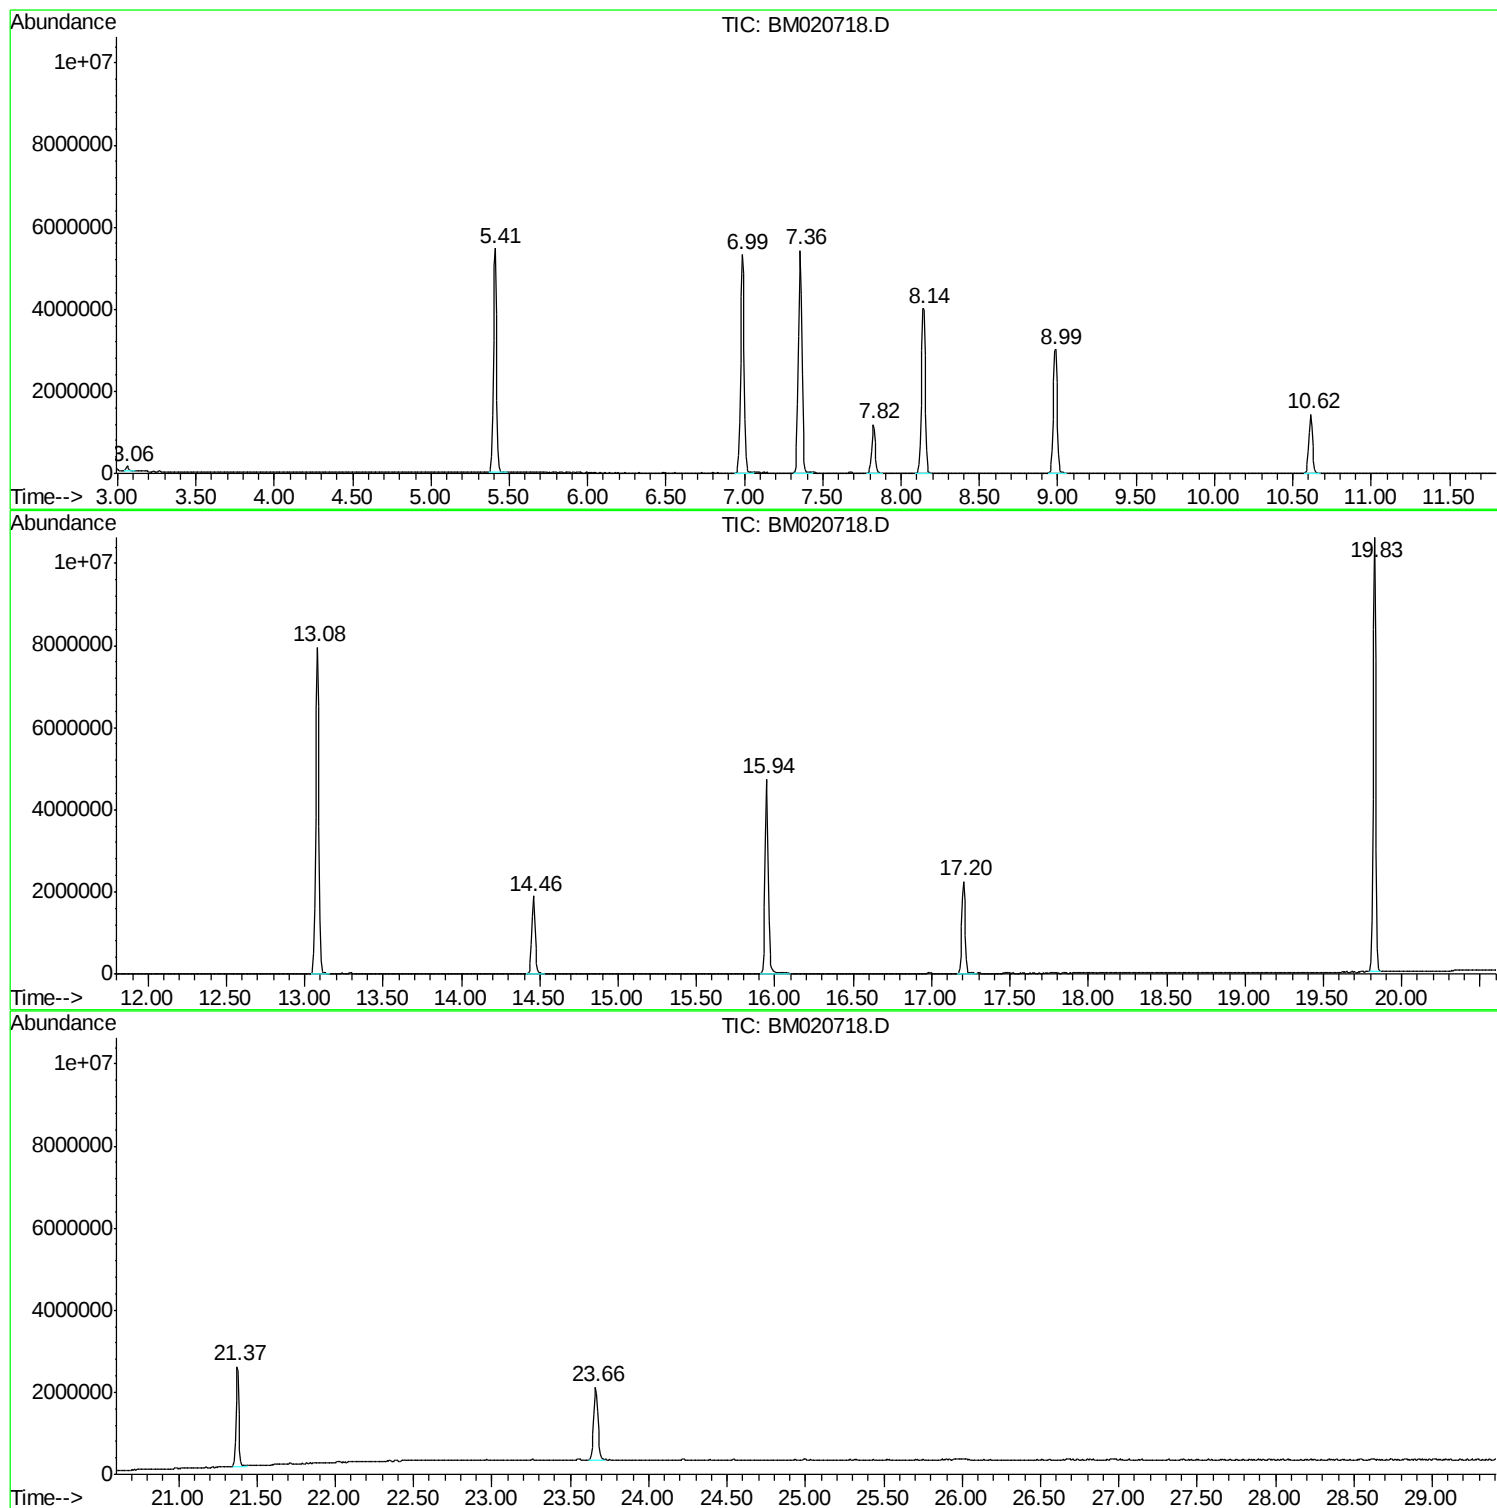

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
Data File : BM020718.D
Acq On : 05 Jun 2019 02:05
Operator : HP/JU
Sample : PB120308BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120308BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.36 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.36	92.80 ng	8561850	1,4-Dichlorobenzene-d4	7.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

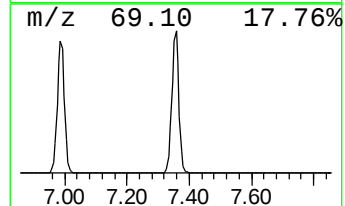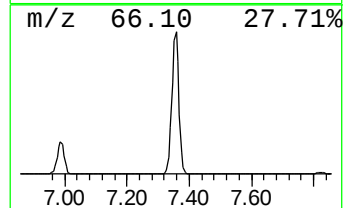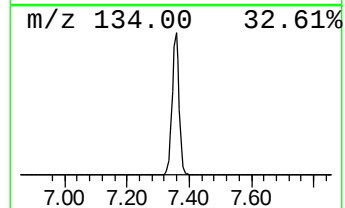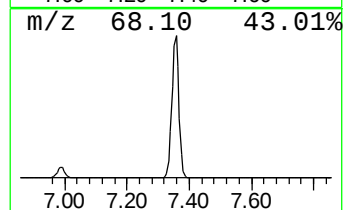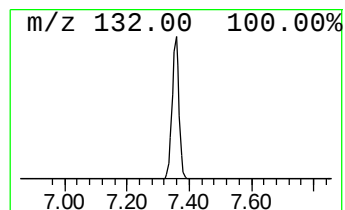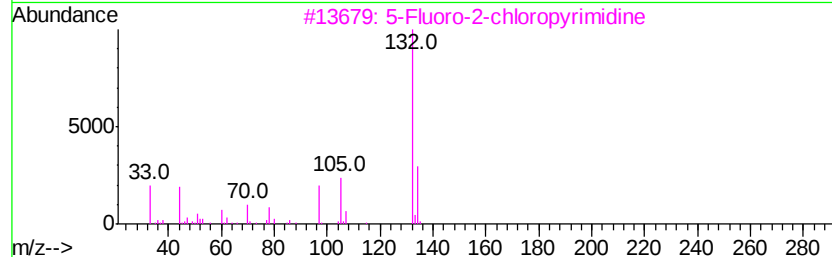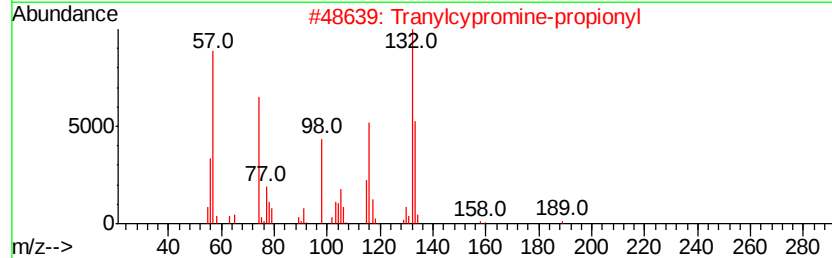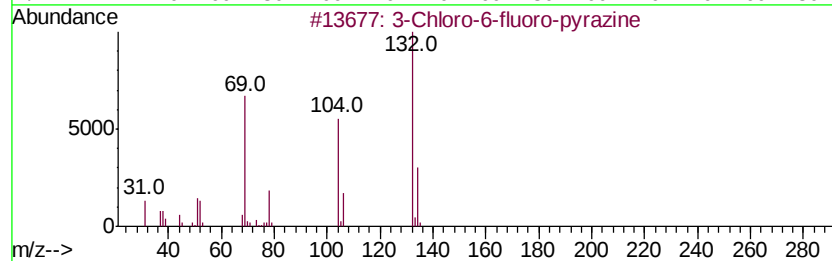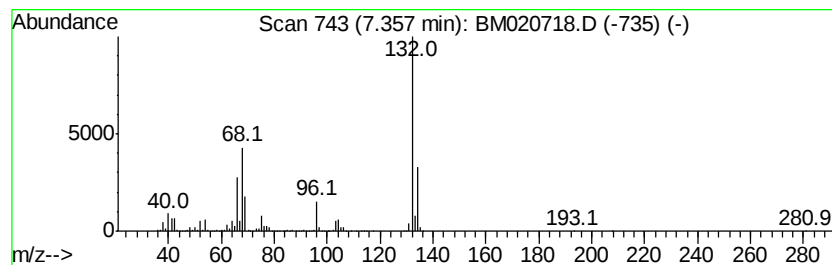

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060419\
Data File : BM020718.D
Acq On : 05 Jun 2019 02:05
Operator : HP/JU
Sample : PB120308BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120308BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.36	7.36	92.8	ng	8561850	1	7.82	1845300	20.0