


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060419\
 Data File : BM020715.D
 Acq On : 04 Jun 2019 23:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM053119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 31 15:48:49 2019

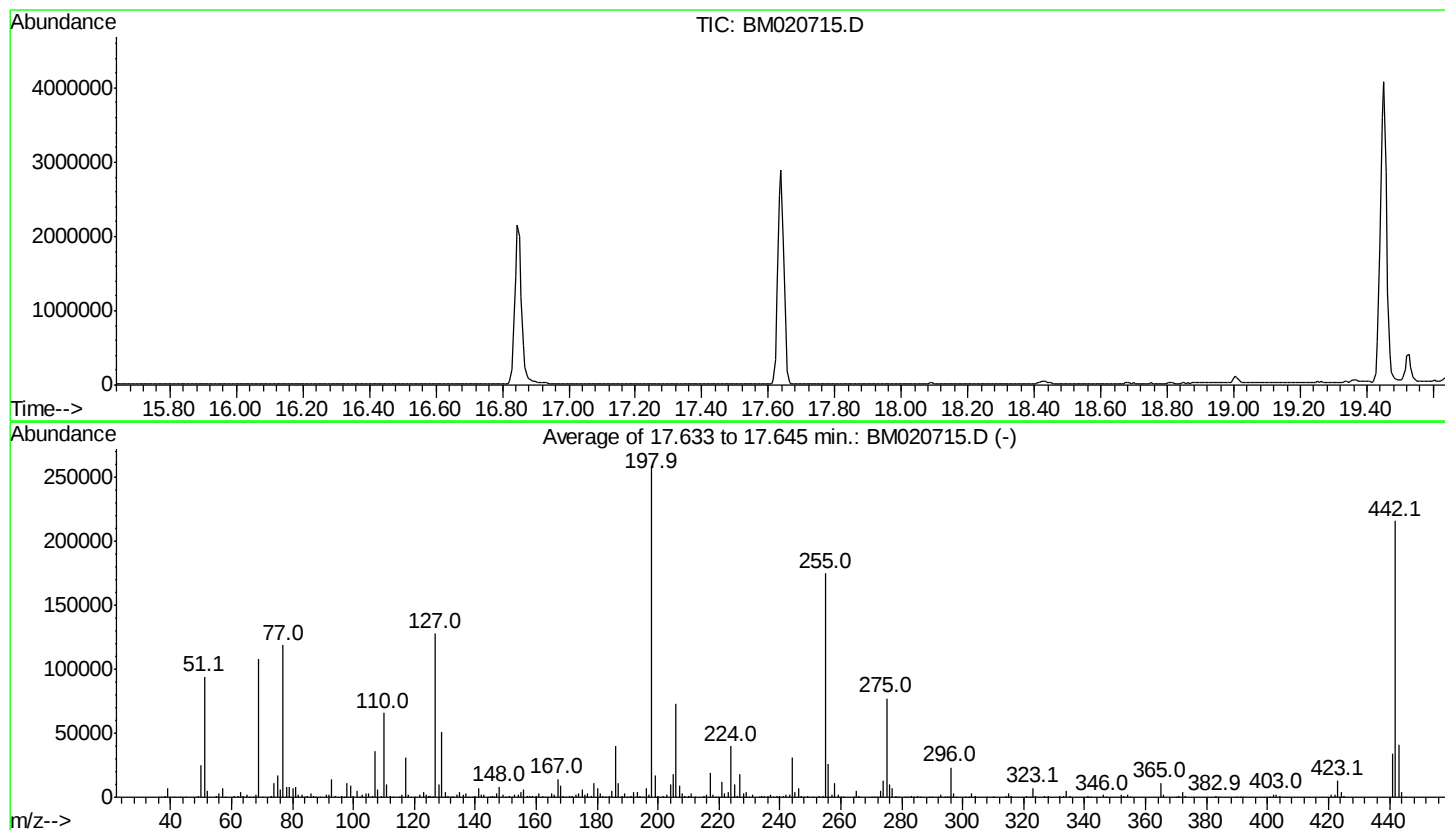

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	94464	PASS
68	69	0.00	2	1.8	1991	PASS
69	198	0.00	100	41.6	107856	PASS
70	69	0.00	2	0.5	513	PASS
127	198	10	80	49.3	127944	PASS
197	198	0.00	2	0.7	1788	PASS
198	198	100	100	100.0	259306	PASS
199	198	5	9	6.6	17184	PASS
275	198	10	60	29.9	77589	PASS
365	198	1	100	4.3	11087	PASS
441	198	0.01	100	13.2	34165	PASS
442	198	50	100	83.4	216149	PASS
443	442	15	24	19.0	41037	PASS