
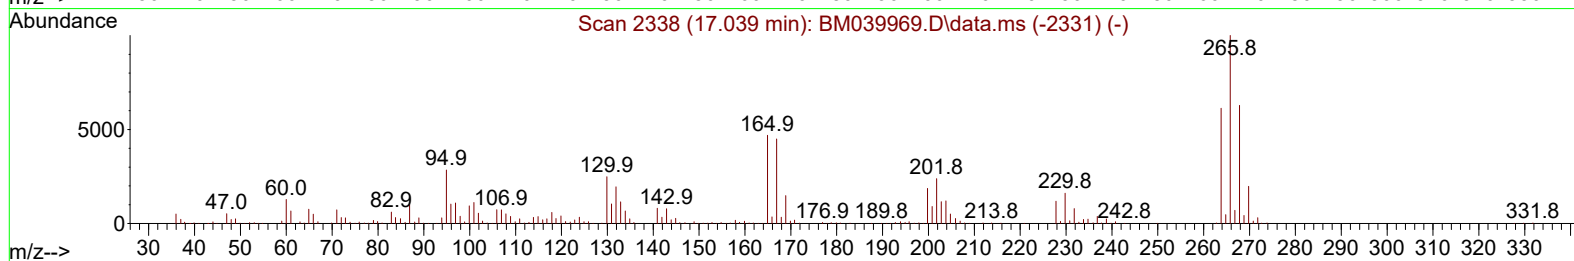
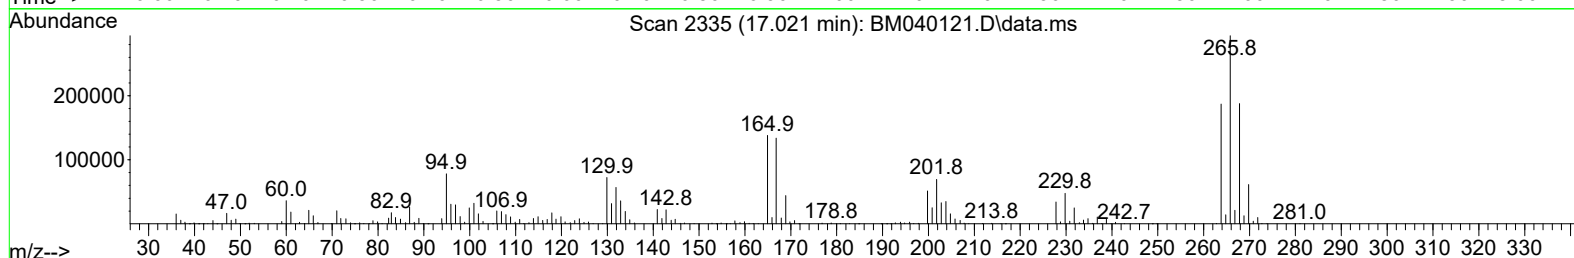


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040121.D
Acq On : 07 Jun 2023 02:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:55:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 16:45:42 2023
Response via : Initial Calibration

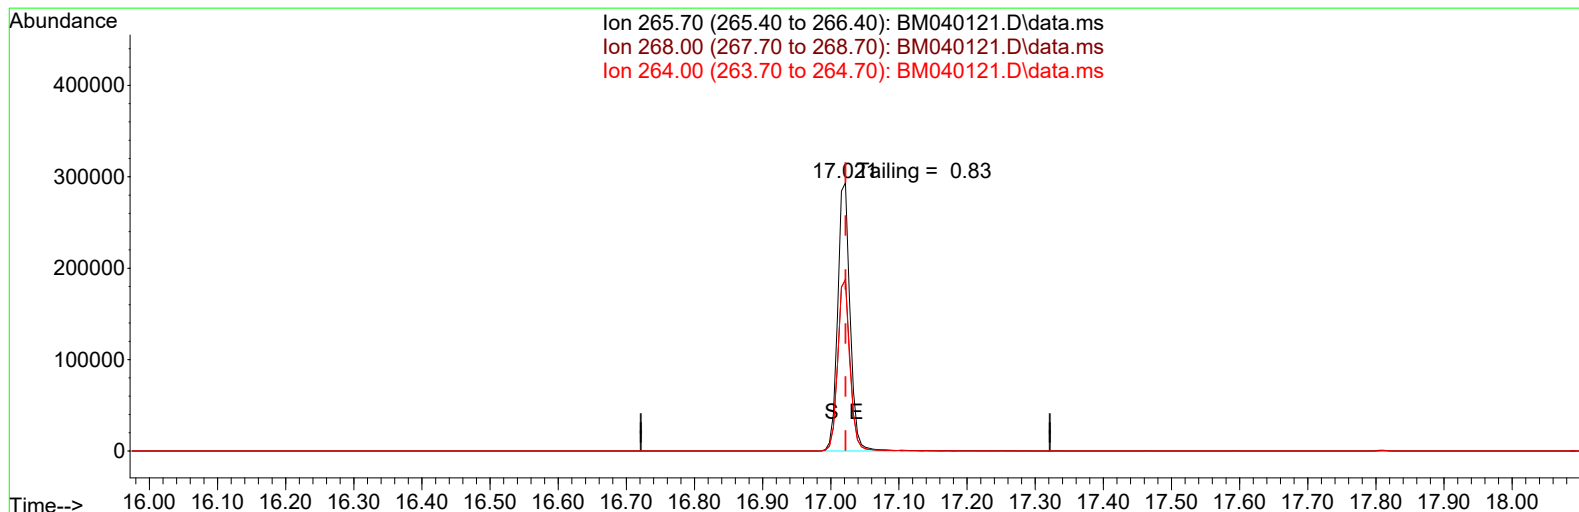

TIC: BM040121.D\data.ms

(70) Pentachlorophenol (C)




17.021min (-0.000) 241738.94 ng

response 370709

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.93
264.00	61.30	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
 Data File : BM040121.D
 Acq On : 07 Jun 2023 02:16
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 07:55:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 06 16:45:42 2023
 Response via : Initial Calibration

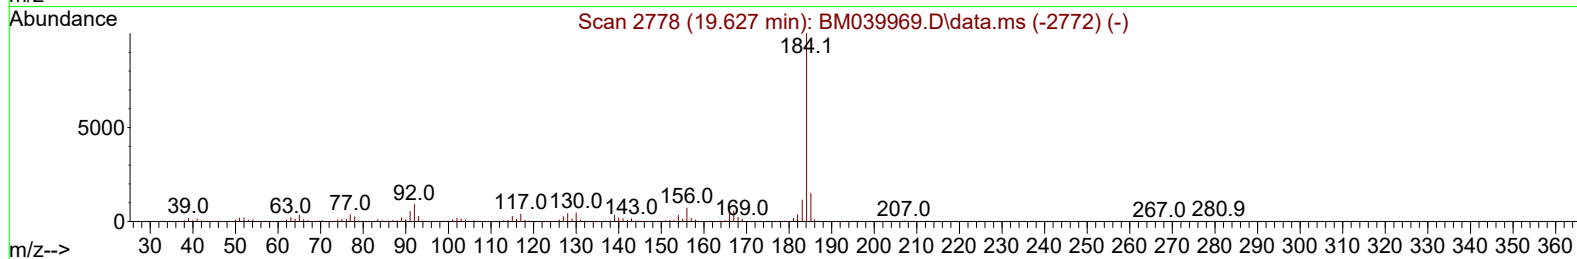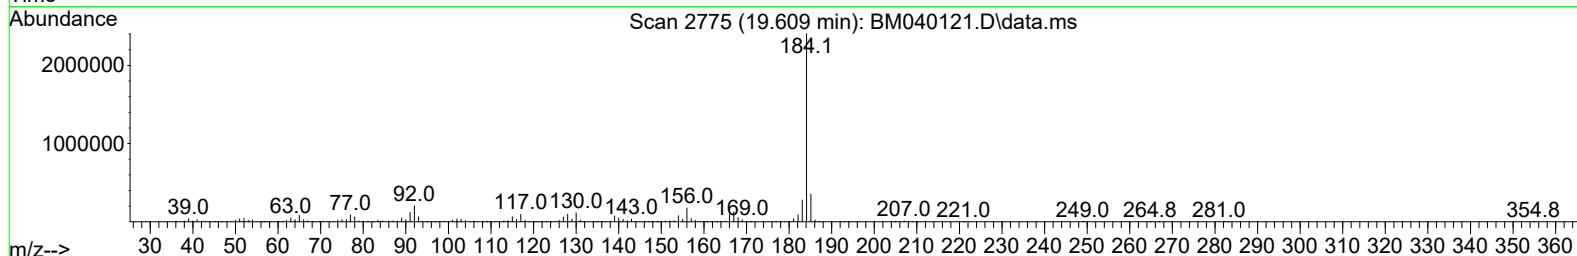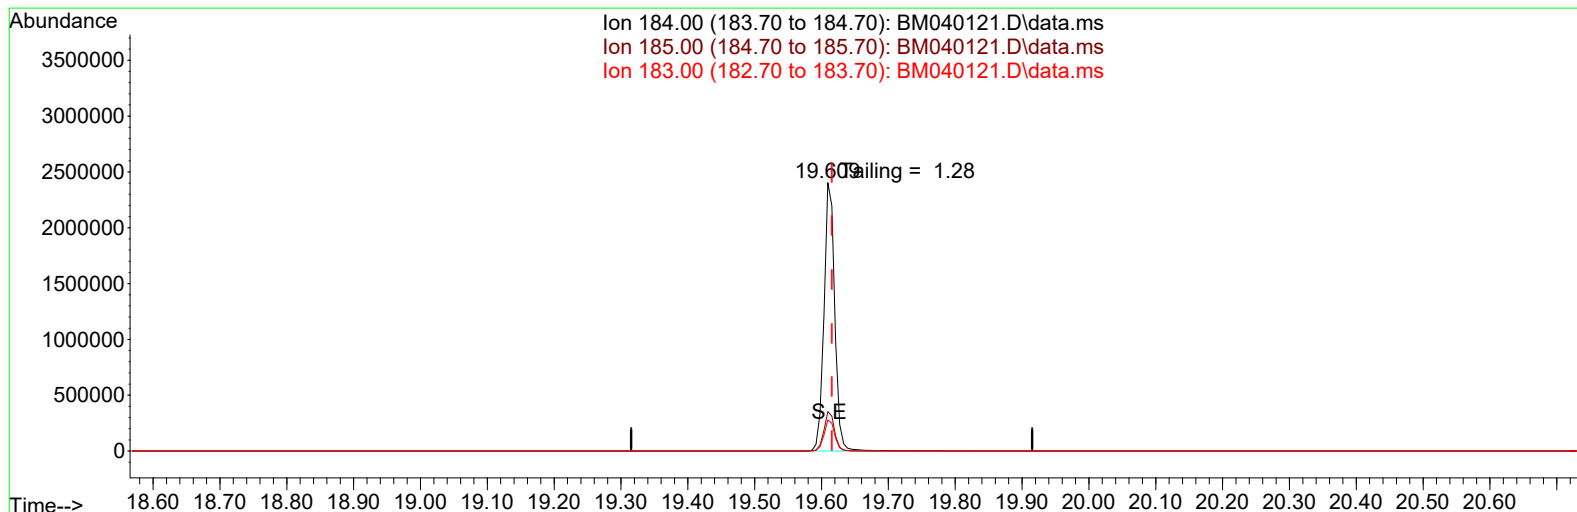

TIC: BM040121.D\data.ms

(77) Benzidine**19.609min (-0.006) 608261.05 ng****response 2692006**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.71
183.00	11.50	11.61
0.00	0.00	0.00