

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
 Data File : BM040104.D
 Acq On : 06 Jun 2023 15:16
 Operator : MA/JU
 Sample : PB153183BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153183BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	377	384	399	rBV	6583382	9269216	41.41%	9.954%
2	7.157	649	658	671	rBV	5948264	9614222	42.95%	10.324%
3	7.992	794	800	812	rBV	1170501	1857698	8.30%	1.995%
4	9.163	991	999	1010	rBV	3613551	5756572	25.72%	6.182%
5	10.810	1271	1279	1288	rBV	1732891	2794990	12.49%	3.001%
6	13.263	1688	1696	1712	rBV	10259309	14631511	65.37%	15.712%
7	14.633	1922	1929	1937	rBV	2620583	3727393	16.65%	4.003%
8	16.115	2174	2181	2203	rBV	7965806	11039584	49.32%	11.855%
9	17.374	2389	2395	2405	rVB	3214900	4303404	19.23%	4.621%
10	19.992	2834	2840	2854	rBV	18414538	22382760	100.00%	24.035%
11	21.550	3100	3105	3116	rBV	3427579	4098335	18.31%	4.401%
12	23.991	3513	3520	3530	rVB	1829491	3648285	16.30%	3.918%




Sum of corrected areas: 93123970

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040104.D
Acq On : 06 Jun 2023 15:16
Operator : MA/JU
Sample : PB153183BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153183BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

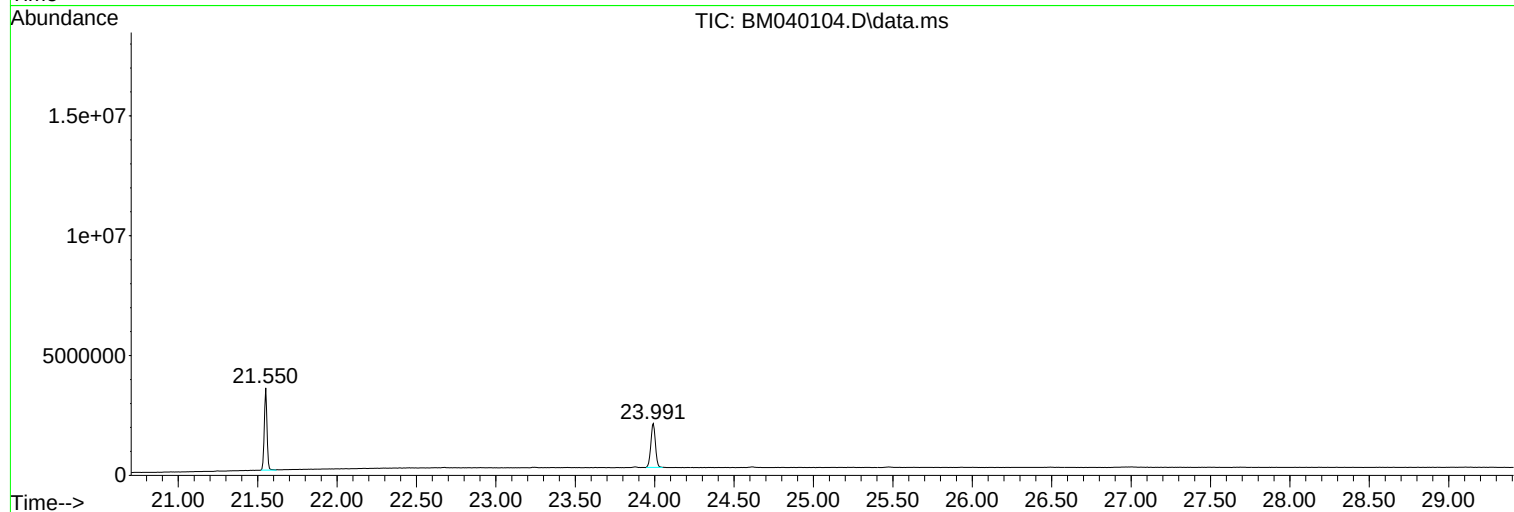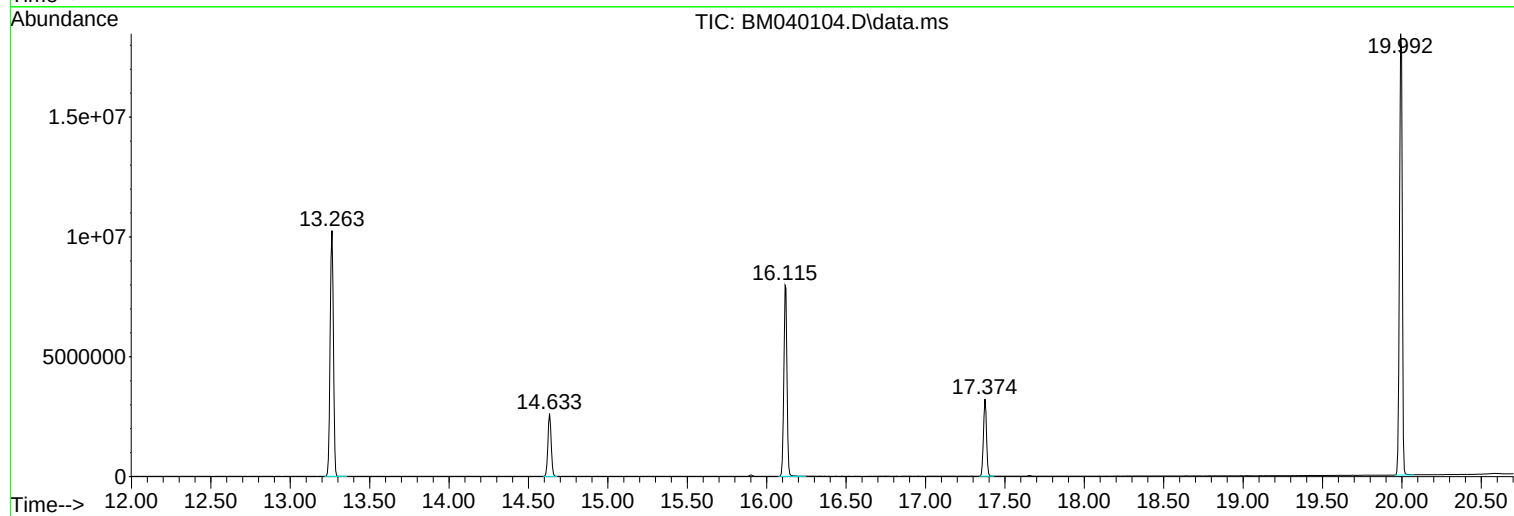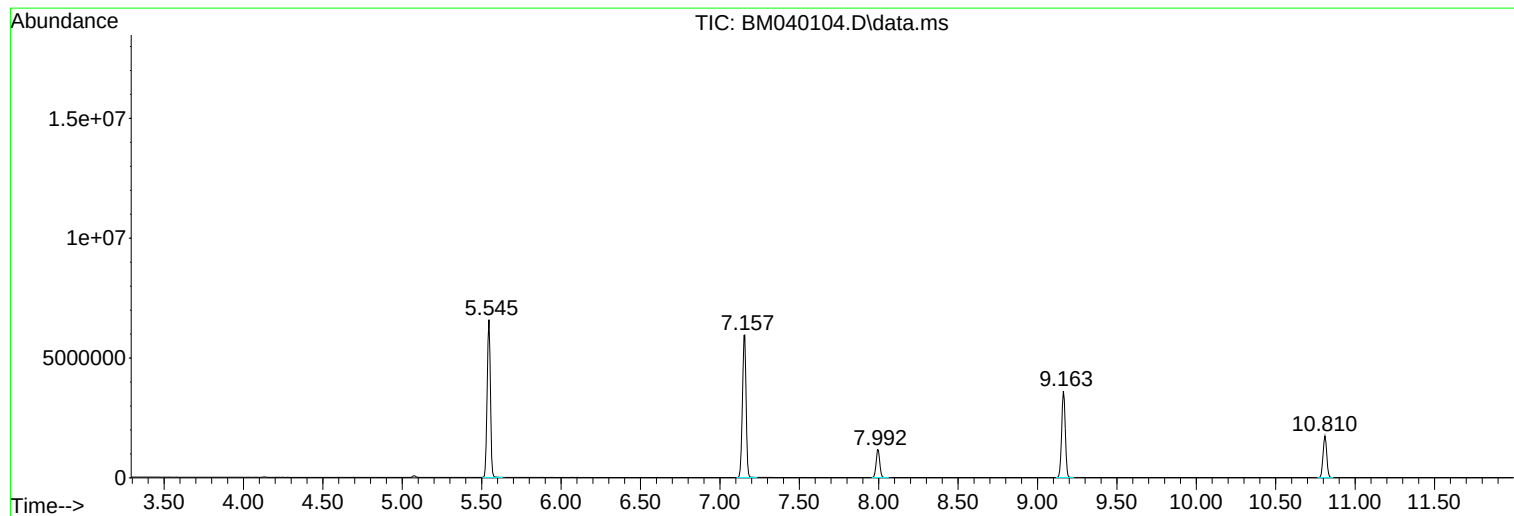

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040104.D
Acq On : 06 Jun 2023 15:16
Operator : MA/JU
Sample : PB153183BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153183BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040104.D
Acq On : 06 Jun 2023 15:16
Operator : MA/JU
Sample : PB153183BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153183BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------