

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040111.D
Acq On : 06 Jun 2023 19:35
Operator : MA/JU
Sample : PB153150TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153150TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	377	384	396	rBV	5520182	7897673	39.01%	9.913%
2	7.151	648	657	677	rBV	5289142	8305904	41.03%	10.425%
3	7.993	794	800	814	rVB	966230	1480412	7.31%	1.858%
4	9.163	990	999	1014	rBV	3018793	4833784	23.88%	6.067%
5	10.810	1271	1279	1291	rBV	1359617	2212073	10.93%	2.777%
6	13.263	1688	1696	1703	rBV	8731044	12183521	60.18%	15.293%
7	14.633	1922	1929	1939	rBV	2042302	2850052	14.08%	3.577%
8	16.116	2174	2181	2203	rBV	7285602	9338390	46.13%	11.721%
9	17.374	2388	2395	2402	rBV	2522412	3385683	16.72%	4.250%
10	19.992	2834	2840	2845	rBV	18153011	20245217	100.00%	25.411%
11	21.550	3099	3105	3115	rBV	2887923	3528513	17.43%	4.429%
12	23.991	3513	3520	3533	rVB	1735838	3408487	16.84%	4.278%




Sum of corrected areas: 79669709

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040111.D
Acq On : 06 Jun 2023 19:35
Operator : MA/JU
Sample : PB153150TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153150TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

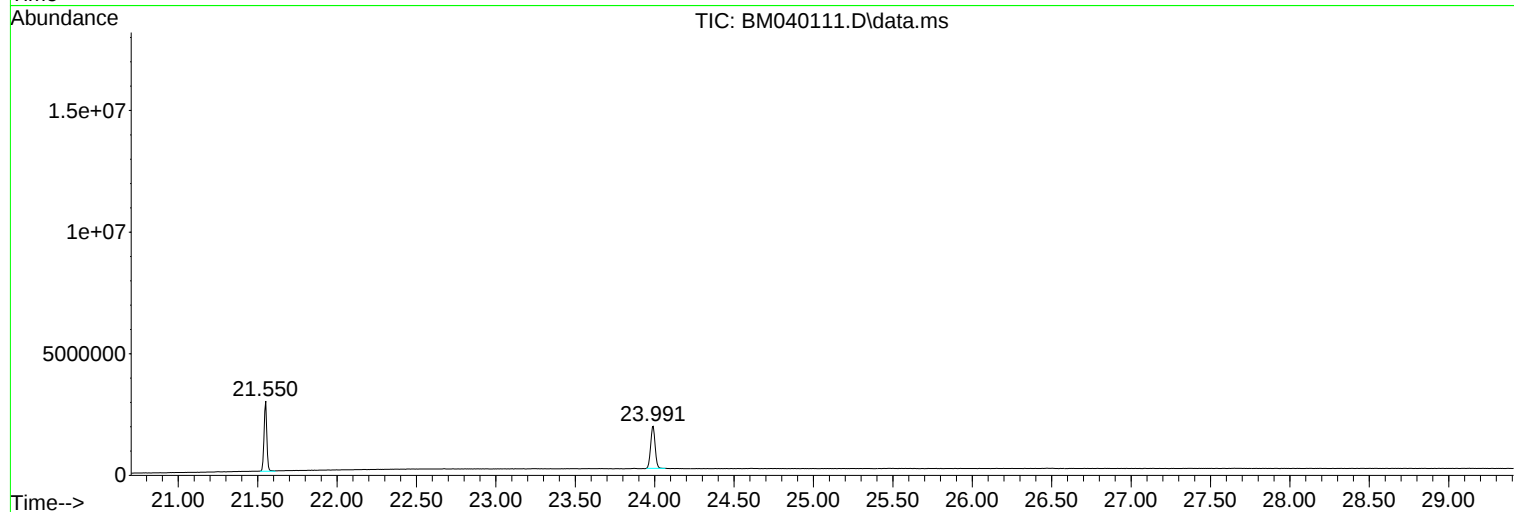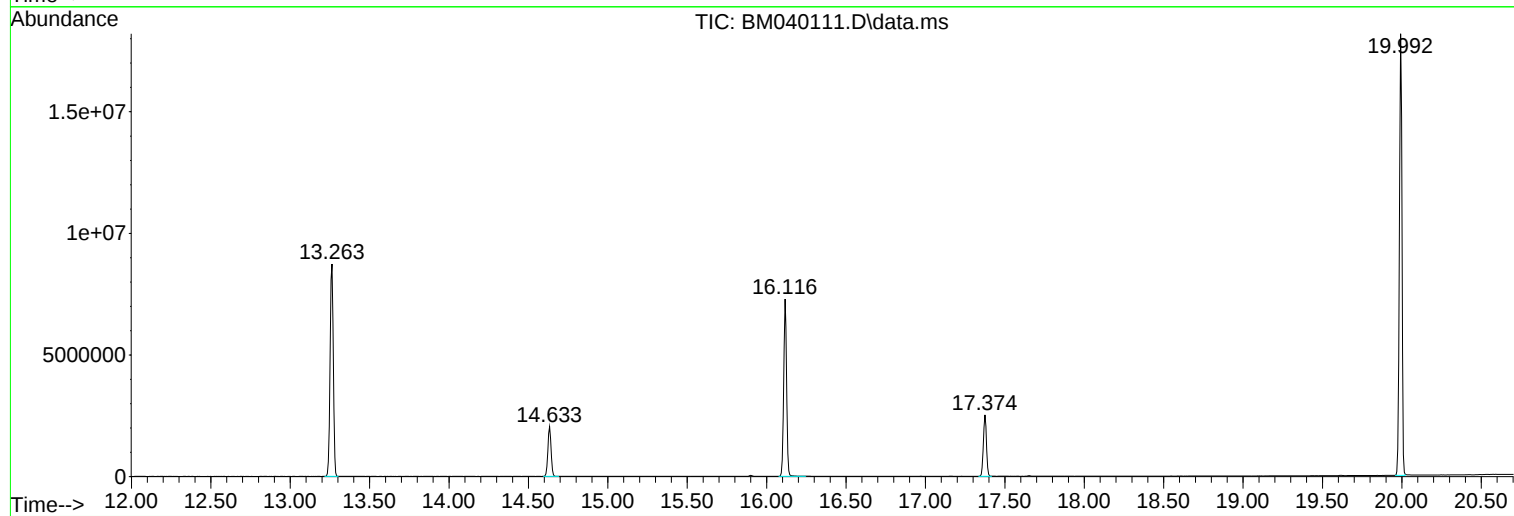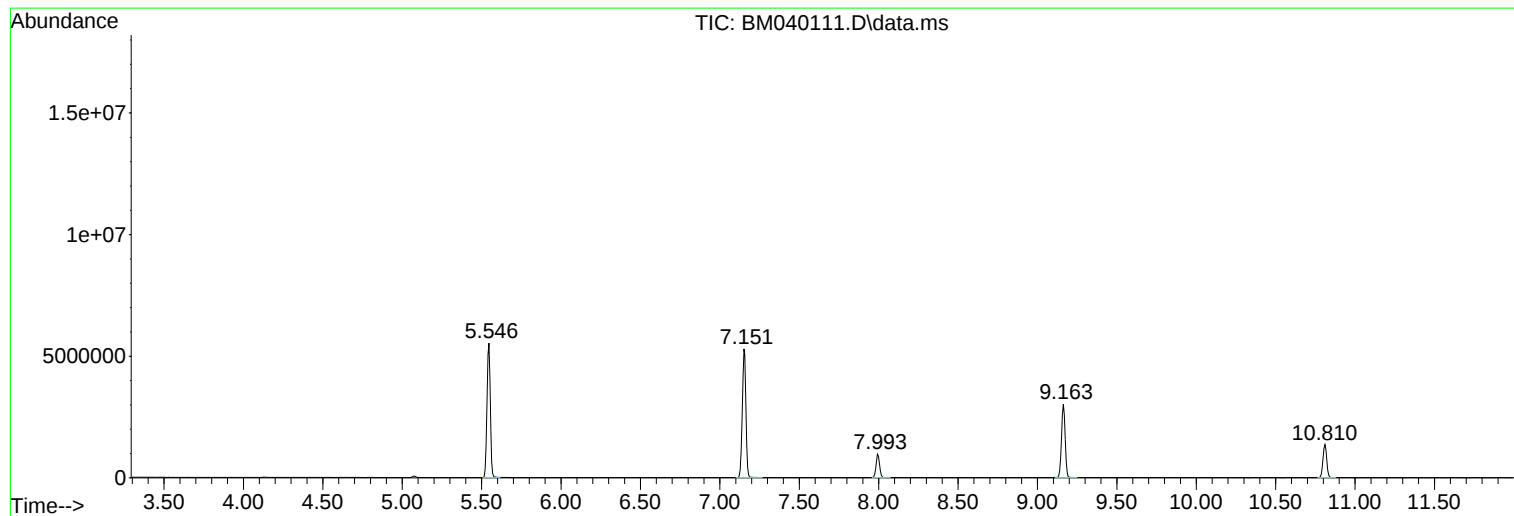

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040111.D
Acq On : 06 Jun 2023 19:35
Operator : MA/JU
Sample : PB153150TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153150TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040111.D
Acq On : 06 Jun 2023 19:35
Operator : MA/JU
Sample : PB153150TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153150TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------