

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040123.D
Acq On : 07 Jun 2023 04:04
Operator : MA/JU
Sample : PB153204BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153204BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	400	rBV	6215260	8963051	43.51%	10.861%
2	7.151	649	657	668	rBV	6103010	9280353	45.05%	11.246%
3	7.992	793	800	810	rBV	1039822	1591381	7.72%	1.928%
4	9.163	988	999	1010	rBV	3250110	5280567	25.63%	6.399%
5	10.804	1269	1278	1289	rBV	1365679	2284810	11.09%	2.769%
6	13.257	1688	1695	1702	rBV	9448423	12763297	61.96%	15.467%
7	14.627	1921	1928	1938	rBV	1991504	2771833	13.45%	3.359%
8	16.115	2174	2181	2198	rBV	7735200	9643660	46.81%	11.686%
9	17.374	2388	2395	2402	rBV	2377605	3203674	15.55%	3.882%
10	19.992	2834	2840	2845	rBV	18245592	20600837	100.00%	24.964%
11	21.544	3099	3104	3113	rBV	2649393	3121007	15.15%	3.782%
12	23.985	3512	3519	3532	rVB	1604617	3016982	14.64%	3.656%




Sum of corrected areas: 82521452

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040123.D
Acq On : 07 Jun 2023 04:04
Operator : MA/JU
Sample : PB153204BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153204BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

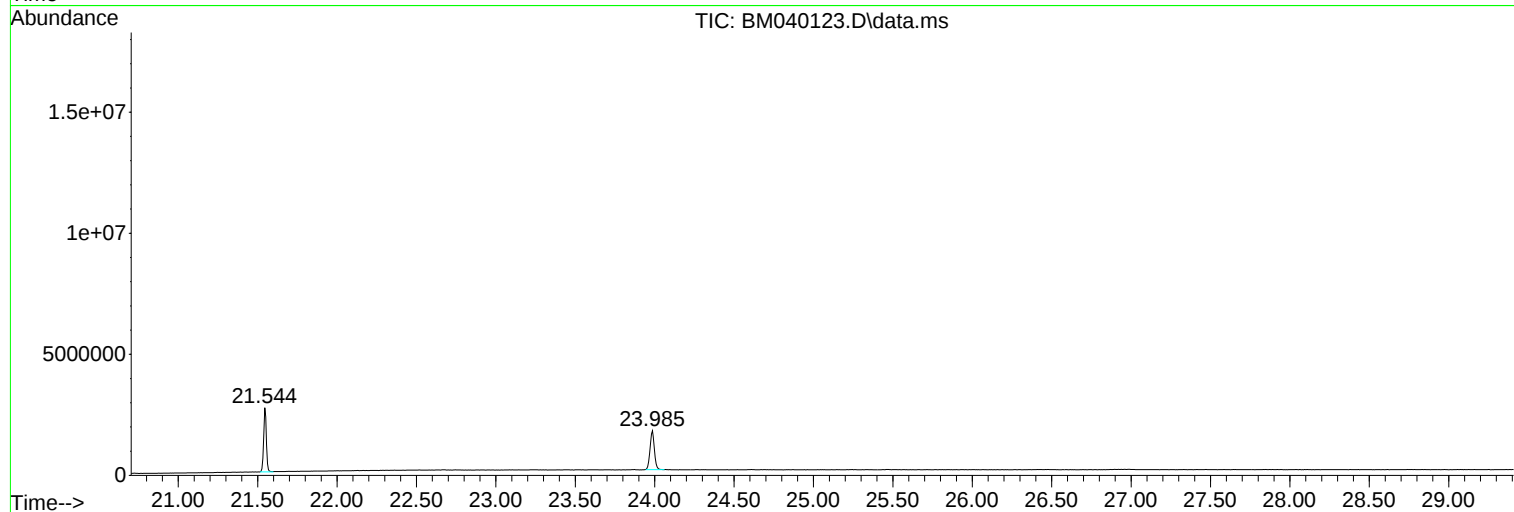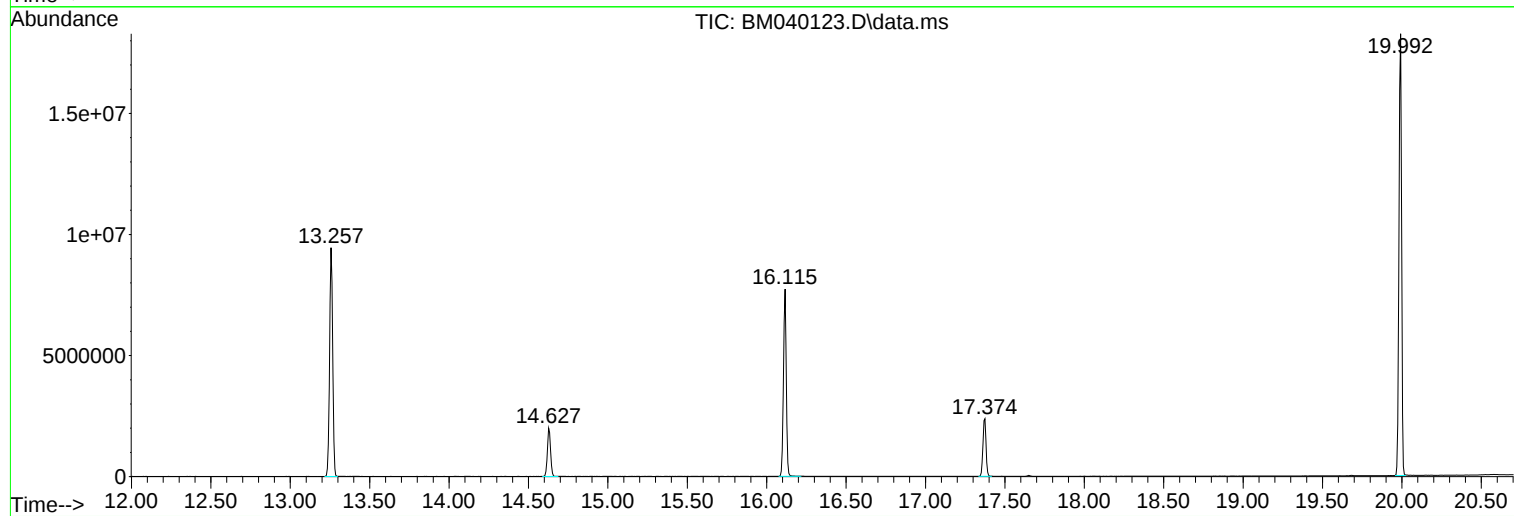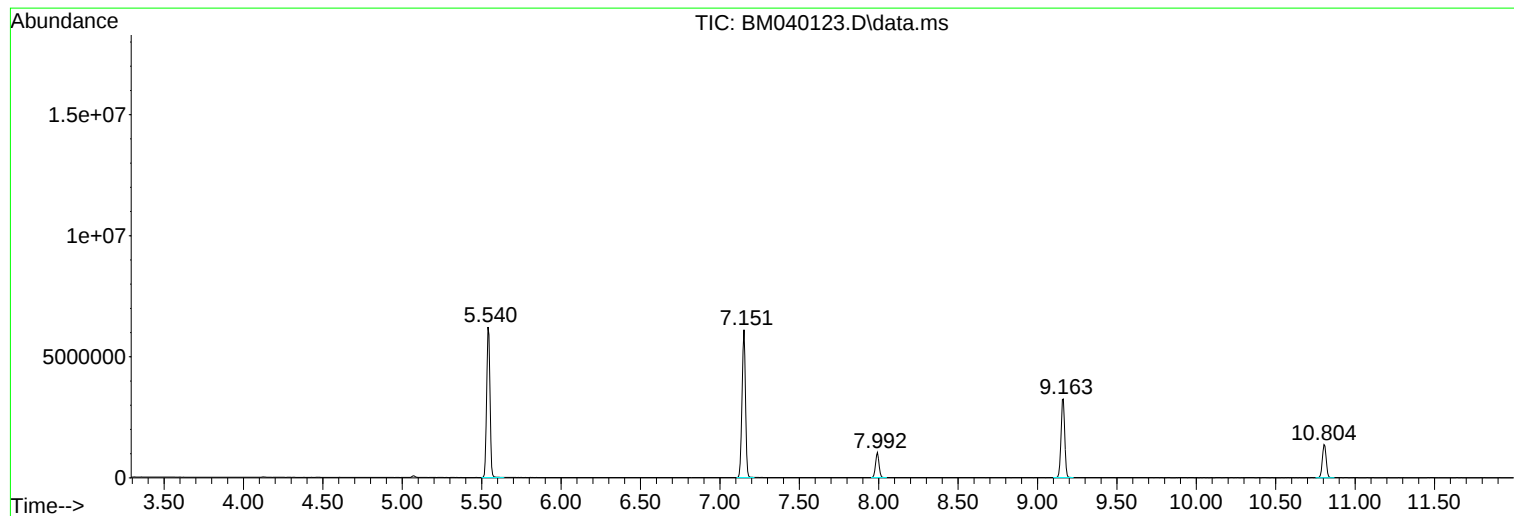

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040123.D
Acq On : 07 Jun 2023 04:04
Operator : MA/JU
Sample : PB153204BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153204BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
Data File : BM040123.D
Acq On : 07 Jun 2023 04:04
Operator : MA/JU
Sample : PB153204BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153204BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------