


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
 Data File : BM040102.D
 Acq On : 06 Jun 2023 13:27
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 16:45:42 2023

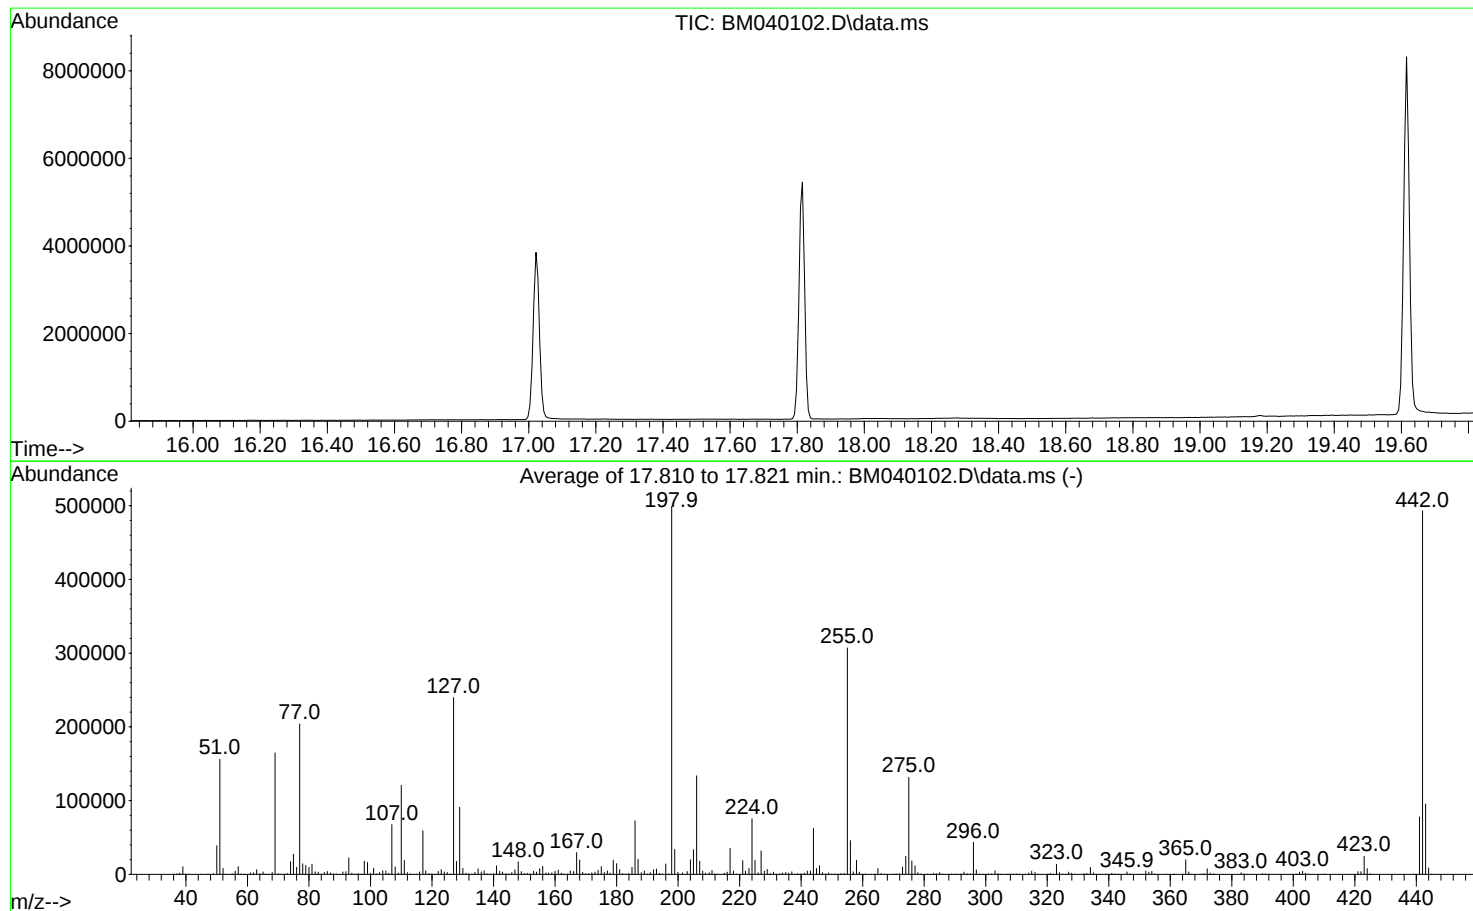

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	156090	PASS
68	69	0.00	2	1.6	2654	PASS
69	198	0.00	100	33.0	164633	PASS
70	69	0.00	2	0.6	936	PASS
127	198	10	80	48.1	239845	PASS
197	198	0.00	2	0.1	517	PASS
198	198	100	100	100.0	498944	PASS
199	198	5	9	6.8	33971	PASS
275	198	10	60	26.4	131565	PASS
365	198	1	100	4.0	19800	PASS
441	198	0.01	100	15.6	77893	PASS
442	442	50	100	100.0	493077	PASS
443	442	15	24	19.4	95560	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_M	<u>BM040102.D</u>
Compound Name	Response	Retention Time
DDT	1710004	20.851
DDD	21590	20.462
DDE	1029	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22619	1732623	1.31

Instrument :
BNA_M
ClientSampleId :
DFTPP