


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060623\
 Data File : BM040121.D
 Acq On : 07 Jun 2023 02:16
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 16:45:42 2023

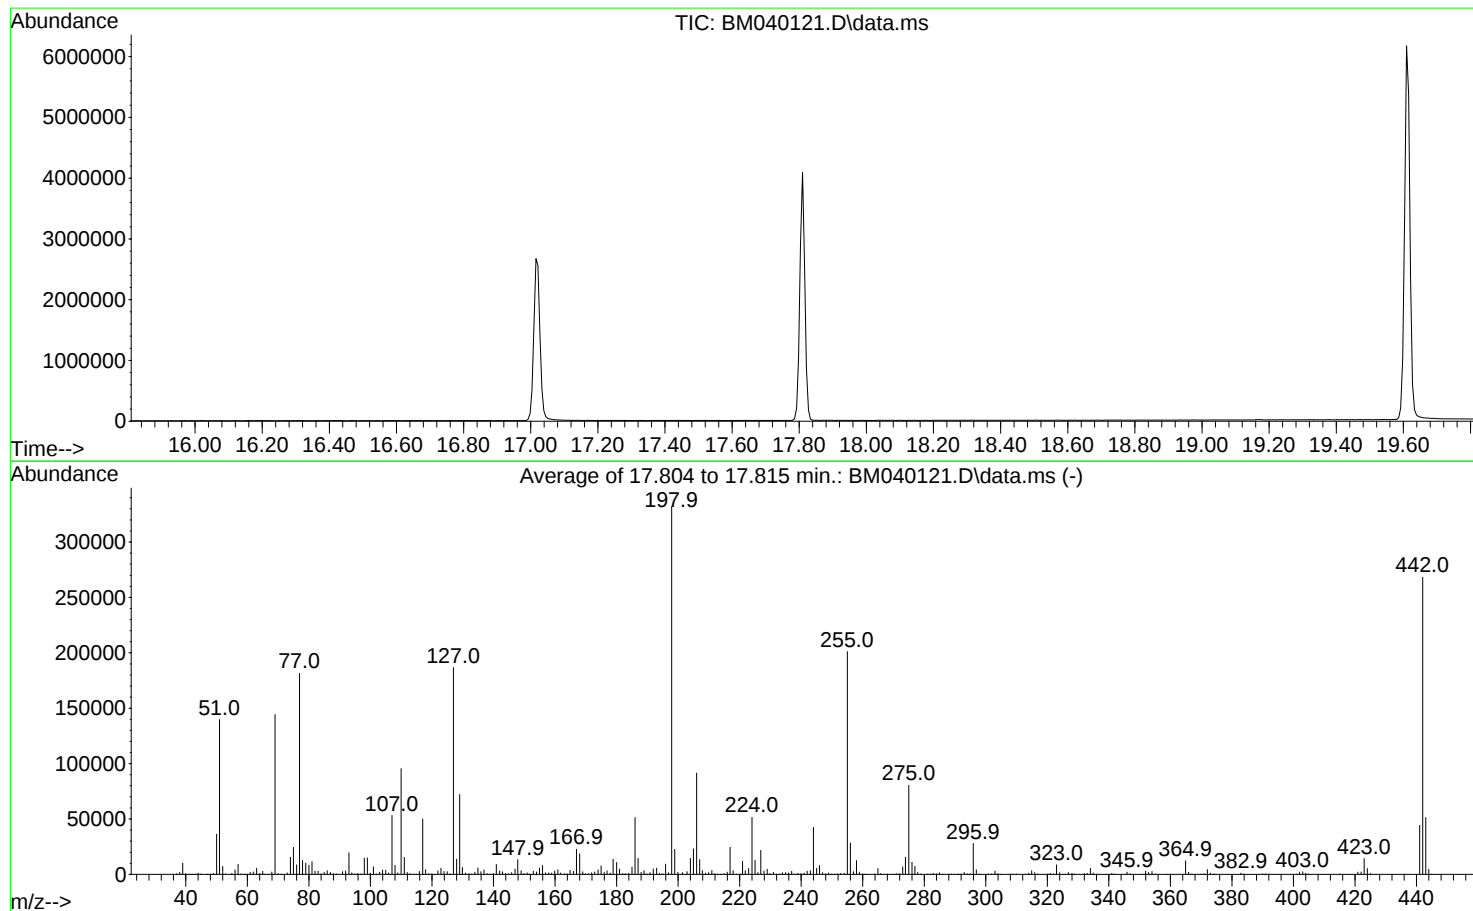

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	139649	PASS
68	69	0.00	2	1.5	2231	PASS
69	198	0.00	100	43.5	144371	PASS
70	69	0.00	2	0.5	734	PASS
127	198	10	80	56.2	186667	PASS
197	198	0.00	2	0.4	1411	PASS
198	198	100	100	100.0	332075	PASS
199	198	5	9	6.8	22595	PASS
275	198	10	60	24.2	80419	PASS
365	198	1	100	3.7	12288	PASS
441	198	0.01	100	13.3	44147	PASS
442	442	50	100	100.0	268224	PASS
443	442	15	24	19.1	51312	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_M	<u>BM040121.D</u>
Compound Name	Response	Retention Time
DDT	1061047	20.839
DDD	10463	20.404
DDE	1822	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12285	1073332	1.14

Instrument :
BNA_M
ClientSampleId :
DFTPP