

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
 Data File : BM050220.D
 Acq On : 06 Jun 2025 18:45
 Operator : RC/JU
 Sample : Q2207-45
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BU-703-COMP-05

Quant Time: Jun 07 01:19:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 16:20:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.786	152	278947	20.000	ng	0.00
21) Naphthalene-d8	10.574	136	1053754	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	580974	20.000	ng	0.00
64) Phenanthrene-d10	17.151	188	1052418	20.000	ng	0.00
76) Chrysene-d12	21.374	240	1021878	20.000	ng	-0.01
86) Perylene-d12	24.362	264	1123026	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	2077013	124.208	ng	0.00
7) Phenol-d6	6.951	99	2457262	111.628	ng	0.00
23) Nitrobenzene-d5	8.933	82	1624226	80.164	ng	-0.01
42) 2,4,6-Tribromophenol	15.892	330	827338	125.199	ng	-0.01
45) 2-Fluorobiphenyl	13.039	172	3222591	75.096	ng	-0.01
79) Terphenyl-d14	19.774	244	4418480	81.939	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050220.D
Acq On : 06 Jun 2025 18:45
Operator : RC/JU
Sample : Q2207-45
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-05

Quant Time: Jun 07 01:19:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

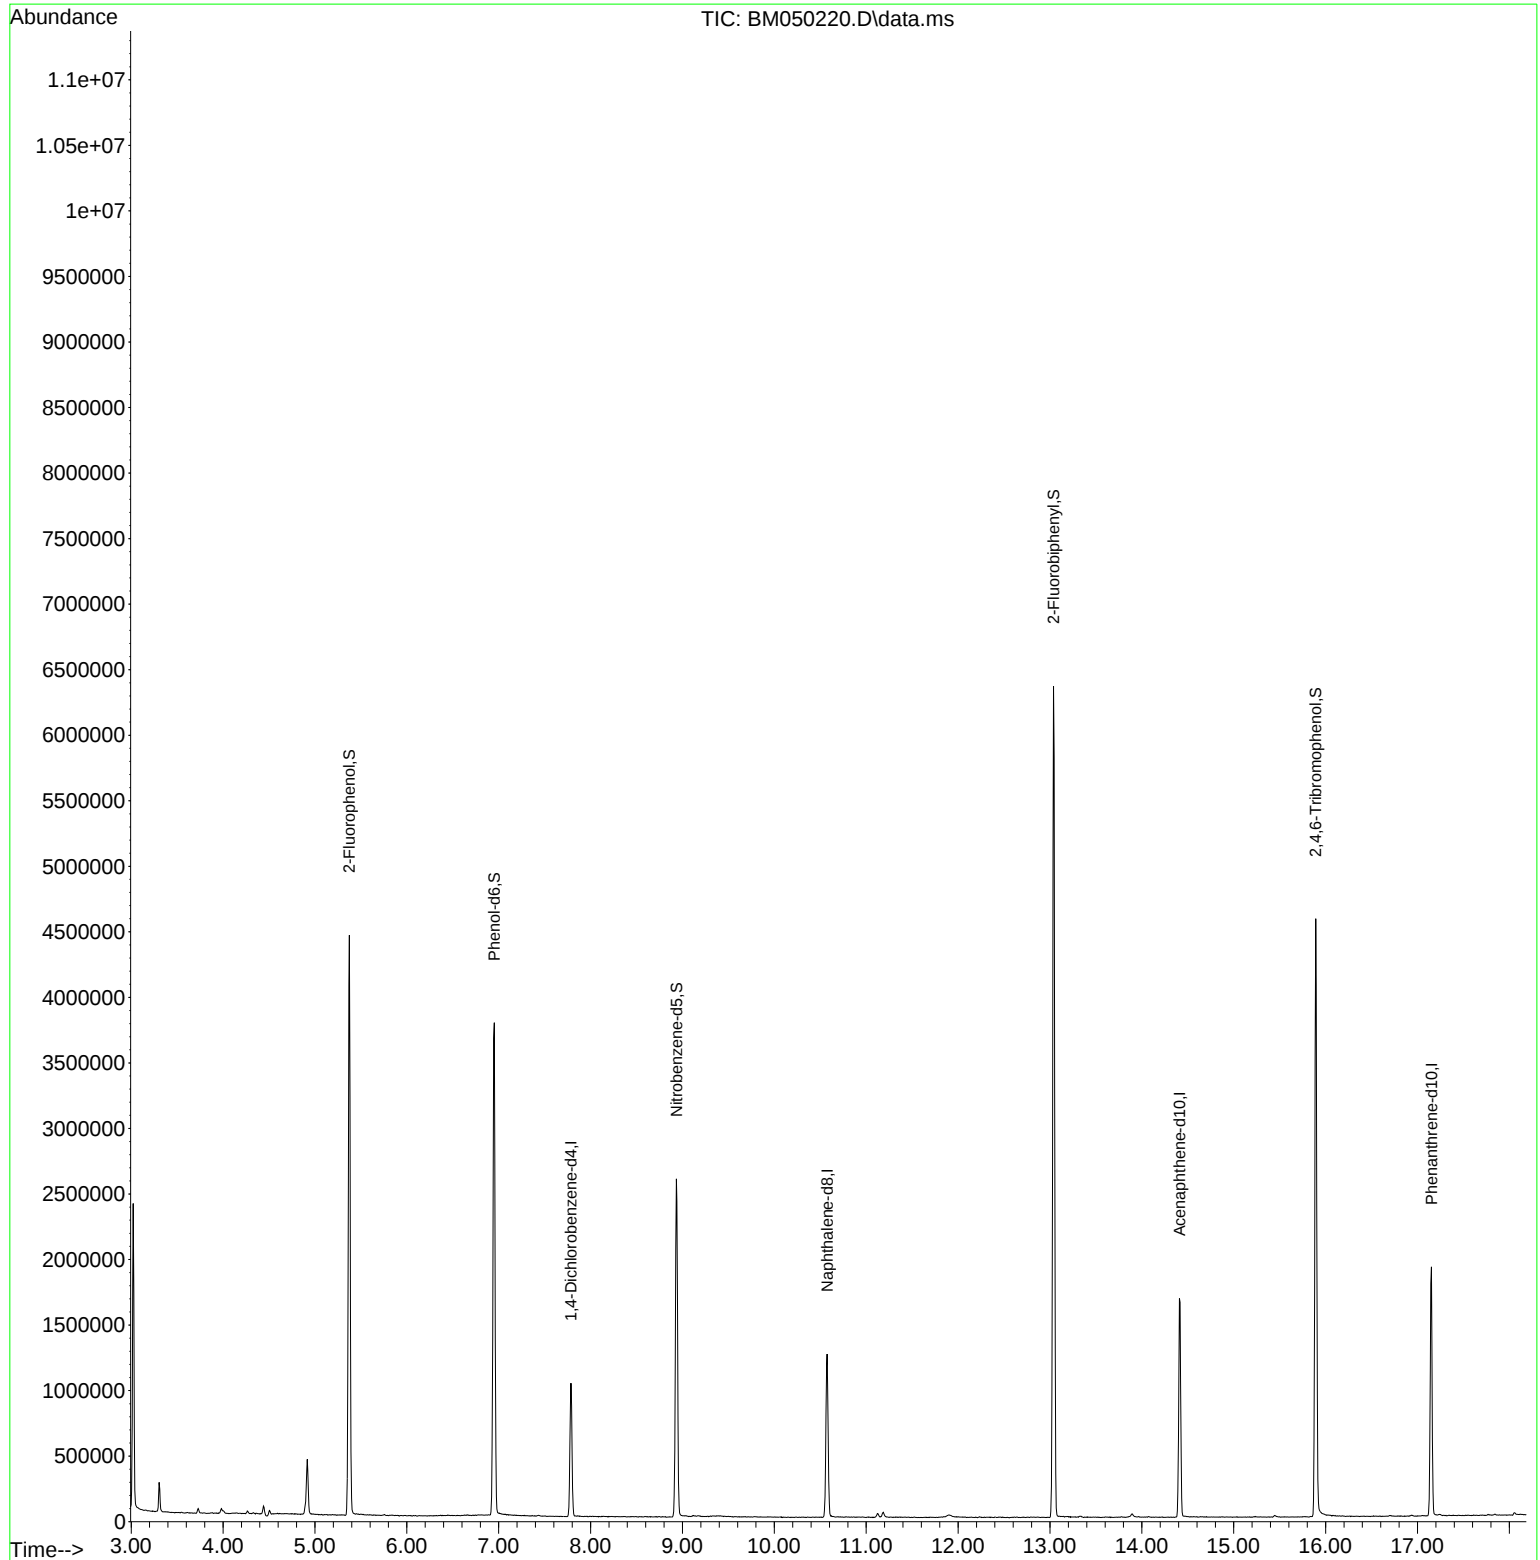

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050220.D
Acq On : 06 Jun 2025 18:45
Operator : RC/JU
Sample : Q2207-45
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-05

Quant Time: Jun 07 01:19:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

