

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
 Data File : BM050230.D
 Acq On : 07 Jun 2025 02:01
 Operator : RC/JU
 Sample : Q2198-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-207-SB02

Quant Time: Jun 07 03:28:35 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 16:20:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	299355	20.000	ng	0.00
21) Naphthalene-d8	10.575	136	1125867	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	622474	20.000	ng	0.00
64) Phenanthrene-d10	17.145	188	1119241	20.000	ng	-0.01
76) Chrysene-d12	21.374	240	1048287	20.000	ng	-0.01
86) Perylene-d12	24.356	264	1143100	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	2234637	124.524	ng	0.00
7) Phenol-d6	6.951	99	2556777	108.230	ng	0.00
23) Nitrobenzene-d5	8.934	82	1795563	82.944	ng	-0.01
42) 2,4,6-Tribromophenol	15.892	330	914676	129.188	ng	-0.01
45) 2-Fluorobiphenyl	13.039	172	3603780	78.380	ng	-0.01
79) Terphenyl-d14	19.774	244	4789764	86.586	ng	-0.01
Target Compounds						
31) Naphthalene	10.622	128	803533	13.804	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050230.D
Acq On : 07 Jun 2025 02:01
Operator : RC/JU
Sample : Q2198-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-207-SB02

Quant Time: Jun 07 03:28:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

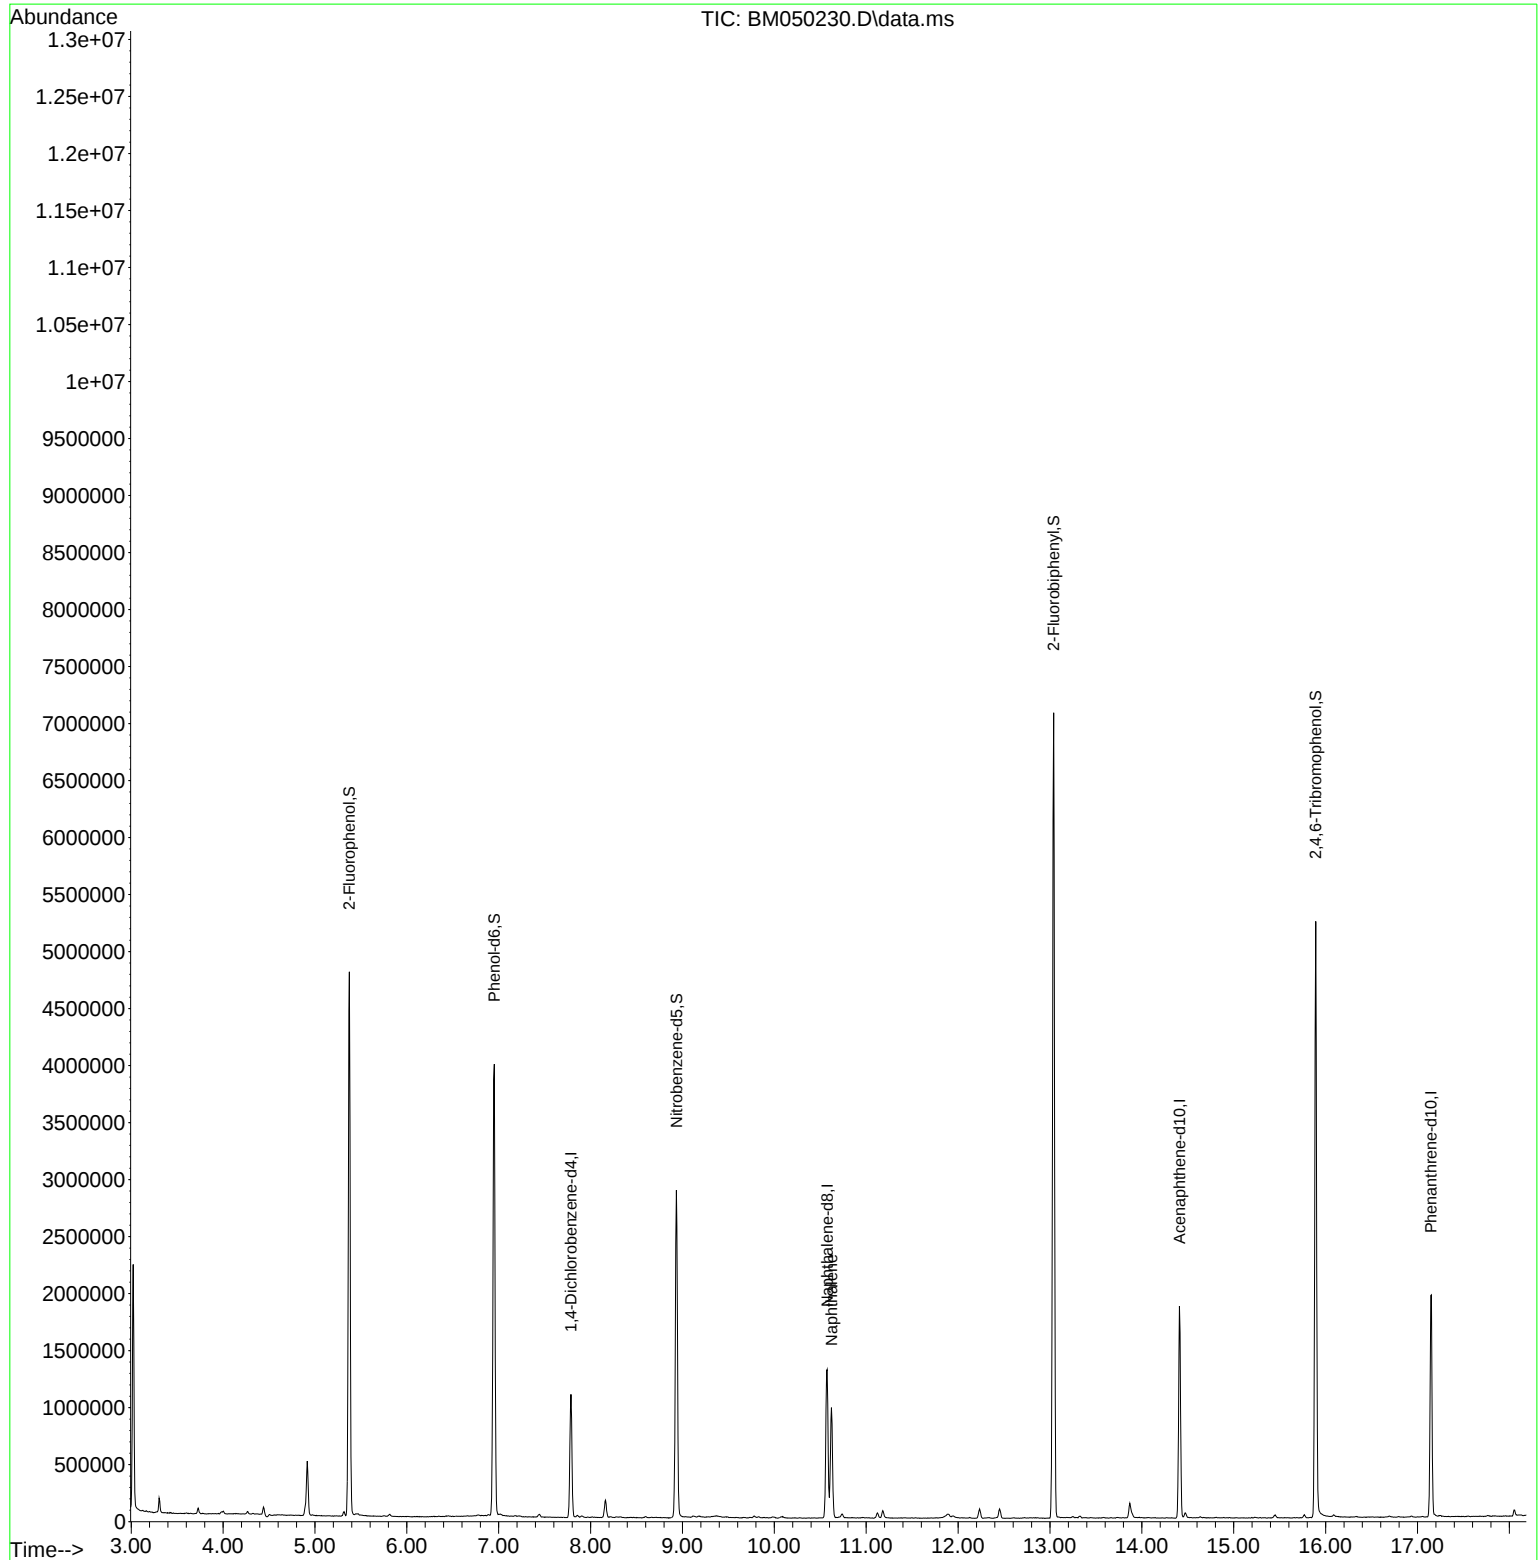

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050230.D
Acq On : 07 Jun 2025 02:01
Operator : RC/JU
Sample : Q2198-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-207-SB02

Quant Time: Jun 07 03:28:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

