
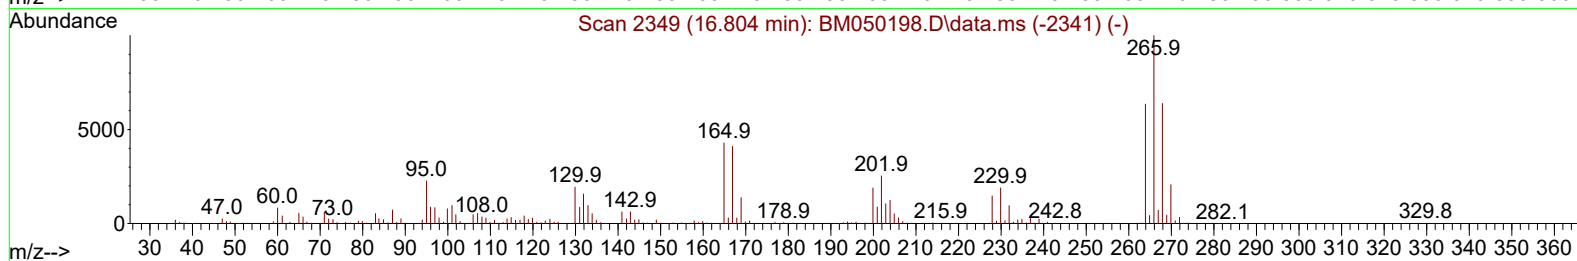
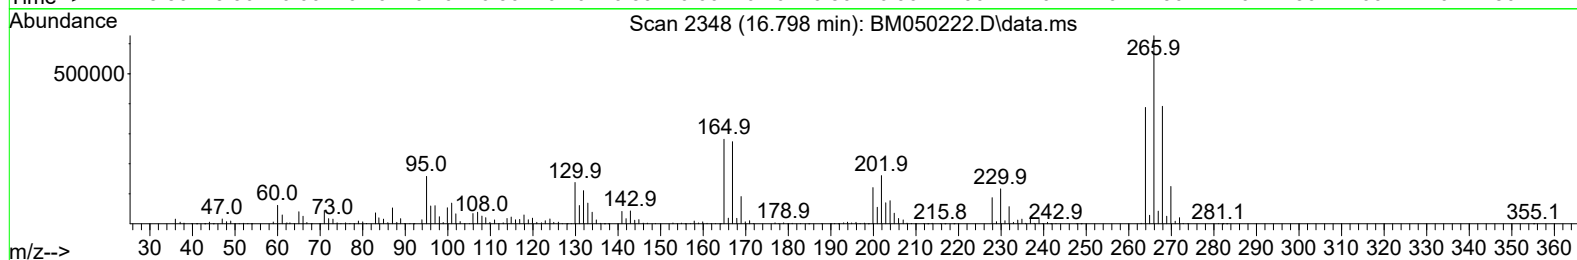


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050222.D
Acq On : 06 Jun 2025 20:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 01:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

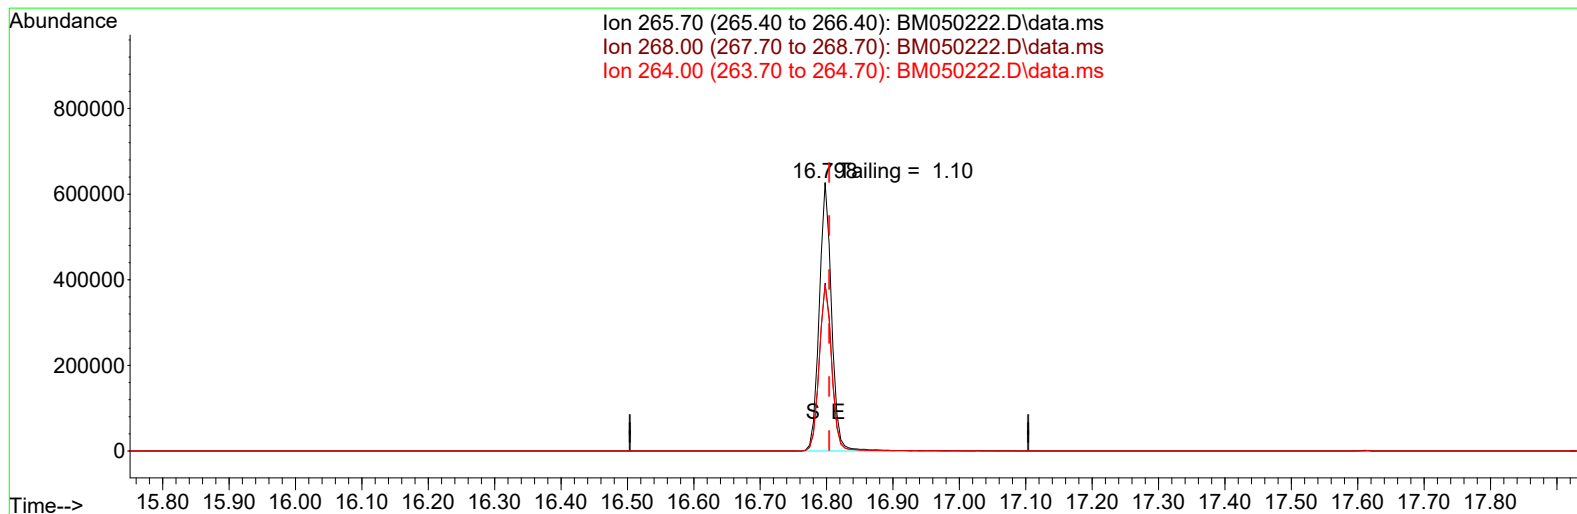

TIC: BM050222.D\data.ms

(70) Pentachlorophenol (C)




16.798min (-0.006) 257431.30 ng

response 809092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.48
264.00	63.50	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050222.D
Acq On : 06 Jun 2025 20:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 01:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

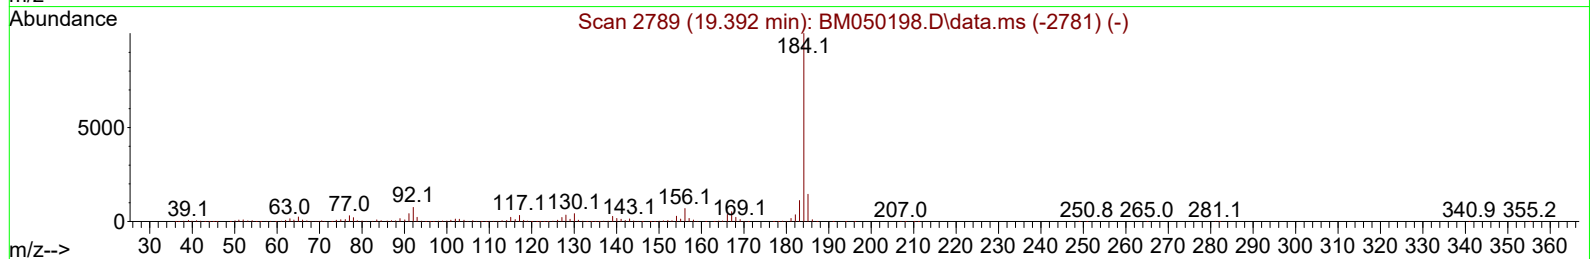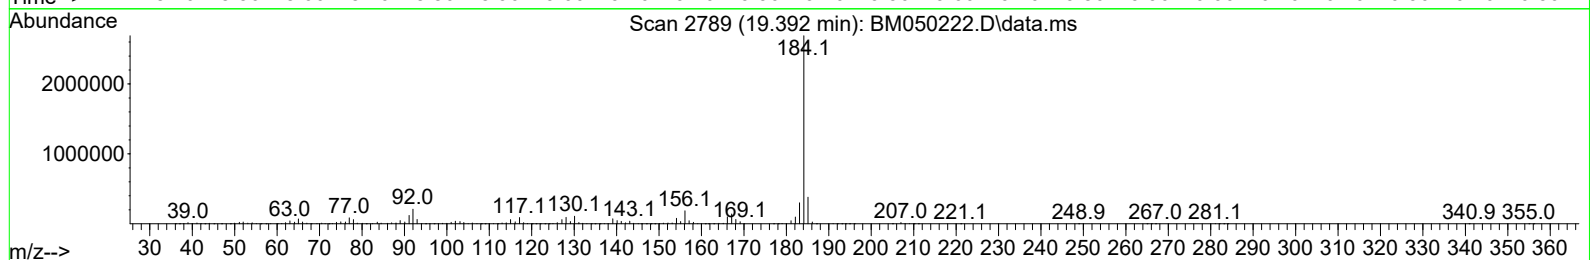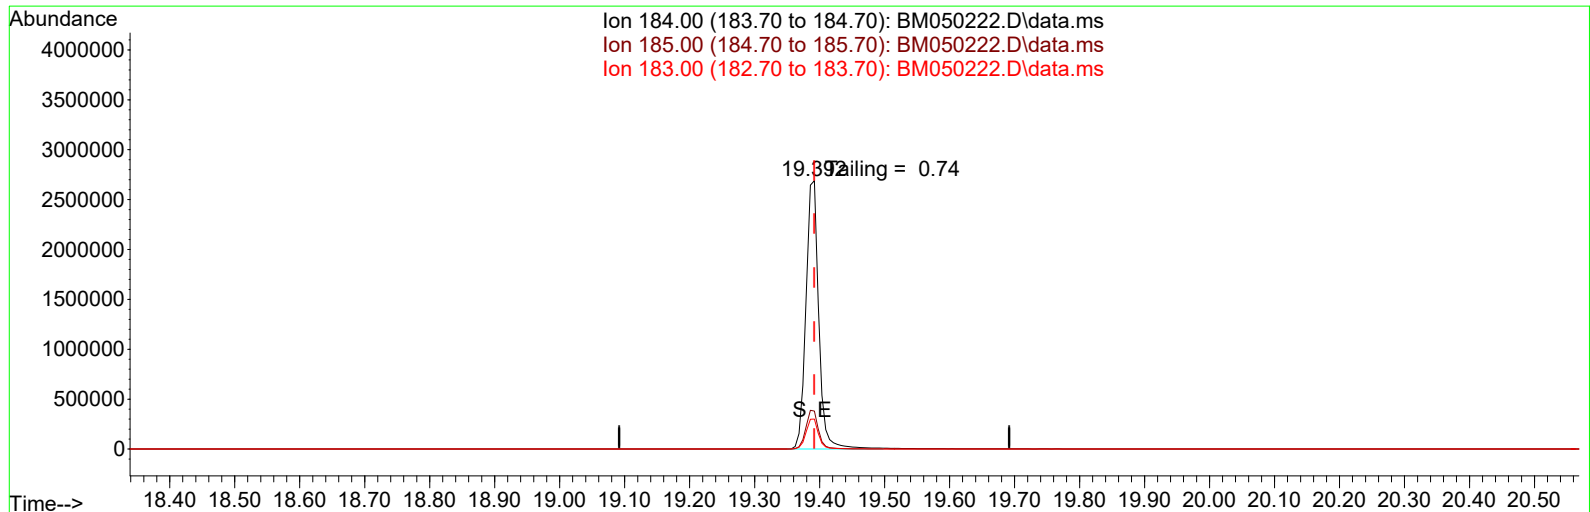

TIC: BM050222.D\data.ms

(77) Benzidine**19.392min (-0.000) 152757.03 ng****response 3707147**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.20	11.19
0.00	0.00	0.00