

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
 Data File : BM050219.D
 Acq On : 06 Jun 2025 18:05
 Operator : RC/JU
 Sample : Q2207-36
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BU-703-COMP-04

Quant Time: Jun 06 18:36:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 05 16:20:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.786	152	287190	20.000	ng	0.00
21) Naphthalene-d8	10.574	136	1092305	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	593608	20.000	ng	0.00
64) Phenanthrene-d10	17.151	188	1065893	20.000	ng	0.00
76) Chrysene-d12	21.374	240	1047961	20.000	ng	-0.01
86) Perylene-d12	24.368	264	1170199	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	2243190	130.296	ng	0.00
7) Phenol-d6	6.951	99	2643851	116.657	ng	0.00
23) Nitrobenzene-d5	8.933	82	1748706	83.262	ng	-0.01
42) 2,4,6-Tribromophenol	15.898	330	875703	129.698	ng	0.00
45) 2-Fluorobiphenyl	13.039	172	3439603	78.448	ng	-0.01
79) Terphenyl-d14	19.780	244	4487113	81.140	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050219.D
Acq On : 06 Jun 2025 18:05
Operator : RC/JU
Sample : Q2207-36
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04


Quant Time: Jun 06 18:36:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

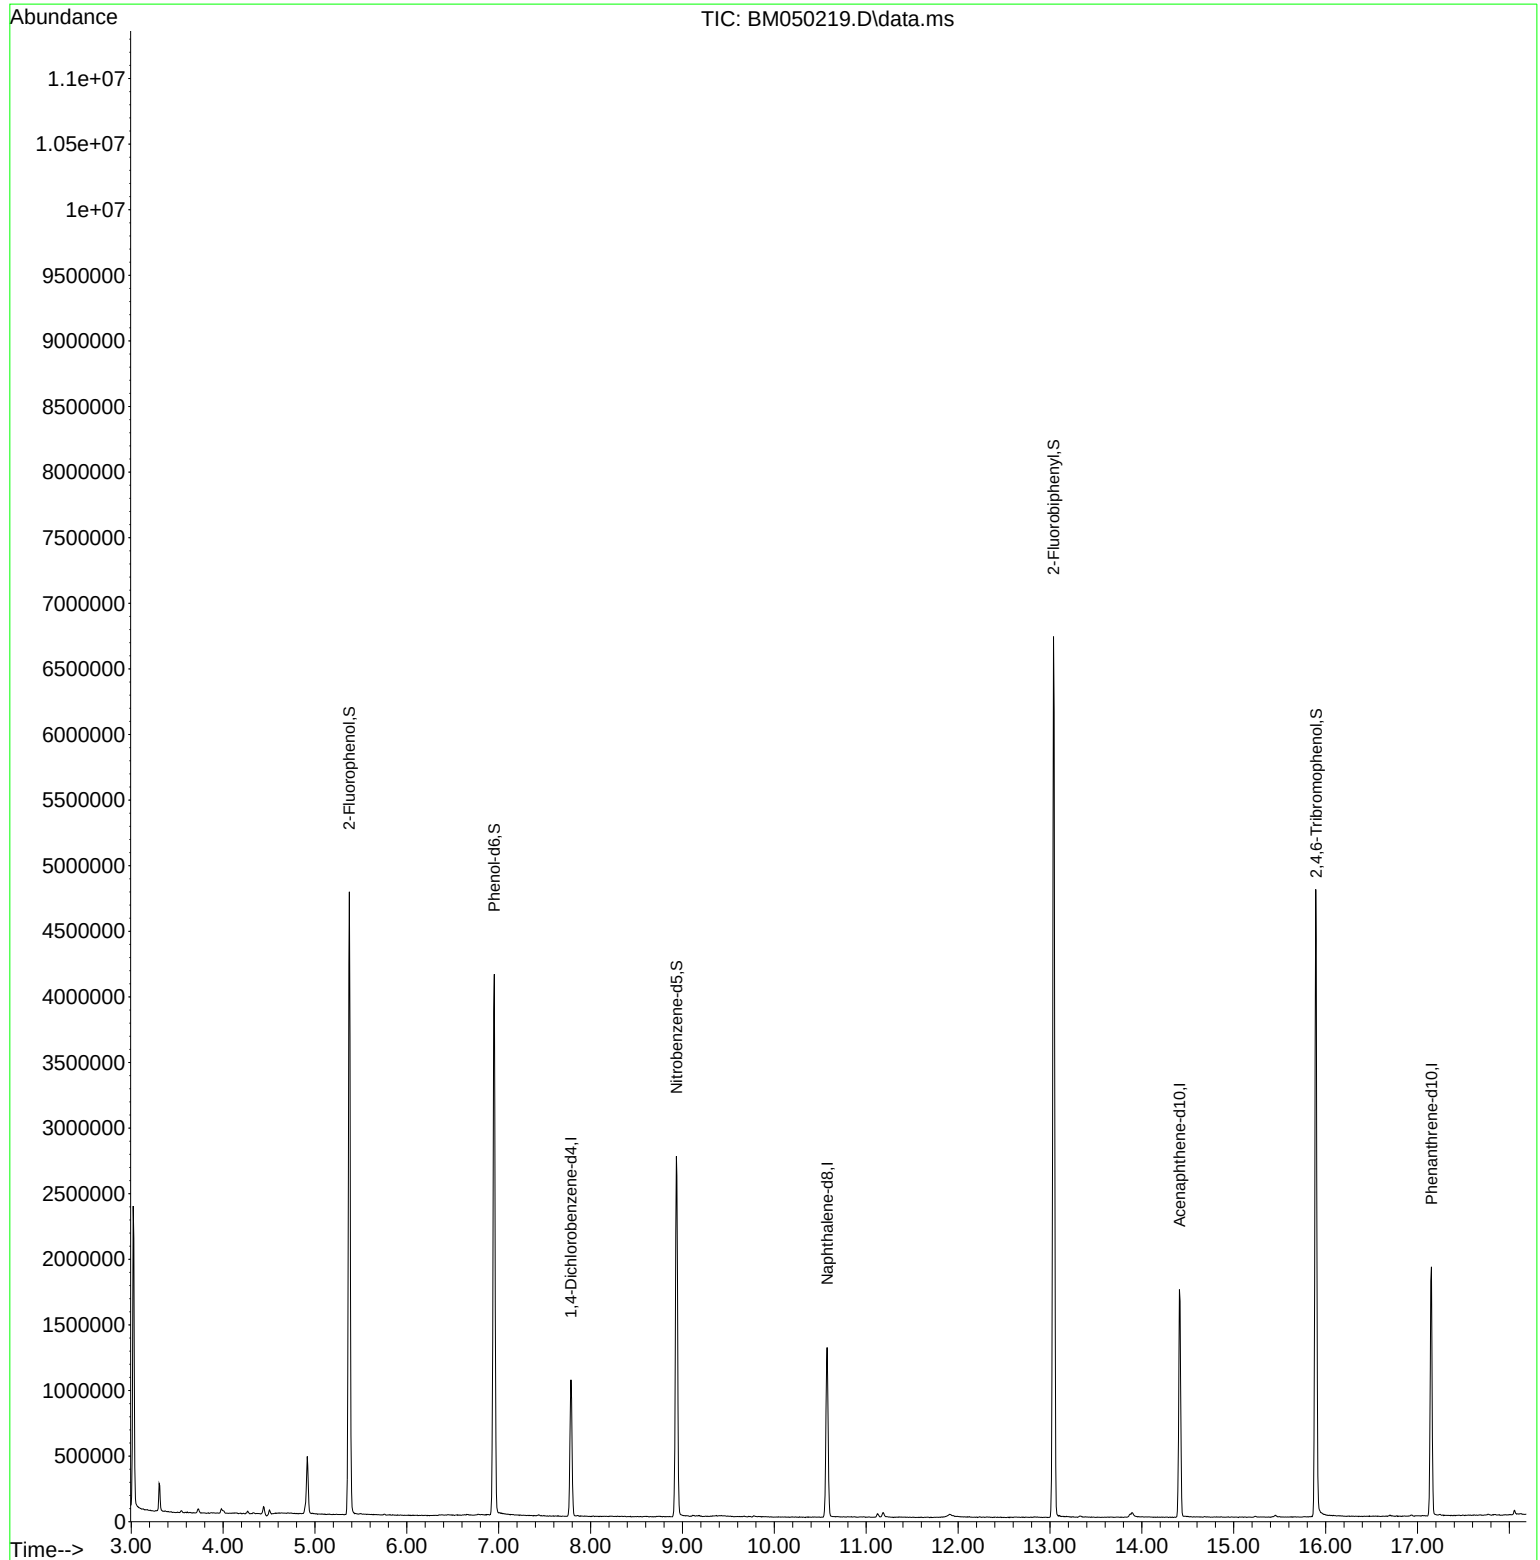


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050219.D
Acq On : 06 Jun 2025 18:05
Operator : RC/JU
Sample : Q2207-36
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04

Quant Time: Jun 06 18:36:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration




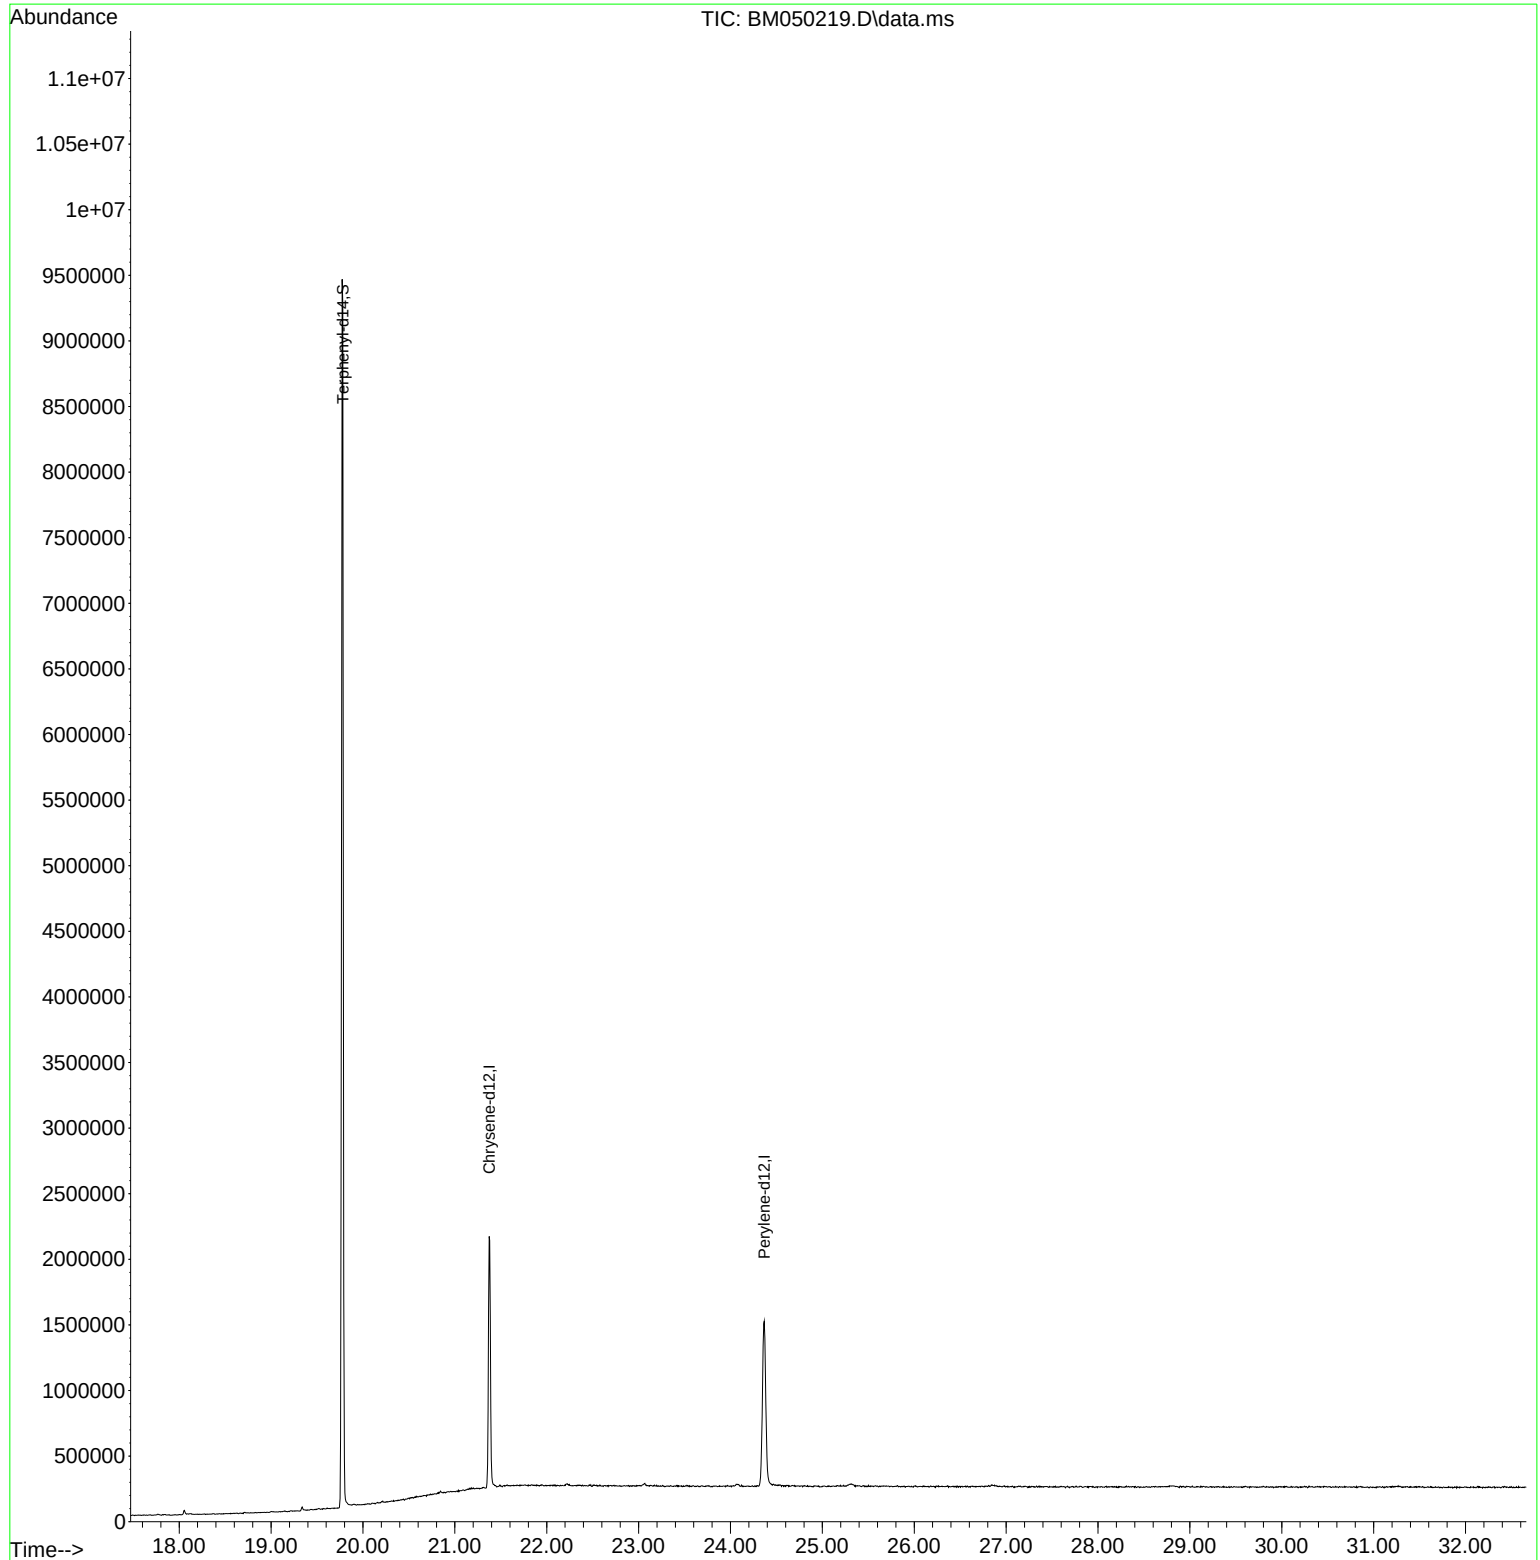


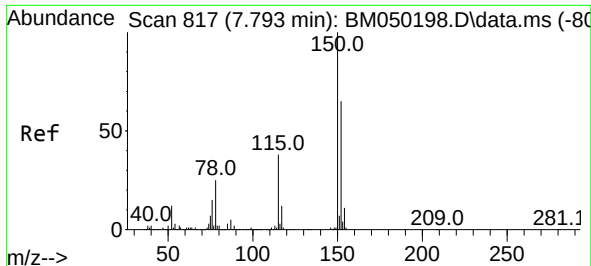

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.786 min Scan# 81
Delta R.T. -0.007 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05




Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04


Tgt Ion:152 Resp: 287190
Ion Ratio Lower Upper
152 100
150 160.4 122.2 183.4
115 62.6 46.3 69.5

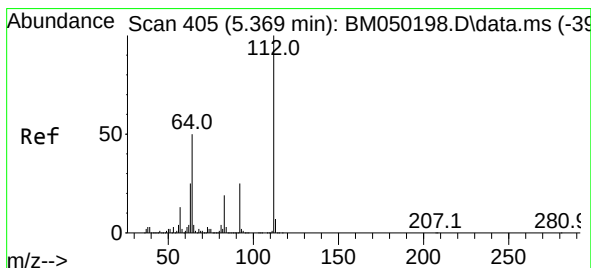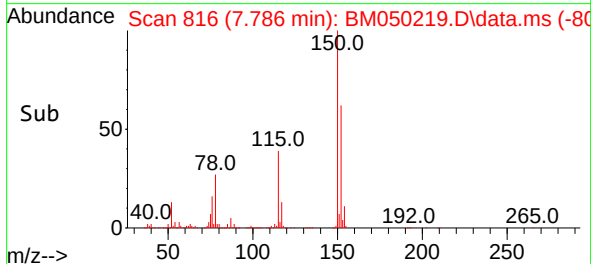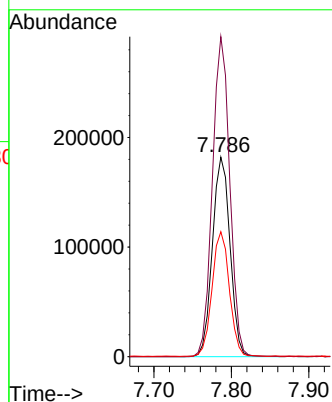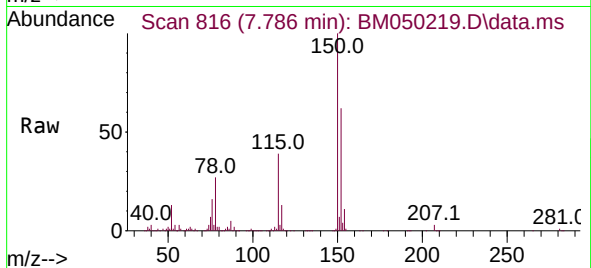

#5
2-Fluorophenol
Concen: 130.296 ng
RT: 5.375 min Scan# 406
Delta R.T. -0.000 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05

Tgt Ion:112 Resp: 2243190
Ion Ratio Lower Upper
112 100
64 50.2 39.8 59.6
63 25.5 19.8 29.8


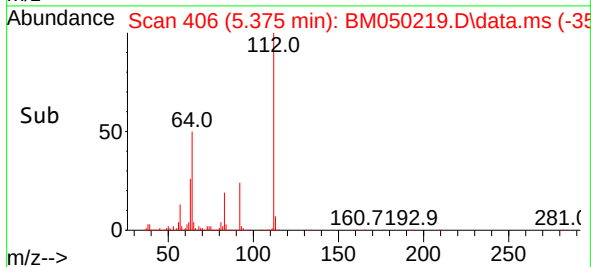
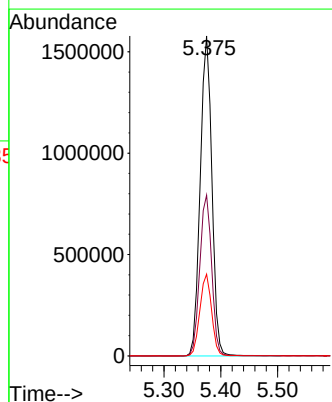
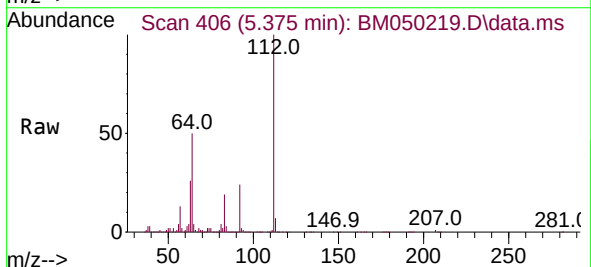


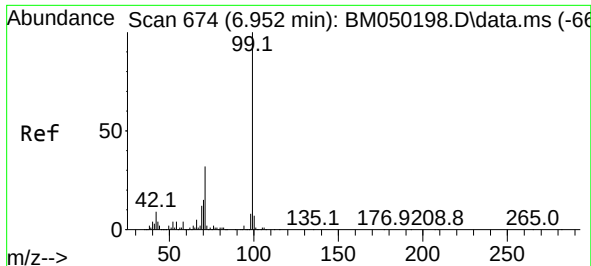

#7
Phenol-d6
Concen: 116.657 ng
RT: 6.951 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05




Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04


Tgt Ion: 99 Resp: 2643851
Ion Ratio Lower Upper
99 100
42 8.4 6.9 10.3
71 32.5 25.3 37.9

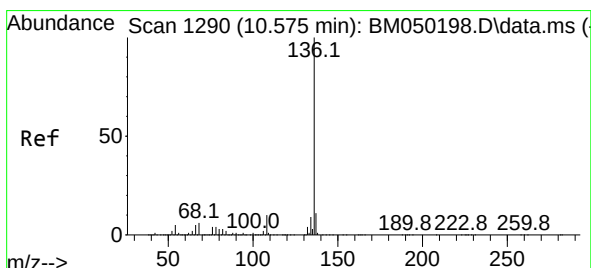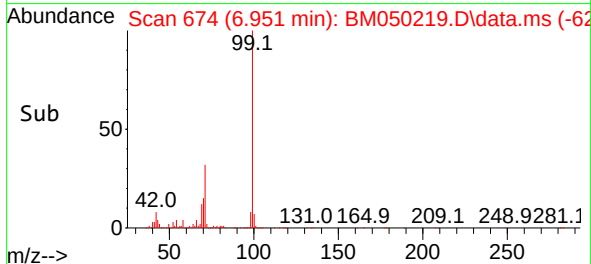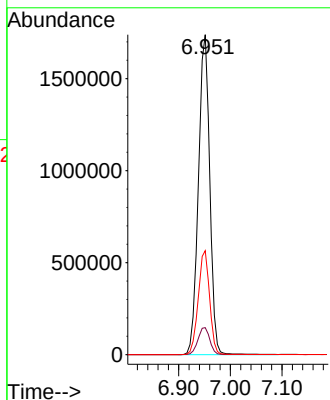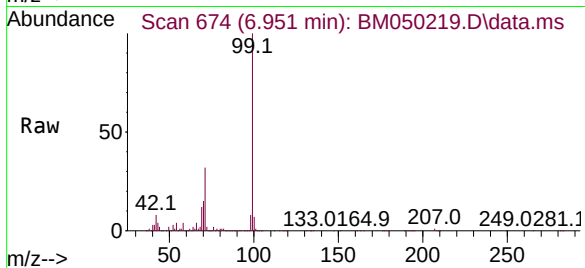

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.574 min Scan# 1290
Delta R.T. -0.006 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05

Tgt Ion: 136 Resp: 1092305
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 5.4 3.8 5.8
68 5.9 4.9 7.3


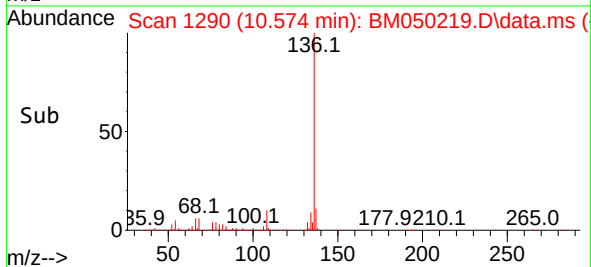
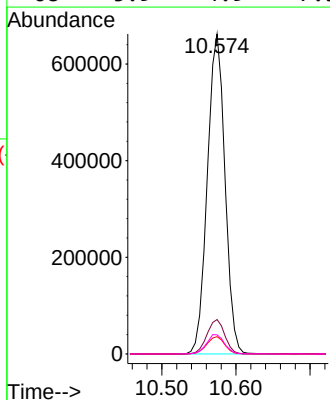
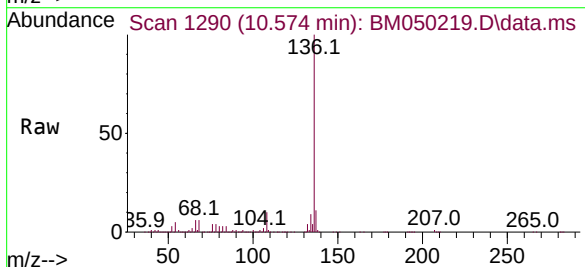


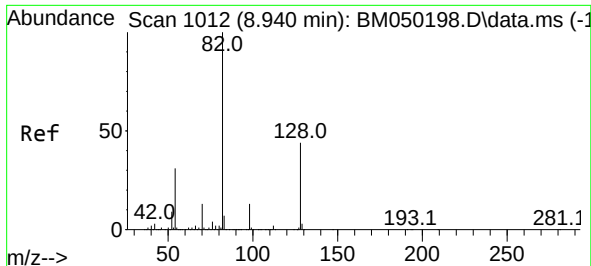

#23
Nitrobenzene-d5
Concen: 83.262 ng
RT: 8.933 min Scan# 1011
Delta R.T. -0.012 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05




Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04


Tgt Ion: 82 Resp: 1748706
Ion Ratio Lower Upper
82 100
128 42.4 35.2 52.8
54 31.3 24.5 36.7

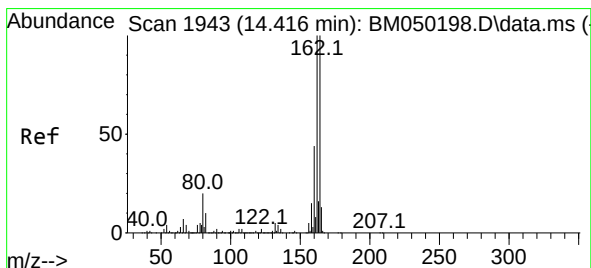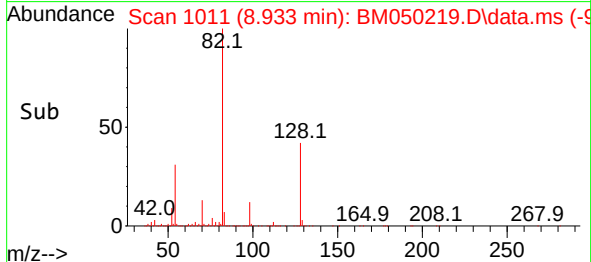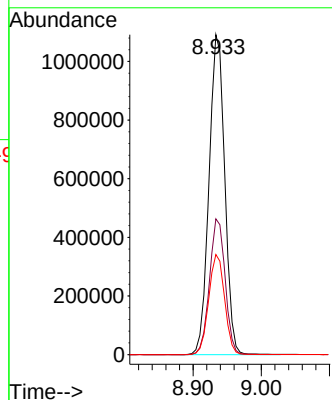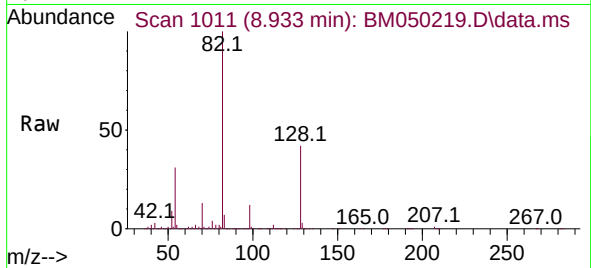

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.410 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05

Tgt Ion:164 Resp: 593608
Ion Ratio Lower Upper
164 100
162 99.6 80.2 120.4
160 46.5 35.7 53.5


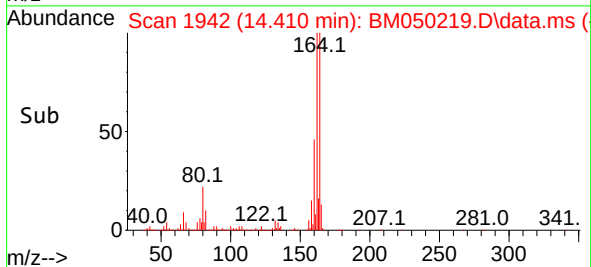
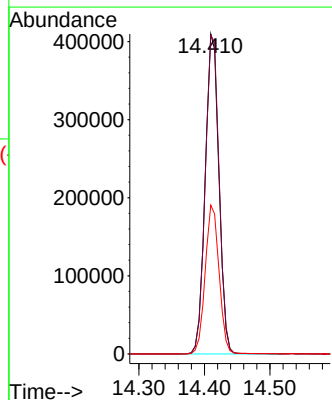
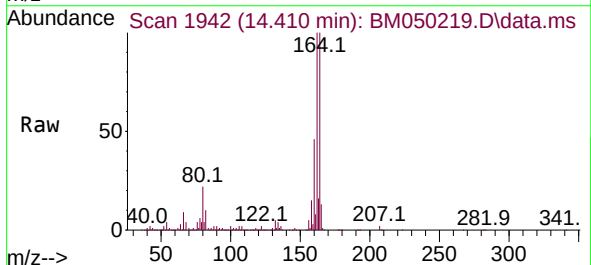


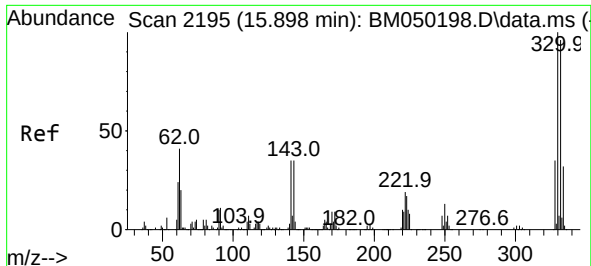

#42
 2,4,6-Tribromophenol
 Concen: 129.698 ng
 RT: 15.898 min Scan# 2195
 Delta R.T. -0.006 min
 Lab File: BM050219.D
 Acq: 06 Jun 2025 18:05




Instrument :
 BNA_M
 ClientSampleId :
 BU-703-COMP-04


Tgt Ion:330 Resp: 875703
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.5 116.3
 141 38.1 28.8 43.2

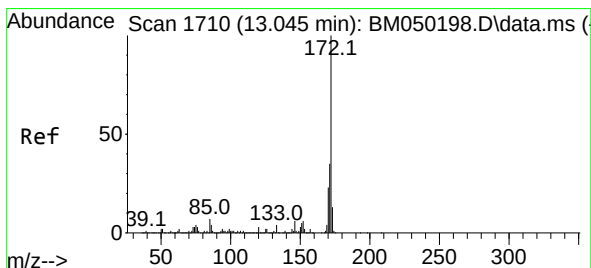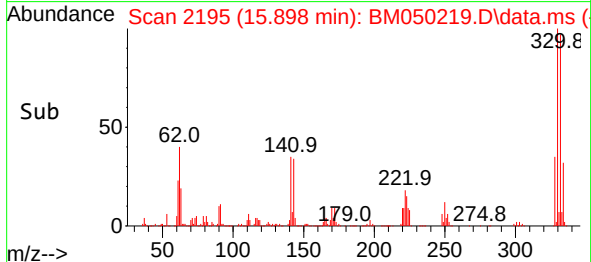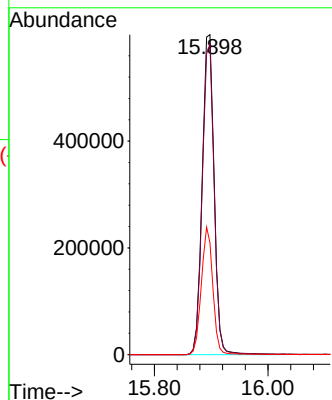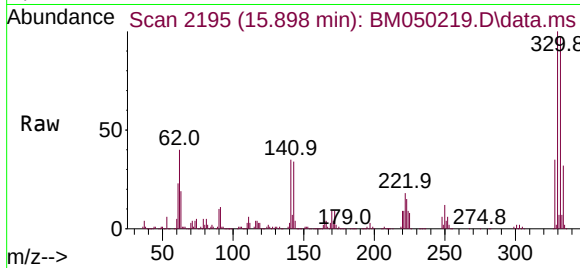

#45
 2-Fluorobiphenyl
 Concen: 78.448 ng
 RT: 13.039 min Scan# 1709
 Delta R.T. -0.012 min
 Lab File: BM050219.D
 Acq: 06 Jun 2025 18:05

Tgt Ion:172 Resp: 3439603
 Ion Ratio Lower Upper
 172 100
 171 35.0 27.8 41.6
 170 23.2 18.6 27.8


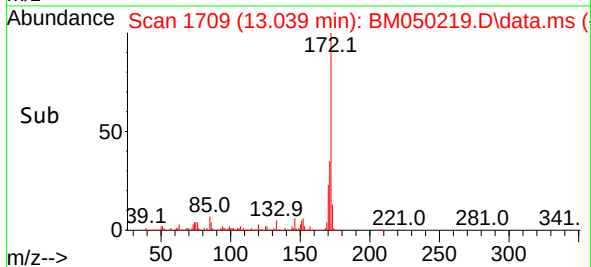
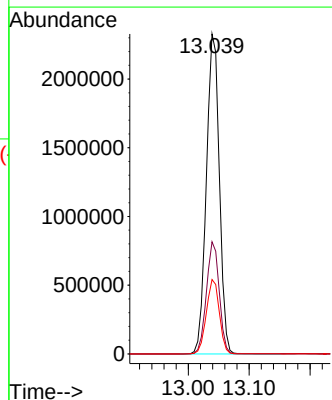
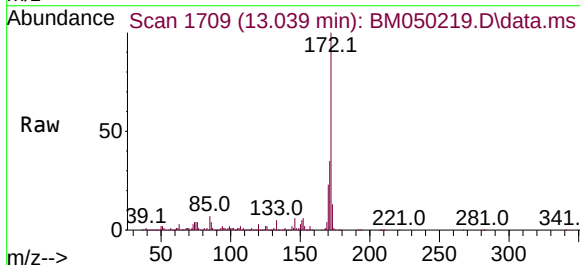


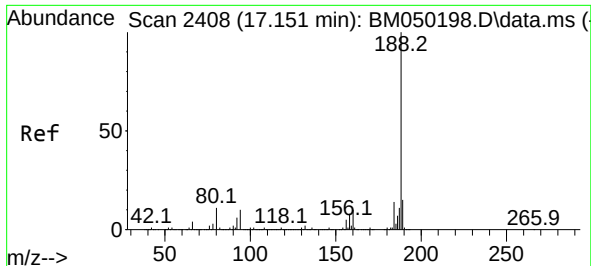

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.151 min Scan# 24
Delta R.T. -0.006 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05




Instrument :
BNA_M
ClientSampleId :
BU-703-COMP-04


Tgt Ion:188 Resp: 1065893
Ion Ratio Lower Upper
188 100
94 9.9 8.1 12.1
80 11.2 8.6 13.0

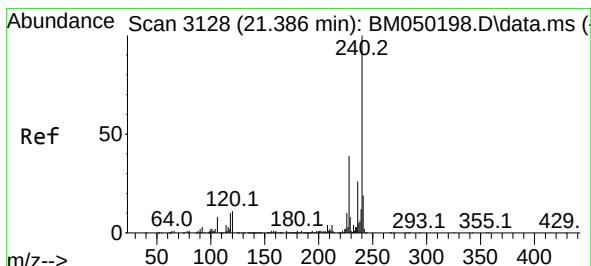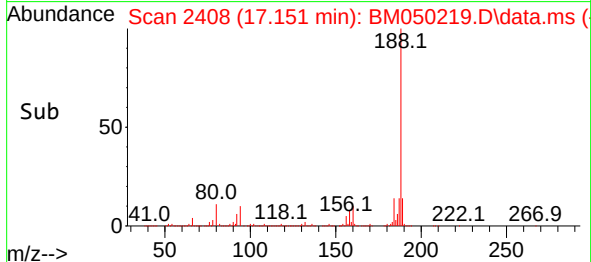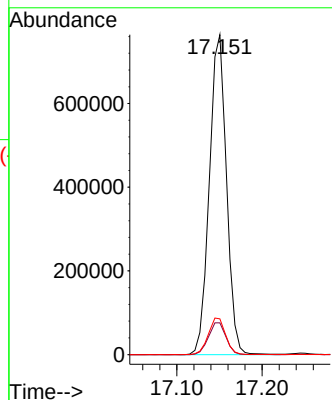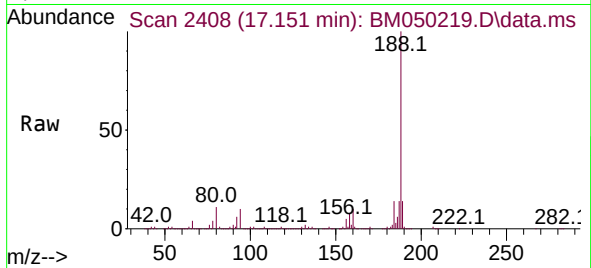

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.374 min Scan# 3126
Delta R.T. -0.012 min
Lab File: BM050219.D
Acq: 06 Jun 2025 18:05

Tgt Ion:240 Resp: 1047961
Ion Ratio Lower Upper
240 100
120 12.6 9.0 13.4
236 25.1 20.7 31.1


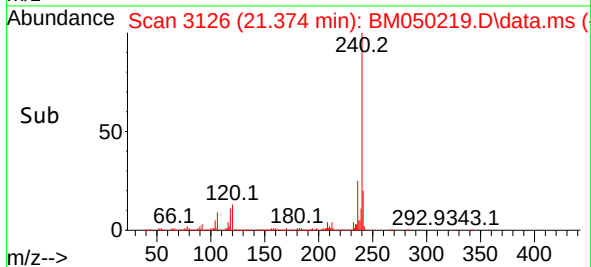
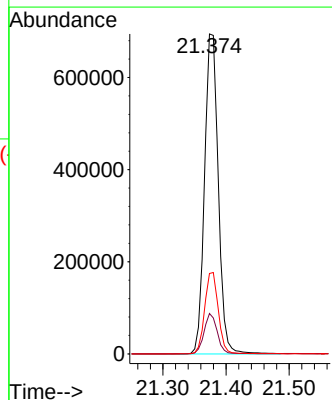
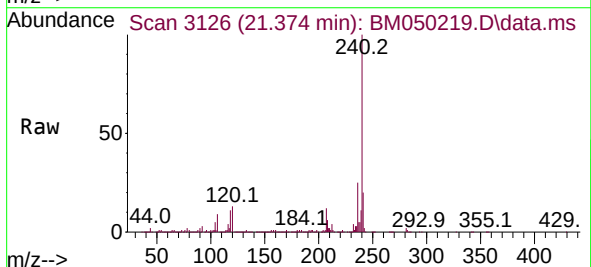


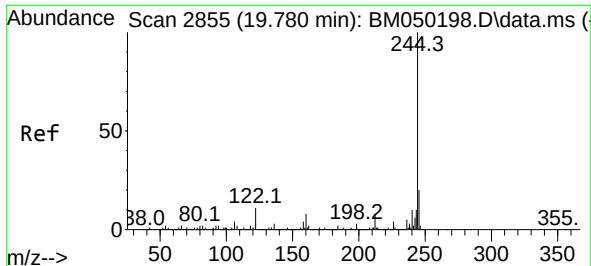

#79
 Terphenyl-d14
 Concen: 81.140 ng
 RT: 19.780 min Scan# 2855
 Delta R.T. -0.006 min
 Lab File: BM050219.D
 Acq: 06 Jun 2025 18:05

Instrument :
 BNA_M
 ClientSampleId :
 BU-703-COMP-04

Tgt Ion:244 Resp: 4487113
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 11.0 8.6 12.8

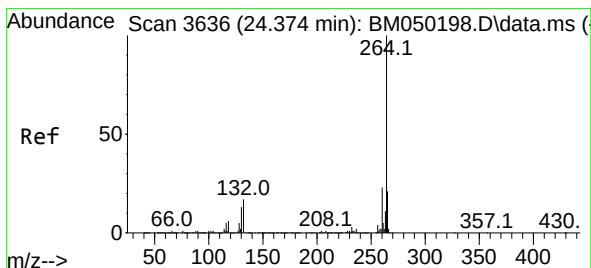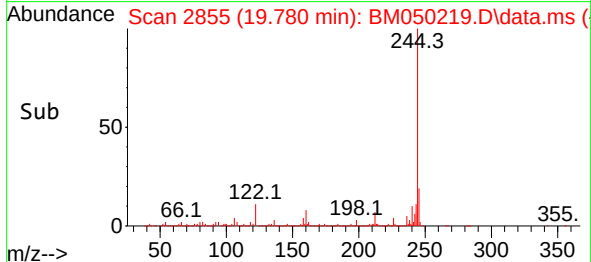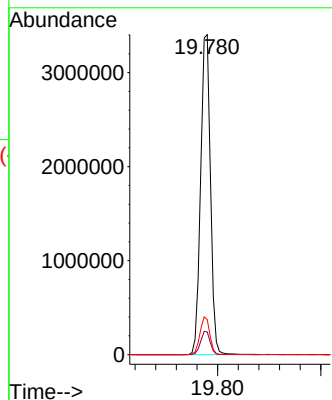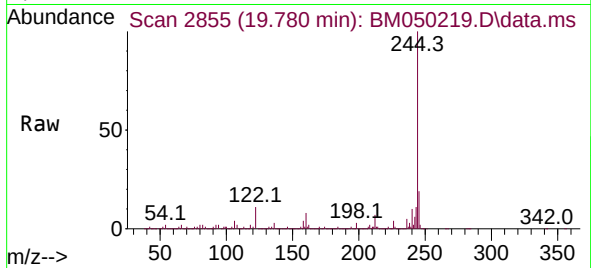

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.368 min Scan# 3635
 Delta R.T. -0.006 min
 Lab File: BM050219.D
 Acq: 06 Jun 2025 18:05

Tgt Ion:264 Resp: 1170199
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.6 28.0
 265 21.4 16.8 25.2

