
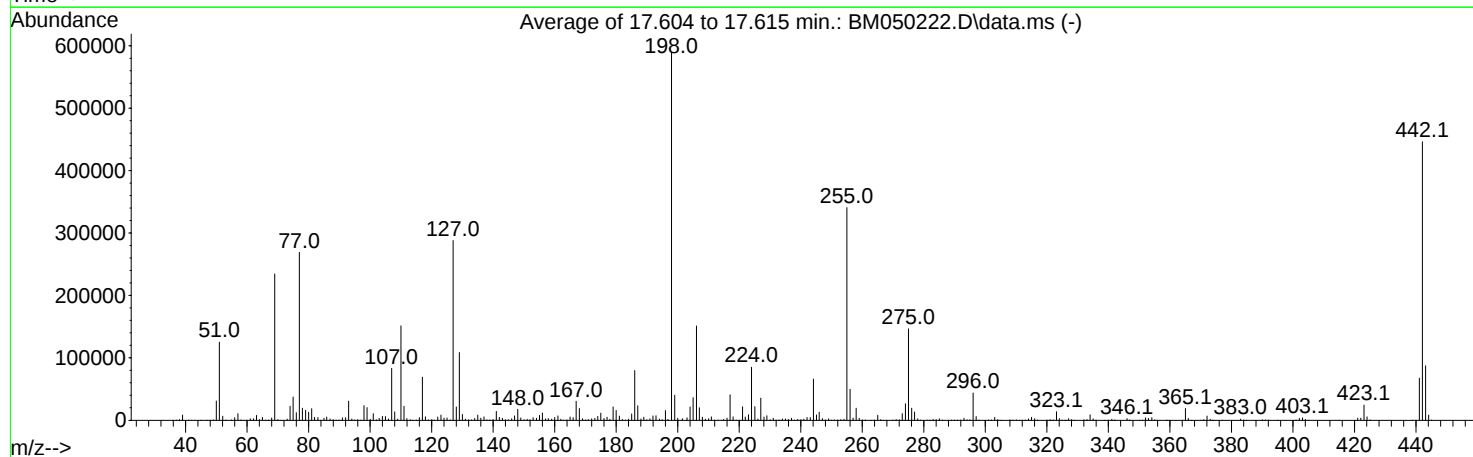


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050222.D
Acq On : 06 Jun 2025 20:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 05 16:20:25 2025

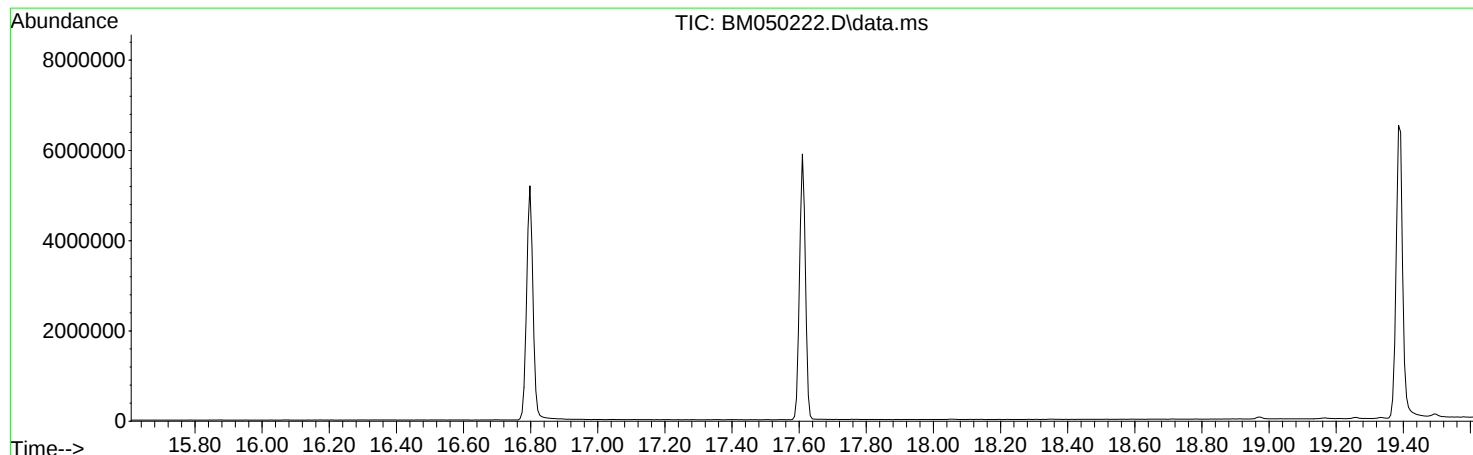




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	125338	PASS
68	69	0.00	2	1.5	3622	PASS
69	198	0.00	100	39.8	234283	PASS
70	69	0.00	2	0.5	1197	PASS
127	198	10	80	48.9	288000	PASS
197	198	0.00	2	0.2	1321	PASS
198	198	100	100	100.0	589269	PASS
199	198	5	9	6.8	40152	PASS
275	198	10	60	24.9	146557	PASS
365	198	1	100	3.2	18967	PASS
441	198	0.01	100	11.5	67659	PASS
442	442	50	100	100.0	446229	PASS
443	442	15	24	19.5	87179	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050222.D
Acq On : 06 Jun 2025 20:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 07 01:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

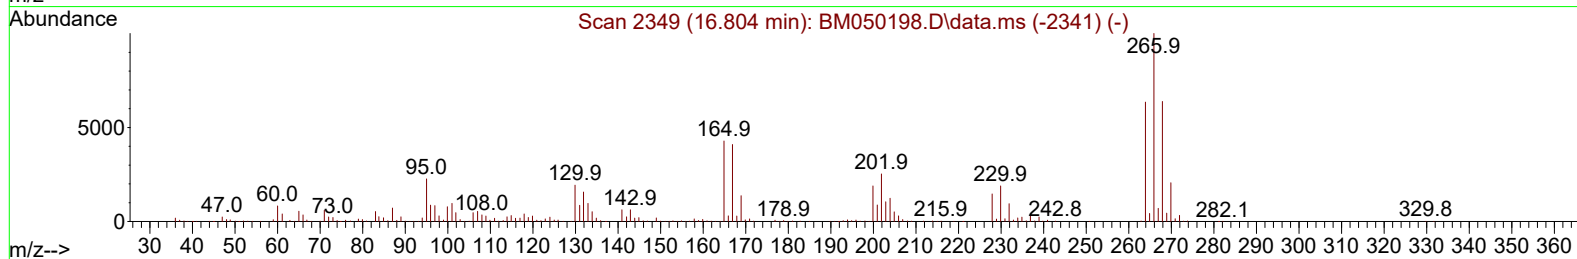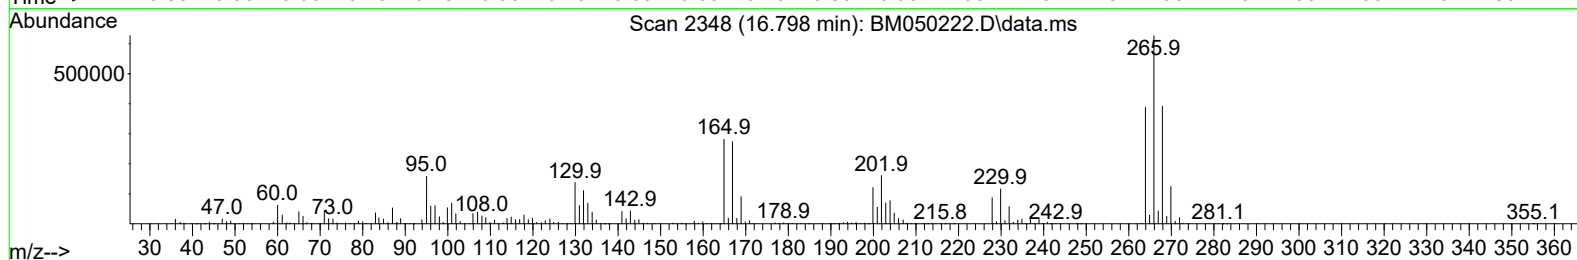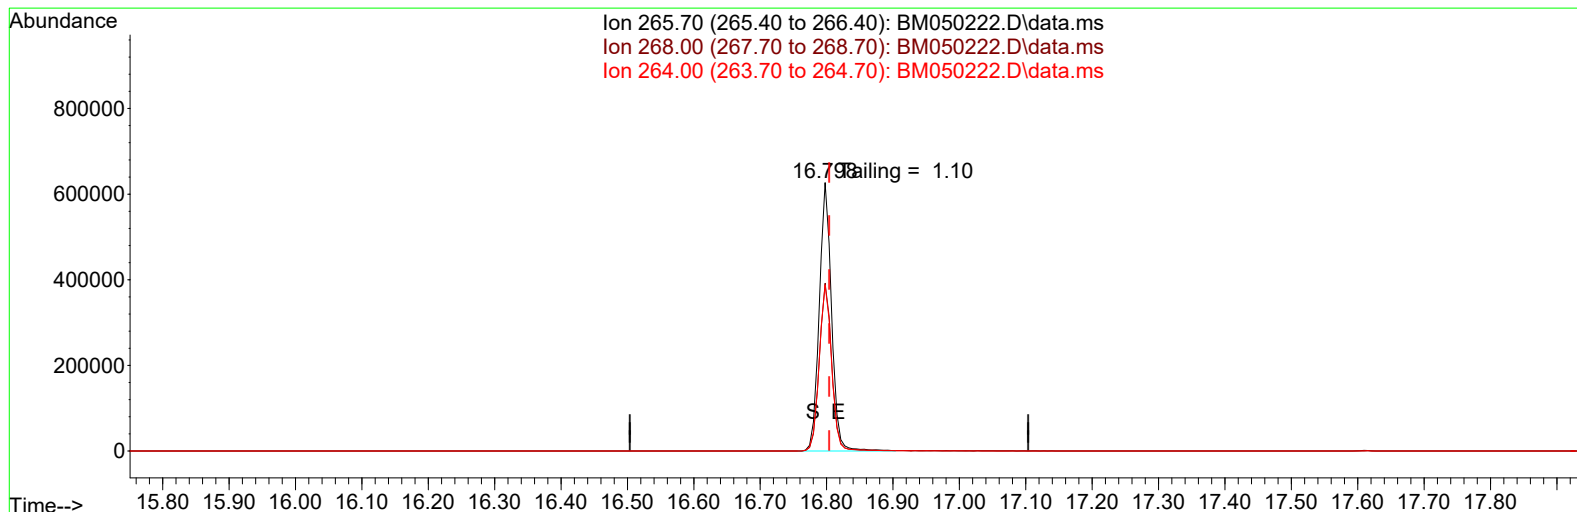

TIC: BM050222.D\data.ms

(70) Pentachlorophenol (C)

16.798min (-0.006) 257431.30 ng




response 809092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.48
264.00	63.50	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050222.D
Acq On : 06 Jun 2025 20:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 07 01:24:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

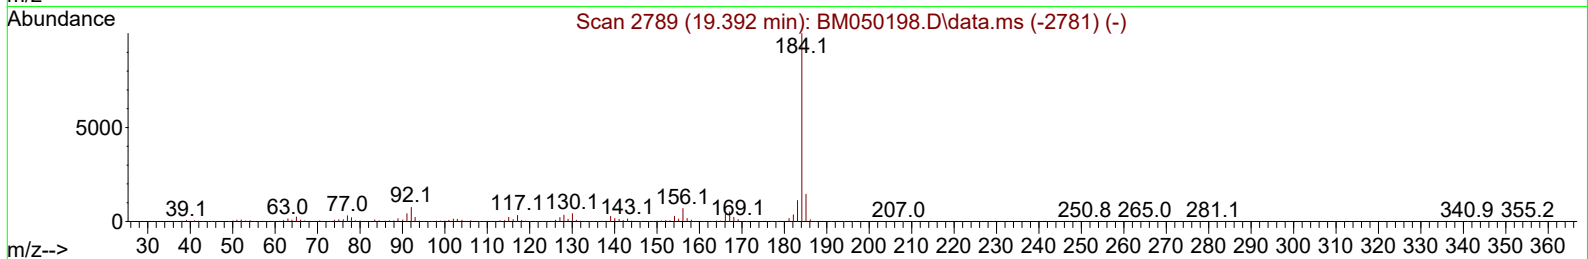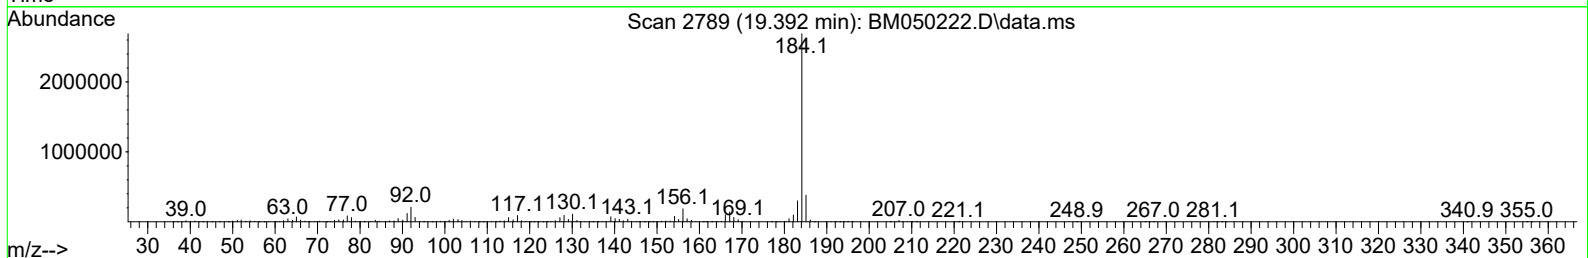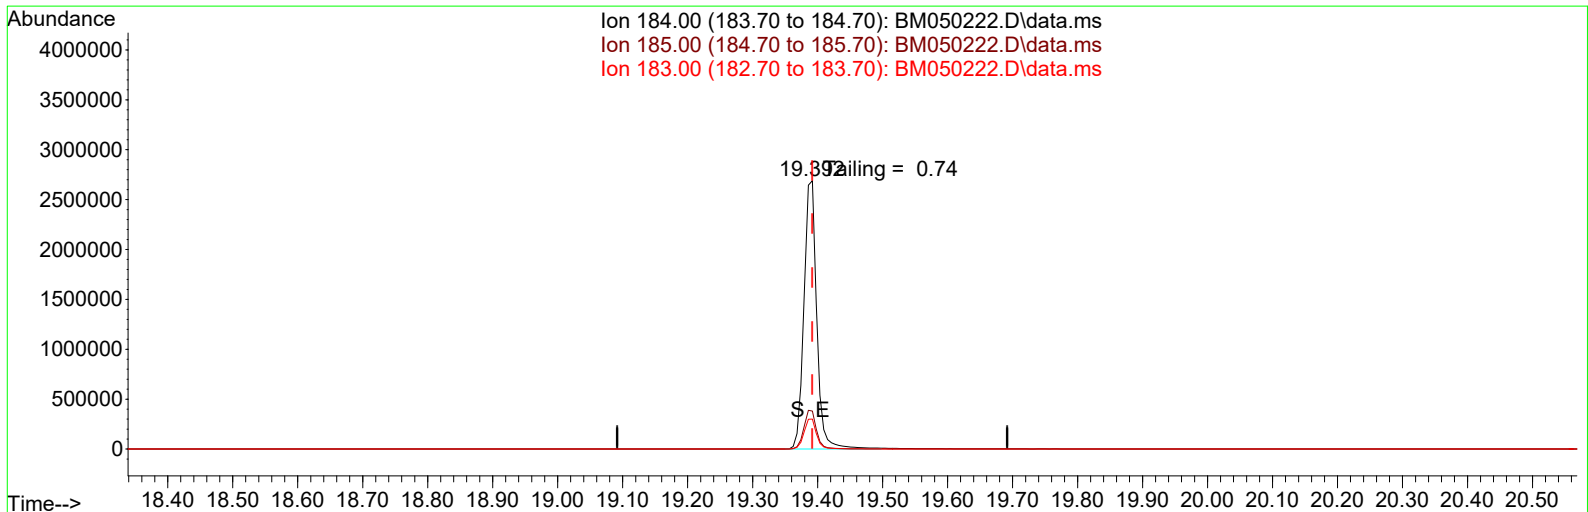

TIC: BM050222.D\data.ms

(77) Benzidine

19.392min (-0.000) 152757.03 ng

response 3707147

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.20	11.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2025	BNA_M	<u>BM050222.D</u>
Compound Name	Response	Retention Time
DDT	1821774	20.627
DDD	19213	20.174
DDE	1595	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20808	1842582	1.13

Instrument :
BNA_M
ClientSampleId :
DFTPP