

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060719\
 Data File : BM020803.D
 Acq On : 07 Jun 2019 14:37
 Operator : HP/JU
 Sample : K3201-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:41:55 AM

Quant Time: Jun 08 01:29:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 08 00:20:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	305925	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1273616	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	714561	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	1426515	20.00	ng/ul	0.00
77) Chrysene-d12	21.38	240	1209981	20.00	ng/ul	0.00
85) Perylene-d12	23.67	264	1368929	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	34899	5.44	ng/uL	0.00
5) Phenol-d5	6.97	99	753942	32.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	481806	34.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	650359	34.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	589719	31.31	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	329306	37.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	370500	41.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	676688	36.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	710663	31.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	2053734	38.86	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	2477499	36.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	243190	26.81	ng/ul	0.00
57) Fluorene-d10	15.45	176	1636920	36.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	148219	20.32	ng/ul	0.00
70) Anthracene-d10	17.30	188	2264404	36.34	ng/ul	0.00
78) Pyrene-d10	19.59	212	2168469	37.08	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.52	264	2178605	35.02	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.00	94	26381	1.095	ng/ul 93
28) Naphthalene	10.65	128	271702	4.542	ng/ul 99
34) 2-Methylnaphthalene	12.26	142	169655	3.861	ng/ul 96
44) Dimethylphthalate	13.91	163	798596	15.089	ng/ul 100
47) Acenaphthylene	14.17	152	130291	2.009	ng/ul# 96
49) Acenaphthene	14.51	153	472080	10.429	ng/ul 98
53) Dibenzofuran	14.85	168	538763	8.415	ng/ul 100
58) Fluorene	15.50	166	540988	10.525	ng/ul 99
69) Phenanthrene	17.24	178	6341729	88.333	ng/ul 99
71) Anthracene	17.33	178	1723546	23.421	ng/ul 99
74) Carbazole	17.60	167	706479	11.039	ng/ul 99
76) Fluoranthene	19.26	202	7111980	86.443	ng/ul 100
79) Pyrene	19.62	202	5838433	78.169	ng/ul 97
82) Benzo(a)anthracene	21.36	228	3694829	48.951	ng/ul 98
83) Bis(2-ethylhexyl)phthalate	21.29	149	258116	5.028	ng/ul 100
84) Chrysene	21.42	228	3154513	45.040	ng/ul 97
87) Benzo(b)fluoranthene	22.98	252	3850483	48.352	ng/ul 99
88) Benzo(k)fluoranthene	23.02	252	1344284m	17.661	ng/ul
90) Benzo(a)pyrene	23.57	252	2623987	34.634	ng/ul 98
91) Indeno(1,2,3-cd)pyrene	25.98	276	1574132	17.591	ng/ul 97
92) Dibenzo(a,h)anthracene	25.98	278	518958	6.845	ng/ul# 89
93) Benzo(a,h,i)perylene	26.70	276	1093240	15.059	ng/ul 99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060719\
Data File : BM020803.D
Acq On : 07 Jun 2019 14:37
Operator : HP/JU
Sample : K3201-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:55 AM

Quant Time: Jun 08 01:29:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 08 00:20:16 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060719\
Data File : BM020803.D
Acq On : 07 Jun 2019 14:37
Operator : HP/JU
Sample : K3201-11
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
C0AC2

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:55 AM

Quant Time: Jun 08 01:29:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 08 00:20:16 2019
Response via : Initial Calibration

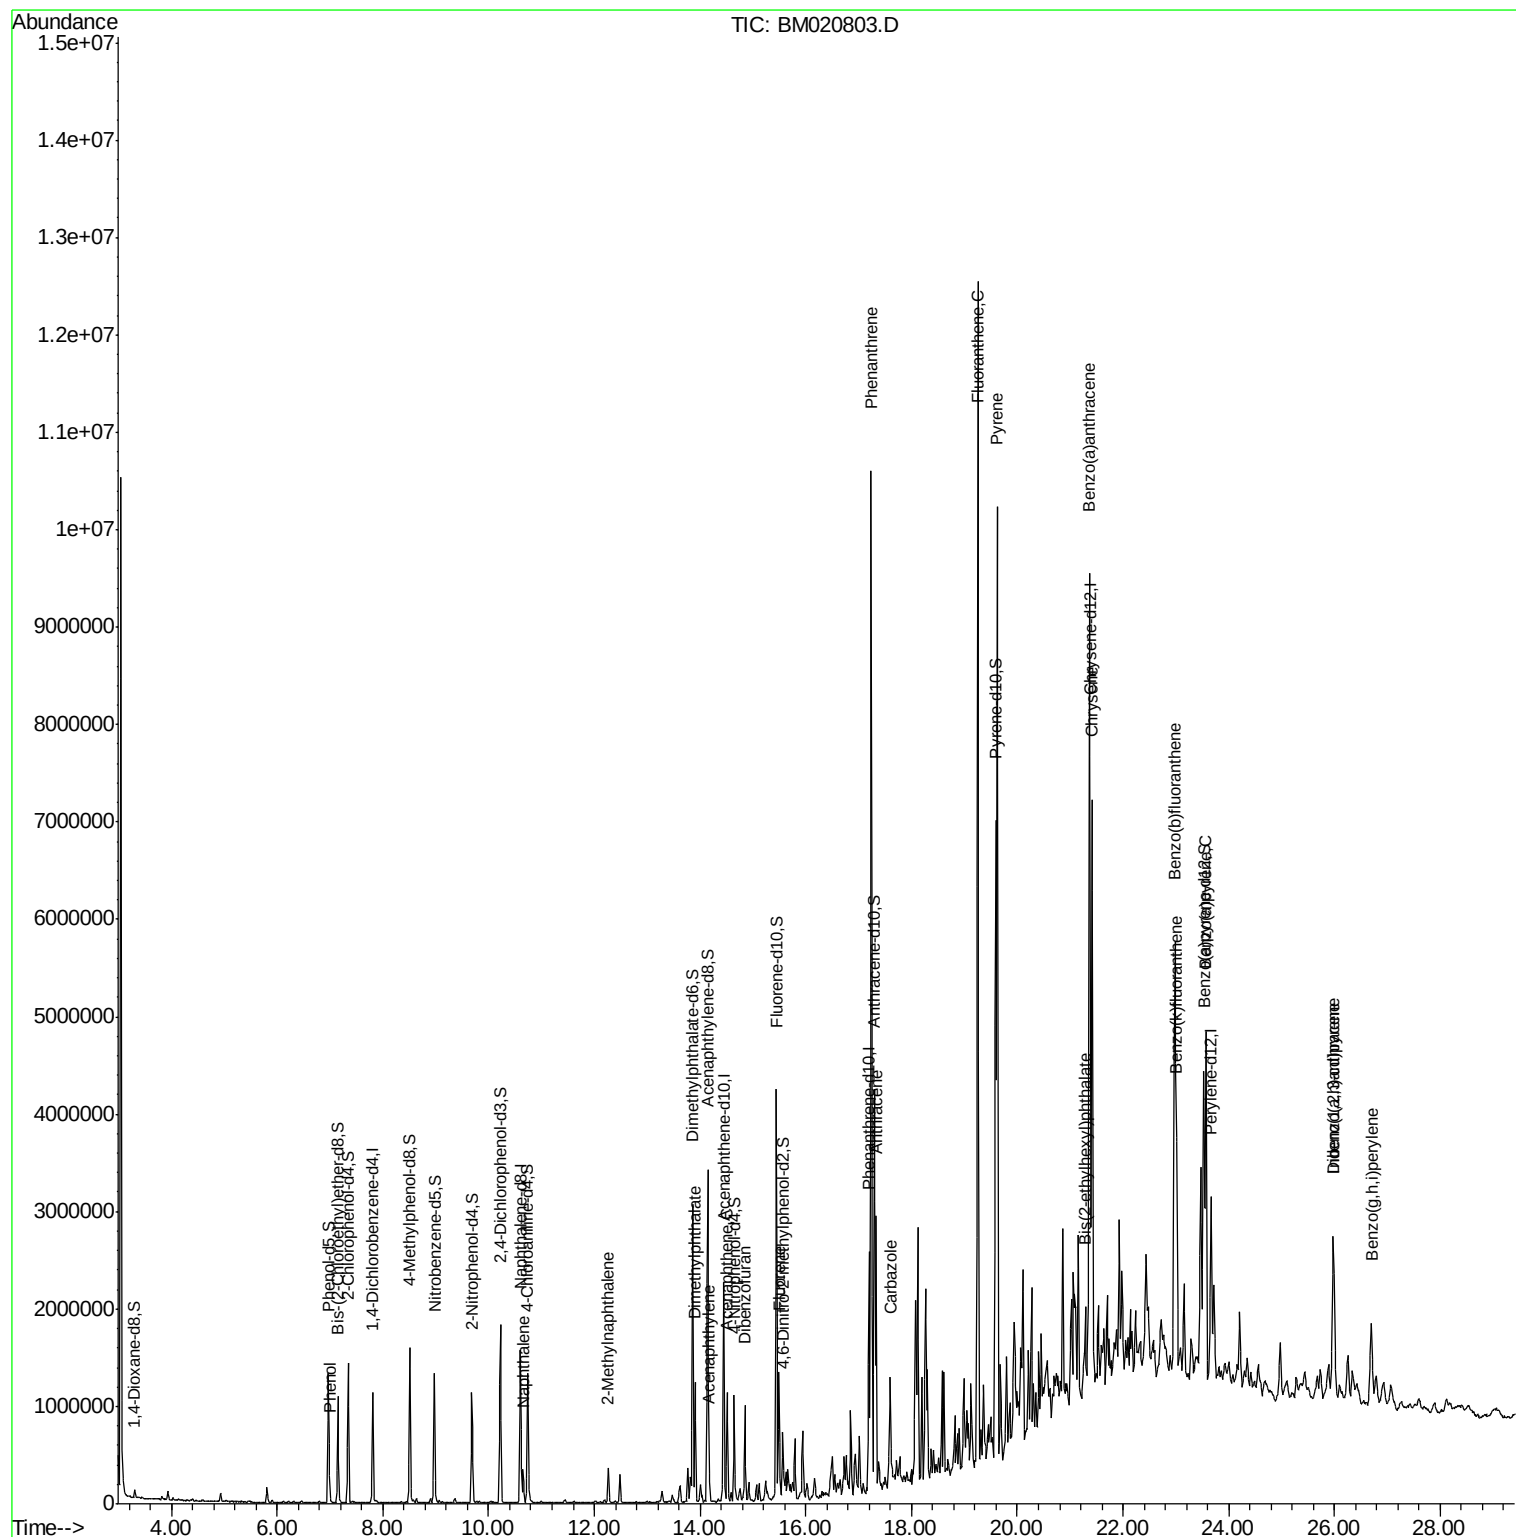

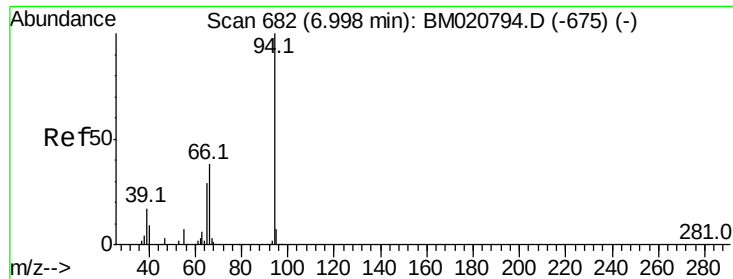

#6

Phenol





Concen: 1.095 ng/ul
 RT: 7.00 min Scan# 682
 Delta R.T. 0.00 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Instrument :
 BNA_M
 ClientSampled :
 C0AC2

Tot Ion	Ratio	Lower	Upper
94	100		
65	30.9	23.3	34.9
66	46.4	32.1	48.1

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:41:55 AM

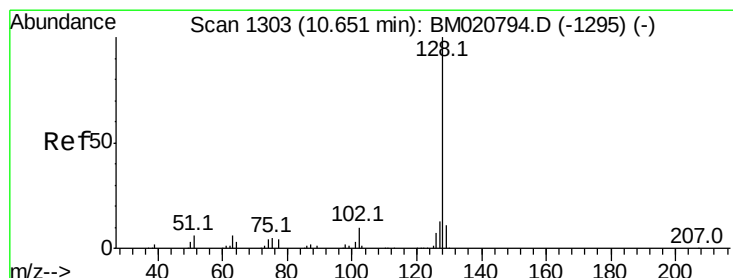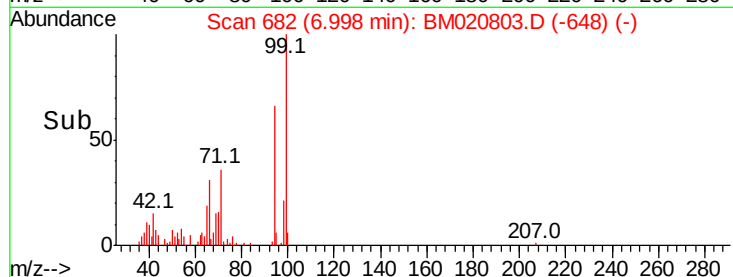
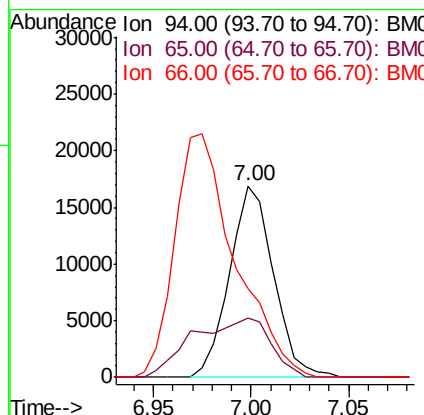
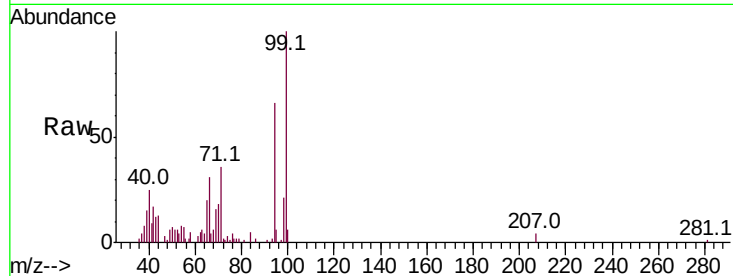



#28

Naphthalene

Concen: 4.542 ng/ul
 RT: 10.65 min Scan# 1303
 Delta R.T. 0.00 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.4	8.6	13.0
127	12.7	10.2	15.2

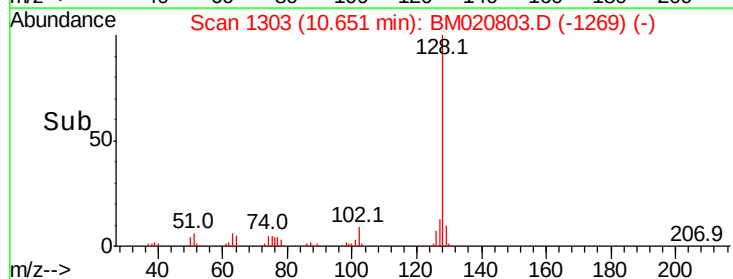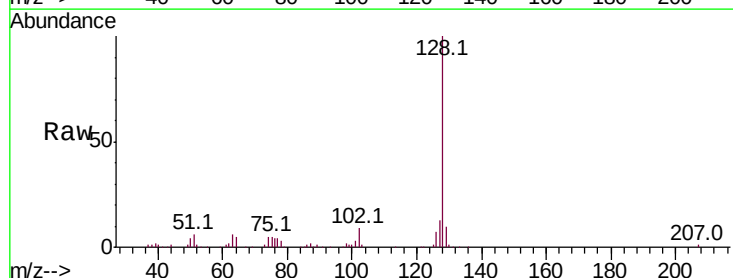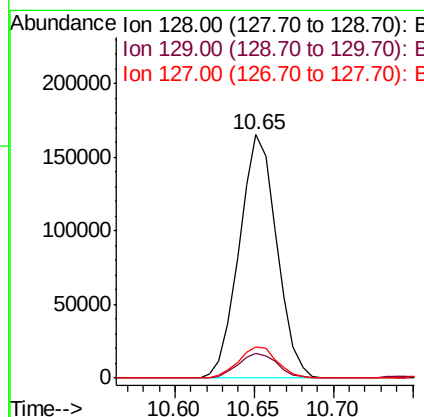

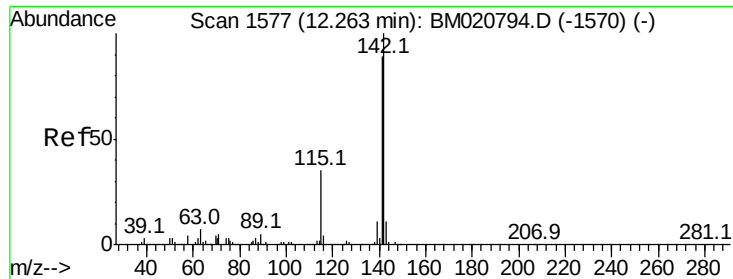





#34
 2-Methylnaphthalene
 Concen: 3.861 ng/ul
 RT: 12.26 min Scan# 1577
 Delta R.T. 0.00 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Tot Ion	Ratio	Lower	Upper
142	100		
141	85.3	71.4	107.0




Manual Integrations
 APPROVED


mohammad
 6/14/2019 8:41:55 AM

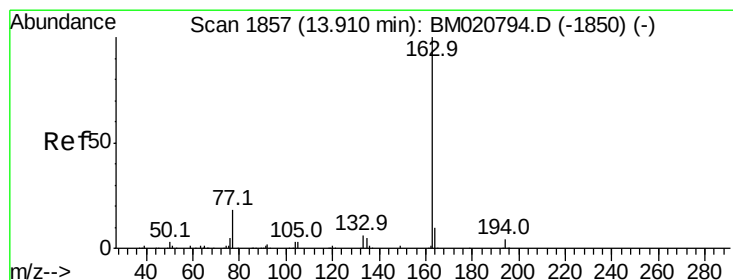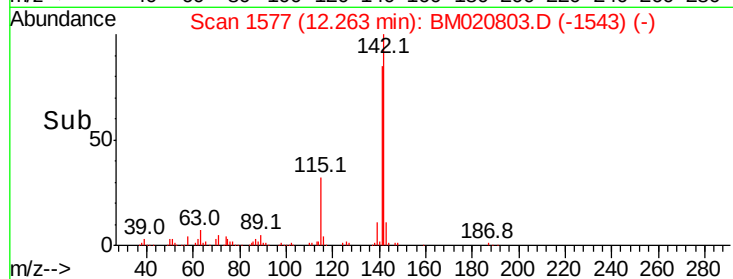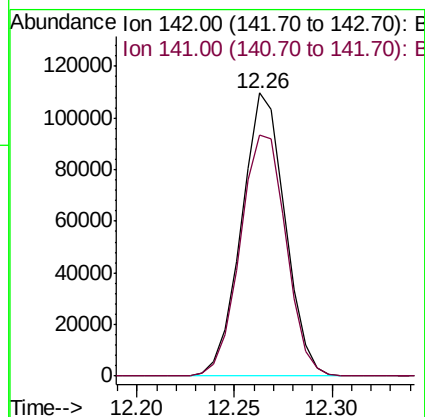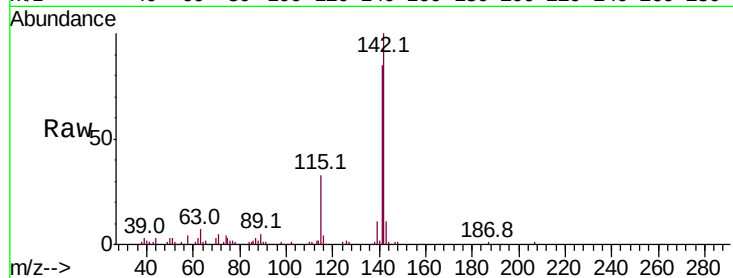

#44
 Dimethylphthalate
 Concen: 15.089 ng/ul
 RT: 13.91 min Scan# 1857
 Delta R.T. 0.00 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.1	8.0	12.0

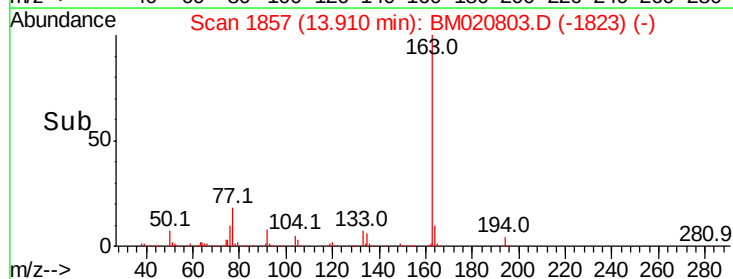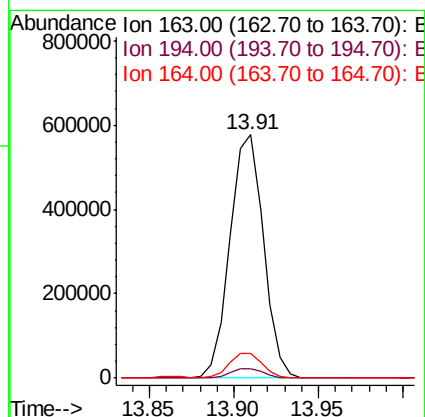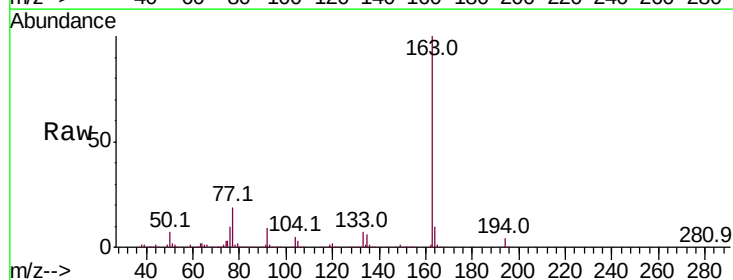

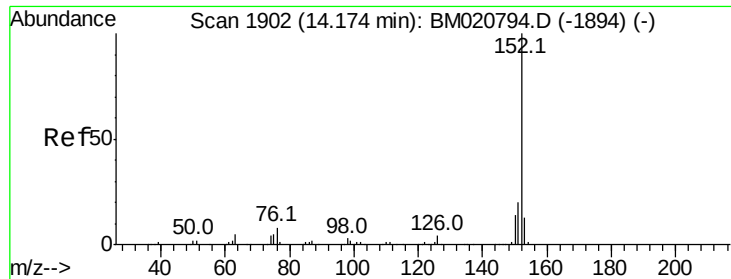

#47

Acenaphthylene

Concen: 2.009 ng/ul

RT: 14.17 min Scan# 1902

Delta R.T. 0.00 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37

Instrument :

BNA_M





ClientSampleId :

C0AC2

Tot Ion:	152	Resp:	130291
Ion Ratio	Lower	Upper	
152	100		
151	19.7	16.2	24.2
153	16.8	10.6	15.8#

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:55 AM

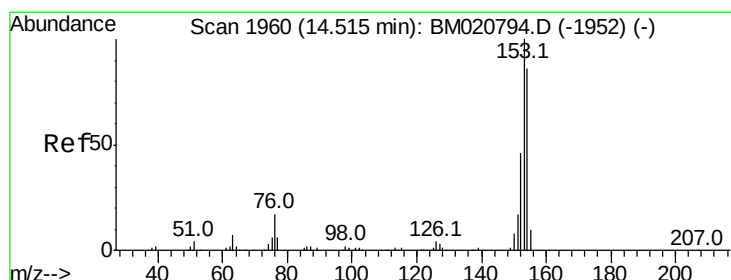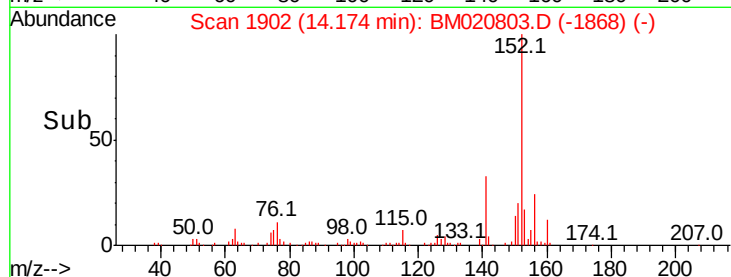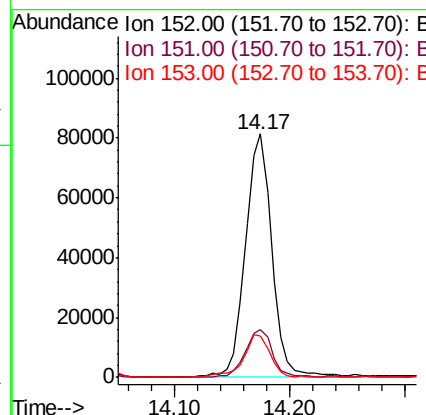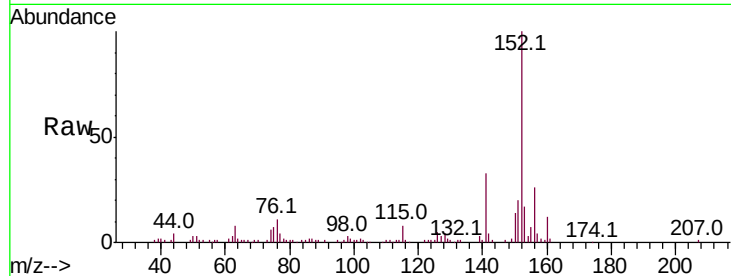

#49

Acenaphthene

Concen: 10.429 ng/ul




RT: 14.51 min Scan# 1959


Delta R.T. -0.01 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37

Tgt Ion:	153	Resp:	472080
Ion Ratio	Lower	Upper	
153	100		
152	47.2	37.3	55.9
154	87.6	68.7	103.1

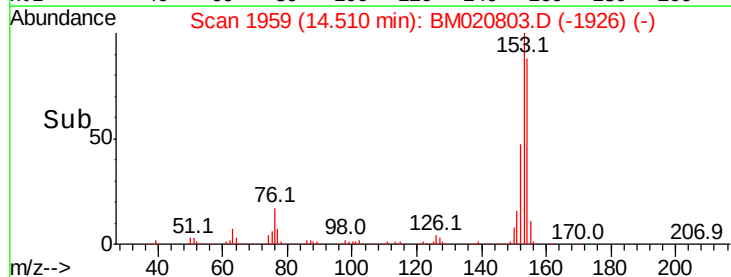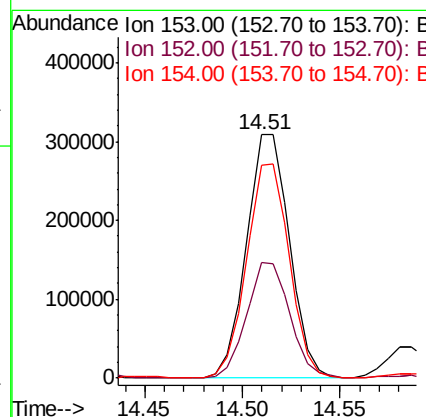

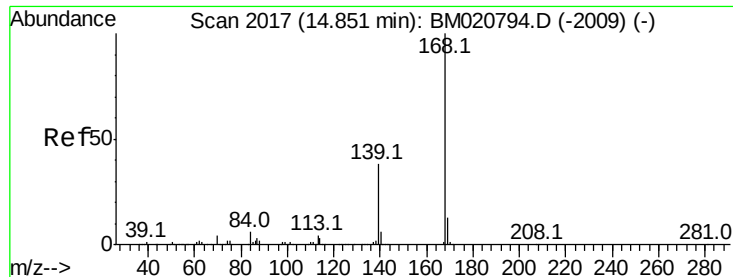

#53

Dibenzenofuran

Concen: 8.415 ng/ul

RT: 14.85 min Scan# 2017

Delta R.T. 0.00 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37

Instrument :

BNA_M

ClientSampleId :

C0AC2

Tot Ion:168 Resp: 538763

Ion Ratio Lower Upper

168 100


139 38.1 30.4 45.6

Manual Integrations

APPROVED

mohammad

6/14/2019 8:41:55 AM

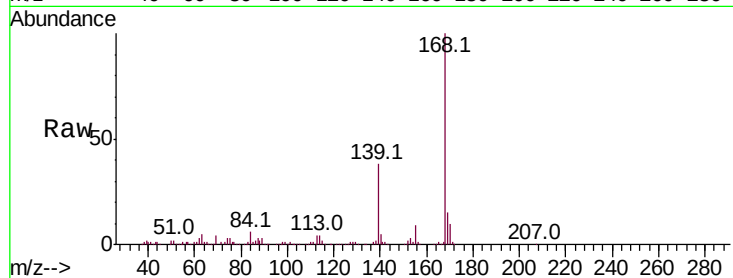

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

400000



300000

200000

100000

0

Time-->

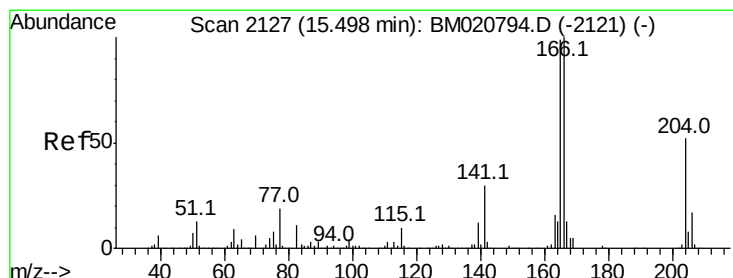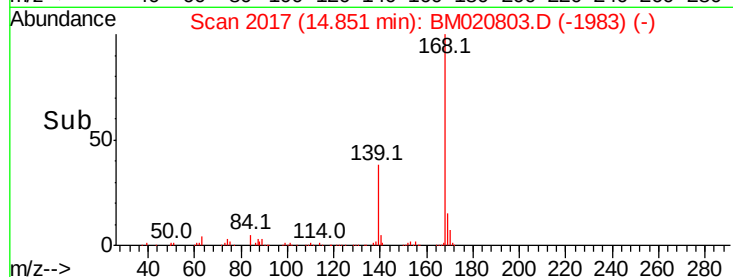

#58

Fluorene

Concen: 10.525 ng/ul

RT: 15.50 min Scan# 2127

Delta R.T. 0.00 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37


Tgt Ion:166 Resp: 540988

Ion Ratio Lower Upper

166 100

165 97.5 78.6 117.8

167 13.9 10.8 16.2

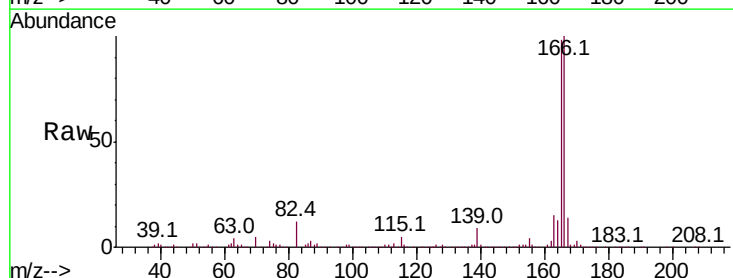

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

500000

400000


300000


200000

100000

0

Time-->

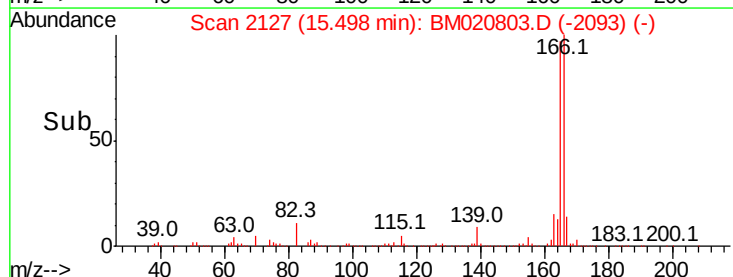

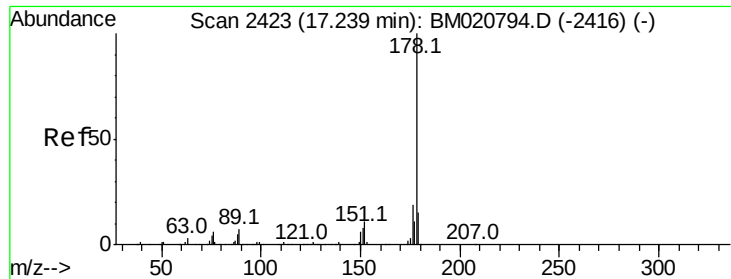





#69
Phenanthrene
Concen: 88.333 ng/ul
RT: 17.24 min Scan# 2423
Delta R.T. 0.00 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Instrument :
BNA_M
ClientSampleId :
C0AC2

Tot Ion:178 Resp: 6341729
Ion Ratio Lower Upper
178 100
179 15.7 12.3 18.5
176 19.3 14.8 22.2



Manual Integrations
APPROVED


mohammad
6/14/2019 8:41:55 AM

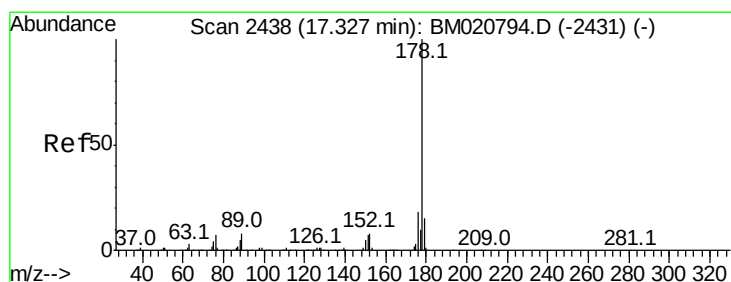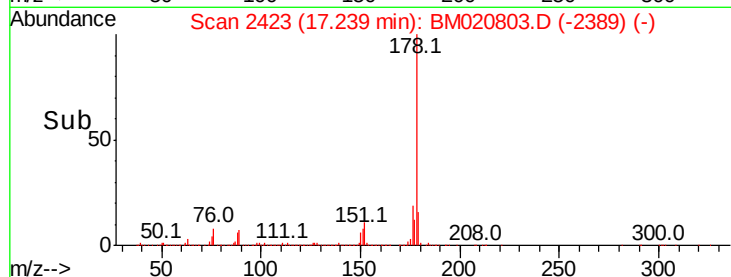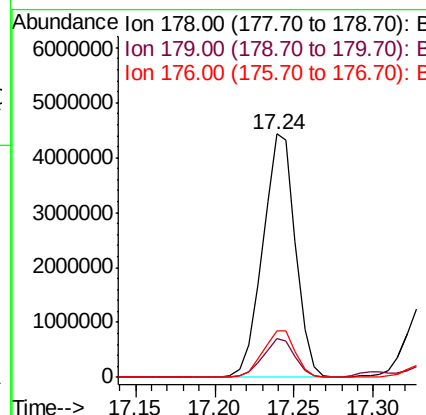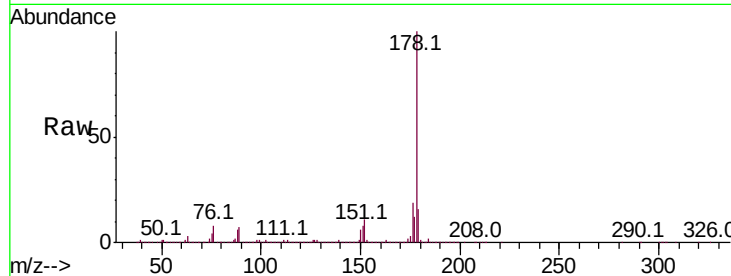

#71
Anthracene
Concen: 23.421 ng/ul
RT: 17.33 min Scan# 2438
Delta R.T. 0.00 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Tgt Ion:178 Resp: 1723546
Ion Ratio Lower Upper
178 100
179 15.6 12.1 18.1
176 18.1 14.9 22.3

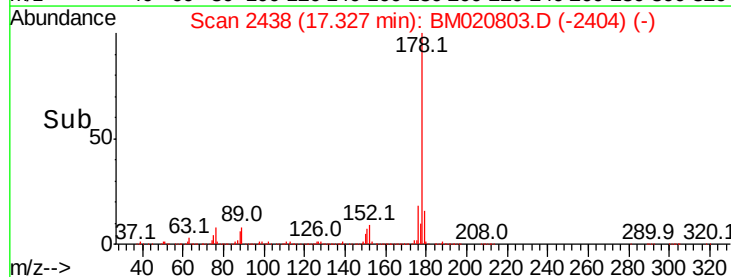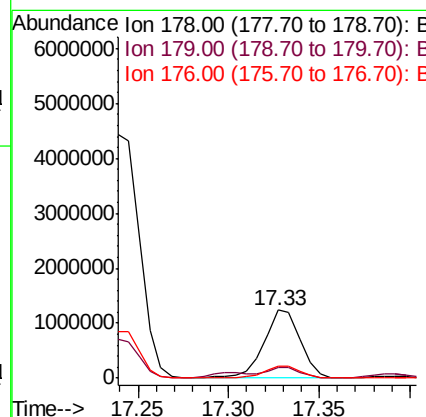

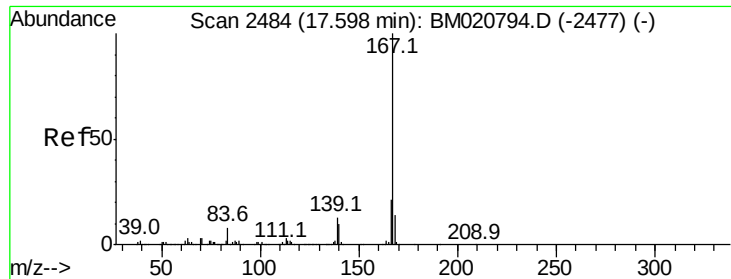





#74
 Carbazole
 Concen: 11.039 ng/ul
 RT: 17.60 min Scan# 2484
 Delta R.T. 0.00 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Tot Ion	Ratio	Lower	Upper
167	100		
166	22.0	17.0	25.6
139	13.2	10.5	15.7




Manual Integrations
 APPROVED


mohammad
 6/14/2019 8:41:55 AM

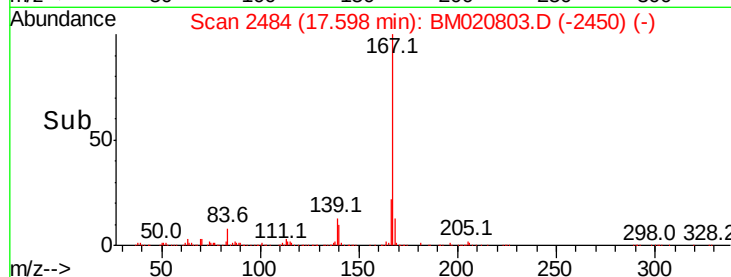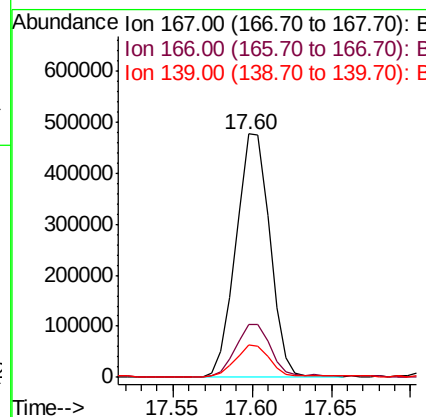

#76
 Fluoranthene
 Concen: 86.443 ng/ul
 RT: 19.26 min Scan# 2766
 Delta R.T. 0.01 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.8	7.9	11.9
100	7.6	6.2	9.4

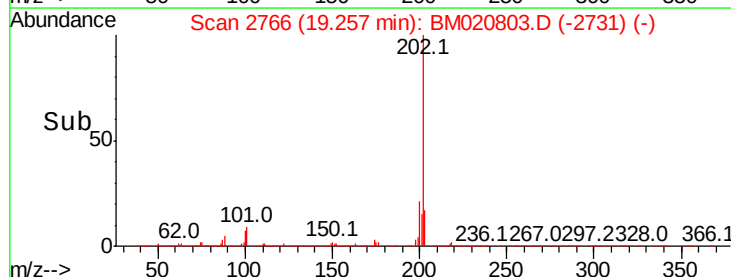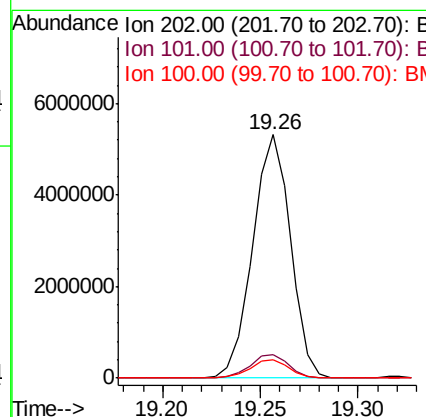

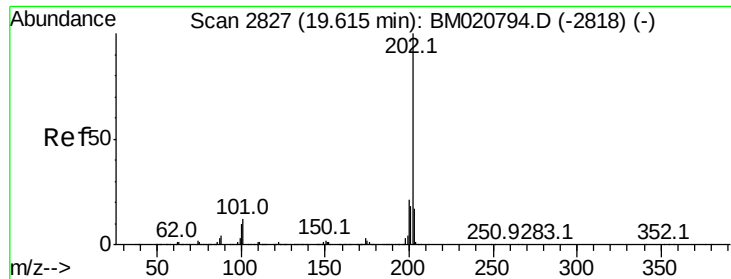





#79
Pvrene
Concen: 78.169 ng/ul
RT: 19.62 min Scan# 2828
Delta R.T. 0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Instrument :
BNA_M
ClientSampleId :
C0AC2

Tot Ion	Ratio	Lower	Upper
202	100		
101	11.2	9.8	14.6
100	9.1	8.0	12.0




Manual Integrations
APPROVED


mohammad
6/14/2019 8:41:55 AM

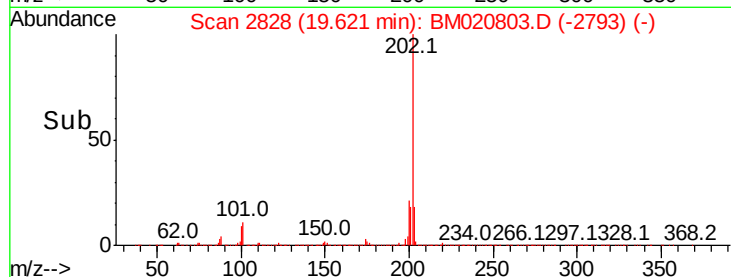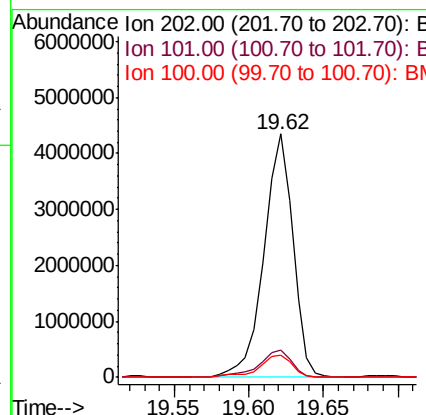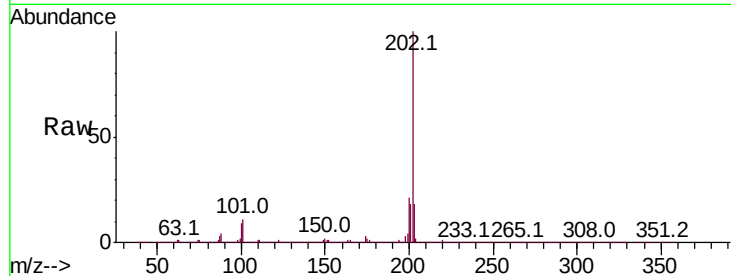

#82
Benzo(a)anthracene
Concen: 48.951 ng/ul
RT: 21.36 min Scan# 3124
Delta R.T. 0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.8	15.6	23.4
226	27.8	21.4	32.2

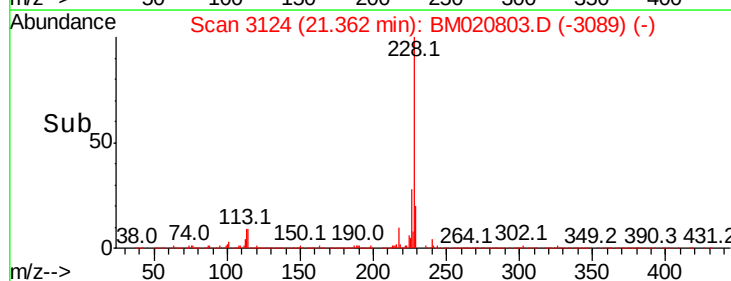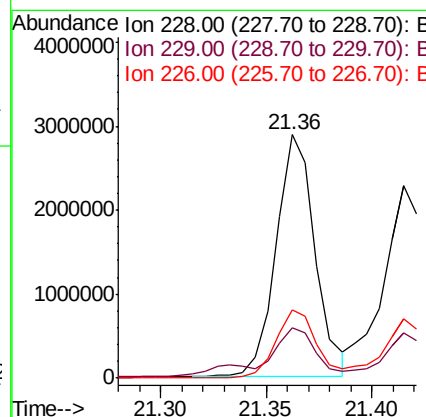

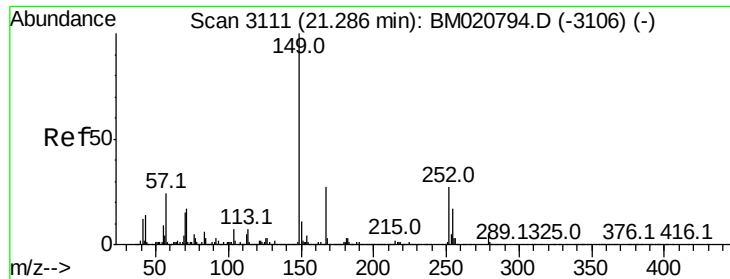





#83
 Bis(2-ethylhexyl)phthalate
 Concen: 5.028 ng/ul
 RT: 21.29 min Scan# 3112
 Delta R.T. 0.01 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Tot Ion	Ratio	Lower	Upper
149	100		
167	27.4	21.9	32.9
279	5.2	4.1	6.1




Manual Integrations
 APPROVED


mohammad
 6/14/2019 8:41:55 AM

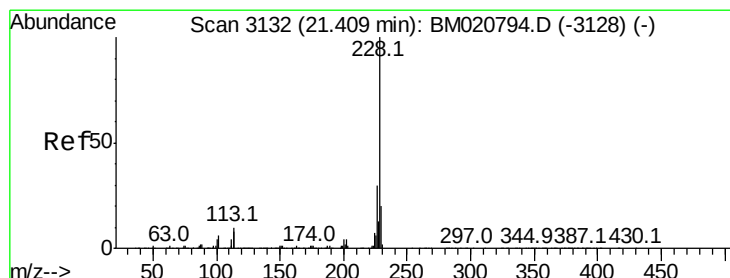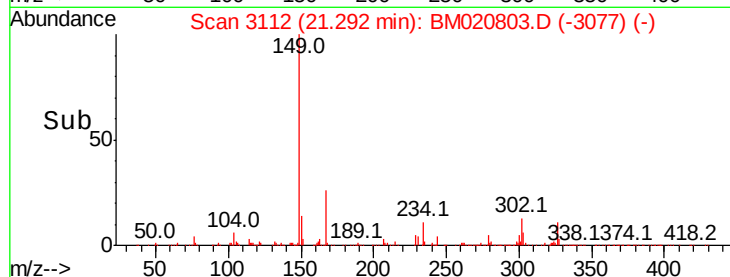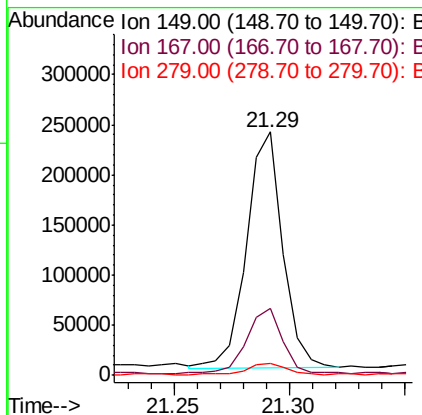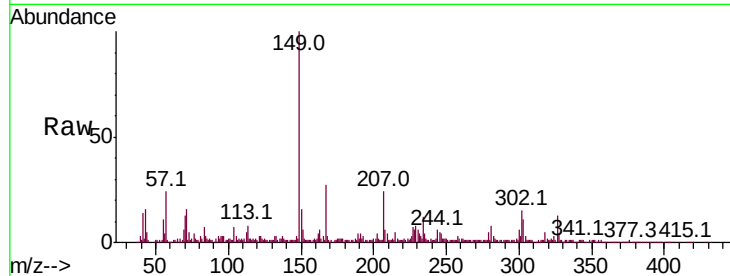

#84
 Chrysene
 Concen: 45.040 ng/ul
 RT: 21.42 min Scan# 3133
 Delta R.T. 0.01 min
 Lab File: BM020803.D
 Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.6	24.4	36.6
229	23.3	16.2	24.2

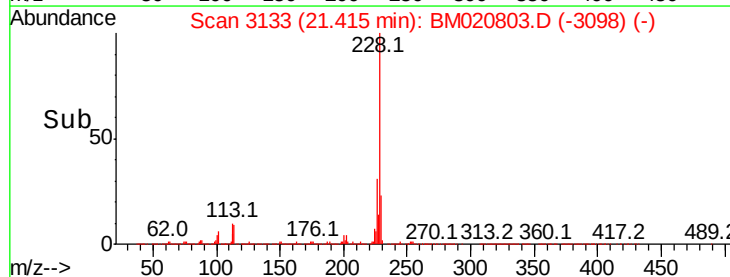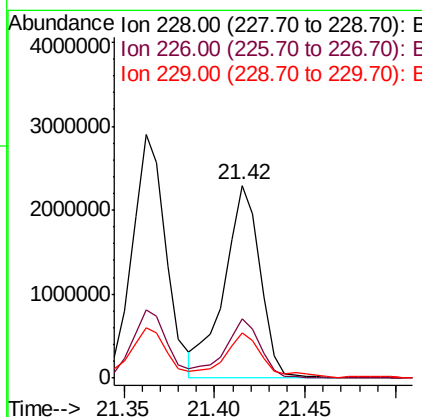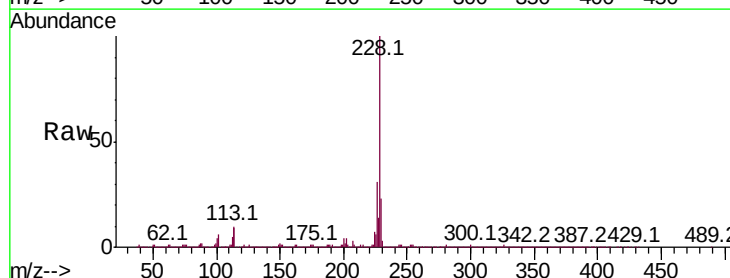

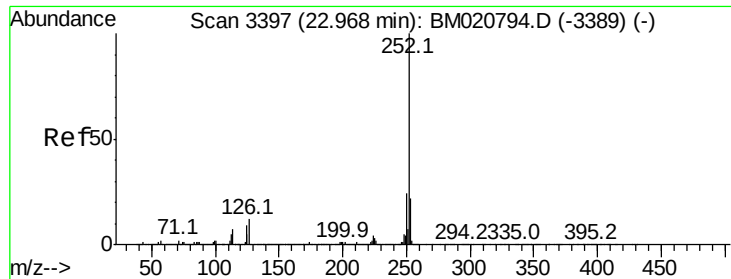





#87
Benzo(b)fluoranthene
Concen: 48.352 ng/ul
RT: 22.98 min Scan# 3399
Delta R.T. 0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Instrument :
BNA_M
ClientSampleId :
C0AC2

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.6	26.4
125	9.3	7.3	10.9




Manual Integrations
APPROVED


mohammad
6/14/2019 8:41:55 AM

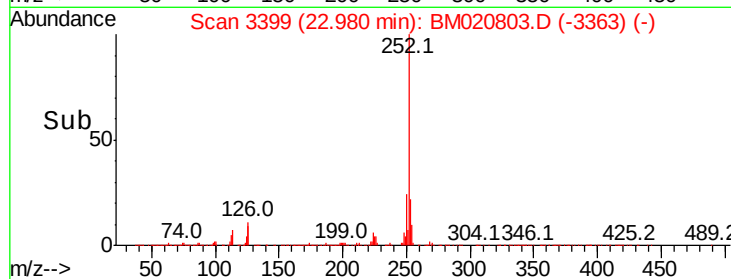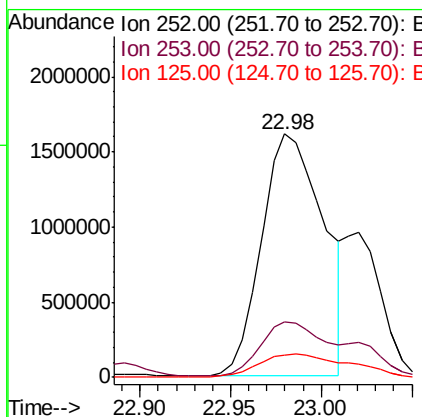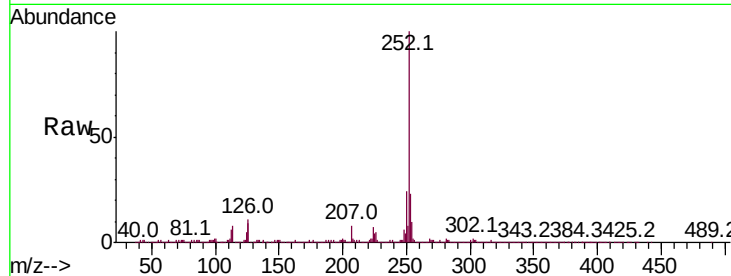

#88
Benzo(k)fluoranthene
Concen: 17.661 ng/ul m
RT: 23.02 min Scan# 3406
Delta R.T. 0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.6	26.4
125	9.2	7.3	10.9

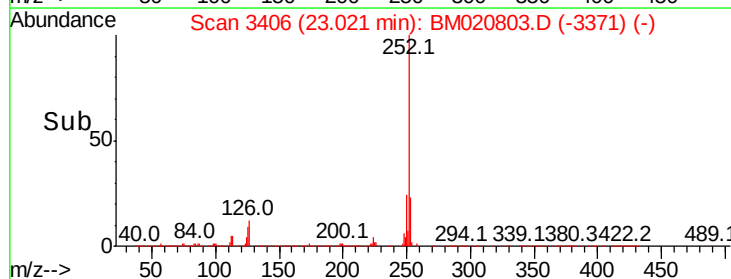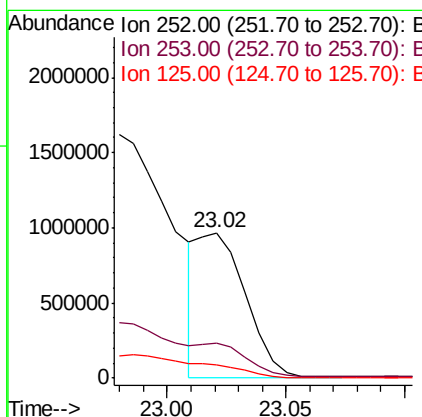

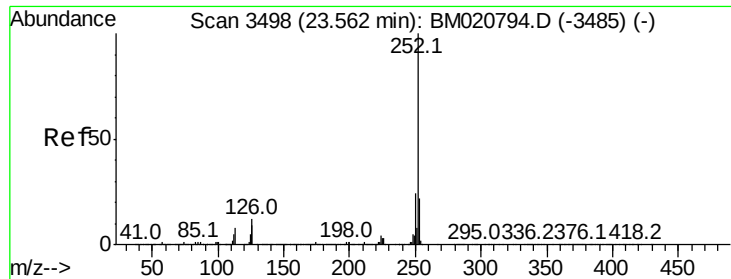

#90

Benzo(a)pyrene

Concen: 34.634 ng/ul

RT: 23.57 min Scan# 3499

Delta R.T. 0.01 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37

Instrument :

BNA_M

ClientSampleId :

C0AC2

Tot Ion:252 Resp: 2623987

Ion Ratio Lower Upper

252 100

253 22.5


125 9.9

17.0 25.6




8.2 12.4

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:55 AM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

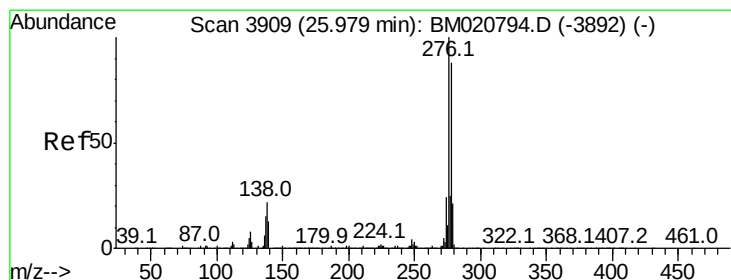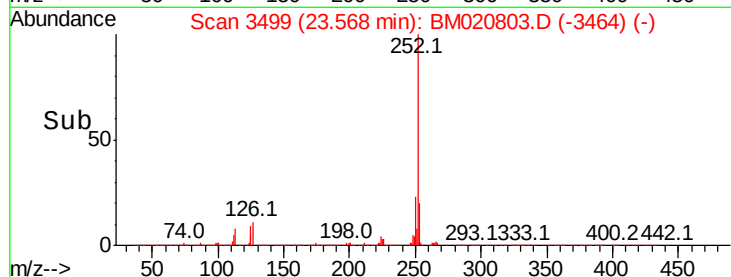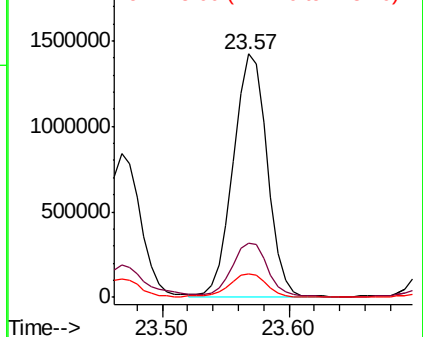

#91

Indeno(1,2,3-cd)pyrene

Concen: 17.591 ng/ul

RT: 25.98 min Scan# 3909

Delta R.T. 0.00 min

Lab File: BM020803.D

Acq: 07 Jun 2019 14:37

Tgt Ion:276 Resp: 1574132

Ion Ratio Lower Upper

276 100




138 19.7


277 25.5

17.8 26.8

20.0 30.0

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

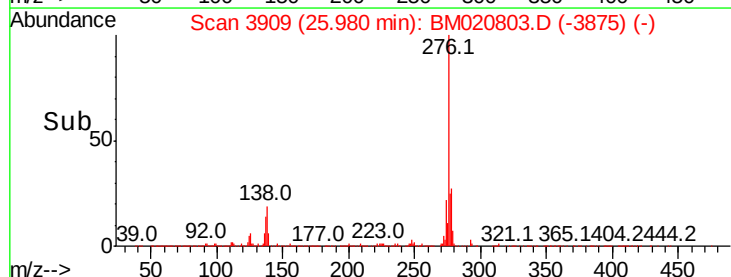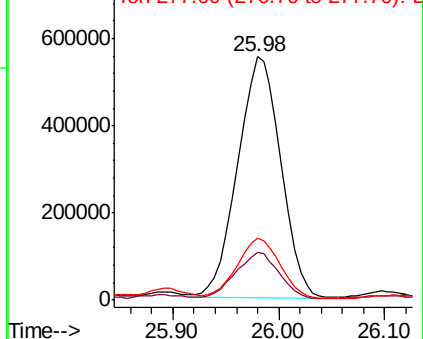

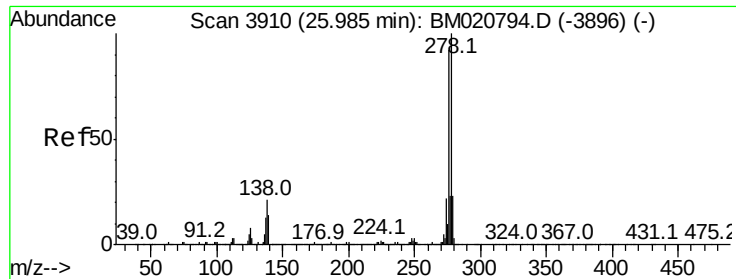





#92
Dibenzo(a,h)anthracene
Concen: 6.845 ng/ul
RT: 25.98 min Scan# 3909
Delta R.T. -0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Instrument :
BNA_M
ClientSampleId :
C0AC2

Tot Ion	Ratio	Lower	Upper
278	100		
139	20.4	11.6	17.4#
279	27.9	18.6	28.0

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:55 AM

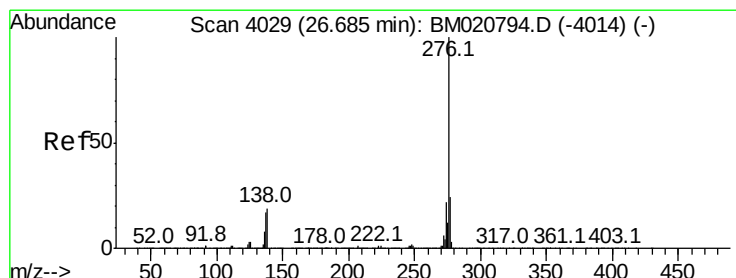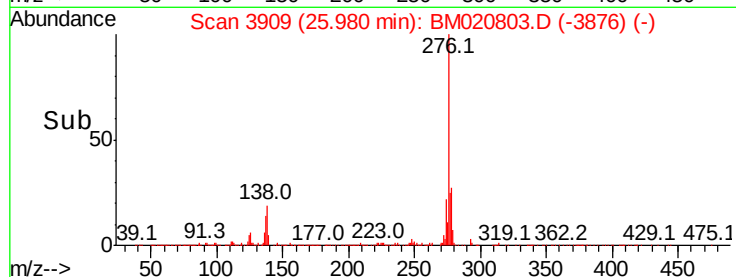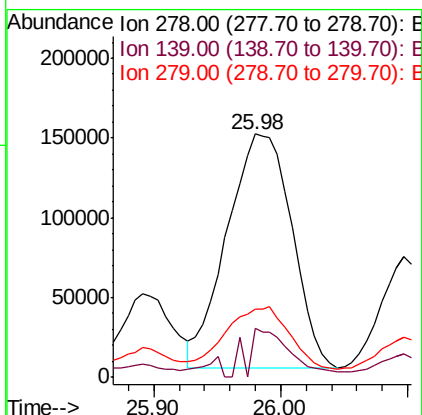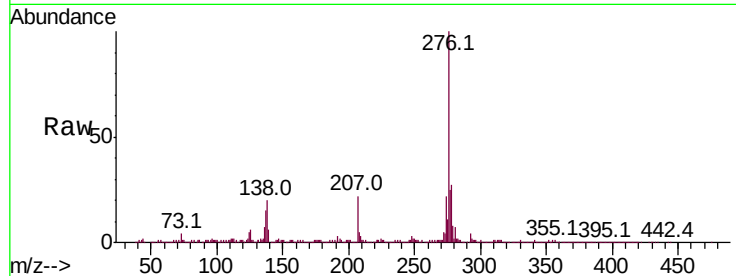

#93
Benzo(g,h,i)perylene
Concen: 15.059 ng/ul
RT: 26.70 min Scan# 4031
Delta R.T. 0.01 min
Lab File: BM020803.D
Acq: 07 Jun 2019 14:37

Tgt Ion	Ratio	Lower	Upper
276	100		
138	20.4	16.6	25.0
277	25.1	19.6	29.4

