

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060719\
 Data File : BM020806.D
 Acq On : 07 Jun 2019 16:26
 Operator : HP/JU
 Sample : K3201-20DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 C0AD1DL

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:41:50 AM

Quant Time: Jun 08 01:43:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 08 00:20:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	300193	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1192901	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	659199	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	1454770	20.00	ng/ul	0.00
77) Chrysene-d12	21.38	240	1378327	20.00	ng/ul	0.00
85) Perylene-d12	23.67	264	1638737	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	9448	1.50	ng/uL	0.00
5) Phenol-d5	6.97	99	141822	6.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	98543	7.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	133641	7.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	103231	5.59	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	63706	7.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	63978	7.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	126071	7.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	137989	6.55	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	392453	8.05	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	476763	7.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	36749	4.39	ng/ul	0.00
57) Fluorene-d10	15.45	176	329987	7.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	16264	2.19	ng/ul	0.00
70) Anthracene-d10	17.29	188	500746	7.88	ng/ul	0.00
78) Pyrene-d10	19.59	212	521611	7.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.52	264	560833	7.53	ng/ul	0.00

Target Compounds

					Ovalue
44) Dimethylphthalate	13.91	163	137096	2.808	ng/ul 100
47) Acenaphthylene	14.17	152	65926	1.102	ng/ul 97
49) Acenaphthene	14.51	153	106474	2.550	ng/ul 99
53) Dibenzofuran	14.85	168	112374	1.903	ng/ul 98
58) Fluorene	15.50	166	140114	2.955	ng/ul 95
69) Phenanthrene	17.24	178	2229267	30.448	ng/ul 99
71) Anthracene	17.33	178	619757	8.258	ng/ul 99
74) Carbazole	17.60	167	142533	2.184	ng/ul 96
76) Fluoranthene	19.26	202	3105234	37.010	ng/ul 99
79) Pyrene	19.62	202	2458529	28.896	ng/ul 99
82) Benzo(a)anthracene	21.36	228	1637716	19.047	ng/ul 97
84) Chrysene	21.42	228	1326443	16.626	ng/ul 97
87) Benzo(b)fluoranthene	22.98	252	1696602	17.797	ng/ul 98
88) Benzo(k)fluoranthene	23.02	252	543084m	5.960	ng/ul
90) Benzo(a)pyrene	23.57	252	1141676	12.588	ng/ul 98
91) Indeno(1,2,3-cd)pyrene	25.98	276	686845	6.412	ng/ul 96
92) Dibenzo(a,h)anthracene	25.98	278	217697	2.398	ng/ul# 90
93) Benzo(g,h,i)perylene	26.69	276	452139	5.203	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060719\
Data File : BM020806.D
Acq On : 07 Jun 2019 16:26
Operator : HP/JU
Sample : K3201-20DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AD1DL

Quant Time: Jun 08 01:43:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 08 00:20:16 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:50 AM

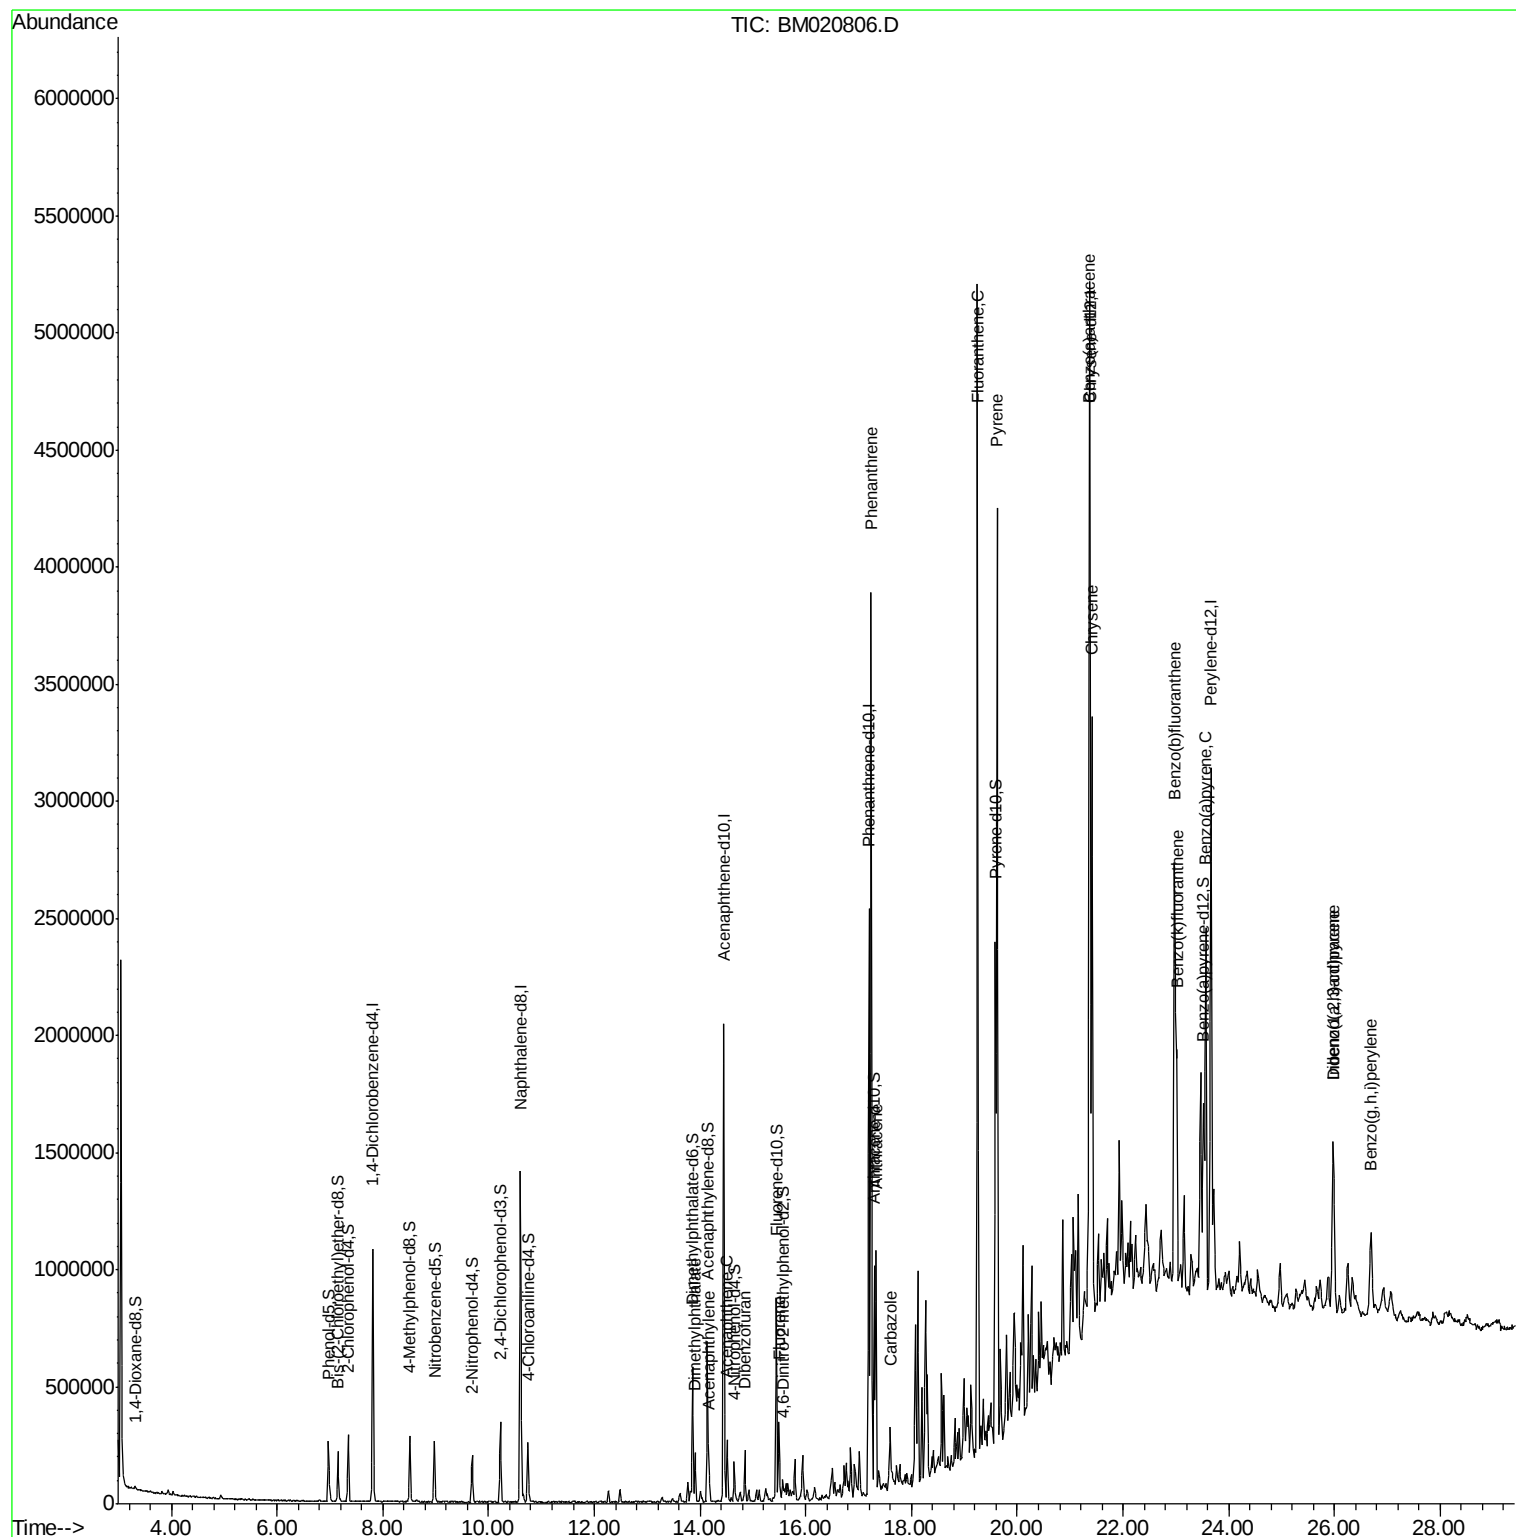

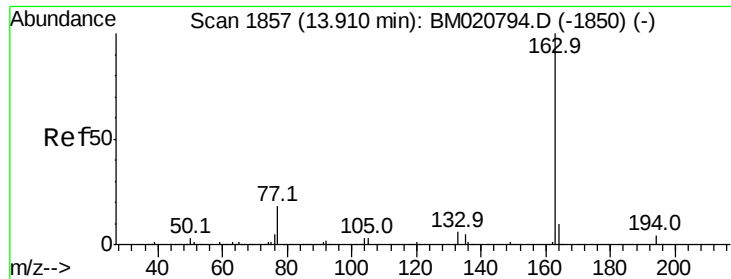

#44

Dimethylphthalate

Concen: 2.808 ng/ul

RT: 13.91 min Scan# 1857

Delta R.T. 0.00 min

Lab File: BM020806.D

Acq: 07 Jun 2019 16:26

Instrument :

BNA_M


ClientSampleId :

C0AD1DL




Tot Ion:	163	Resp:	137096
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.2	4.8
164	10.0	8.0	12.0

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:50 AM

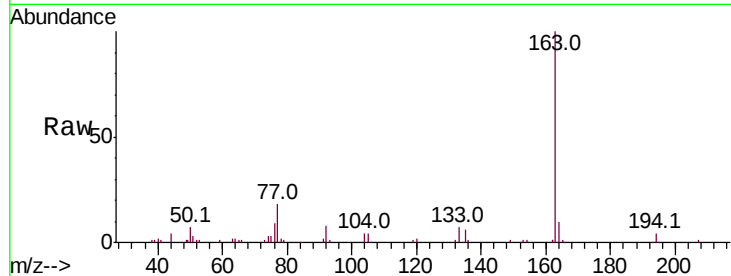

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

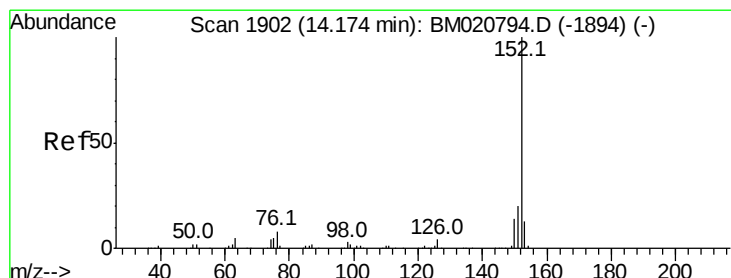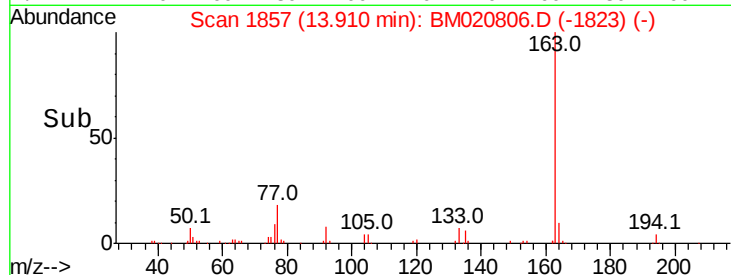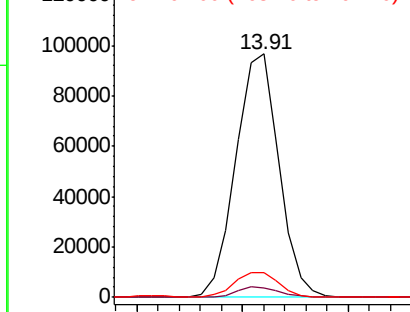

#47

Acenaphthylene

Concen: 1.102 ng/ul


RT: 14.17 min Scan# 1902

Delta R.T. 0.00 min



Lab File: BM020806.D


Acq: 07 Jun 2019 16:26

Tgt Ion:	152	Resp:	65926
Ion Ratio	Lower	Upper	
152	100		
151	20.0	16.2	24.2
153	15.7	10.6	15.8

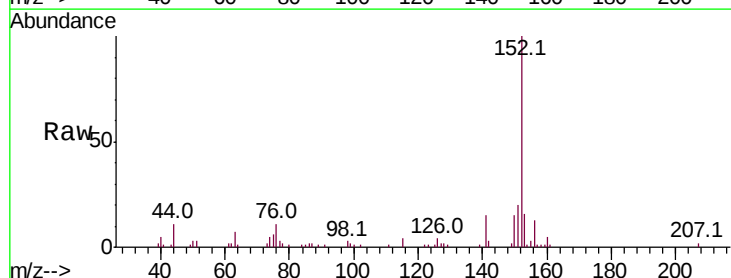

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

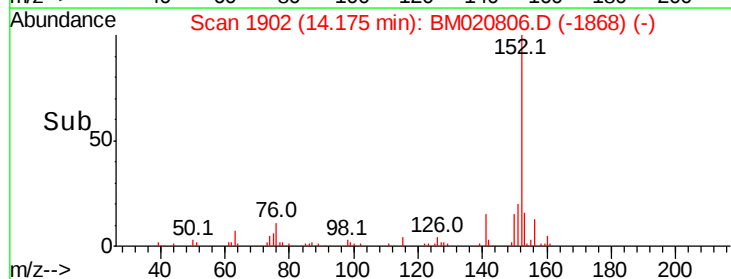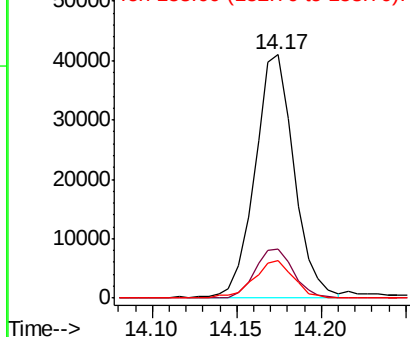

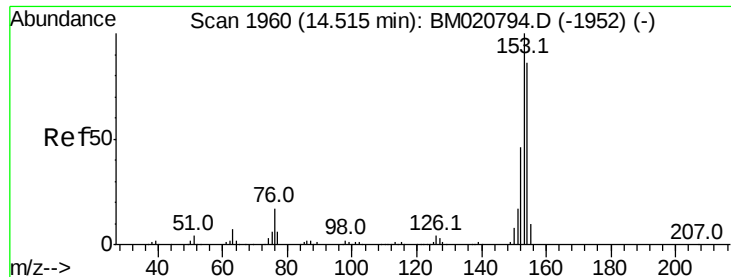


#49
Acenaphthene
Concen: 2.550 ng/ul
RT: 14.51 min Scan# 1959
Delta R.T. -0.01 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Instrument :
BNA_M
ClientSampleId :
C0AD1DL




Tot Ion	Ratio	Lower	Upper
153	100		
152	48.1	37.3	55.9
154	86.3	68.7	103.1

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:50 AM

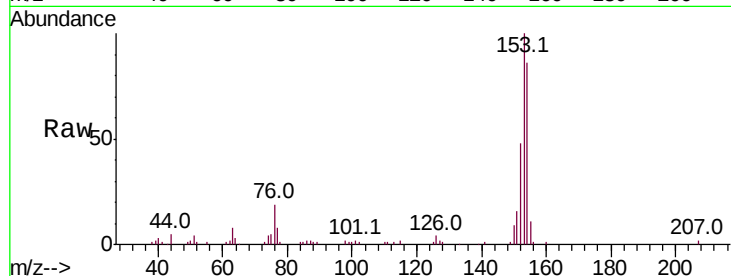


Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

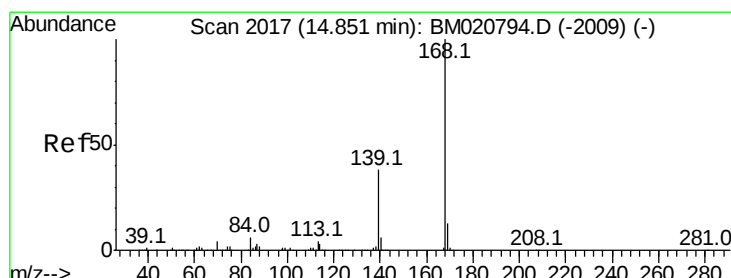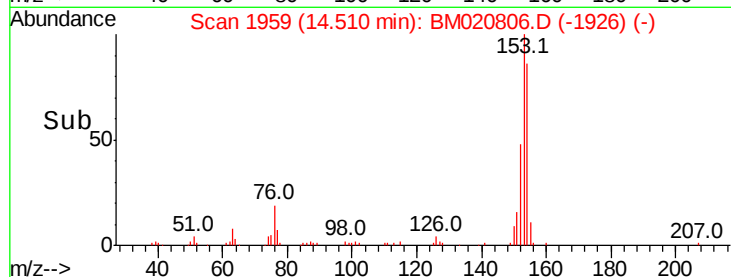
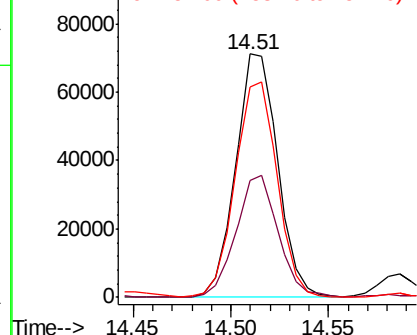



#53
Dibenzofuran
Concen: 1.903 ng/ul
RT: 14.85 min Scan# 2017
Delta R.T. 0.00 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Lower	Upper
168	100		
139	37.1	30.4	45.6

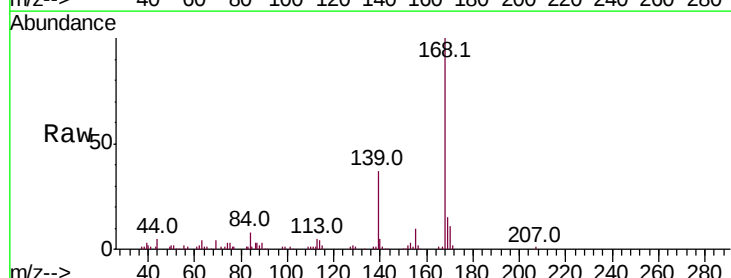

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E

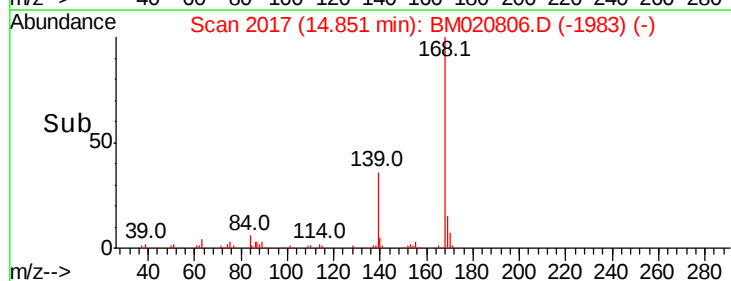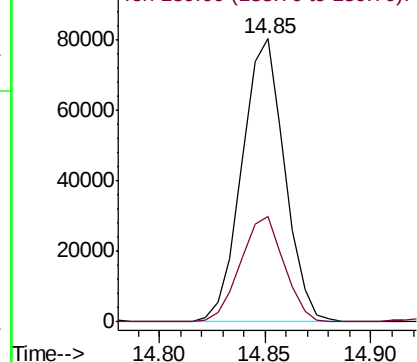

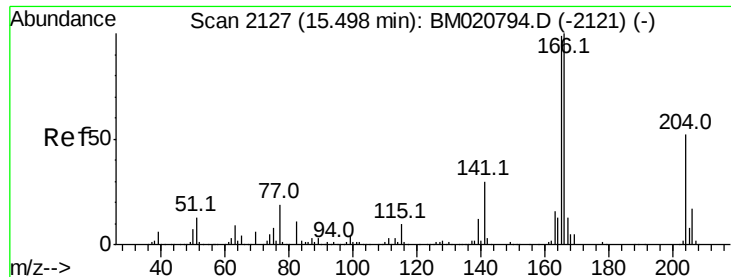





#58
 Fluorene
 Concen: 2.955 ng/ul
 RT: 15.50 min Scan# 2127
 Delta R.T. 0.00 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26

Instrument :
 BNA_M
 ClientSampleId :
 C0AD1DL

Tot Ion	Ratio	Resp	Lower	Upper
166	100	140114		
165	103.6	78.6	117.8	
167	14.6	10.8	16.2	




Manual Integrations
 APPROVED


mohammad
 6/14/2019 8:41:50 AM

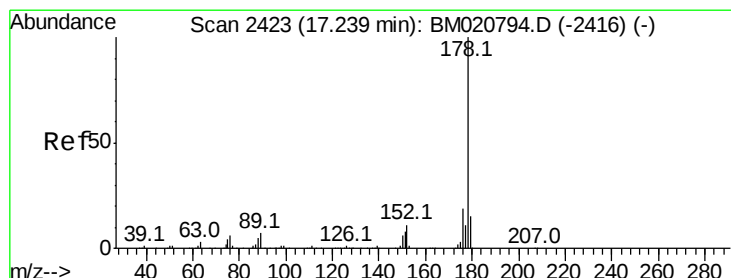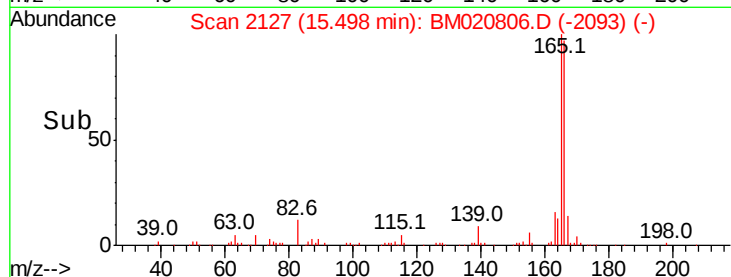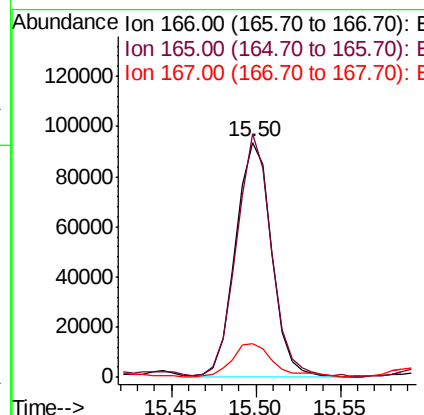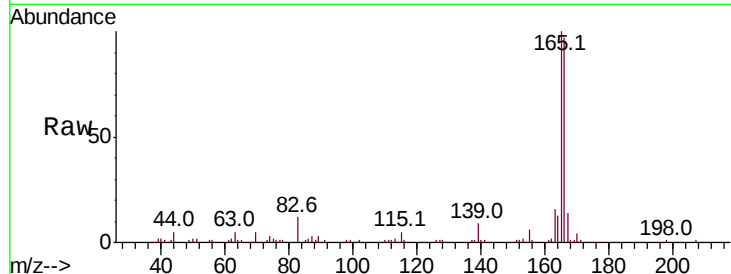

#69
 Phenanthrene
 Concen: 30.448 ng/ul
 RT: 17.24 min Scan# 2423
 Delta R.T. 0.00 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	2229267		
179	15.3	12.3	18.5	
176	19.0	14.8	22.2	

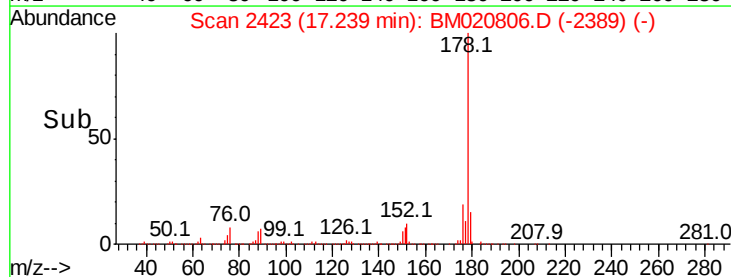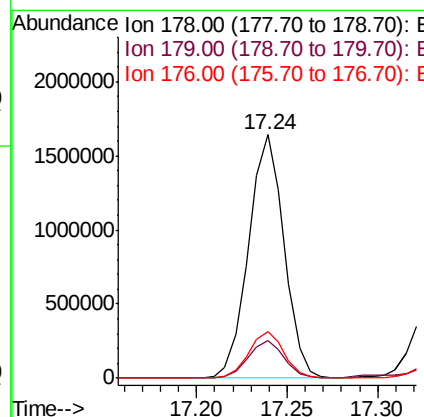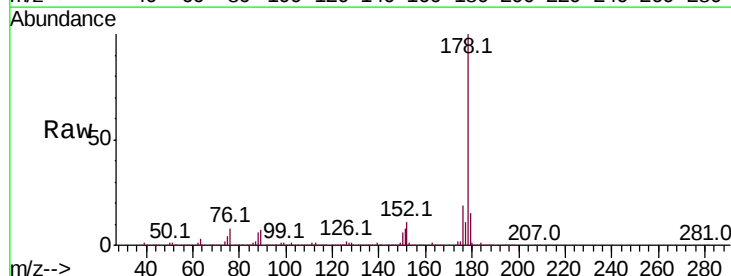

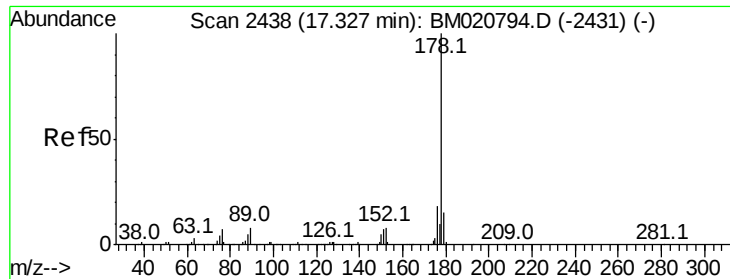





#71
 Anthracene
 Concen: 8.258 ng/ul
 RT: 17.33 min Scan# 2438
 Delta R.T. 0.00 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26

Instrument :
 BNA_M
 ClientSampleId :
 C0AD1DL

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.8	12.1	18.1
176	18.4	14.9	22.3




Manual Integrations
 APPROVED


mohammad
 6/14/2019 8:41:50 AM

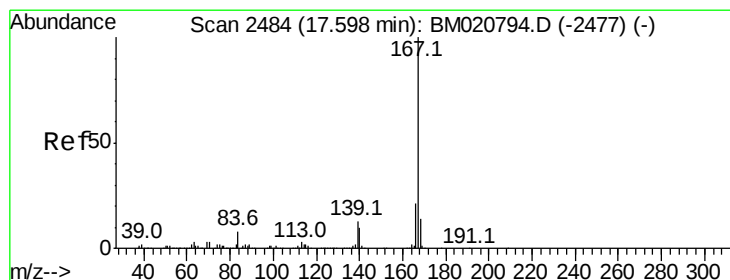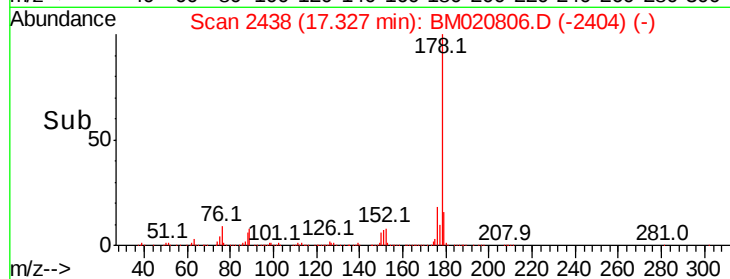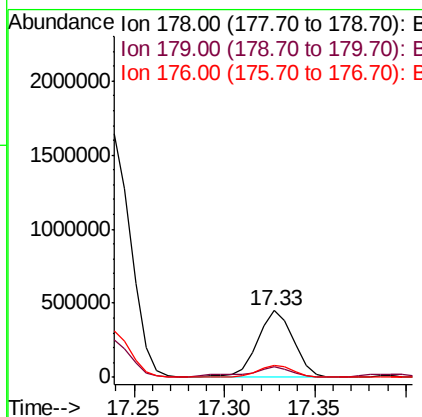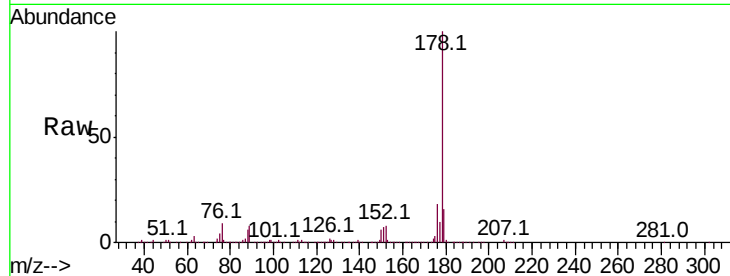

#74
 Carbazole
 Concen: 2.184 ng/ul
 RT: 17.60 min Scan# 2484
 Delta R.T. 0.00 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Lower	Upper
167	100		
166	23.8	17.0	25.6
139	13.8	10.5	15.7

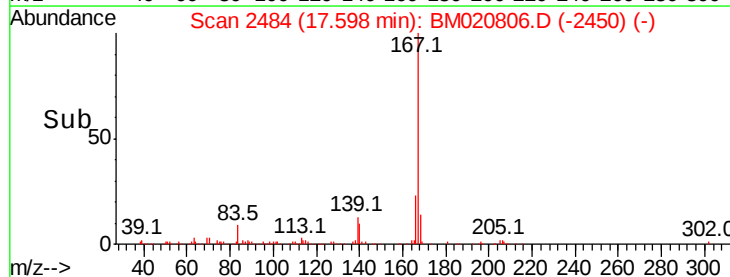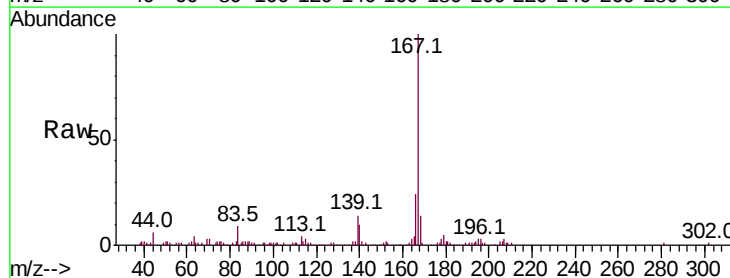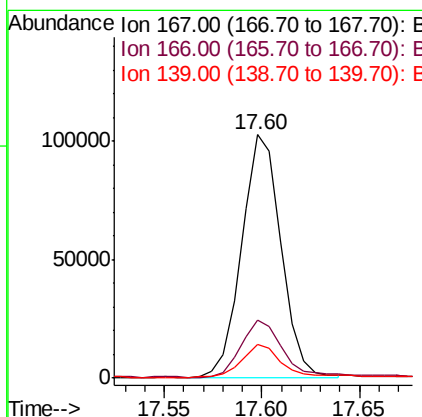

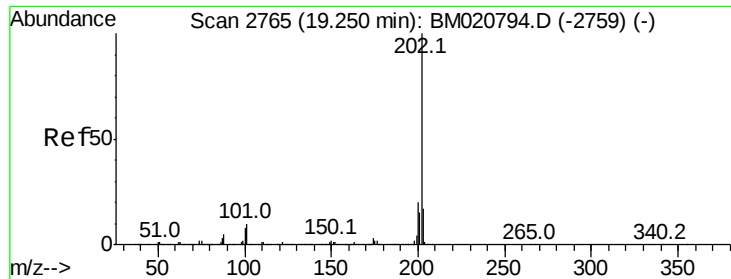


#76
 Fluoranthene
 Concen: 37.010 ng/ul
 RT: 19.26 min Scan# 2766
 Delta R.T. 0.01 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26

Instrument :
 BNA_M
 ClientSampleId :
 C0AD1DL

Tot Ion	Ratio	Lower	Upper
202	100		
101	9.6	7.9	11.9
100	7.3	6.2	9.4

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:41:50 AM



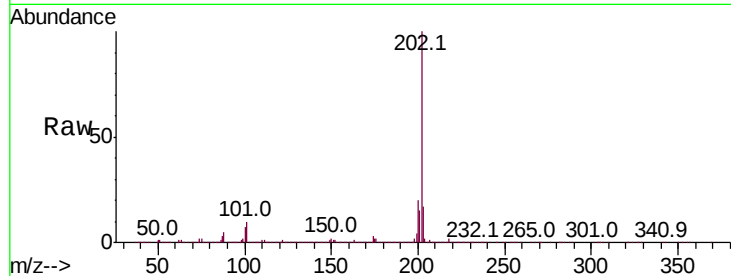


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

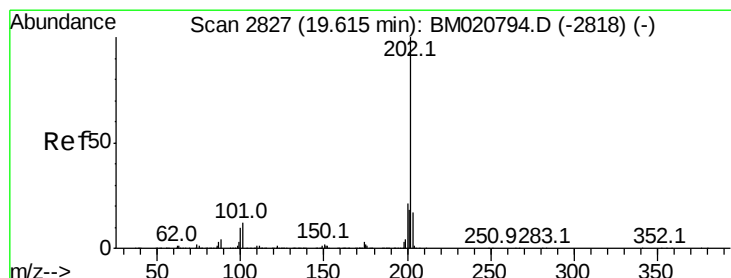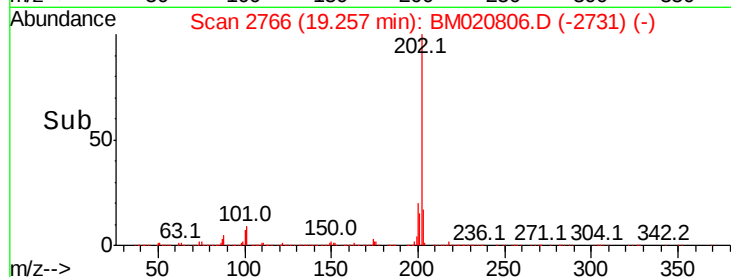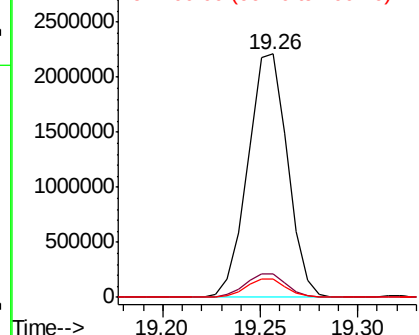

#79
 Pyrene
 Concen: 28.896 ng/ul
 RT: 19.62 min Scan# 2827
 Delta R.T. 0.00 min
 Lab File: BM020806.D
 Acq: 07 Jun 2019 16:26




Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.4	9.8	14.6
100	10.3	8.0	12.0


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

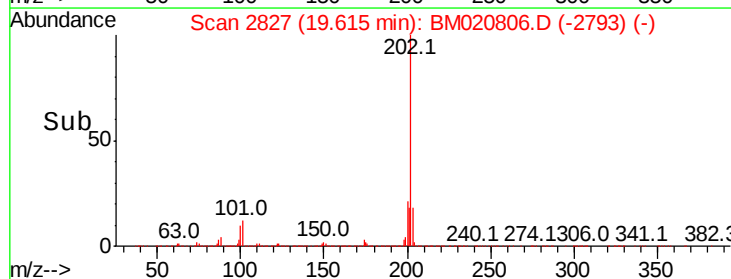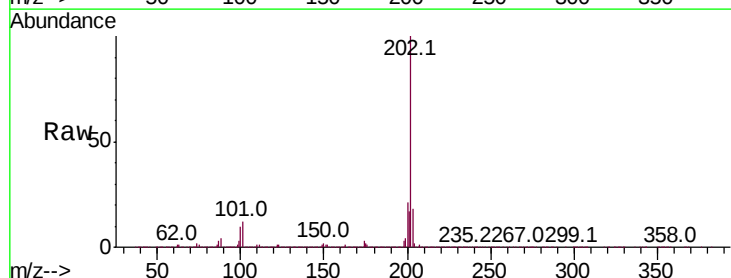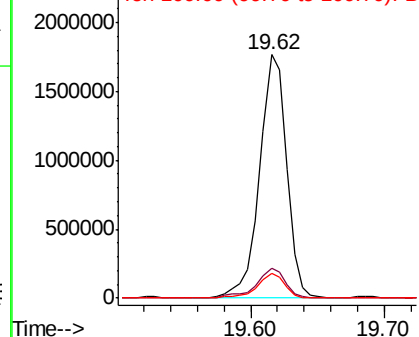

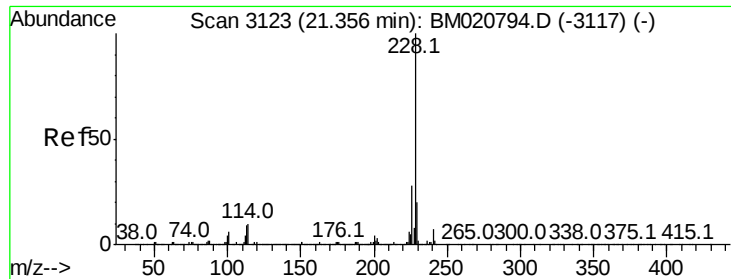





#82
Benzo(a)anthracene
Concen: 19.047 ng/ul
RT: 21.36 min Scan# 3124
Delta R.T. 0.01 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Instrument :
BNA_M
ClientSampleId :
C0AD1DL

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.8	15.6	23.4
226	28.2	21.4	32.2




Manual Integrations
APPROVED


mohammad
6/14/2019 8:41:50 AM

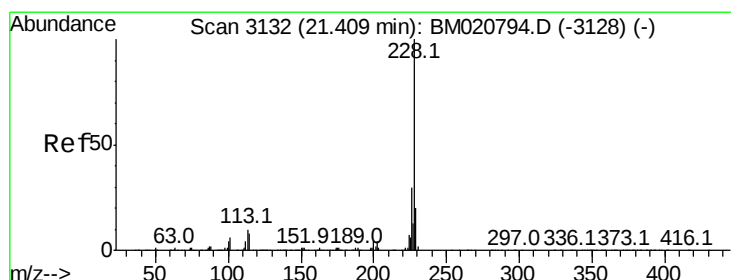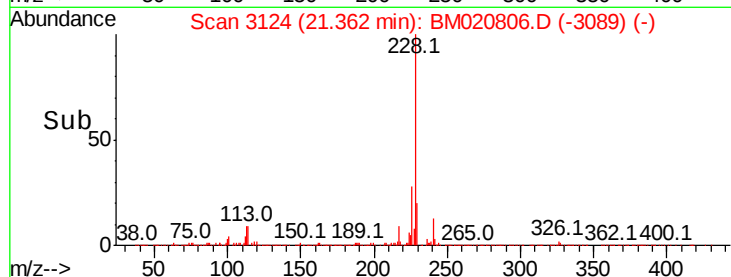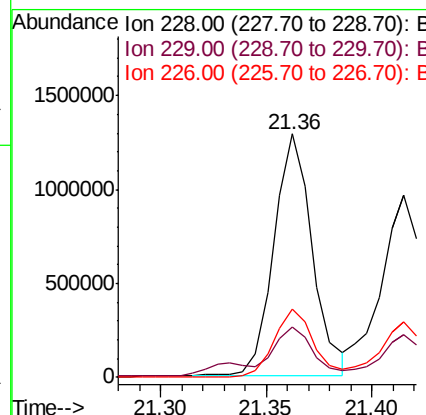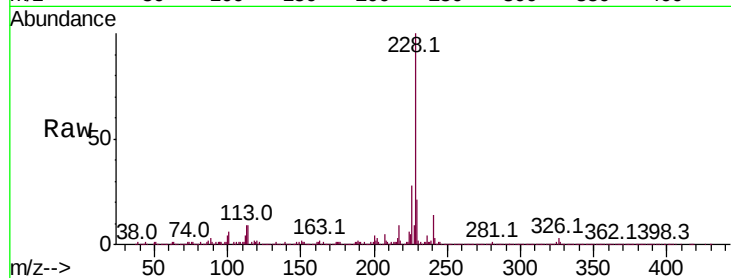

#84
Chrysene
Concen: 16.626 ng/ul
RT: 21.42 min Scan# 3133
Delta R.T. 0.01 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.4	36.6
229	23.1	16.2	24.2

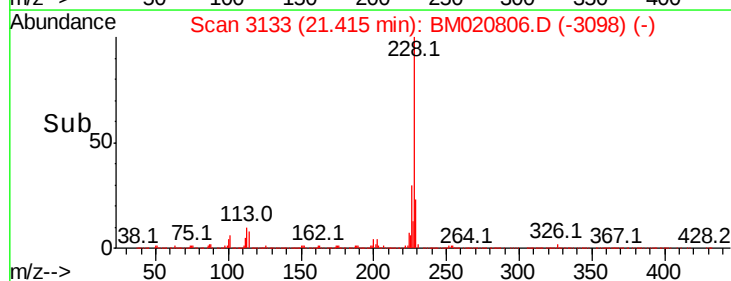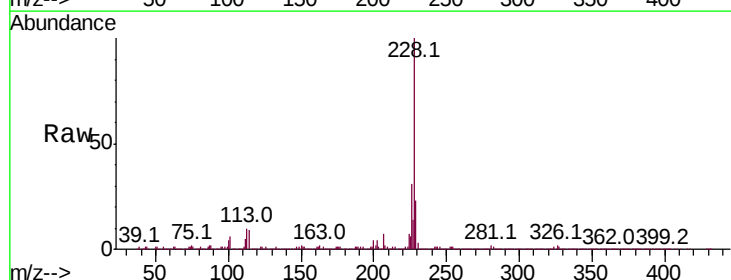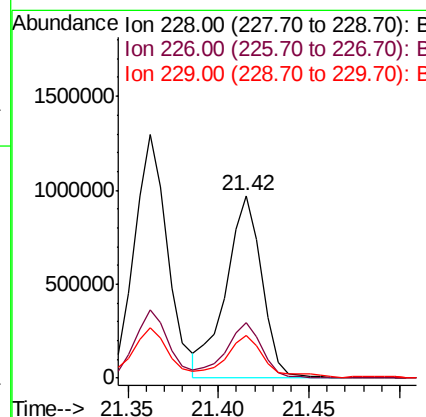

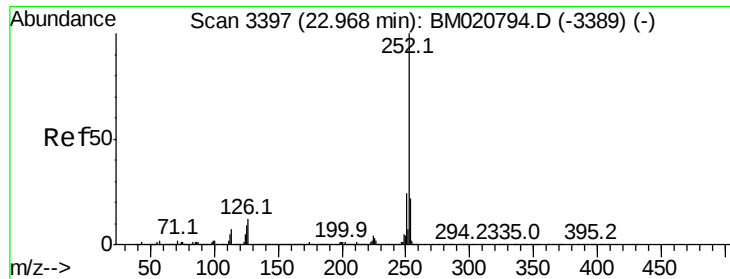

#87

Benzo(b)fluoranthene

Concen: 17.797 ng/ul

RT: 22.98 min Scan# 3399

Delta R.T. 0.01 min

Lab File: BM020806.D

Acq: 07 Jun 2019 16:26





Instrument :
BNA_M

ClientSampleId :
C0AD1DL

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.6	26.4
125	9.6	7.3	10.9

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:50 AM

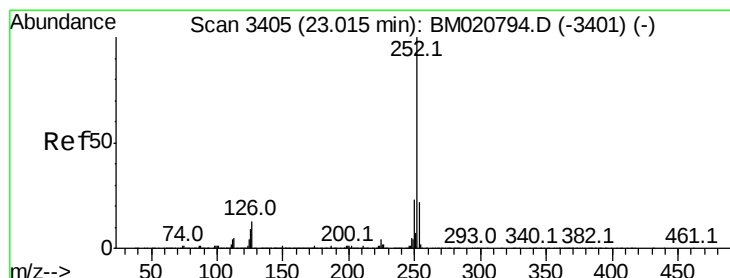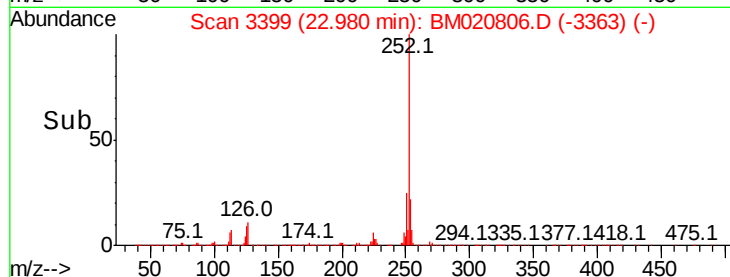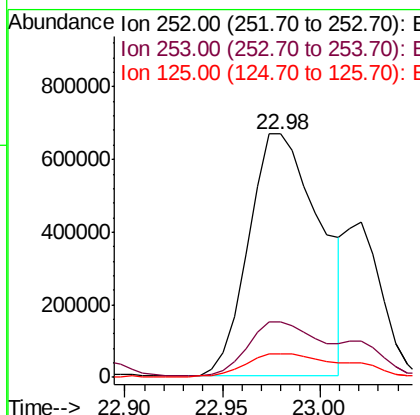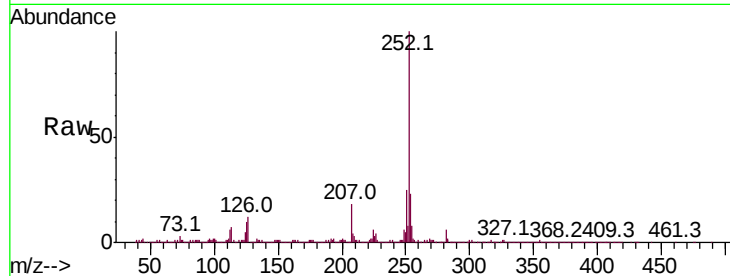

#88

Benzo(k)fluoranthene

Concen: 5.960 ng/ul m




RT: 23.02 min Scan# 3406


Delta R.T. 0.01 min

Lab File: BM020806.D

Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.6	26.4
125	9.3	7.3	10.9

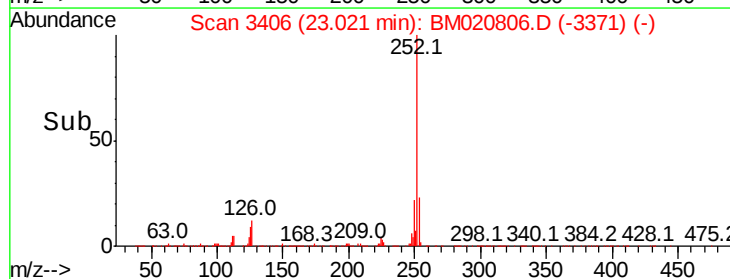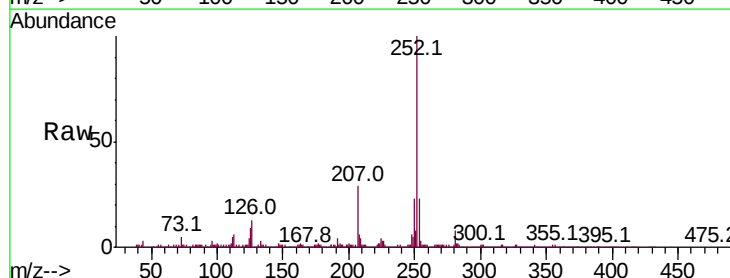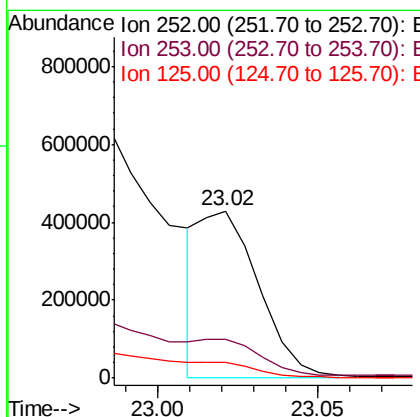

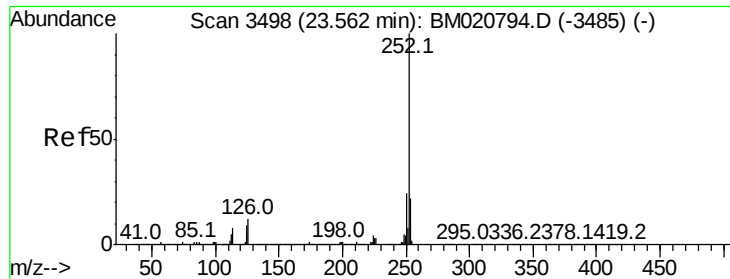

#90

Benzo(a)pyrene

Concen: 12.588 ng/ul

RT: 23.57 min Scan# 3499

Delta R.T. 0.01 min

Lab File: BM020806.D

Acq: 07 Jun 2019 16:26

Instrument :

BNA_M

ClientSampleId :

C0AD1DL

Tot Ion:252 Resp: 1141676

Ion Ratio Lower Upper

252 100


253 22.3 17.0 25.6

125 9.8 8.2 12.4

Manual Integrations
APPROVED

mohammad

6/14/2019 8:41:50 AM



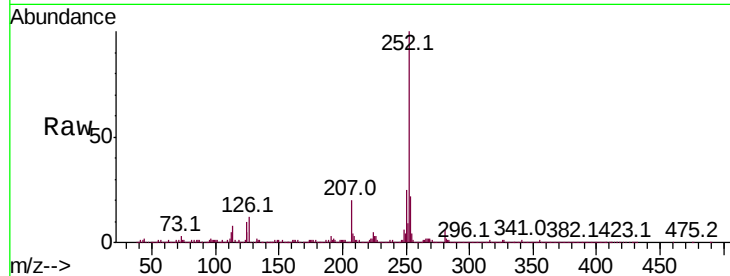


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

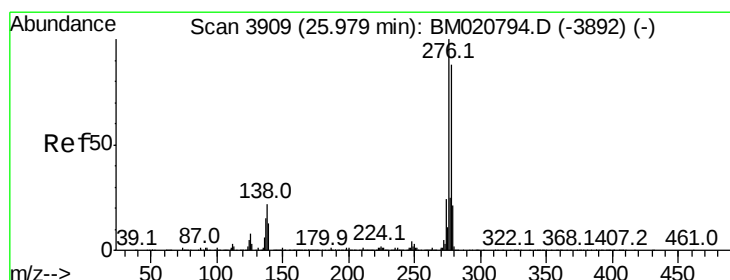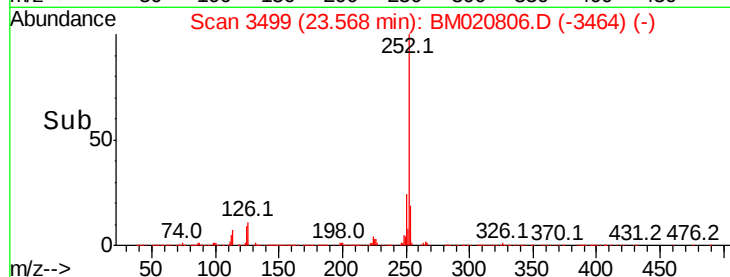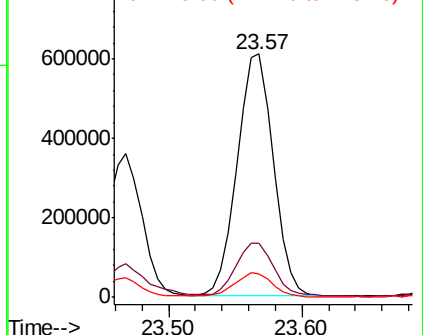

#91

Indeno(1,2,3-cd)pyrene

Concen: 6.412 ng/ul

RT: 25.98 min Scan# 3909

Delta R.T. 0.00 min

Lab File: BM020806.D

Acq: 07 Jun 2019 16:26

Tgt Ion:276 Resp: 686845

Ion Ratio Lower Upper

276 100

138 18.9 17.8 26.8




277 24.4 20.0 30.0


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

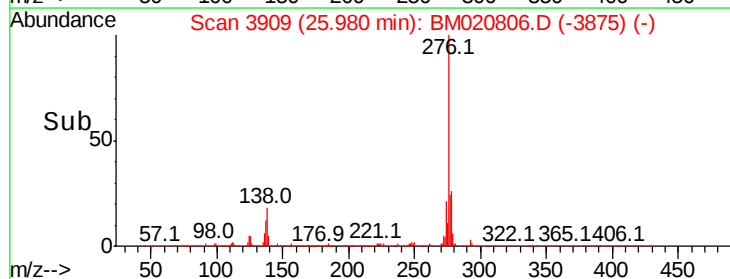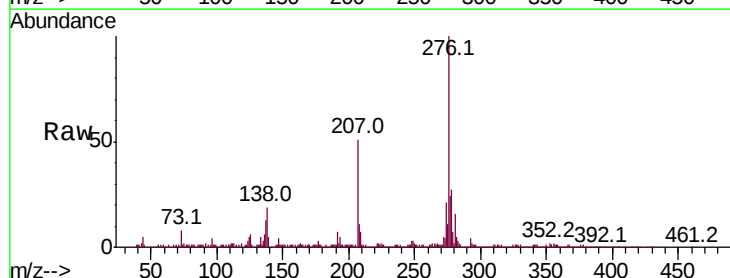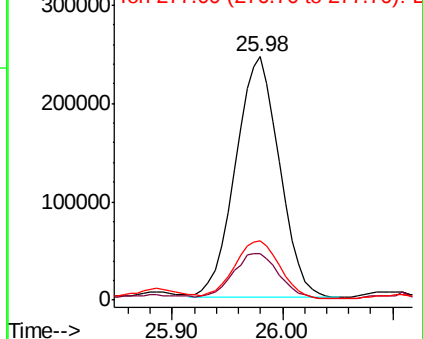

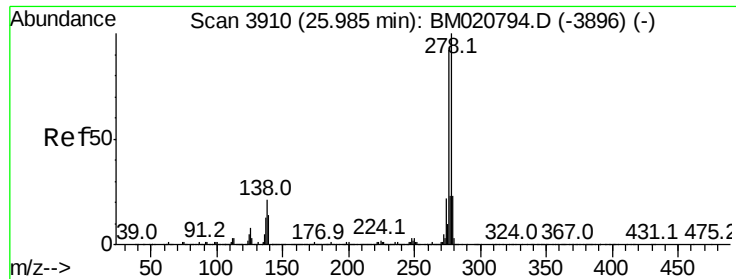





#92
Dibenzo(a,h)anthracene
Concen: 2.398 ng/ul
RT: 25.98 min Scan# 3909
Delta R.T. -0.01 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Instrument :
BNA_M
ClientSampleId :
C0AD1DL

Tot Ion	Ratio	Lower	Upper
278	100		
139	19.9	11.6	17.4#
279	27.2	18.6	28.0

Manual Integrations
APPROVED

mohammad
6/14/2019 8:41:50 AM

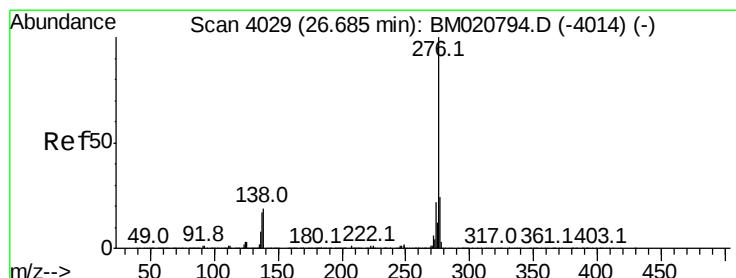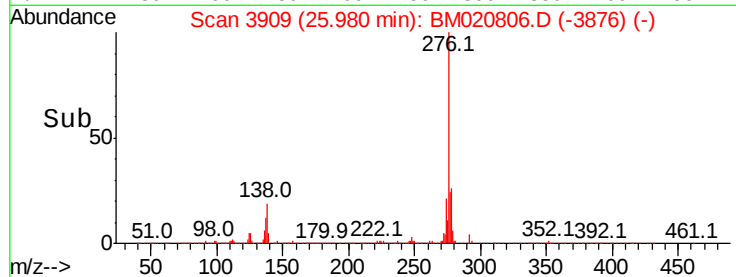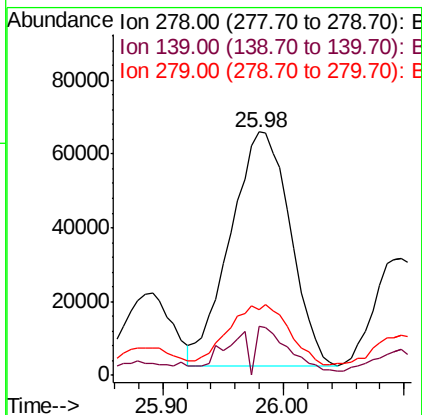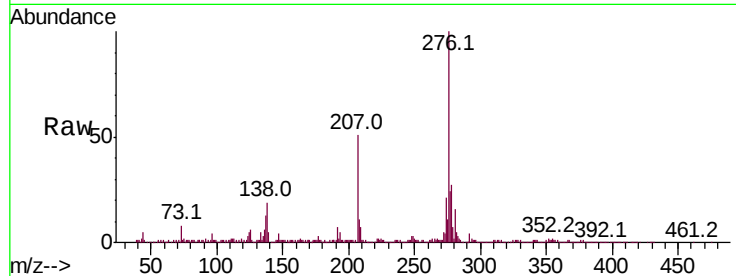

#93
Benzo(g,h,i)perylene
Concen: 5.203 ng/ul
RT: 26.69 min Scan# 4030
Delta R.T. 0.01 min
Lab File: BM020806.D
Acq: 07 Jun 2019 16:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	20.1	16.6	25.0
277	25.3	19.6	29.4

