
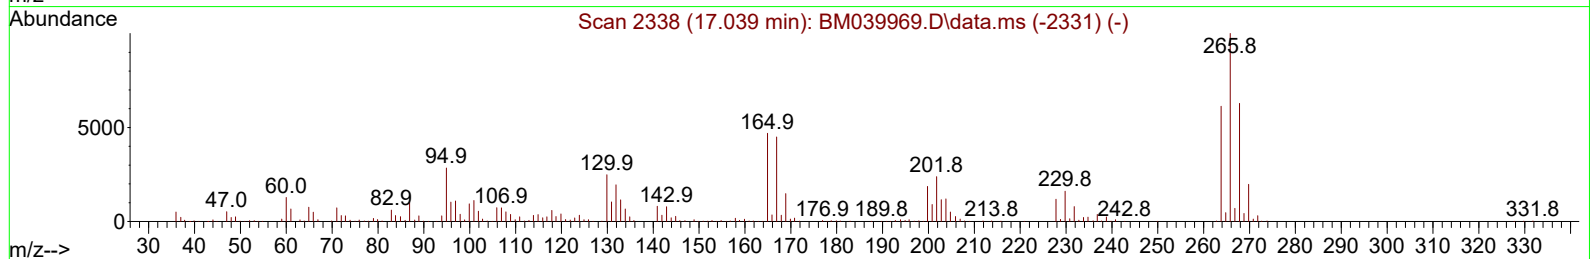
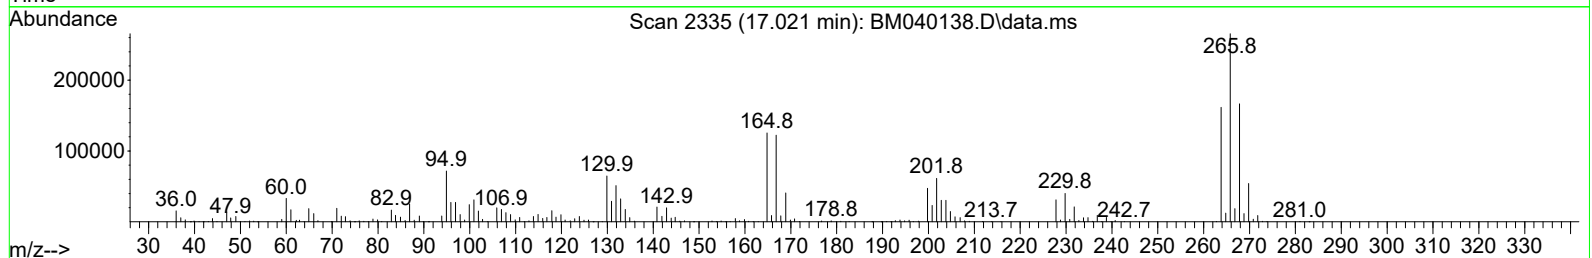


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060723\  
Data File : BM040138.D  
Acq On : 07 Jun 2023 13:07  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 15:20:30 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM052323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 06 16:45:42 2023  
Response via : Initial Calibration

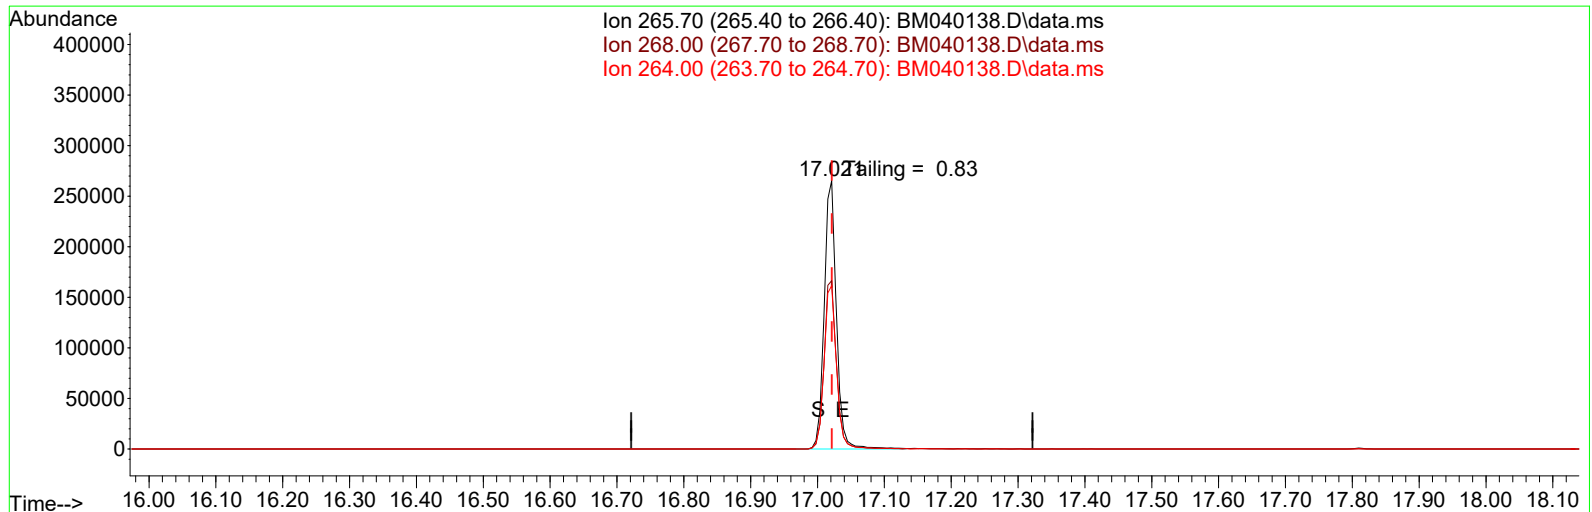

TIC: BM040138.D\data.ms

**(70) Pentachlorophenol (C)**




**17.021min (-0.000) 195736.52 ng**

**response 335859**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.80  | 62.74  |
| 264.00 | 61.30  | 60.89  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060723\  
 Data File : BM040138.D  
 Acq On : 07 Jun 2023 13:07  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 15:20:30 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM052323.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 06 16:45:42 2023  
 Response via : Initial Calibration

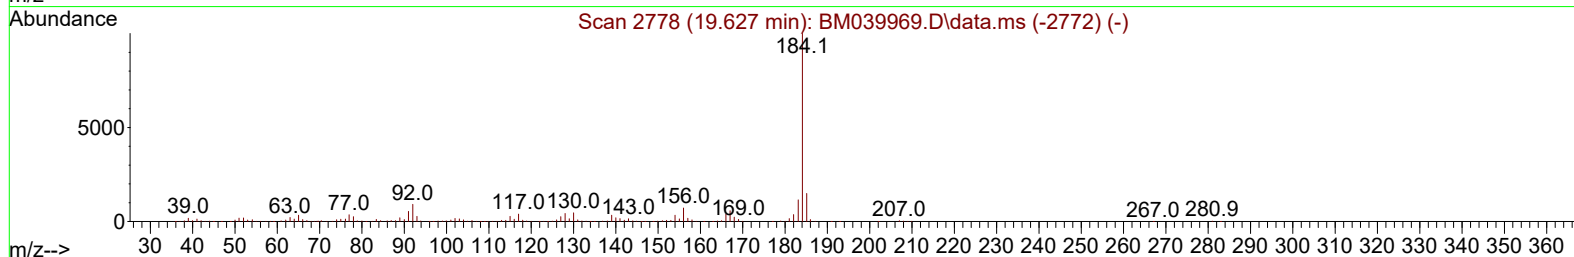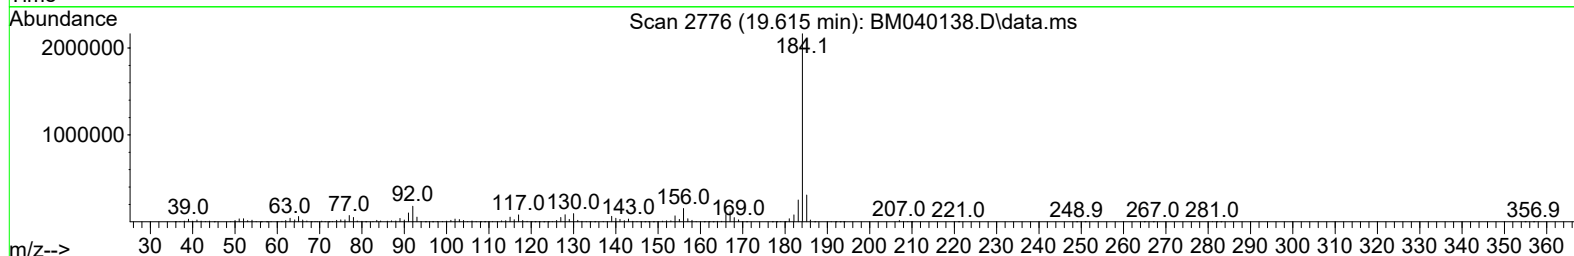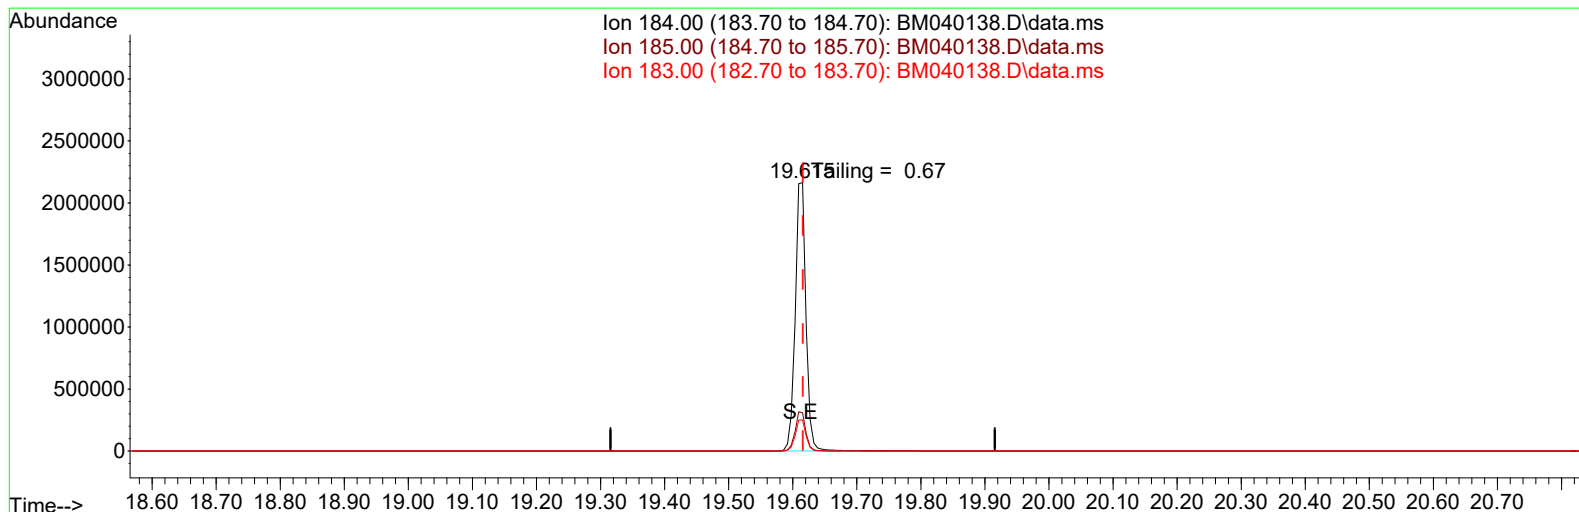

TIC: BM040138.D\data.ms

**(77) Benzidine****19.615min (-0.000) 268265.07 ng****response 2516183**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.25  |
| 183.00 | 11.50  | 11.60  |
| 0.00   | 0.00   | 0.00   |