

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
Data File : BM040140.D
Acq On : 07 Jun 2023 14:19
Operator : MA/JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153266BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	397	rBV	5057124	7269687	39.77%	10.568%
2	7.151	647	657	668	rBV	4884599	7640210	41.80%	11.107%
3	7.993	792	800	808	rBV	731467	1169695	6.40%	1.700%
4	9.157	990	998	1009	rBV	2704525	4192058	22.94%	6.094%
5	10.804	1271	1278	1290	rBV	1033480	1674675	9.16%	2.434%
6	13.257	1688	1695	1708	rBV	7877552	10515913	57.53%	15.287%
7	14.627	1921	1928	1937	rBV	1538483	2089259	11.43%	3.037%
8	16.116	2174	2181	2196	rBV	6155168	8283120	45.32%	12.041%
9	17.368	2388	2394	2407	rBV	1903073	2513341	13.75%	3.654%
10	19.992	2834	2840	2845	rBV	16278730	18277589	100.00%	26.570%
11	21.545	3099	3104	3110	rBV	2136922	2606582	14.26%	3.789%
12	23.986	3512	3519	3530	rBV	1370258	2557481	13.99%	3.718%




Sum of corrected areas: 68789610

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
Data File : BM040140.D
Acq On : 07 Jun 2023 14:19
Operator : MA/JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153266BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

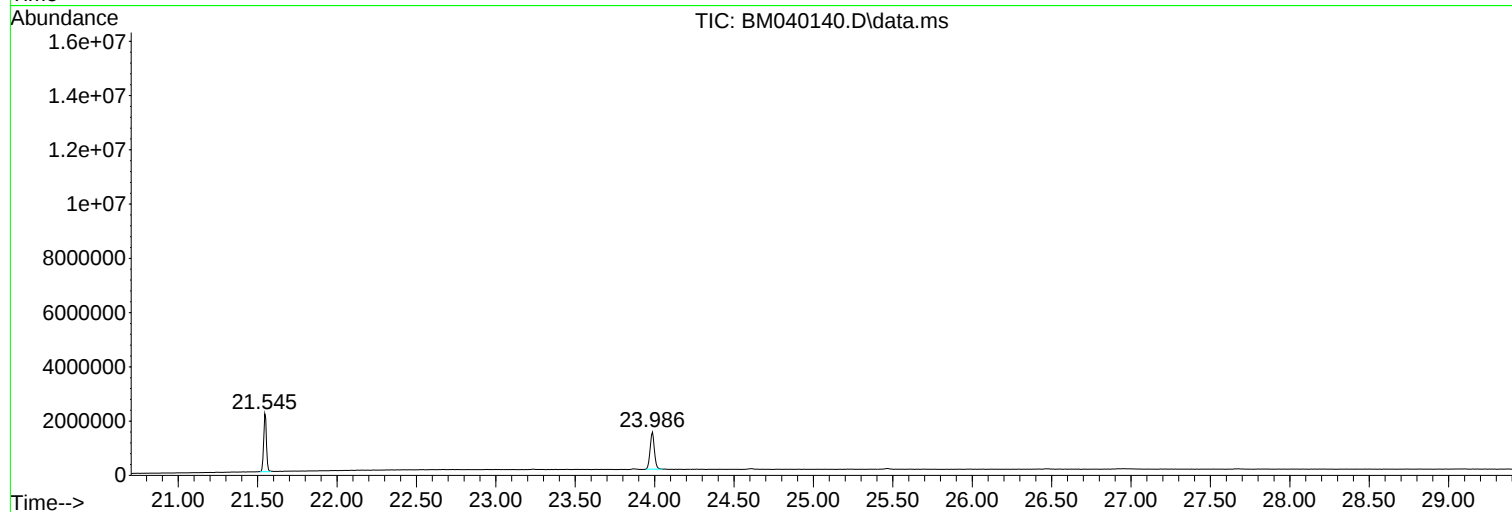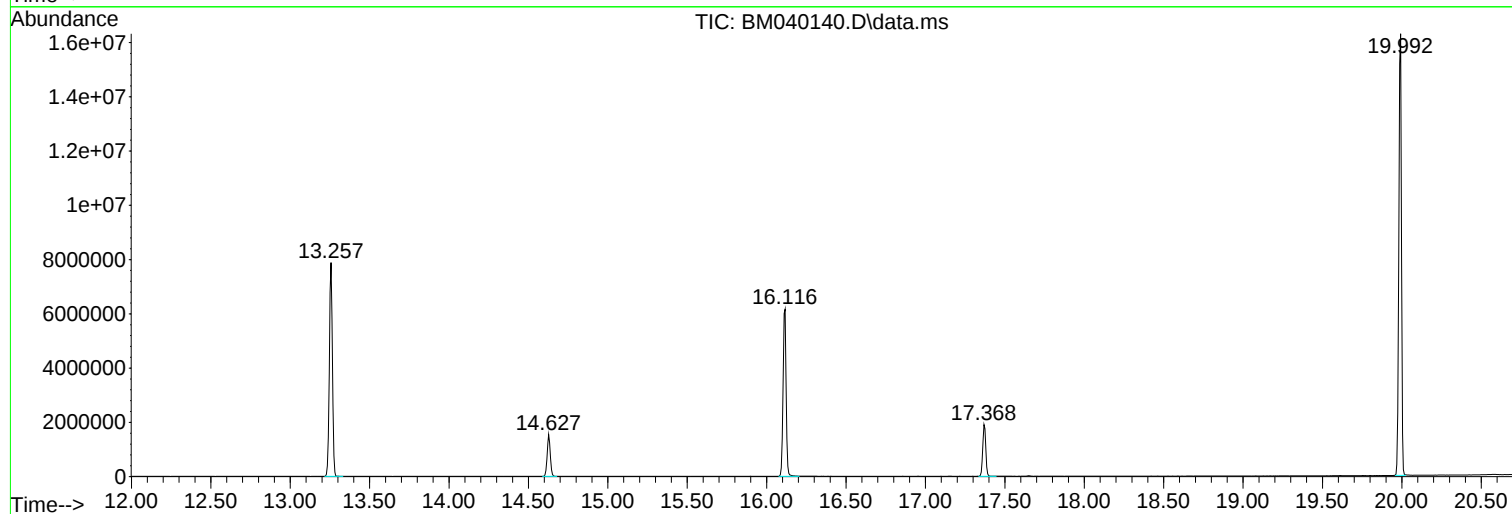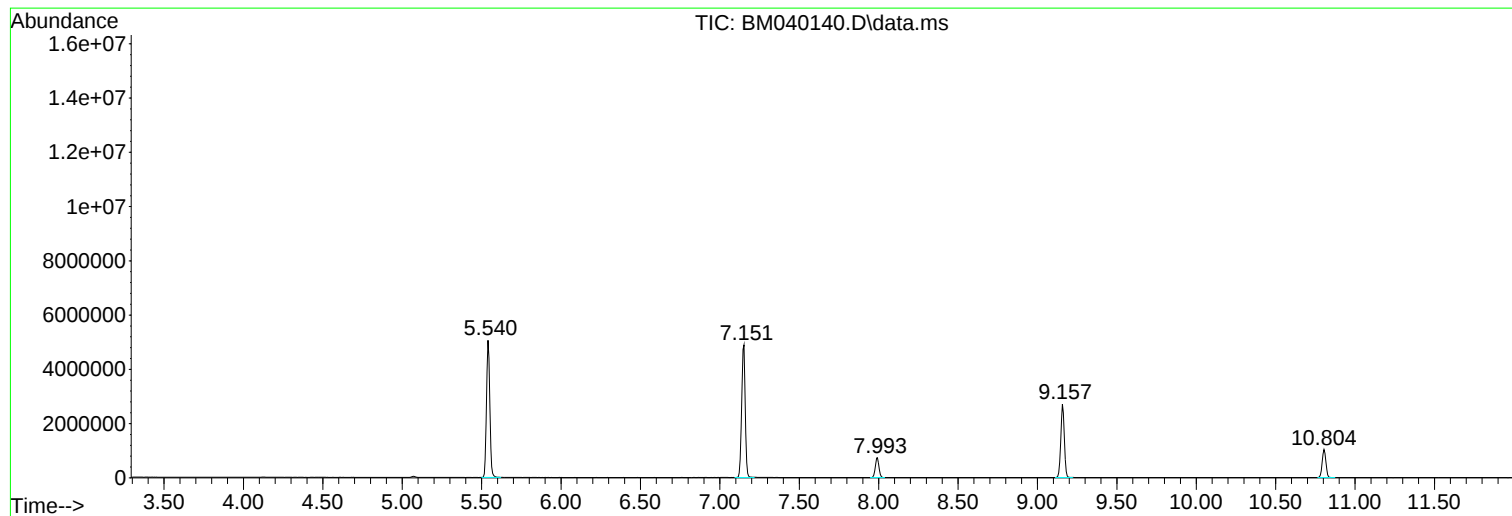

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
Data File : BM040140.D
Acq On : 07 Jun 2023 14:19
Operator : MA/JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153266BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
Data File : BM040140.D
Acq On : 07 Jun 2023 14:19
Operator : MA/JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153266BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------