
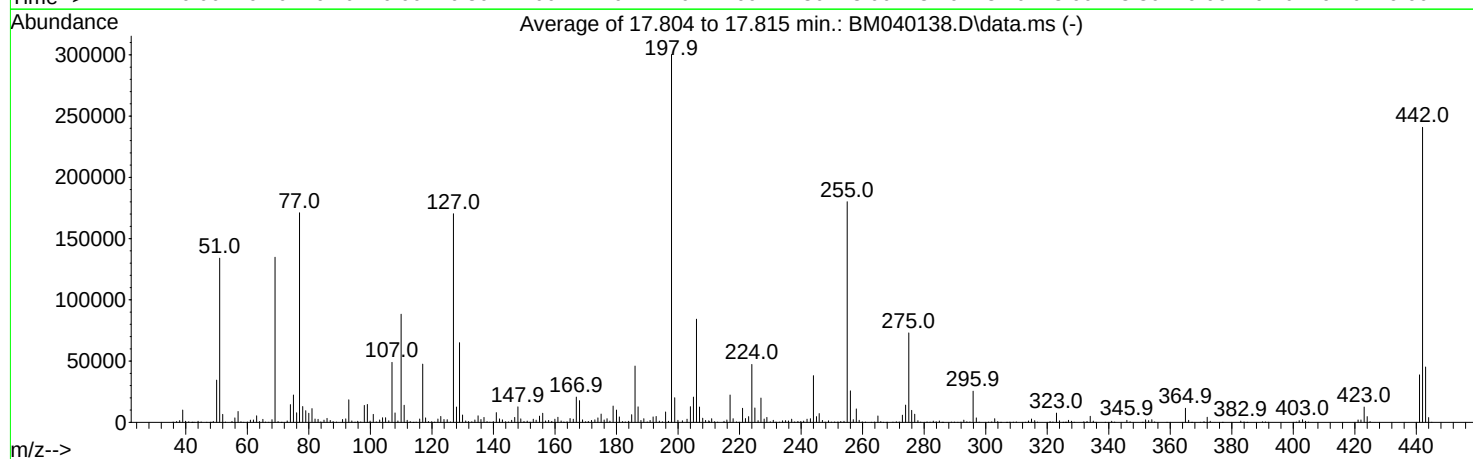


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
 Data File : BM040138.D
 Acq On : 07 Jun 2023 13:07
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 16:45:42 2023

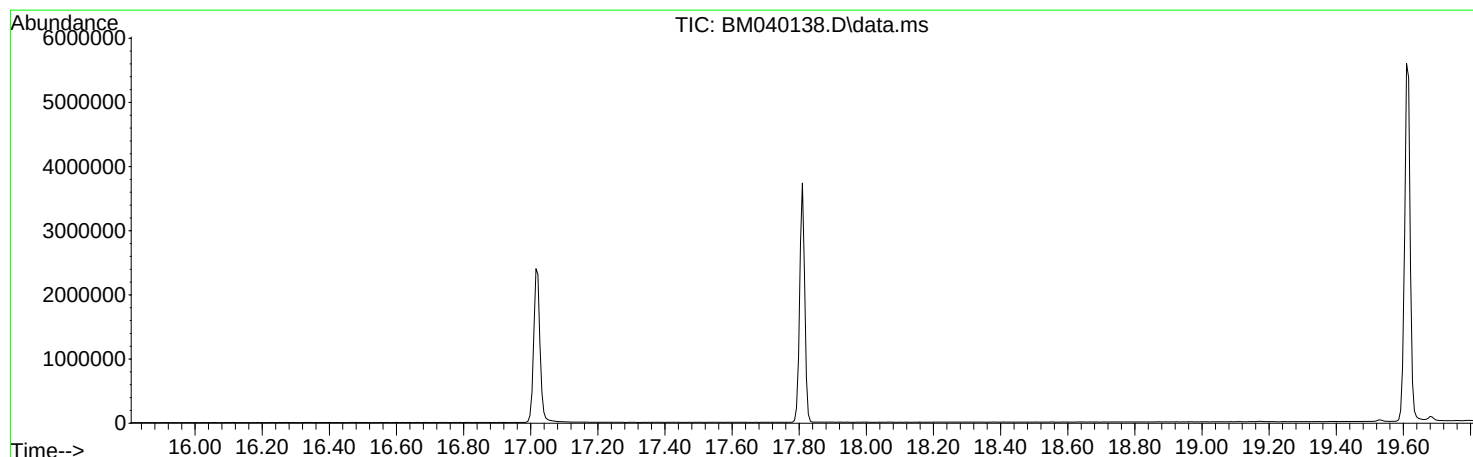

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	134072	PASS
68	69	0.00	2	1.7	2230	PASS
69	198	0.00	100	44.9	134840	PASS
70	69	0.00	2	0.5	722	PASS
127	198	10	80	56.7	170325	PASS
197	198	0.00	2	0.3	952	PASS
198	198	100	100	100.0	300267	PASS
199	198	5	9	6.7	20165	PASS
275	198	10	60	24.3	73021	PASS
365	198	1	100	3.8	11449	PASS
441	198	0.01	100	12.9	38792	PASS
442	442	50	100	100.0	240896	PASS
443	442	15	24	18.8	45181	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/7/2023	BNA_M	<u>BM040138.D</u>
Compound Name	Response	Retention Time
DDT	1047583	20.845
DDD	14808	20.403
DDE	1360	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16168	1063751	1.52

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
 Data File : BM040138.D
 Acq On : 07 Jun 2023 13:07
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 15:20:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 06 16:45:42 2023
 Response via : Initial Calibration

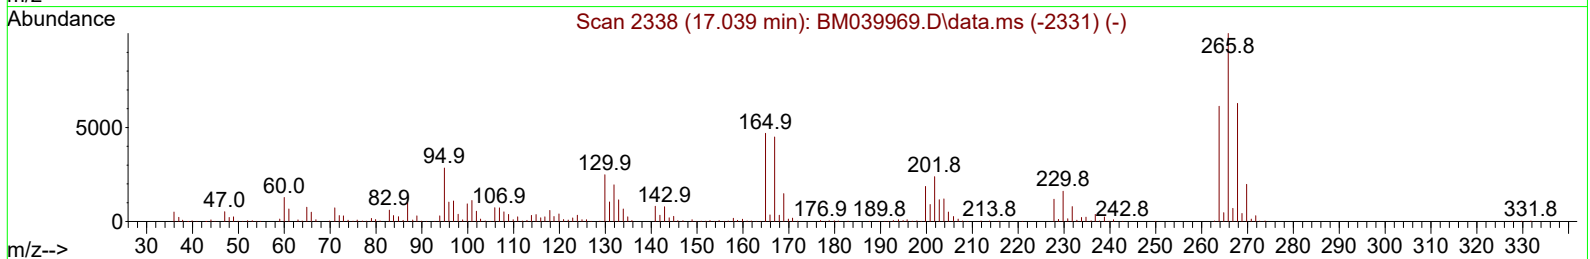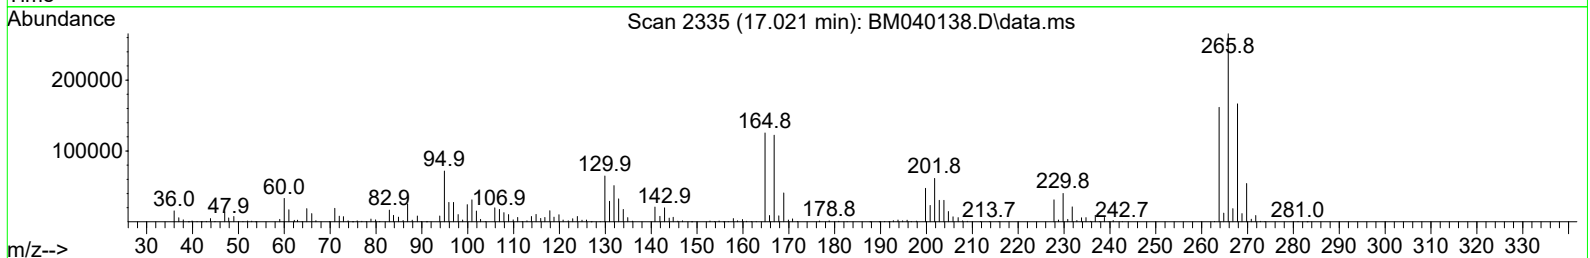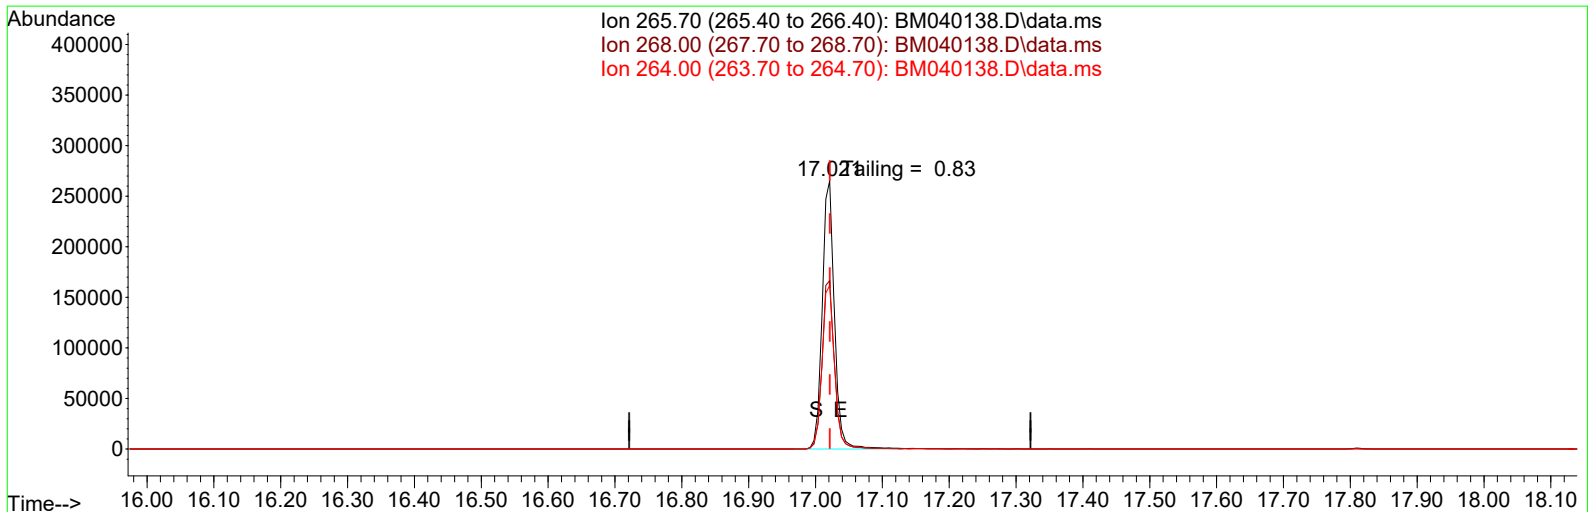

TIC: BM040138.D\data.ms

(70) Pentachlorophenol (C)

17.021min (-0.000) 195736.52 ng




response 335859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.74
264.00	61.30	60.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060723\
 Data File : BM040138.D
 Acq On : 07 Jun 2023 13:07
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 15:20:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 06 16:45:42 2023
 Response via : Initial Calibration

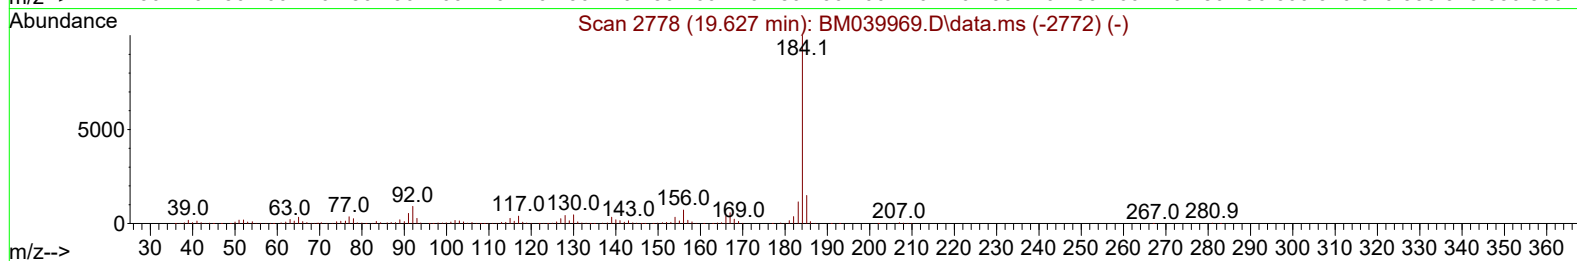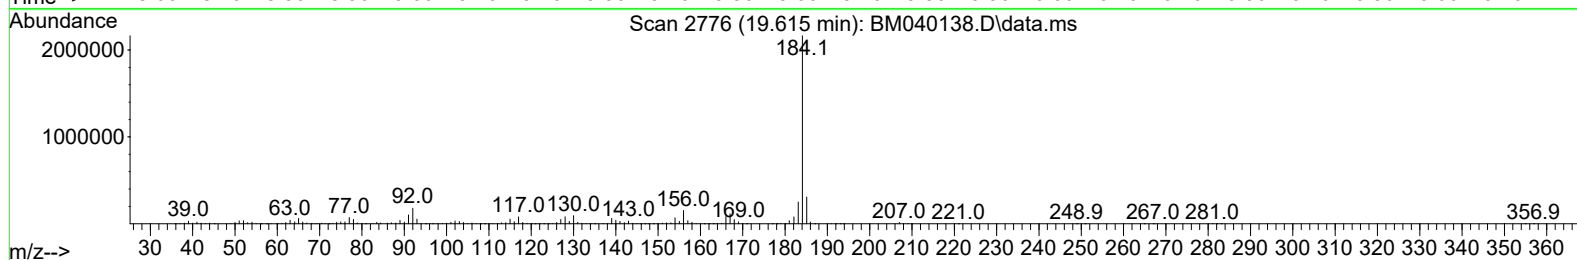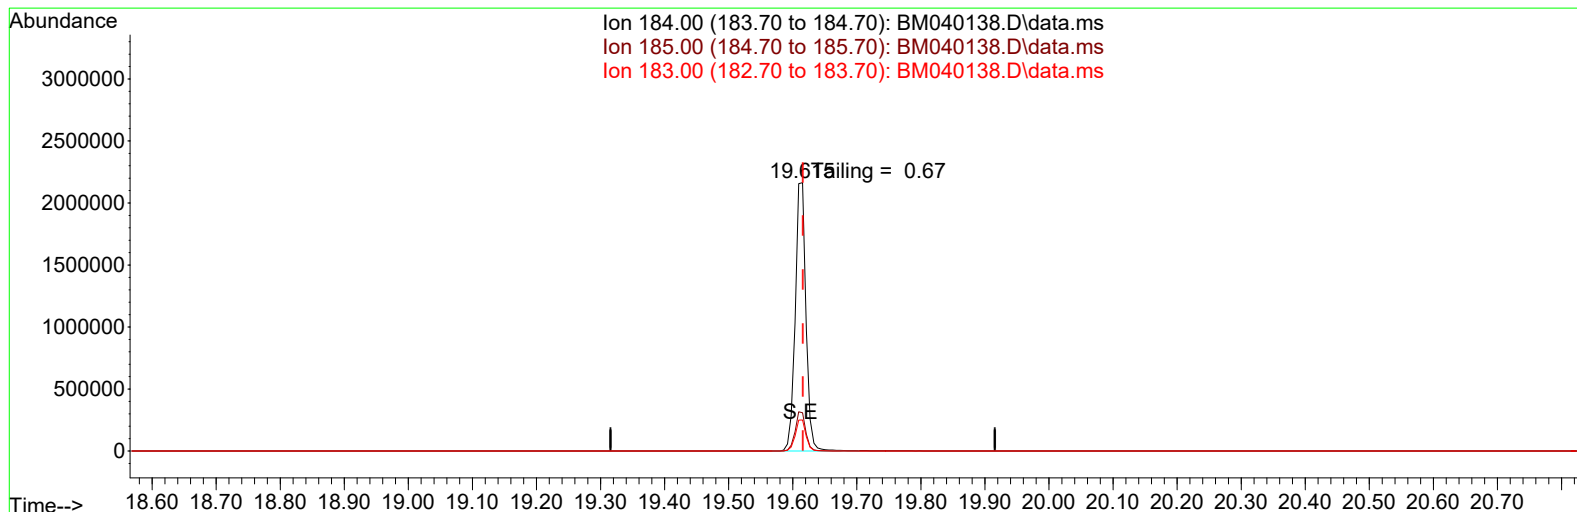

TIC: BM040138.D\data.ms

(77) Benzidine

19.615min (-0.000) 268265.07 ng

response 2516183

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.25
183.00	11.50	11.60
0.00	0.00	0.00